

DIKMA[®]
A reliable partner for your lab

CHROMATOGRAPHY

2012/2013



Dikma Technologies Inc.
www.dikmatech.com

Table of Contents

HPLC Columns.....	3
Endeavorsil™ Columns	5
Leapsil™ Columns.....	15
Inspire™ Columns	21
Spursil™ Columns	31
Bio-Bond™ Columns.....	52
Platisil™ Columns.....	54
EasyGuard™ Guard Columns.....	55
Preparative Chromatography	56
GC Columns.....	64
GC Column Selection.....	64
GC Guard Columns.....	66
DikmaCap™ (DM) Capillary Columns.....	67
Sample Preparation	101
ProElut™ SPE Cartridges	102
ProElut™ QuEChERS	119
ProElut™ Liquid-Liquid Extraction	123
ProMax™ Syringe Filters.....	124
Autosampler Vials.....	126
Applications and Index.....	129
HPLC Applications	130
GC Applications	151
SPE Applications	213
Compound Index.....	233
Product Index	240

Terms and Conditions

1. CONDITIONS

The information published by Dikma is, to the best of its knowledge, correct and accurate but is not guaranteed to be so. Dikma assumes no responsibility with respect thereto and has not verified the values or specifications stated experimentally and does not guarantee their accuracy. The sale of any products by Dikma does not waive any patent restrictions connected with those products. Buyer agrees and represents that it is buying for its own end use only, and not for resale. Buyer warrants that they have sufficient knowledge, training, facilities and skills to safely use and store products provided under this agreement.

2. USE OF PRODUCTS

The products offered are for laboratory or manufacturing use only. They are not intended for medicinal or food use.

3. QUALITY

All purchases are subject to Dikma approval notwithstanding prior payments, and if not in accordance with the specifications at Dikma sole option, may be returned to Dikma at Buyer's expense for transportation. Dikma reserves the right to change product specifications, quantities, designs or prices without notice and without liability for such changes.

4. PRICE

The price(s) set forth in any Dikma Order Acknowledgement are firm and shall not be changed without the prior written consent of Dikma. If no price is specified in this Purchase Order, the goods shall be invoiced at the current list price.

5. PAYMENT

Payment will be due thirty (30) days from receipt on approved credit. All shipments are F.O.B. factory.

6. SHIPMENT

Shipment of the goods shall be made in accordance with customary shipping practices for such goods. Unless otherwise stated in the Order Acknowledgement, no charge will be allowed for packing, boxing, cartage or insurance and Buyer shall absorb and pre-pay all shipping and insurance charges. Goods ordered in error or duplicated from a mailed-in order not clearly marked "CONFIRMING" will be subject to a 20% restocking charge, if approved by Dikma.

7. DELIVERY

Buyer shall notify Dikma immediately of any situation that may delay or threaten to delay the timely acceptance of services and/or receipt of goods. Dikma, at its option, may cancel all or any portion of this Order Acknowledgement without liability. Acceptance of all or part of the goods, or payment therefore, or failure to notify Buyer promptly shall not waive or affect Dikma's right to cancel the order or recover damages.

8. RETURNS

No returns will be accepted without prior authorization, and are subject to approval by Dikma. If it is necessary to return goods to Dikma for any reason, please contact your Technical Representative for forwarding instructions. This procedure will prevent delays and enable us to resolve the situation to your satisfaction. Dikma is not liable for goods returned without authorization. Returns must be sent through a traceable carrier.

9. WARRANTY

Dikma will repack, replace, or refund charges on any column at our discretion at no cost if a column fails to perform satisfactorily. Columns being returned must have prior return authorization granted by Dikma. Defective products must be accompanied by a written explanation of failure. Approval is subject to the following exclusions:

- a. All columns must be tested upon receipt and all deficiencies must be reported to Dikma no later than 15 days after the date of receipt of the column.
- b. Maximum warranty period is limited to 60 days on HPLC columns unless previously agreed upon. However, columns may not be returned for refund or credit after 30 days or without prior authorization.
- c. Removal of column end-fittings automatically voids column warranty.
- d. Column performance warranty is limited to the conditions of the original test chromatogram.
- e. Physical damage to the column due to misuse, abuse, or mishap, including mechanical shock.
- f. Chemical damage to the packing material due to operation at incorrect chemical conditions, temperatures, or pressures.
- g. Failure due to high backpressures caused by improper solvent or sample filtration practices causing particulate build-up or precipitation or sample fouling in the column or end-fitting.
- h. Incorrect selection of packing material made by customer for their particular use or incompatibility of equipment, etc.

For products supplied by, but not manufactured by Dikma, the warranty is limited by the terms of the original manufacturer's warranty.

HPLC Columns

Endeavorsil™ Columns	5
Leapsil™ Columns	15
Inspire™ Columns	21
Spursil™ Columns	31
Bio-Bond™ Columns	52
Platisil™ Columns	54
EasyGuard™ Guard Columns	55
Preparative Chromatography	56



Dikma HPLC Columns


About Dikma HPLC Columns

Dikma has over 15 years of R&D experience in HPLC columns. Dikma HPLC columns have been widely used by pharmaceutical manufacturers. We offer columns of ultimate performance and maximum versatility to address the challenges and increasing needs of today's chromatographic laboratories.

The quality of packing material is the basis for all good chromatographic separation. Dikma is in a unique position to control the manufacturing process from start to finish, from making the high-purity (99.999%) raw silica to applying different bonding chemistries. Furthermore, to ensure the high performance and robustness of our columns, we maintain tight specifications during all stages of the manufacturing process and follow rigid, audited ISO 9001 procedures to guarantee reproducible products. The end results that get delivered to you are columns that perform at their best, and offer you highly reproducible batch-to-batch results without alteration of HPLC conditions.

Dikma silica of ultra-purity and incredible smoothness

Dikma silica is extremely pure (99.999%) and free of metals. Meticulous care is given to the quality control of surface smoothness, particle shape uniformity, pore structure and pore consistency to ensure uniformity of particle structure and enhanced mechanical strength. Low percentages of fines from damaged silica particles strengthen the column bed, leading to low backpressure and enhanced column performance and lifetime.



Features of Endeavorsil™ Columns


- Combined speed, resolution and sensitivity
- Reduced analysis time and solvent waste
- High efficiency combined with high selectivity generates more information and productivity
- Superior column performance at higher pressure
- Excellent separation characteristics over wide pH range




Endeavorsil™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Purity (%)	Phase density (µmol/m ²)	Carbon loading (%)	pH range	Endcapping
C18	1.8	120	300	> 99.999	3.5	20	1.5 - 9	Yes

Speed

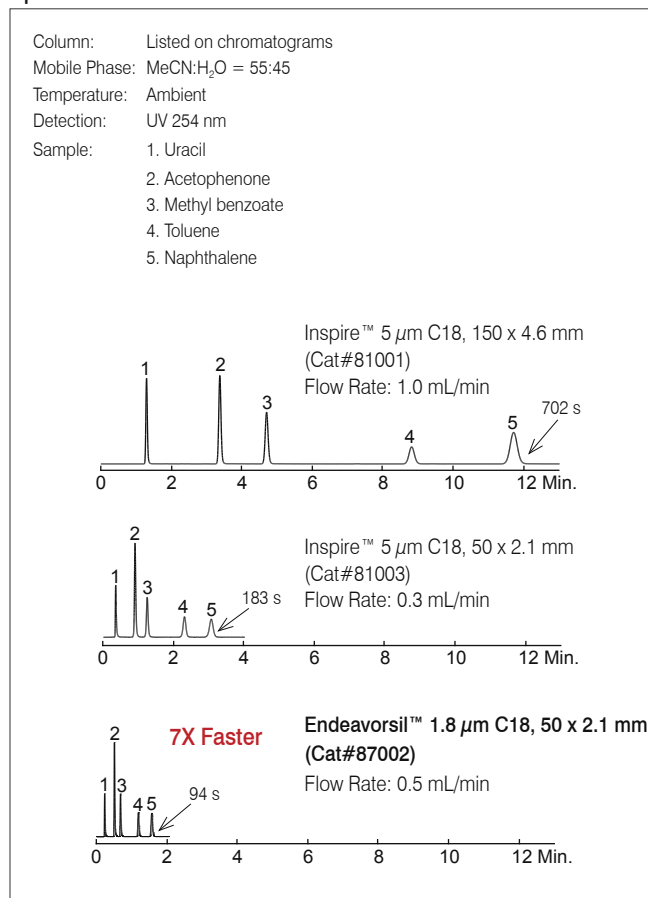

Selectivity*

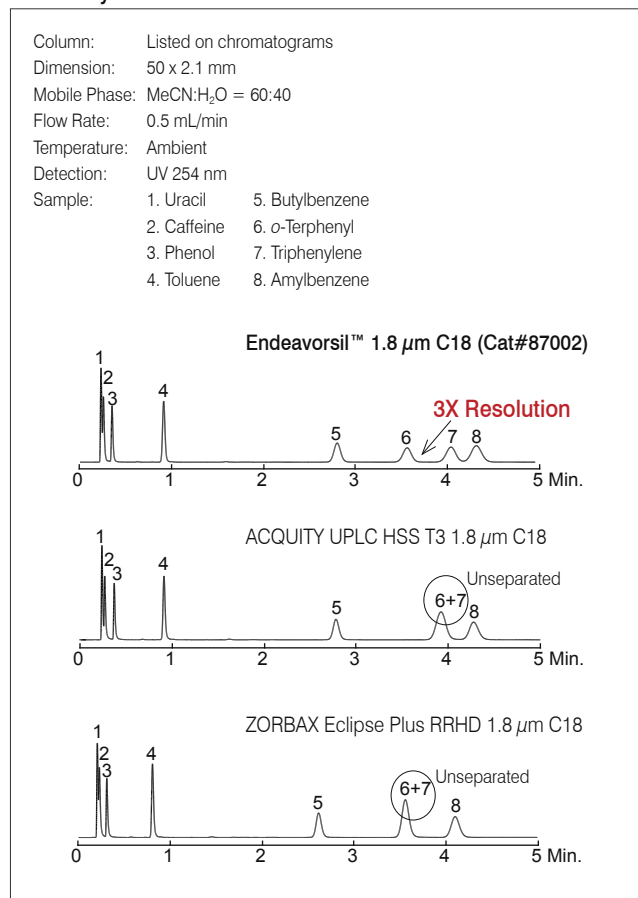

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.





Endeavorsil™ Ordering Information

1.8 µm Microbore Columns (2.1 mm)

Phase	30 x 2.1	Price	50 x 2.1	Price	100 x 2.1	Price
Endeavorsil™ C18	87001	\$715	87002	\$725	87003	\$735




Separation of Hydrophobic, Polar and Basic Mixture*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:20 mM phosphate buffer (pH 7) = 80:20
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Butyl paraben
 3. Dipropyl phthalate
 4. Naphthalene
 5. Acenaphthene
 6. Amitriptyline

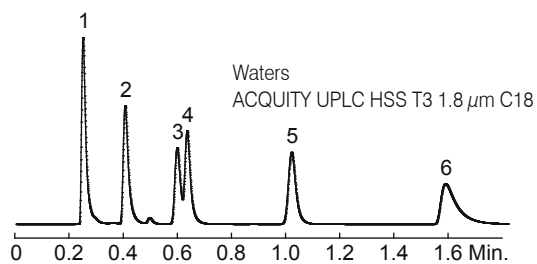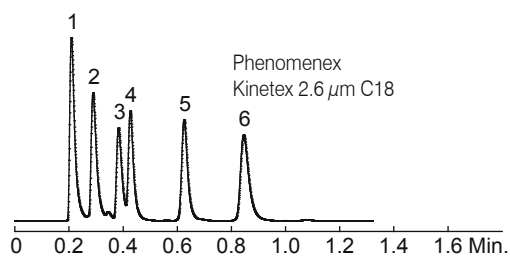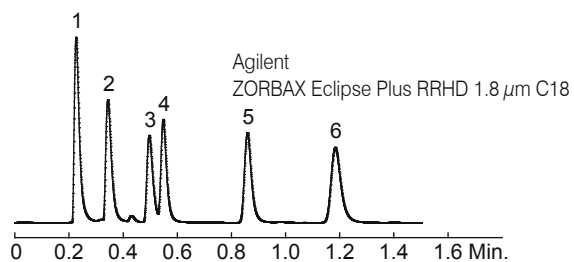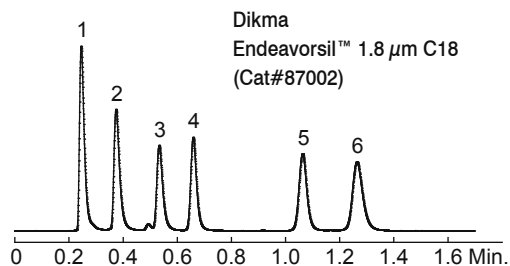

Strong Basic Compounds at Neutral pH

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:20 mM phosphate buffer (pH 7) = 65:35
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Pyridine
 2. Codeine
 3. Quinine
 4. Nortriptyline
 5. Diphenhydramine

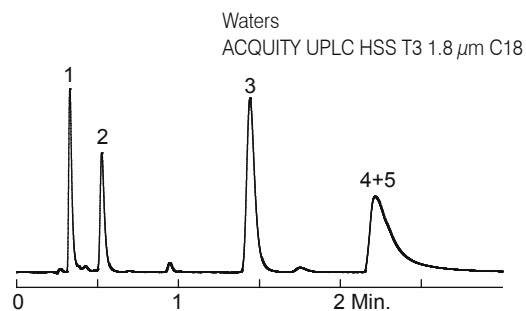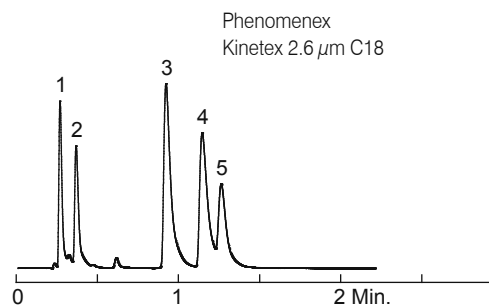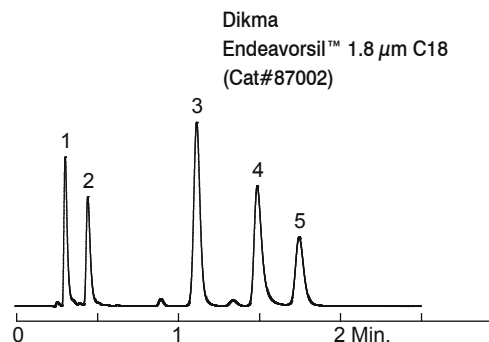

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


Cold Medicine*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 35:65
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Doxylamine
 2. Acetaminophen
 3. Acetanilide
 4. Acetylsalicylic acid
 5. Salicylic acid


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

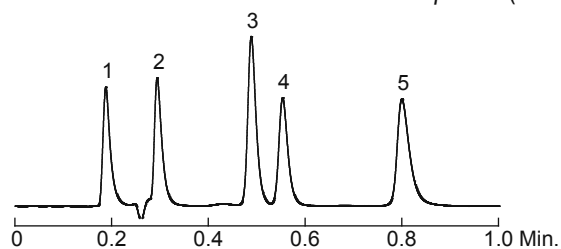


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

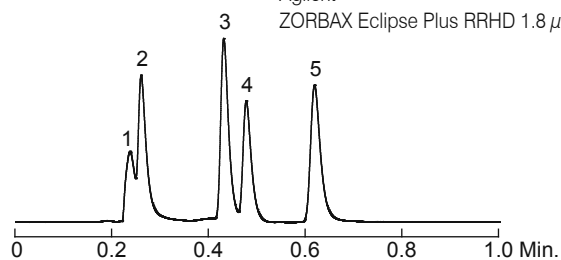

Phenomenex
 Kinetex 2.6 μm C18

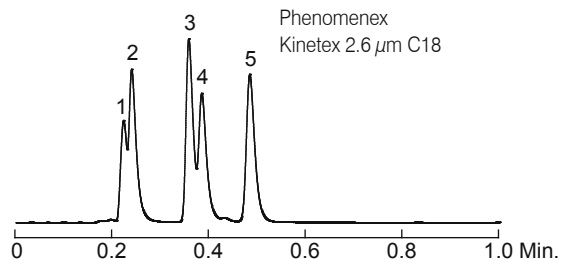


Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

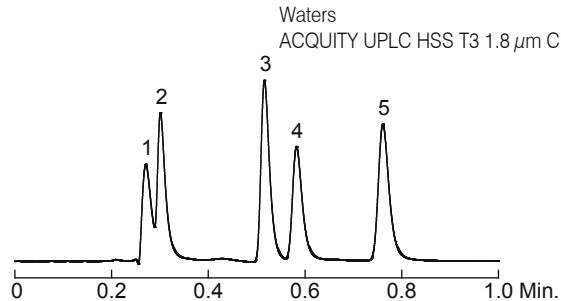


Water-Soluble Vitamins

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 10 mM NH₄COOH, pH 3
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Pyridoxamine
 2. L-Ascorbic acid
 3. Pyridoxal
 4. Nicotinamide


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

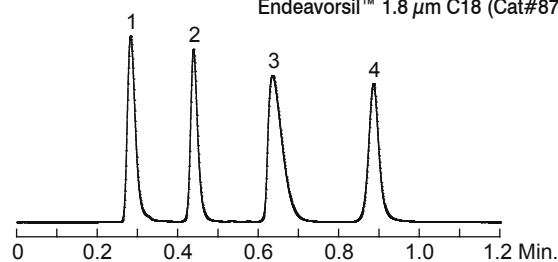


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

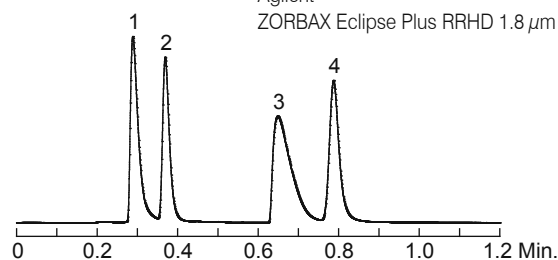

Phenomenex
 Kinetex 2.6 μm C18

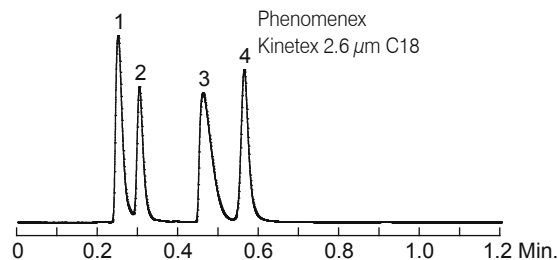

Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

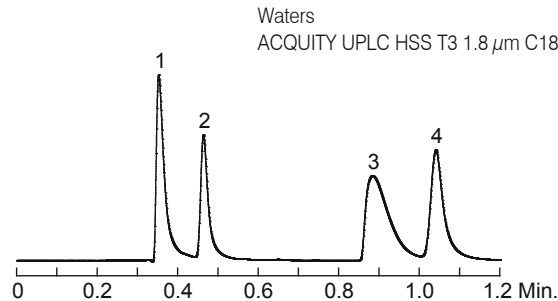

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.


*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Endeavorsil™


Galushko Test*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:H₂O = 50:50
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Aniline
 3. Phenol
 4. Benzene
 5. Toluene


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

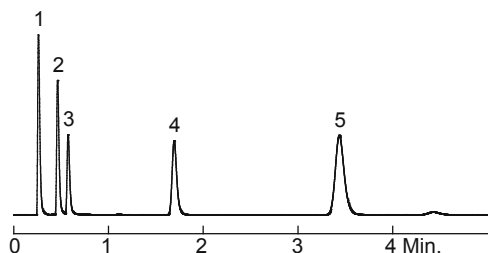


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

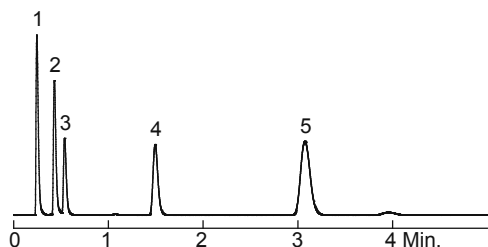

Phenomenex
 Kinetex 2.6 μm C18

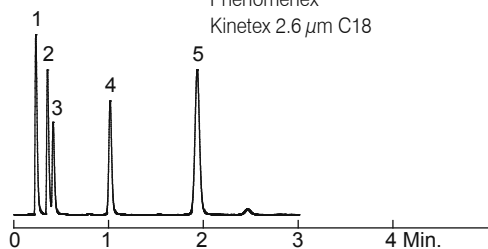


Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

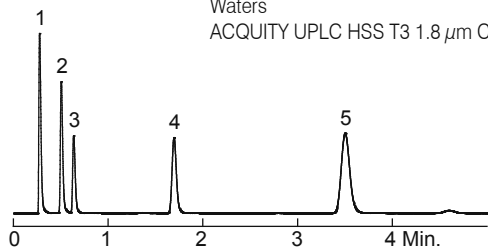


Verzele Test

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:0.5% CH₃COONa (pH 7.8) = 60:40
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Acetylacetone
 2. 1-Nitronaphthalene
 3. Naphthalene


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

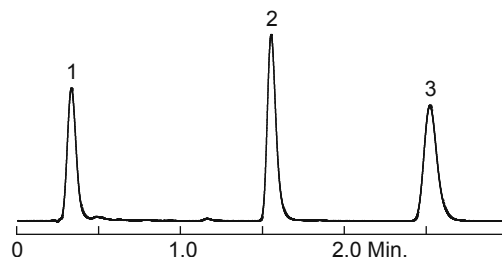


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

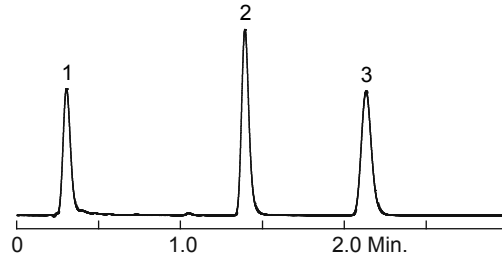

Phenomenex
 Kinetex 2.6 μm C18

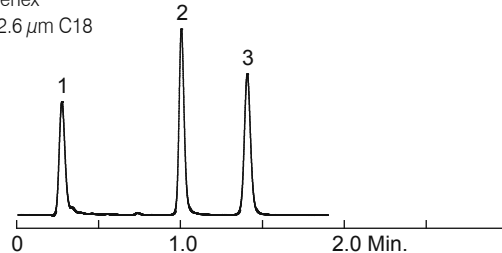

Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

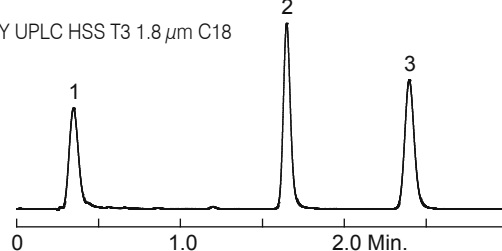

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


Parabens*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeCN:20 mM K₂HPO₄ (pH 7) = 50:50
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Methyl paraben
 2. Ethyl paraben
 3. Propyl paraben
 4. Butyl paraben


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

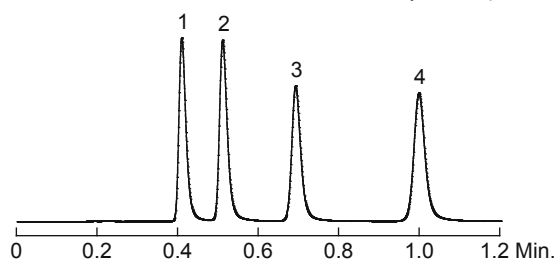


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

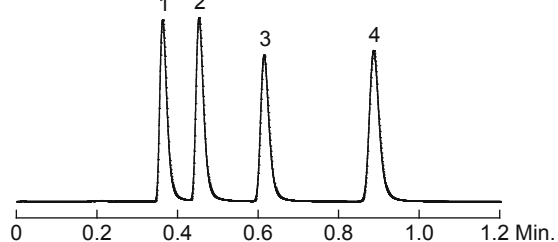

Phenomenex
 Kinetex 2.6 μm C18

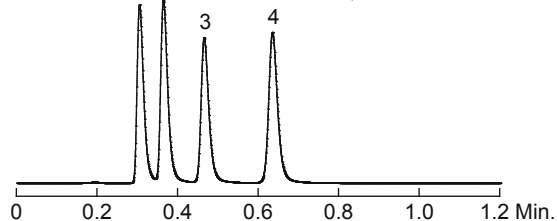


Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

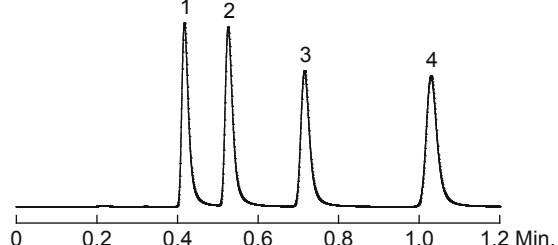


Catecholamines

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% TFA in H₂O
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample: 1. Norepinephrine
 2. Epinephrine
 3. Dopamine


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

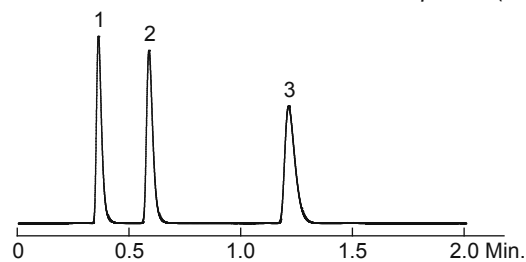


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

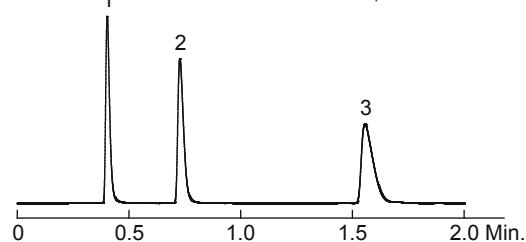

Phenomenex
 Kinetex 2.6 μm C18

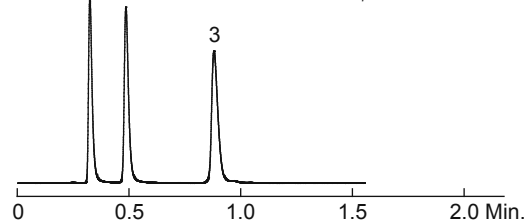

Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

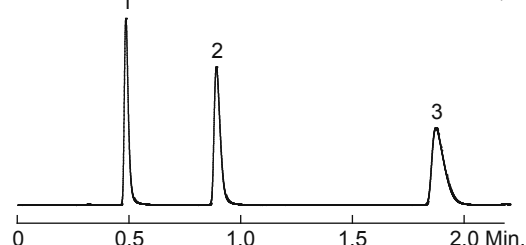

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.





*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Endeavorsil™





β-Blockers at Neutral pH*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 30:70
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Metoprolol
 4. Labetolol
 5. Propranolol

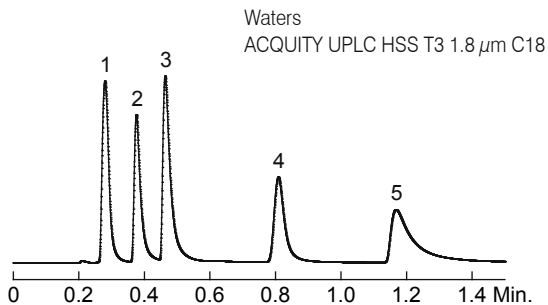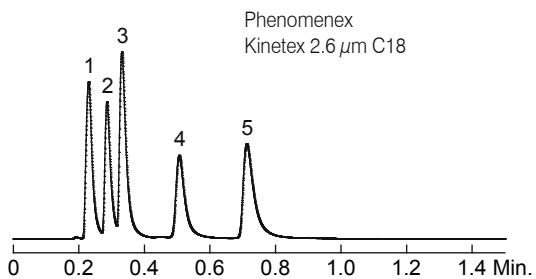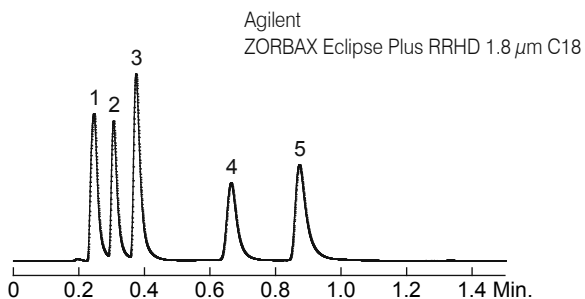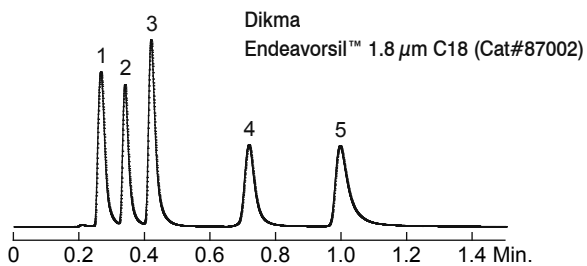

β-Blockers at Low pH

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 25:75
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Acebutolol
 4. Metoprolol
 5. Labetolol
 6. Propranolol
 7. Alprenolol

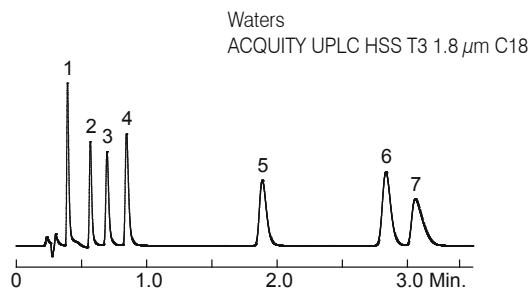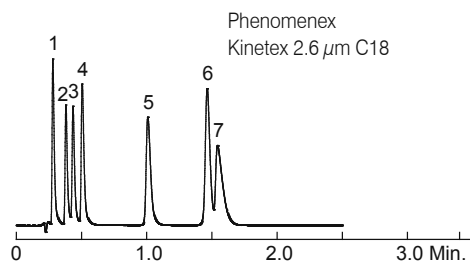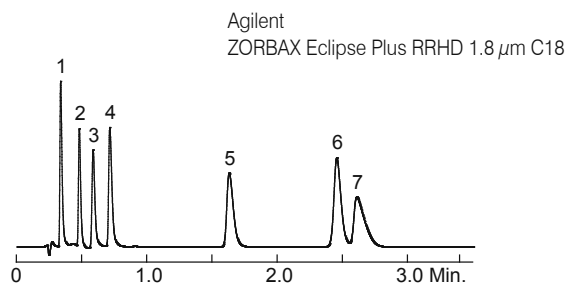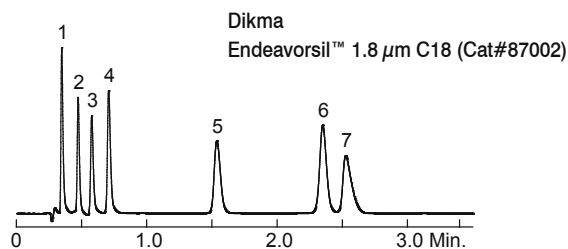

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


TCAs at Low pH*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 35:65
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Doxepin 4. Amitriptyline
 2. Desipramine 5. Trimipramine
 3. Nortriptyline 6. Clomipramine


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

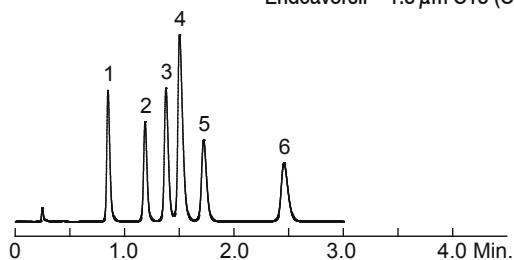


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

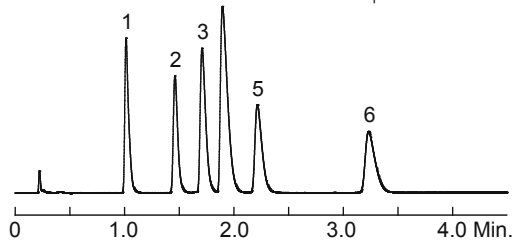

Phenomenex
 Kinetex 2.6 μm C18

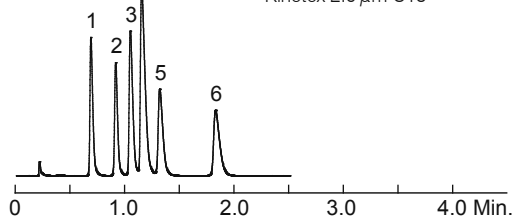


Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

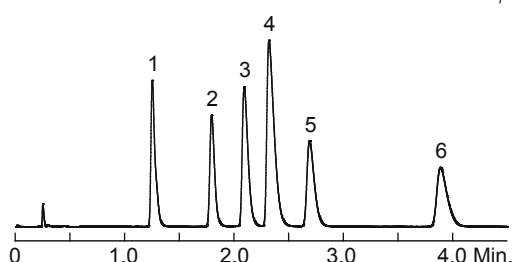


Anticlers

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:10 mM CH₃COONH₄ (pH 7) = 35:65
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample: 1. Famotidine
 2. Ranitidine
 3. Cimetidine
 4. Nizatidine


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

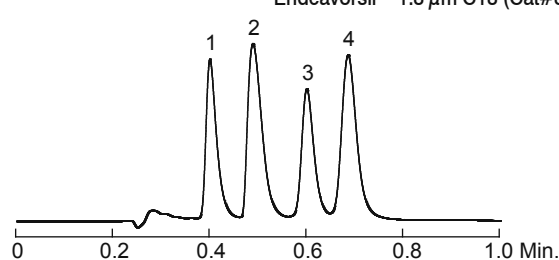


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

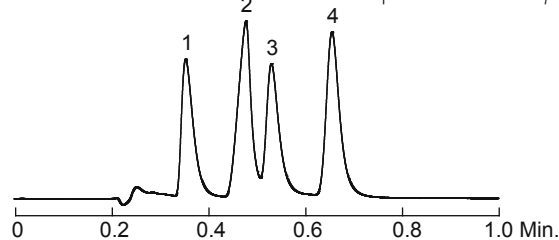

Phenomenex
 Kinetex 2.6 μm C18

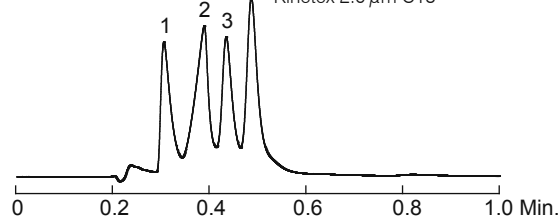

Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

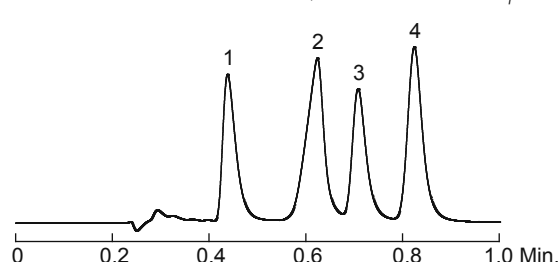

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.





*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Endeavorsil™





Polar Acids*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid 4. Salicylic acid
 2. Homovanillic acid 5. *p*-Chlorobenzoic acid
 3. Sorbic acid 6. *p*-Nitrobenzoic acid

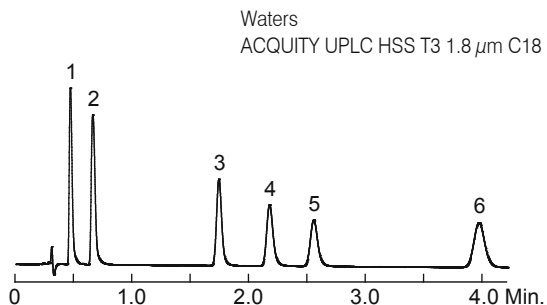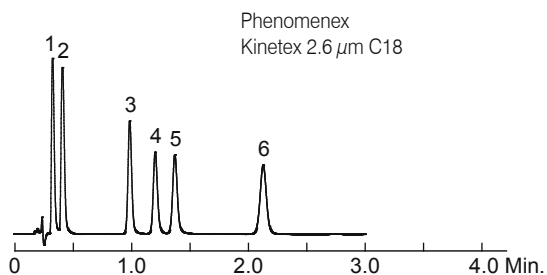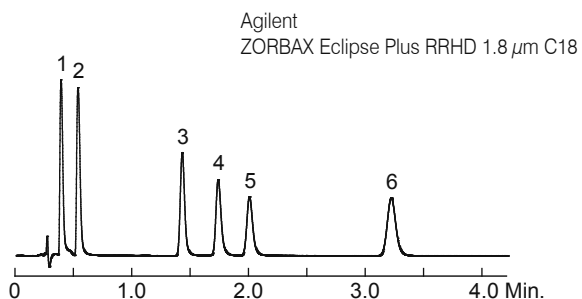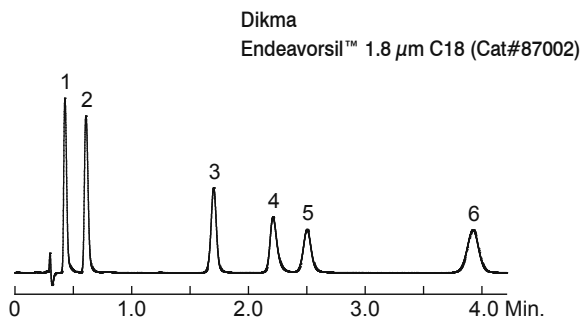

Acidic Compounds

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *L*-Ascorbic acid 4. Acetylsalicylic acid
 2. *p*-Aminobenzoic acid 5. Sorbic acid
 3. Homovanillic acid 6. Salicylic acid

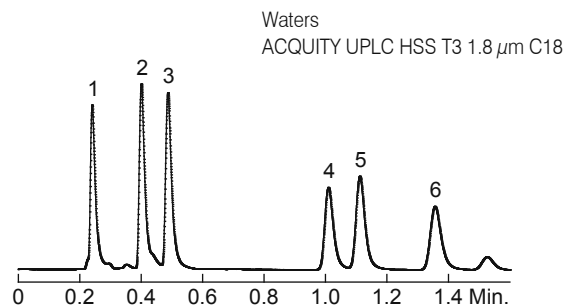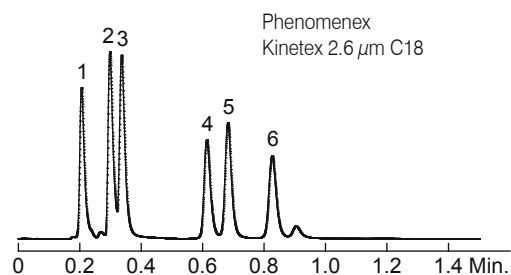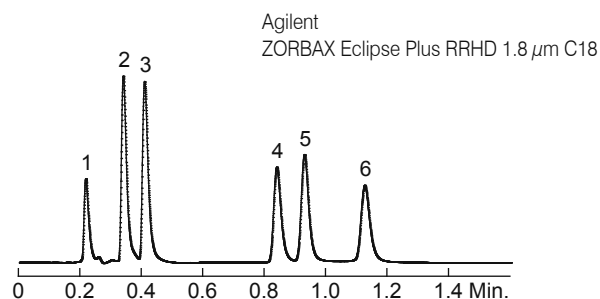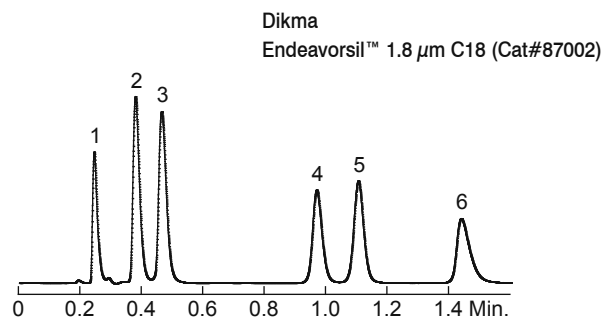





*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.





Anti-inflammatories*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 50:50
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Phenacetin 4. Fenoprofen
 2. Tolmetin 5. Flurbiprofen
 3. Ketoprofen 6. Ibuprofen

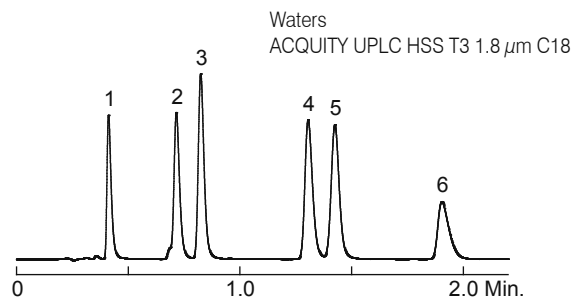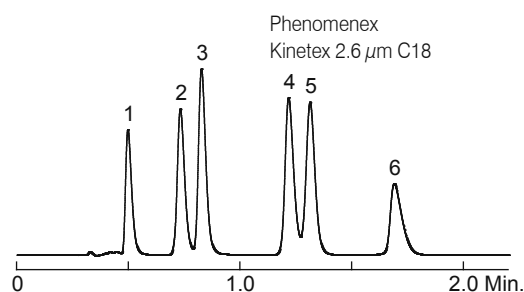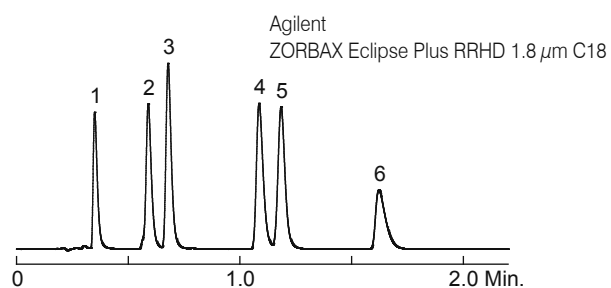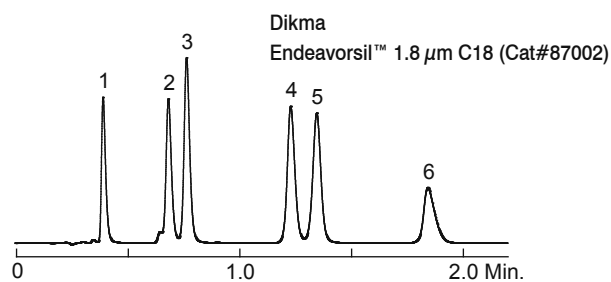

Antibacterials

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Sulfanilamide 6. Sulfamethoxazole
 2. Carbadox 7. Sulfisoxazole
 3. Sulfamerazine 8. Oxolinic acid
 4. Sulfamethoxy-pyridazine 9. Sulfadimethoxine
 5. Furazolidone 10. Sulfaquinoxaline

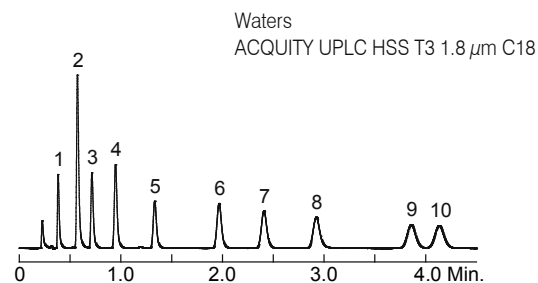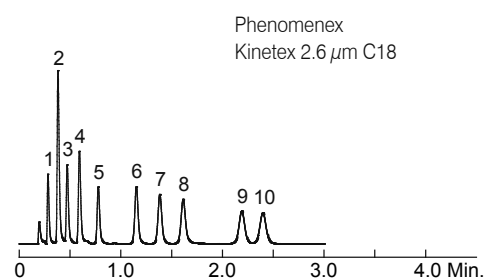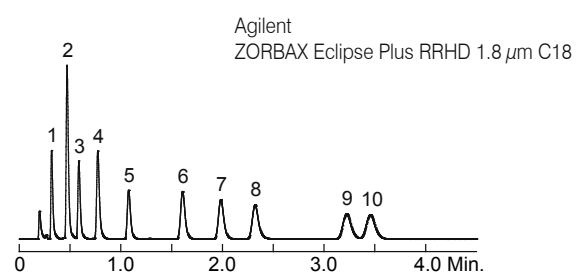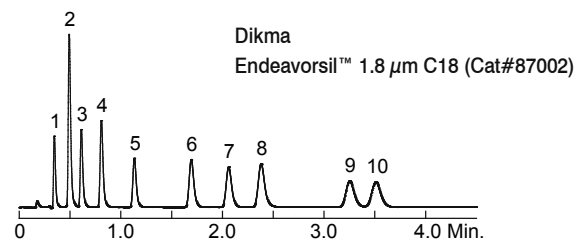

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.


*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Endeavorsil™


Antifungals*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 30:70
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Acetylsalicylic acid
 3. Benzoic acid
 4. Salicylic acid


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

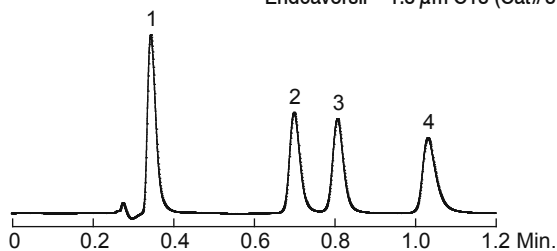


Agilent
 ZORBAX Eclipse Plus RRHD 1.8 μm C18

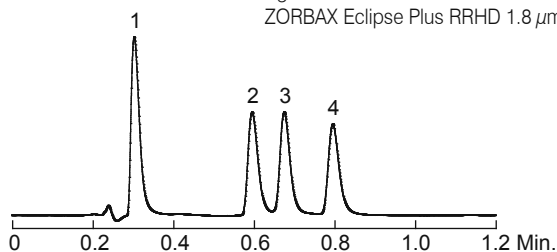

Phenomenex
 Kinetex 2.6 μm C18

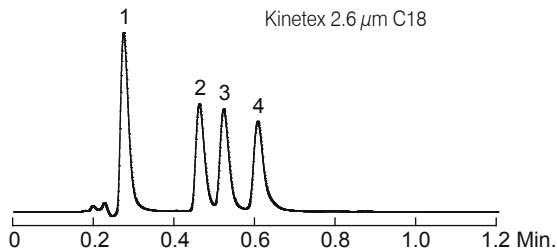


Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

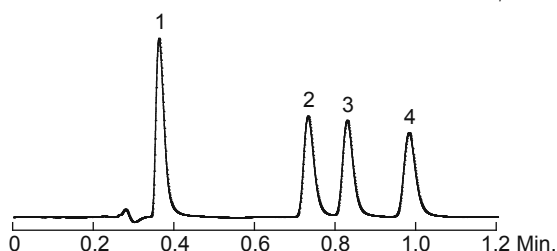


Steroids

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:H₂O = 50:50
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Prednisone
 2. Prednisolone
 3. Dexamethasone
 4. Hydrocortisone 21-acetate
 5. 11-α-Hydroprogesterone


Dikma
 Endeavorsil™ 1.8 μm C18 (Cat#87002)

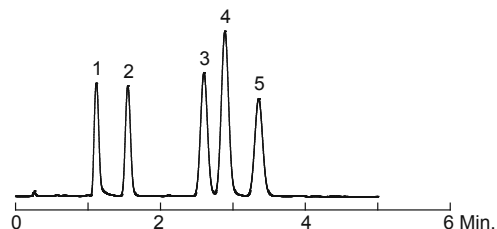

Phenomenex
 Kinetex 2.6 μm C18

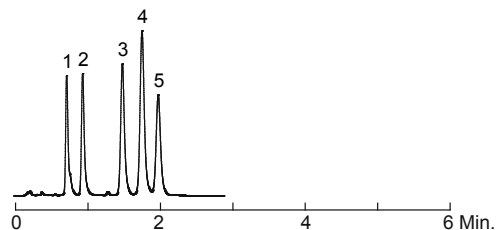

Waters
 ACQUITY UPLC HSS T3 1.8 μm C18

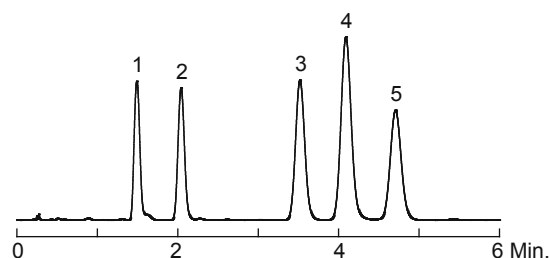

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*Kinetex is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


Features of Leapsil™ Columns

- Ultra fast separation without compromising resolution
- Compatible with all HPLC and UHPLC instruments
- Method development flexibility
- Wide pH stability
- Full spectrum of phases and selectivities


Leapsil™ Material Characteristics

Bonded phase	Particle size (μm)	Pore size (Å)	Surface area (m ² /g)	Purity (%)	Phase density (μmol/m ²)	Carbon loading (%)	pH range	Endcapping
C18	2.7	100	440	> 99.999	3.9	27	1.5 - 10	Yes

Speed

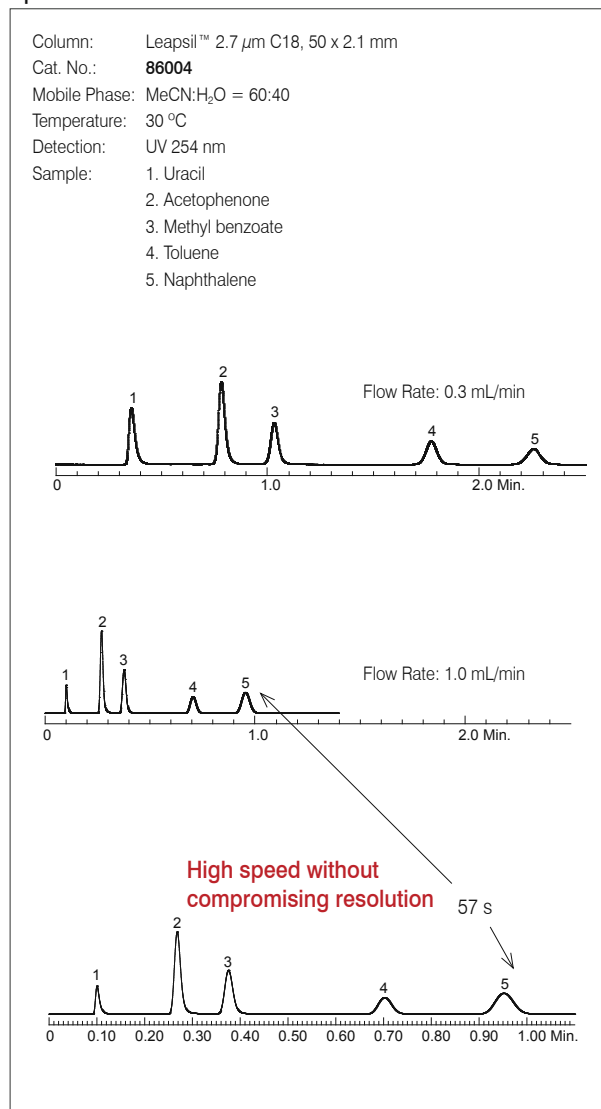

Selectivity*

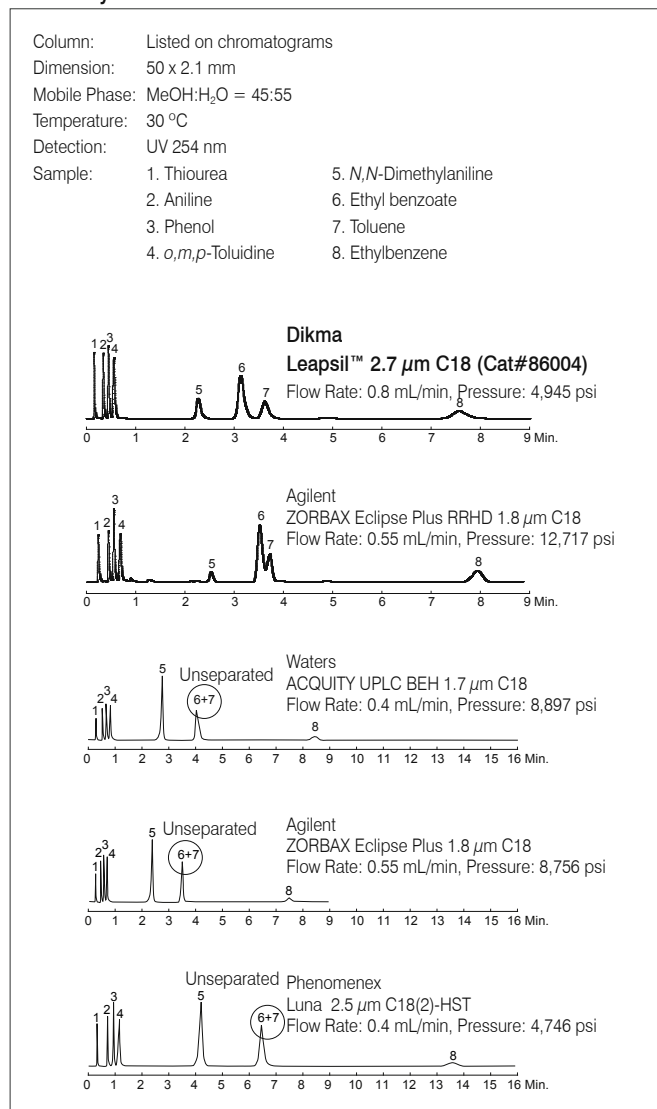

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*BEH Technology is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


*ACQUITY UPLC is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

*Luna is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.


Galushko Test*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:H₂O = 50:50
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Aniline
 3. Phenol
 4. Benzene
 5. Toluene


Dikma
Leapsil™ 2.7 μm C18 (Cat#86004)

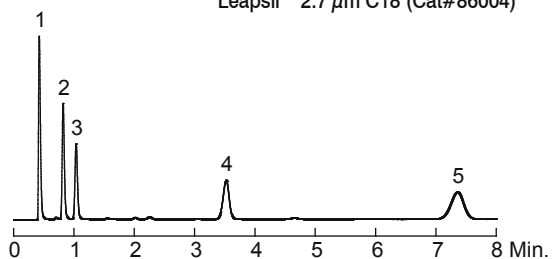

Agilent
Pursuit XRs ULTRA 2.8 μm C18

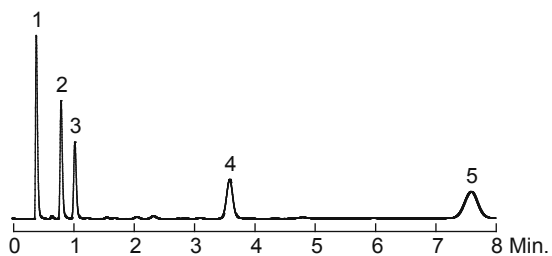


Phenomenex
Luna 2.5 μm C18(2)-HST

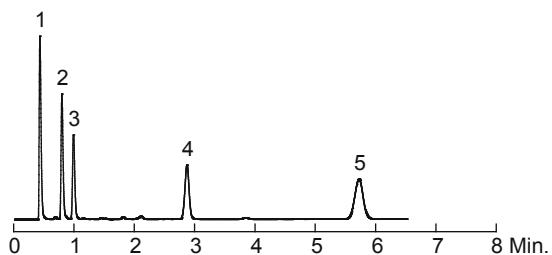


Steroids

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeOH:H₂O = 55:45
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Prednisone
 2. Prednisolone
 3. Betamethasone
 4. Cortisone 21-acetate
 5. 11-α-Hydroprogesterone


Dikma
Leapsil™ 2.7 μm C18 (Cat#86004)

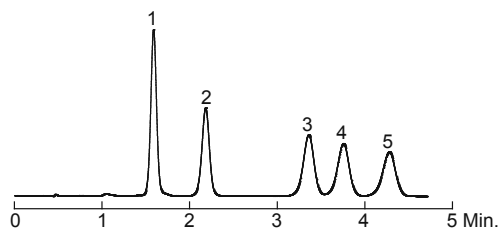

Agilent
Pursuit XRs ULTRA 2.8 μm C18

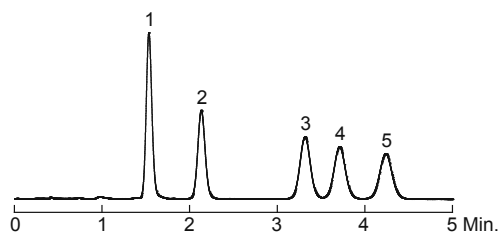



Phenomenex
Luna 2.5 μm C18(2)-HST

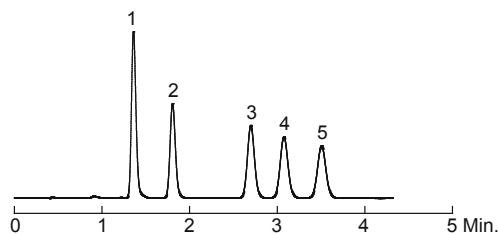



*Pursuit is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.
 *Luna is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

β-Blockers at Neutral pH*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 25:75
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample:
 1. Nadolol
 2. Pindolol
 3. Metoprolol
 4. Labetolol
 5. Propranolol

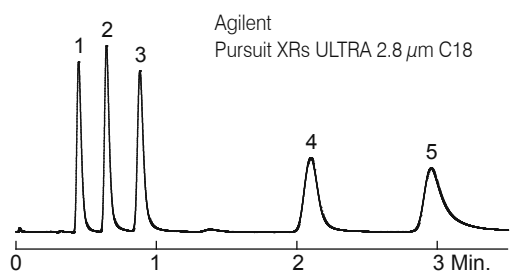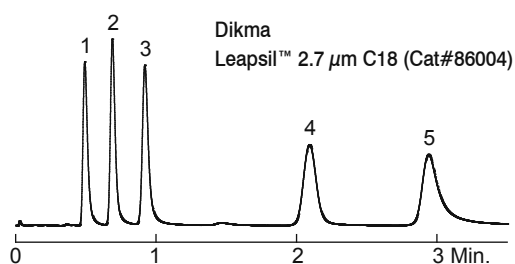**β-Blockers at Low pH**

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 25:75
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample:
 1. Nadolol
 2. Pindolol
 3. Acebutolol
 4. Metoprolol
 5. Labetolol
 6. Propranolol

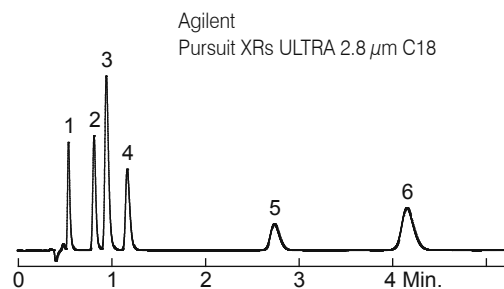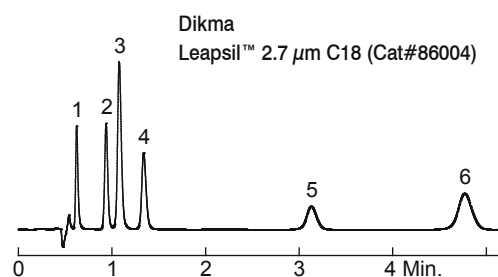


*Pursuit is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


TCAs at Low pH*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Doxepin
 2. Protriptyline
 3. Nortriptyline
 4. Amitriptyline
 5. Trimipramine
 6. Clomipramine

Dikma
Leapsil™ 2.7 μm C18 (Cat#86004)

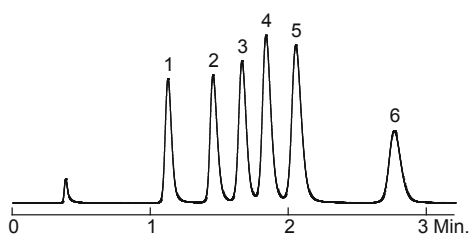


Agilent
Pursuit XRs ULTRA 2.8 μm C18

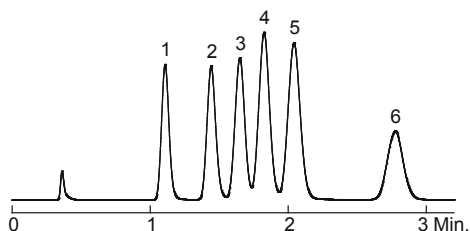


Polar Acids

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Homovanillic acid
 3. Sorbic acid
 4. Salicylic acid
 5. *p*-Nitrobenzoic acid
 6. *p*-Toluic acid

Dikma
Leapsil™ 2.7 μm C18 (Cat#86004)

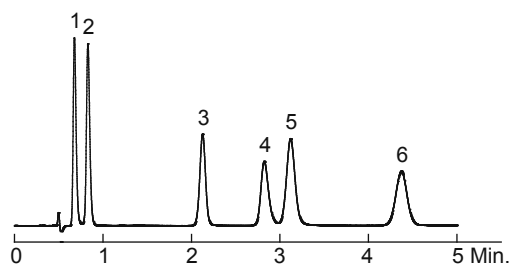

Agilent
Pursuit XRs ULTRA 2.8 μm C18

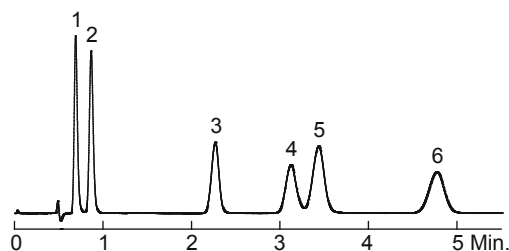


*Pursuit is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


Acidic Compounds*

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. L-Ascorbic acid
 2. *p*-Aminobenzoic acid
 3. Homovanillic acid
 4. Acetylsalicylic acid
 5. Sorbic acid
 6. Salicylic acid

Dikma
 Leapsil™ 2.7 μm C18 (Cat#86004)

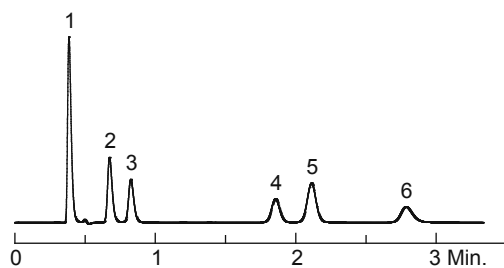


Agilent
 Pursuit XRs ULTRA 2.8 μm C18

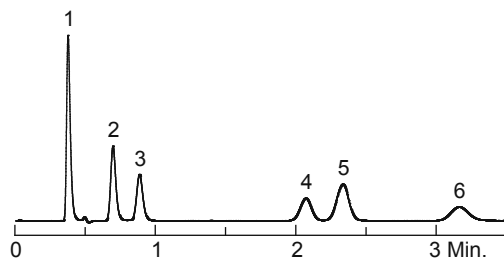


Antibacterials

Column: Listed on chromatograms
 Dimension: 50 x 2.1 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Sulfanilamide
 2. Carbadox
 3. Sulfamerazine
 4. Sulfamethazine
 5. Sulfamethoxypridazine
 6. Furazolidone
 7. Sulfamethoxazole
 8. Sulfisoxazole
 9. Oxolinic acid
 10. Sulfadimethoxine

Dikma
 Leapsil™ 2.7 μm C18 (Cat#86004)

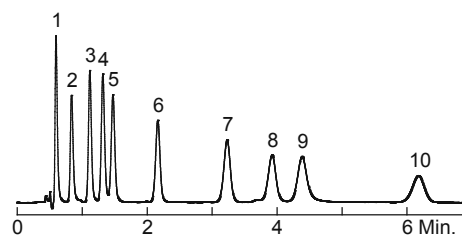

Agilent
 Pursuit XRs ULTRA 2.8 μm C18

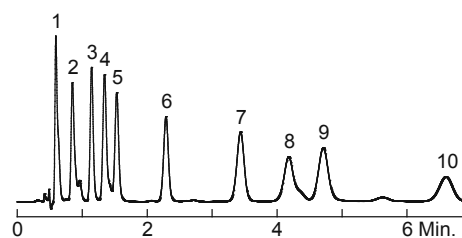

*Pursuit is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

Leapsil™

Leapsil™ Ordering Information

2.7 μm Microbore Columns (2.1 mm)

Phase	50 x 2.1	Price	100 x 2.1	Price	150 x 2.1	Price
Leapsil™ C18	86004	\$463	86005	\$562	86006	\$662

2.7 μm Analytical Columns (3.0 mm)

Phase	50 x 3.0	Price	100 x 3.0	Price	150 x 3.0	Price
Leapsil™ C18	86007	\$463	86008	\$562	86009	\$662

2.7 μm Analytical Columns (4.6 mm)

Phase	50 x 4.6	Price	100 x 4.6	Price	150 x 4.6	Price
Leapsil™ C18	86001	\$463	86002	\$562	86003	\$662

Features of Inspire™ Columns

- Rapid separations with outstanding resolution
- Advanced bonding technologies
- High efficiency and outstanding lifetime
- Excellent separation characteristics over wide pH range
- Superior batch-to-batch reproducibility
- Choose from a variety of phases and hardware formats



Inspire™ columns are engineered with high purity raw silica, proprietary bonding techniques, tightly controlled manufacturing processes, and column packing procedures that provide today's chromatographic laboratories with HPLC columns of unrivaled performance.

Inspire™ Material Characteristics


Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Purity (%)	Phase density (µmol/m ²)	Carbon loading (%)	pH range	Endcapping
C18	3, 5, 10	100	440	> 99.999	3.9	27	1 - 11	Yes
C8	3, 5, 10	100	440	> 99.999	4.2	17	1 - 11	Yes

Superior Batch-to-batch Reproducibility

Reproducibility is essential for the selection of a HPLC column. Today's chemists often need to establish new analytical methods to evaluate the latest pharmaceutical and biopharmaceutical products. The column they select has to provide the same chromatographic results over the entire lifespan of the new drug product. Chemists doing QA / QC also need a well-producible column, which ensures the accuracy of analytical results and high productivity of chromatographic laboratories. Inspire™ columns undergo rigorous quality control testing to ensure long-term reproducibility, letting you increase your laboratory's productivity and allowing for easier method transfer between labs.

Reproducibility Test

Five randomly selected batches demonstrated excellent reproducibility in the example shown:

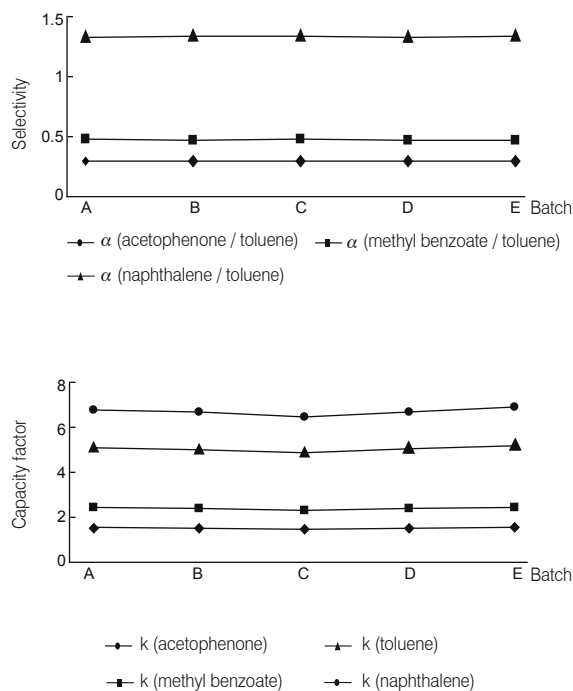


Long Lifetime

Columns that last longer not only save your money, but also save your time in establishing and verifying methods for a new column. Inspire™ columns deliver guaranteed, consistent performance in optimizing the two key factors that control column lifetime: the packing material and the mechanical stability of the packed bed.

Lifetime Test

Column: Inspire™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Nadolol 5. Labetolol
 2. Pindolol 6. Propranolol
 3. Acebutolol 7. Alprenolol
 4. Metoprolol

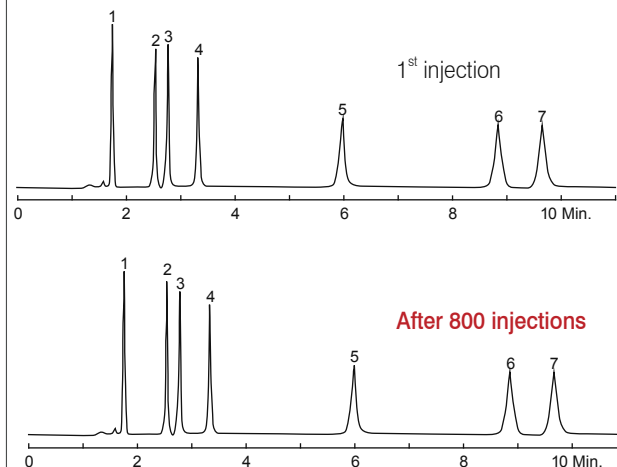

Inspire™ columns can last over 800 injections with minimal loss in efficiency, symmetry and retention time.

Stable from pH 1 - 11

Generally, the cause of shortened column lifetime relates to exposure under extreme pH mobile phases, which leads to hydrolysis of the bonded phase at low pH and dissolution of silica at high pH. The hydrolysis can also lead to significant changes in analyte retention time, making method reproducibility requirements difficult to achieve.





Dikma incorporates proprietary bonding and endcapping techniques, making Inspire™ packing much more stable across a broad pH range when compared to conventionally prepared material. Our packing platform also effectively resists the typical ligand hydrolysis and silica dissolution seen with conventional columns. In both low pH and high pH tests, Inspire™ C18 columns undergo elution over 1,440 hours and show very little loss of retention time, capacity factor and symmetry, exhibiting their unsurpassed endurance and stability.

pH Stability Test

Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: 81001
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Pyridine
 3. Phenol
 4. Benzene

pH 1

pH 11

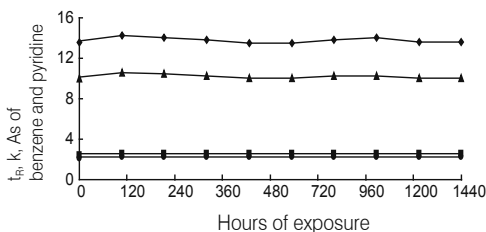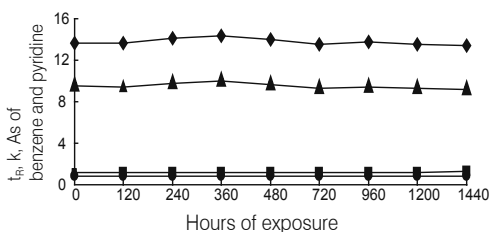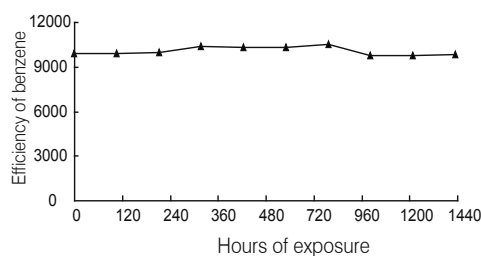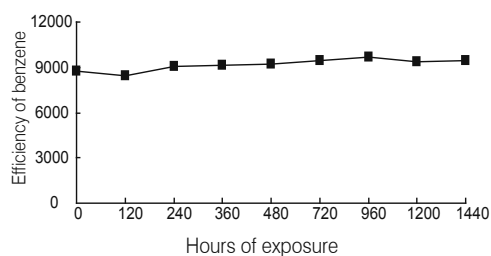

■ As (pyridine)
 ◆ As (benzene)
 ▲ k (benzene)
 ● t_R (benzene)

Flush solution (pH 1)

Mobile Phase: 1% TFA in MeCN:1% TFA in H₂O = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient

Flush solution (pH 11)

Mobile Phase: MeCN:20 mM phosphate buffer = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient

Efficient Method Development


Inspire™ columns provide chromatographic laboratories with advanced performance and robust, rugged methods that can be achieved across the entire log *P* range of -2 to 8, simplifying the method validation and transfer process.

In the test below, aspartame, reserpine, cortisone and dioctyl phthalate are chosen to evaluate the Inspire™ columns with a sample representative of molecules encountered in drug discovery. The compounds vary in polarity (log *P* = -2 to 8) and molecular weight (MW 294 to 608). High quality separation of these components demonstrates the broad applicability of Inspire™ C18 to a range of compounds with drug-like properties.

Tang, L.; Fitch, W.L.; Alexander, M.S.; Dolan J.W. *Anal. Chem.*, 2000, 72, 5211 - 5218.

LC / MS Performance Test Mix

Column: Inspire™ 5 μm C18
 Dimension: 150 x 4.6 mm
 Cat. No.: 81001
 Mobile Phase: A: 0.05% HCOOH in MeCN
 B: 0.05% HCOOH in H₂O
 Gradient: 10 - 90% A in 5 min, hold at 90% A for 5 min
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Aspartame
 2. Reserpine
 3. Cortisone
 4. Dioctyl phthalate

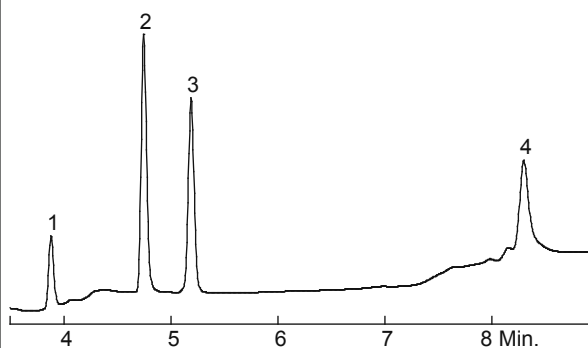


Engelhardt Test

The Engelhardt test is a stringent test we use to verify the selectivity of Inspire™ columns. It is based solely on stationary phase chemistry. In this test, aniline elutes before phenol and the three toluidine isomers coelute, indicating that the acidic silanol groups of Inspire™ columns are deactivated.

Engelhardt Test

Column: Inspire™ 5 μm C18
 Dimension: 150 x 4.6 mm
 Cat. No.: 81001
 Mobile Phase: MeOH:H₂O = 55:45
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Thiourea
 2. Aniline
 3. Phenol
 4. *o,m,p*-Toluidine
 5. *N,N*-Dimethylaniline
 6. Ethyl benzoate
 7. Toluene
 8. Ethylbenzene

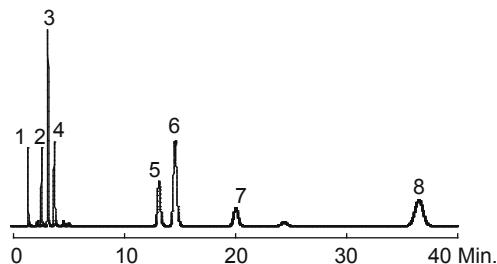

Excellent Peak Shapes with Basic Molecules - but simple mobile phase*

Column: Inspire™ 5 μm C18, 150 x 4.6 mm

Cat. No.: 81001


Mobile Phase: A: 0.1% TFA in H₂O
B: 0.1% TFA in MeCN
A:B = 60:40

Flow Rate: 1.0 mL/min

Temperature: Ambient

Detection: UV 254 nm

Sample: 1. Nordoxepin
2. Doxepin
3. Desipramine
4. Nortriptyline
5. Amitriptyline
6. Trimipramine
7. Clomipramine

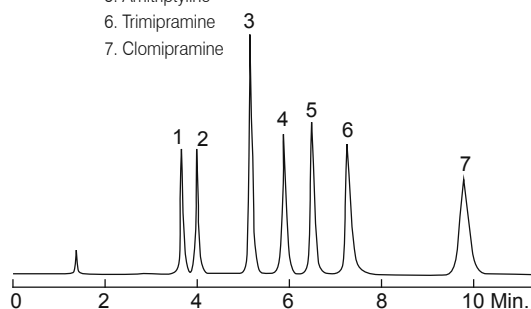

Column: SunFire™ 5 μm C18, 150 x 4.6 mm


Mobile Phase: A: H₂O
B: MeOH
C: 100 mM CH₃COONH₄, pH 6.0
A:B:C = 18:72:10

Flow Rate: 1.0 mL/min

Temperature: 30 °C

Detection: UV 254 nm

Sample: 1. Desipramine
2. Nortriptyline
3. Doxepin
4. Imipramine
5. Amitriptyline

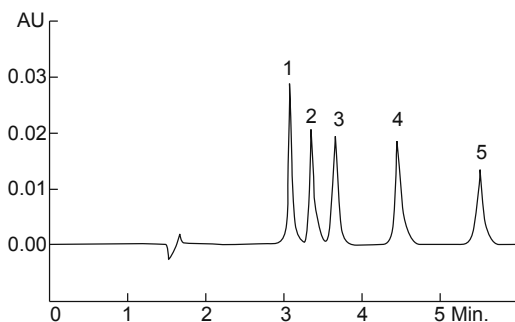

Antihistamines at High pH*

Column: Listed on chromatograms

Dimension: 150 x 4.6 mm




Mobile Phase: MeOH:5 mM NH₄HCO₃ (pH 10) = 75:25

Flow Rate: 1.0 mL/min

Temperature: Ambient

Detection: UV 254 nm

Sample: 1. Maleic acid
2. Pheniramine
3. Doxylamine
4. Chlorpheniramine
5. Brompheniramine
6. Diphenhydramine

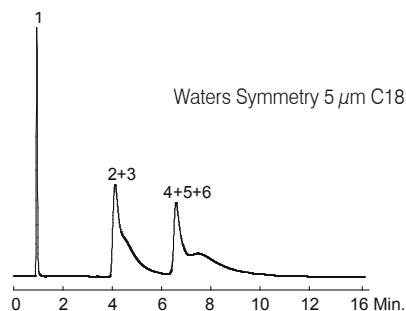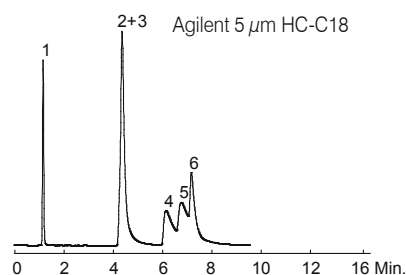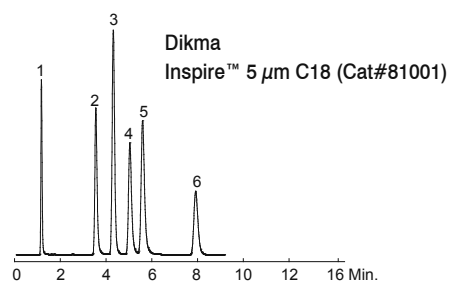

*SunFire is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

*Symmetry is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


TCAs at High and Neutral pHs

Basic compounds tend to tail on alkyl phases because of the interaction with the silanols on the silica surface. This can often cause increased retention but loss in performance (peak shape). The most sensitive measurement of silanol interactions is achieved using highly basic probes with a pH 7 mobile phase. At this pH, many of the residual silanols are in their ionized form, and the basic probes are completely protonated. The protonated bases interact with the ionized silanols by an ion-exchange mechanism, and the degree of tailing is a direct measure of silanol activity. Inspire™ columns provide more symmetrical peaks and greater resolution for TCAs at high and neutral pHs, demonstrating their outstanding bonding and endcapping techniques.


TCAs at High pH*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:5 mM NH₄HCO₃ (pH 10) = 80:20
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Nordoxepin 5. Imipramine
 2. Doxepin 6. Amitriptyline
 3. Desipramine 7. Trimipramine
 4. Nortriptyline


Dikma
 Inspire™ 5 μm C18 (Cat#81001)



Phenomenex Gemini 5 μm C18




Kromasil 5 μm C18




TCAs at Neutral pH*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 2:1
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Desipramine
 2. Nortriptyline
 3. Imipramine
 4. Amitriptyline
 5. Trimipramine


Dikma
 Inspire™ 5 μm C18 (Cat#81001)



Agilent 5 μm HC-C18



Waters XBridge 5 μm C18



*XBridge is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

*Gemini is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.




*Kromasil is a registered trademark of Eka Chemicals AB. Dikma Technologies Inc. is not affiliated with the above company.

Ultimate Performance

High phase density results in increased analyte-bonded phase interactions. These interactions impart greater selectivity and retention, leading to enhanced resolution.

Antibacterials*


Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Sulfanilamide
 2. Carbadox
 3. Sulfapyridine
 4. Sulfamerazine
 5. Thiamphenicol
 6. Sulfamethoxyipyridazine
 7. Furazolidone
 8. Sulfamethoxazole
 9. Sulfisoxazole
 10. Oxolinic acid

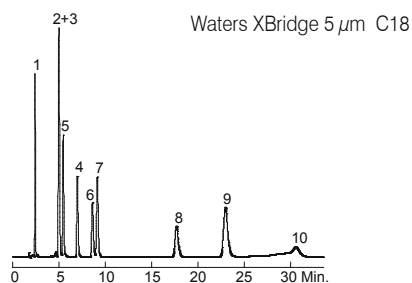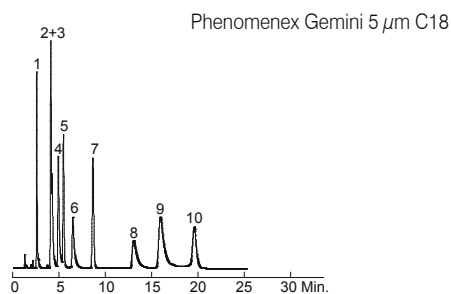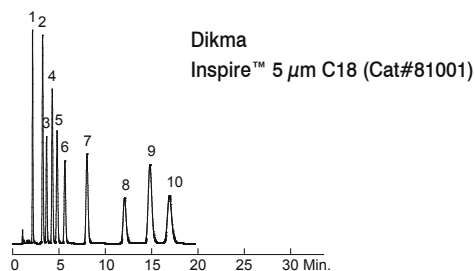


*XBridge is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.
 *Gemini is a registered trademark of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

Separation of Cephalosporin Antibiotics at Different Mobile Phase Conditions


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:25 mM phosphate buffer (pH 3) = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Cefadroxil 5. Cefazoline
 2. Ceftazidime 6. Cefoxitin
 3. Cefaclor 7. Cefradine
 4. Cephalexin

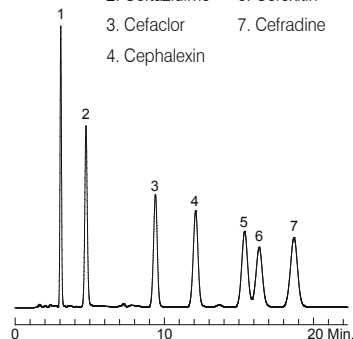

Mobile Phase: MeOH:100 mM acetate buffer = 20:80
 Flow Rate: 1.0 mL/min
 Detection: UV 254 nm
 Sample: 1. Cefadroxil 4. Cefoxitin
 2. Cefuroxime 5. Cefradine
 3. Cefaclor

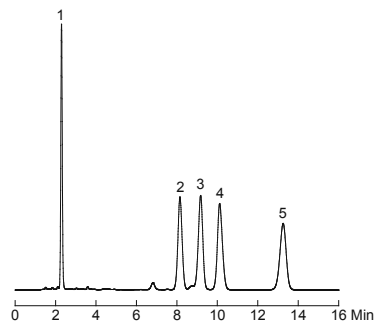


Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Detection: UV 230 nm
 Sample: 1. Ceftazidime 5. Cephalexin
 2. Cefadroxil 6. Cefoxitin
 3. Cefazoline 7. Cefradine
 4. Cefaclor

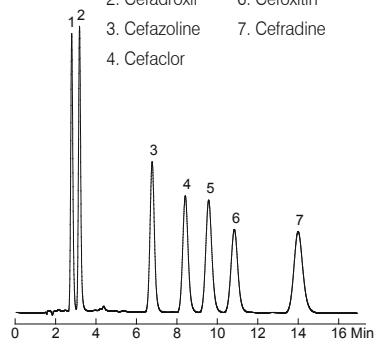


Separation of TCAs and Benzos*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Nitrozepam 6. Triazolam
 2. Nordoxepin 7. Nortriptyline
 3. Alprazolam 8. Clonazepam
 4. Diazepam 9. Trimipramine
 5. Oxazepam


Dikma
 Inspire™ 5 μm C18 (Cat#81001)

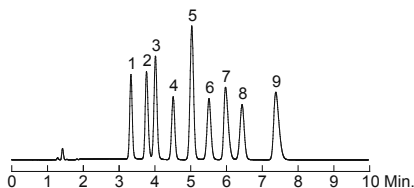


Dikma
 Spursil™ 5 μm C18-EP (Cat#82101)

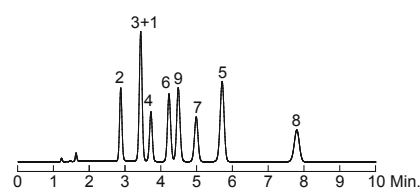


GL Science
 Inertsil 5 μm ODS-3

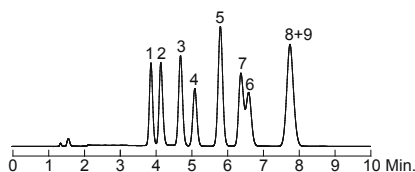


Agilent
 ZORBAX 5 μm Bonus-PP

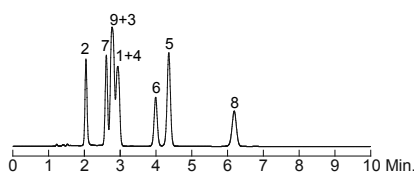


Agilent
 ZORBAX Eclipse 5 μm XDB-C18

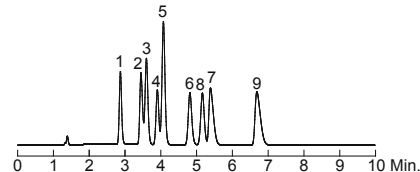


Waters
 SymmetryShield 5 μm RP18

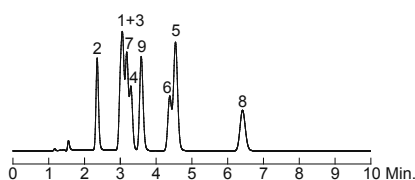


Waters
 XBridge 5 μm C18

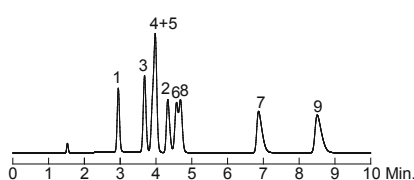


Waters
 Symmetry 5 μm C18

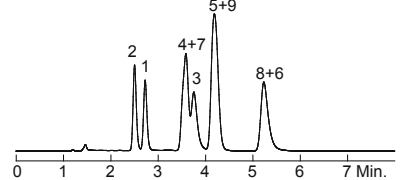


Phenomenex
 Luna 5 μm C18(2)

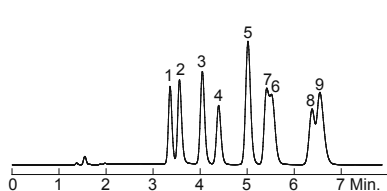


Phenomenex
 Gemini 5 μm C18

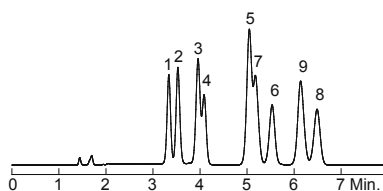


Eka Chemicals AB
 Kromasil 5 μm C18

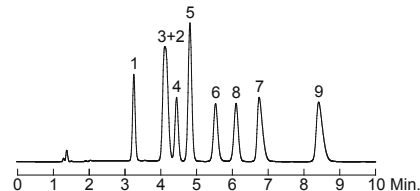


Thermo Scientific
 Hypersil 5 μm BDS C18

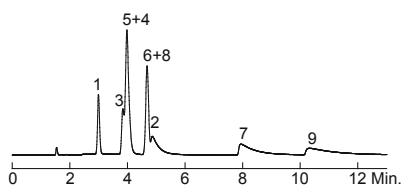

Beckman Coulter
 Ultrasphere 5 μm C18

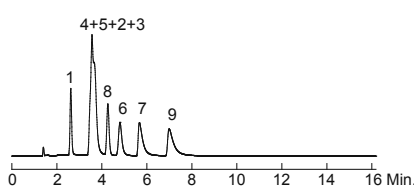

Separation Methods Technologies
 OD-5-100 5 μm C18

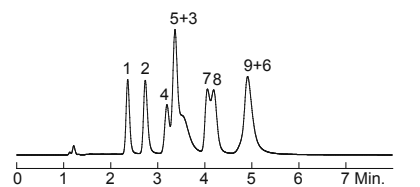


*The comparative data presented here may not be representative for all applications.


Organic Acids*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 25 mM KH₂PO₄, pH 2.5
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Oxalic acid
 2. Tartaric acid
 3. Malic acid
 4. Lactic acid
 5. Acetic acid
 6. Citric acid
 7. Fumaric acid
 8. Succinic acid


Dikma
 Inspire™ 5 μm C18 (Cat#81001)

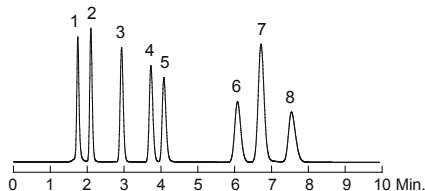


Dikma
 Spursil™ 5 μm C18 (Cat#82001)

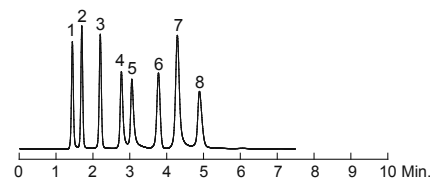


Agilent
 ZORBAX 5 μm SB-C18

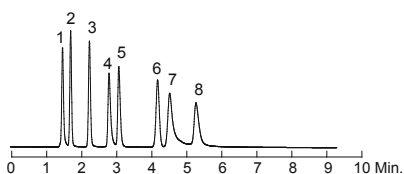


Agilent
 ZORBAX Eclipse 5 μm XDB-C18

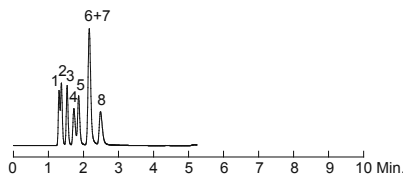


Phenomenex
 Gemini 5 μm C18

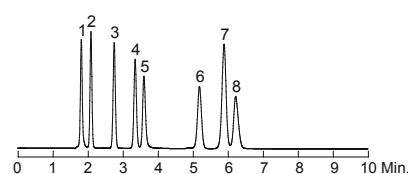


Phenomenex
 Luna 5 μm C18(2)

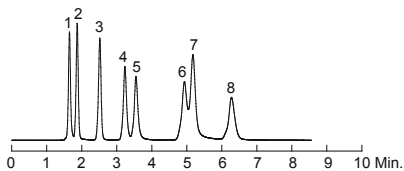


Waters
 XBridge 5 μm C18

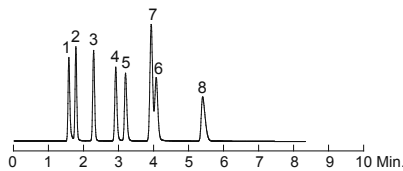


Waters
 Symmetry 5 μm C18

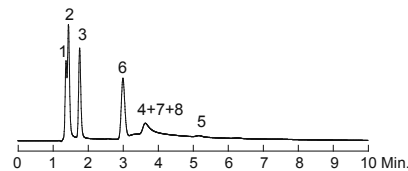


Thermo Scientific
 Hypersil 5 μm BDS C18

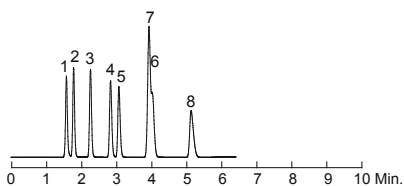

Beckman Coulter
 Ultrasphere 5 μm C18

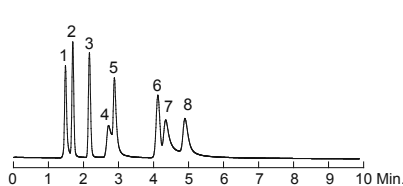

Separation Methods Technologies
 OD-5-100 5 μm C18

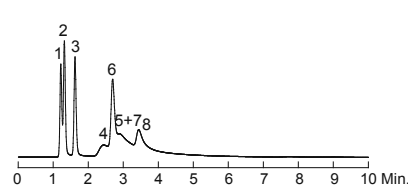


*The comparative data presented here may not be representative for all applications.


Flavonoids

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:0.085% H₃PO₄ = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Gallic acid
 2. Catechin
 3. Caffeic acid
 4. Vanillic acid
 5. *p*-Coumaric acid
 6. Quercitrin
 7. Myricetin

Dikma
 Inspire™ 5 μm C18 (Cat#81001)




Dikma
 Spursil™ 5 μm C18 (Cat#82001)




Herbicides

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 2.0 mL/min
 Temperature: Ambient
 Detection: UV 214 nm
 Sample: 1. Dalapon
 2. 2,4-D
 3. 2,4,5-T

Dikma
 Inspire™ 5 μm C18 (Cat#81001)



Dikma
 Spursil™ 5 μm C18 (Cat#82001)



Inspire™ Ordering Information

3 μm Microbore Columns (2.1 mm)

Guard Cartridge, 2/pk

Phases	30 x 2.1	Price	50 x 2.1	Price	100 x 2.1	Price	150 x 2.1	Price	250 x 2.1	Price	10 x 2.1	Price
Inspire™ C18	81030	\$333	81004	\$353	81012	\$523	81013	\$572	81015	\$602	6501	\$149
Inspire™ C8	81130	333	81104	353	81112	523	81113	572	81115	602	6502	149

3 μm Analytical Columns (3.0 mm)

Phases	30 x 3.0	Price	50 x 3.0	Price	100 x 3.0	Price	150 x 3.0	Price	250 x 3.0	Price	10 x 2.1	Price
Inspire™ C18	81029	\$333	81021	\$353	81022	\$523	81023	\$572	81024	\$602	6501	\$149
Inspire™ C8	81129	333	81121	353	81122	523	81123	572	81124	602	6502	149

3 μm Analytical Columns (4.6 mm)

Phases	30 x 4.6	Price	50 x 4.6	Price	100 x 4.6	Price	150 x 4.6	Price	250 x 4.6	Price	10 x 4.0	Price
Inspire™ C18	81031	\$333	81016	\$353	81017	\$523	81018	\$572	81020	\$602	6601	\$149
Inspire™ C8	81131	333	81116	353	81117	523	81118	572	81120	602	6602	149

5 μm Microbore Columns (2.1 mm)

Phases	30 x 2.1	Price	50 x 2.1	Price	100 x 2.1	Price	150 x 2.1	Price	250 x 2.1	Price	10 x 2.1	Price
Inspire™ C18	81033	\$323	81003	\$343	81007	\$508	81002	\$557	81009	\$587	6503	\$149
Inspire™ C8	81133	323	81103	343	81107	508	81102	557	81109	587	6504	149

5 μm Analytical Columns (3.0 mm)

Phases	30 x 3.0	Price	50 x 3.0	Price	100 x 3.0	Price	150 x 3.0	Price	250 x 3.0	Price	10 x 2.1	Price
Inspire™ C18	81032	\$323	81025	\$343	81026	\$508	81027	\$557	81028	\$587	6503	\$149
Inspire™ C8	81132	323	81125	343	81126	508	81127	557	81128	587	6504	149

5 μm Analytical Columns (4.6 mm)

Phases	30 x 4.6	Price	50 x 4.6	Price	100 x 4.6	Price	150 x 4.6	Price	250 x 4.6	Price	10 x 4.0	Price
Inspire™ C18	81034	\$323	81010	\$343	81011	\$508	81001	\$557	81006	\$587	6603	\$149
Inspire™ C8	81134	323	81110	343	81111	508	81101	557	81106	587	6604	149

EasyGuard™ Guard Holder: Cat#6220, Price: \$99

5 μm and 10 μm Semi-preparative Columns

Guard Cartridge, 2/pk

Phases	Particle Size (μm)	250 x 4.6		250 x 10.0		150 x 21.2		250 x 21.2		10 x 10.0		10 x 21.2	
		Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
Inspire™ C18	5	81006	\$587	81038	\$1,291	81045	\$2,691	81039	\$2,891	6505	\$195	6506	\$311
Inspire™ C8	5	81106	587	81138	1,291	81145	2,691	81139	2,891	6507	195	6508	311
Inspire™ Diol	5	81247	587	81238	1,291	81245	2,691	81239	2,891	6509	195	6510	311
Inspire™ C18	10	81035	383	81036	1,092	81046	2,291	81037	2,491	6511	195	6512	311
Inspire™ C8	10	81135	383	81136	1,092	81146	2,291	81137	2,491	6513	195	6514	311
Inspire™ Diol	10	81235	383	81236	1,092	81246	2,291	81237	2,491	6515	195	6516	311

10 mm Guard Holder: Cat#6221, Price: \$199, 21.2 mm Guard Holder: Cat#6222, Price: \$299

10 μm Packing Materials

Phases	Particle Size (μm)	100 G		1 KG	
		Cat. No.	Price	Cat. No.	Price
Inspire™ C18	10	85001	Inquire	85002	Inquire
Inspire™ C8	10	85101	Inquire	85102	Inquire
Inspire™ Diol	10	85021	Inquire	85022	Inquire

Features of Spursil™ Columns

- Combine high purity silica with unique polar modification technology
- Unique selectivity and enhanced resolution
- Silanol shielding for excellent peak shape
- Improved water wettability and stable retention in highly aqueous mobile phase conditions
- Excellent retention for polar compounds
- Extended range pH stability
- Choose from a variety of selectivities and hardware formats

Spursil™ polar-modified phases are based on ultra high-purity silica and novel polar modification technology. The unique bonded phases maximize polar retention and selectivity, while virtually eliminating silanol activity. The resulting polar-modified packing material contains a surface which is easily “wetted” with polar eluents and can run in highly aqueous conditions. The polar group also seems to play a role in base deactivation. We have seen some evidence that hydrogen bonding occurs between certain polar linkers and the silica surface, thereby decreasing the interaction of such silanols with basic components in the sample. Additionally, polar-modified phases often provide selectivity quite different from standard C18 phases.

Standard reversed-phase columns, particularly C18 columns, often suffer from “phase collapse” and the retention of the compounds is severely diminished when used in combination with highly aqueous phases. This phenomenon is substantially reduced with Spursil™ because the polar modifications make the phase less hydrophobic and more wettable. Polar-modified phases remain fully extended in aqueous phases, allowing increased interaction between samples and the bonded phase. Spursil™ columns show good retention of polar compounds which tend to elute in the void volume on standard ODS phases.

Spursil™ columns are available in 3, 5, and 10 micron particle sizes, column lengths are ranging from 30 mm to 250 mm, and column dimensions are ranging from 2 mm to 21.2 mm. Ten micron preparative materials are available in bulk form.

Spursil™ Material Characteristics



Bonded phase	Particle size (μm)	Pore size (Å)	Surface area (m ² /g)	Purity (%)	Phase density (μmol/m ²)	Carbon loading (%)	pH range	Endcapping
C18	3, 5, 10	100	440	> 99.999	3.5	25	1.5 - 10	Yes
C18-EP	3, 5, 10	100	440	> 99.999	3.4	24	1.5 - 10	Yes

High Efficiency

A chromatographic efficiency test is run on all columns. Plates per column and USP tailing factor are measured for each column to confirm packing efficiency. The USP tailing factor, a measure of peak symmetry at 5% of peak height, is a stringent indicator of peak shape. The test analytes are neutral hydrophobic compounds chromatographed in a acetonitrile:water mobile phase. The retention, selectivity, efficiency and peak symmetry of these molecules are measured to provide specifications for column performance.

Performance Test

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:H₂O = 60:40
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Acetophenone
 3. Methyl benzoate
 4. Toluene
 5. Naphthalene

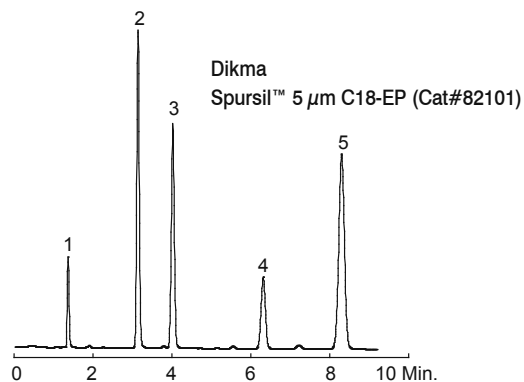
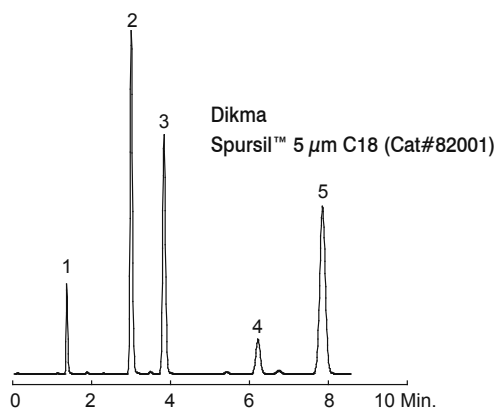


Batch-to-Batch Reproducibility of Spursil™ C18

Reproducibility is imperative to any application in the laboratory. A new column may be interesting, but if the retentivity and selectivity are not consistent, it has little value in a validated method. Dikma has designed reproducibility into the Spursil™ family starting with tight specifications on the surface area, pore size and particle size of the silica. Bonding procedures are transferred to production through a manufacturing transfer validation procedure. All Spursil™ columns are manufactured at our ISO 9001 registered facility. This ISO 9001 registration provides quality oversight into all aspects of the manufacturing process, leading to a product that consistently meets exact specifications.

Reproducibility Test

Five randomly selected batches demonstrated excellent reproducibility in the example shown



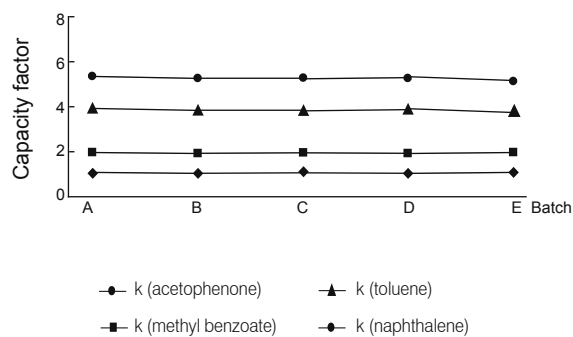
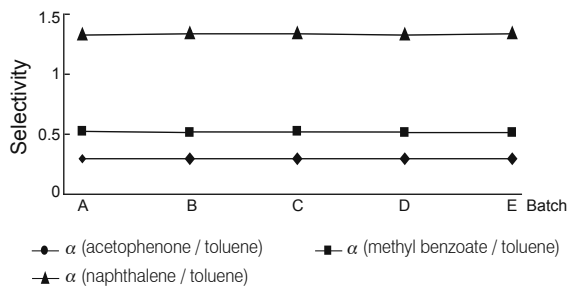


Wide pH Range

One of the most important parameters in choosing a column is lifetime. Columns that last longer save time and money. Column failure often occurs because of hydrolytic instability of the stationary phase and silica as well as mechanical instability of the column packing (voiding). The high phase coverage of all Spursil™ products plus proprietary endcapping creates a phase that is more stable against hydrolytic attack. Dikma's narrow specifications on surface area of the silica help to create a more consistent and well-packed column that minimizes shifting of the column bed during use. This reduces the chance of voiding. With Spursil™ columns, there is no worry about bonded phase hydrolysis, dissolution of the silica particle, or bonded phase collapse. The polar groups make the Spursil™ columns highly stable in hydrophilic conditions, from pH 1.5 to 10 and from 0 to 100% aqueous. All Spursil™ columns are tested at pH 1.5 and pH 10 under "real world" conditions with basic and acidic compounds to ensure good peak symmetry.

pH Stability Test

Column: Spursil™ 5 μ m C18, 150 x 4.6 mm
 Cat. No.: 82001
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Pyridine
 3. Phenol
 4. Benzene

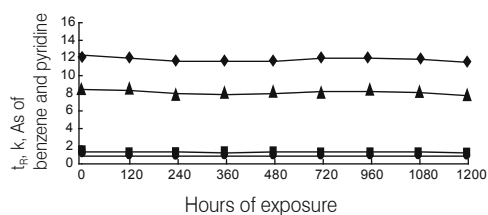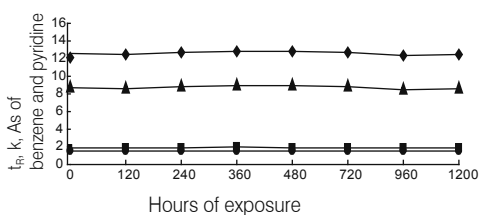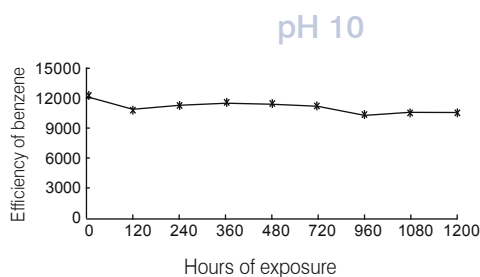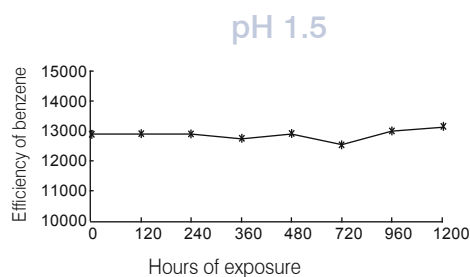

■ As (pyridine) ◆ As (benzene) ▲ k (benzene) ● t_R (benzene)

Flush solution (pH 1.5)

Mobile Phase: 1% TFA in MeCN:1% TFA in H₂O = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient

Flush solution (pH 10)

Mobile Phase: MeCN:20 mM phosphate buffer = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient


Unique Selectivity

Spursil™ analytical HPLC columns are designed to provide enhanced retention and selectivity for highly polar compounds in the reversed-phase mode, as well as compatibility with highly aqueous mobile phases. These phases offer several advantages over traditional alkyl bonded phases including a unique selectivity, improved peak shape for basic compounds, and the ability to operate in highly aqueous mobile phases. These polar-modified columns give the same range of application but alternative selectivity compared to traditional alkyl bonded phases. Spursil™ phases provide additional charge density to adjacent silanol through electron delocalization, thereby removing mixed-mode interactions and improving peak symmetry. The best methods employ simple mobile phases. Spursil™ columns enable separation scientists who work with polar compounds to consistently deliver robust methods with good selectivity and excellent peak shape.


Cold Medicine

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA
 in H₂O = 35:65
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Doxylamine
 2. Acetanilide
 3. Acetylsalicylic acid
 4. Dextromethorphan
 5. Diphenhydramine

Dikma
Spursil™ 5 μm C18 (Cat#82001)




Dikma
Spursil™ 5 μm C18-EP (Cat#82101)




Polar Acids*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:0.1% TFA in H₂O = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Maleic acid
 2. Procainamide
 3. *o*-Toluamide
 4. *p*-Hydroxybenzoic acid


Dikma
Spursil™ 5 μm C18 (Cat#82001)




Phenomenex
Gemini 5 μm C18



Agilent
ZORBAX 5 μm Bonus-RP




Waters
SymmetryShield 5 μm RP18




Polar Compounds*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 10 mM HCOONH₄, pH 3
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Thiourea
 2. Cytosine
 3. Adenine
 4. Uridine


Dikma
Spursil™ 5 μm C18 (Cat#82001)




Dikma
Spursil™ 5 μm C18-EP (Cat#82101)



Phenomenex
Luna 5 μm C18(2)



Phenomenex
Gemini 5 μm C18



*Gemini and Luna are registered trademarks of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


*SymmetryShield is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Outstanding Performance

Our Spursil™ family of reversed-phase columns, each prepared from the same high-purity silica, differ from one another solely and predictably in the hydrophobicity and polarity inherent in the stationary phase chemistry. The outstanding performance of Spursil™ columns allows users who are developing methods to achieve the right separation the first time, even with a simple mobile phase. This means faster development of HPLC methods, and more robust methods being transferred to QA / QC labs.


Anti-inflammatories

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
Cat. No.: **82001**
Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 55:45
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Phenacetin
2. Tolmetin
3. Ketoprofen
4. Fenopropfen
5. Flurbiprofen
6. Diclofenac
7. Ibuprofen

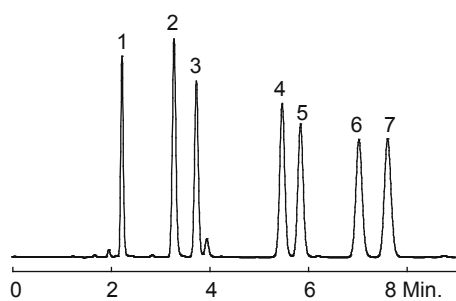

Steroids

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
Cat. No.: **82001**
Mobile Phase: MeOH:H₂O = 55:45
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Prednisone
2. Cortisone
3. Prednisolone
4. Dexamethasone
5. Hydrocortisone 21-acetate
6. 11-α-Hydroxyprogesterone

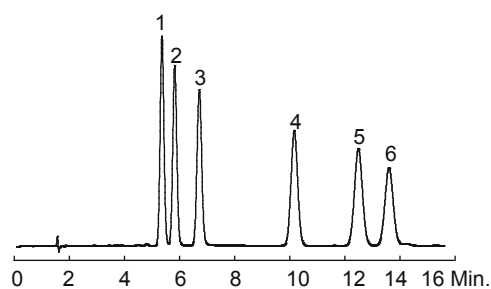


Our Solution for Working Under Highly Aqueous Conditions

The separation of polar compounds under highly aqueous mobile phase conditions is not reproducible with conventional reversed-phase materials. A proprietary derivatization procedure enables Spursil™ columns to be penetrated by water without losing their hydrophobic property. This allows polar compounds to be separated with excellent peak shape and remarkable reproducibility. The separations of water-soluble vitamins and amino acids illustrate the features of the Spursil™ columns in improving selectivity and peak shape and optimizing retention.


Water-Soluble Vitamins

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: MeOH:10 mM K₂HPO₄ (pH 7) = 3:97
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. L-Ascorbic acid
 2. Orotic acid
 3. Pyridoxamine
 4. Pyridoxal
 5. Pyridoxol
 6. Nicotinamide
 7. Thiamine



Amino acids

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: 20 mM KH₂PO₄ (pH 2.5 by H₃PO₄)
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Citrulline
 2. Valine
 3. Methionine
 4. Tyrosine




Although they are designed for use in highly aqueous mobile phase conditions, Spursil™ columns are completely compatible with highly organic mobile phases. The ability to cover the full range of mobile phase composition, from 100% aqueous to 100% organic, is useful for developing gradient methods for analyzing complex samples. High phase density allows highly organic mobile phase for the best desolvation and MS sensitivity.


Tocopherols*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 295 nm
 Sample: 1. δ-Tocopherol
 2. γ-Tocopherol
 3. α-Tocopherol


Dikma Spursil™ 5 μm C18 (Cat#82001)



Agilent ZORBAX 5 μm Bonus-RP



Waters SymmetryShield 5 μm RP18

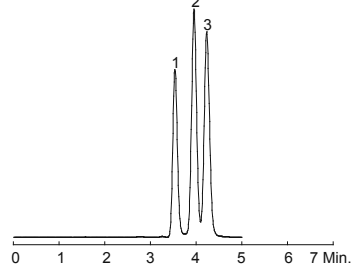

*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*SymmetryShield is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Superior Peak Shape and Resolution for Basic Analytes


The most sensitive measurement of silanol interactions is achieved using highly basic probes with a pH 7 mobile phase. At this pH, many of the residual silanols are in their ionized form, and the basic probes are completely protonated. The protonated bases interact with the ionized silanols by an ion-exchange mechanism, and the degree of tailing is a direct measure of silanol activity. Basic compounds tend to tail on alkyl phases because of the interaction with the silanols on the silica surface. This can often cause increased retention but loss in performance (peak shape). Polar-modified phases shield the silica surface and provide improved peak shape. The separation of a complex mixture of tricyclic antidepressants, having both hydrophobic and polar characteristics, demonstrates the unique selectivity of Spursil™ columns, and the power of stationary phase manipulation in HPLC method development. The polar groups in Spursil™ phases impart a unique selectivity with good separation not observed in traditional alkyl phases. The peak symmetries and efficiency values obtained for these drugs, which are considered to be difficult HPLC candidates, furnish a good measure of performance of these columns for similar problem drugs compared to traditional alkyl columns.

TCAs at Neutral pH*


Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 2:1
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample:
 1. Desipramine
 2. Nortriptyline
 3. Imipramine
 4. Amitriptyline
 5. Trimipramine

Dikma


Spursil™ 5 μm C18 (Cat#82001)




Agilent 5 μm TC-C18



Waters XBridge 5 μm C18



Agilent 5 μm HC-C18



*XBridge is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


β-Blockers at Low and High pHs

β-Blockers are highly basic compounds that tend to give poor peak shape and resolution on conventional C18 and C8 HPLC columns. Spursil™ columns are packed with ultra pure silica and proprietary C18 and C8 bonding and endcapping technologies, resulting in greater peak shape and resolution.


β-Blockers at Low pH*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Metoprolol
 4. Labetolol
 5. Propranolol
 6. Alprenolol


Dikma
 Spursil™ 5 μm C18 (Cat#82001)



Agilent
 ZORBAX 5 μm Bonus-RP




Waters
 SymmetryShield 5 μm RP18




β-Blockers at High pH

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:5 mM NH₄HCO₃ (pH 10) = 70:30
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Pindolol
 2. Metoprolol
 3. Bisoprolol
 4. Propranolol
 5. Alprenolol


Dikma
 Spursil™ 5 μm C18 (Cat#82001)



Agilent
 ZORBAX 5 μm Bonus-RP



Waters
 SymmetryShield 5 μm RP18



*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*SymmetryShield is a trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


Steric Selectivity

Steric selectivity is often the most critical parameter in method development. Dikma had that in mind when designing the Spursil™ line, creating the C18 and C8 columns when small differences in retention and selectivity are desired. The Spursil™ C18-EP can create larger differences in selectivity for resolving difficult pairs or confirming identity. The Spursil™ line of HPLC columns demonstrates Dikma's commitment to solving real-life problems in selectivity and throughput with advanced technology. The separation of bibenzyl and *trans*-stilbene shows the key performance characteristics of improved shape selectivity for similar structure analytes.


Steric Selectivity*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:H₂O = 80:20
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *N,N*-Dimethylaniline
 2. Ethylbenzene
 3. Propylbenzene
 4. Bibenzyl
 5. *trans*-Stilbene


Dikma
 Spursil™ 5 μm C18-EP (Cat#82101)



Agilent
 ZORBAX 5 μm Bonus-RP



Waters
 XBridge 5 μm C18




Enhanced Polar Retention

Conventional C18 columns often provide less retention for polar compounds. Spursil™ C18-EP column exhibits enhanced retention of polar compounds due to its unique embedded polar group design for the stationary phase. Enhanced retention of polar compounds results in a column that is compatible with the high aqueous mobile phases necessary for retaining these polar compounds.


Parabens*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:20 mM K₂HPO₄ (pH 7) = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Methyl paraben
 2. Ethyl paraben
 3. Propyl paraben
 4. Butyl paraben


Dikma
 Spursil™ 5 μm C18-EP (Cat#82101)




Dikma
 Spursil™ 5 μm C18 (Cat#82001)



Agilent
 ZORBAX 5 μm Bonus-RP



Waters
 SymmetryShield 5 μm RP18




*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.


*SymmetryShield and XBridge are trademarks of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Caffeine Metabolites*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:1% CH₃COOH in H₂O = 10:90
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uric acid
 2. Xanthine
 3. 7-Methylxanthine
 4. 1-Methyluric acid
 5. 3-Methylxanthine
 6. 1,3-Dimethyluric acid
 7. Theobromine
 8. 1,7-Dimethylxanthine
 9. Theophylline

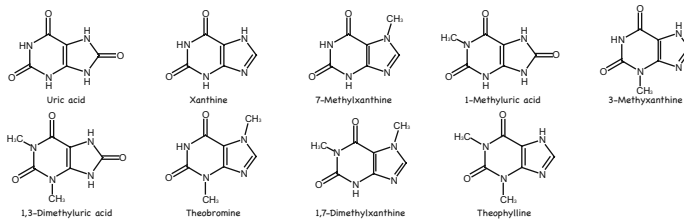


Dikma
 Spursil™ 5 μm C18 (Cat#82001)




The separation of nine caffeine metabolites, each a geostereoisomer of similar structure, demonstrates the resolving power for positional isomers. The Spursil™ C18 column completes this separation in less than 13 minutes, with remarkable selectivity.


Thermo Scientific
 Hypersil 5 μm BDS C18




Agilent
 ZORBAX 5 μm Bonus-RP



Waters
 SymmetryShield 5 μm RP18




Phenomenex
 Gemini 5 μm C18




Water-Soluble Vitamins*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:10 mM K₂HPO₄ (pH 7) = 3:97
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. L-Ascorbic acid
 2. Orotic acid
 3. Pyridoxamine
 4. Pyridoxal
 5. Pyridoxol
 6. Nicotinamide
 7. Thiamine


Dikma
 Spursil™ 5 μm C18 (Cat#82001)




Waters
 XBridge 5 μm C18




Waters
 SymmetryShield 5 μm RP18




Agilent
 ZORBAX 5 μm Bonus-RP



Phenomenex
 Gemini 5 μm C18



Phenomenex
 Luna 5 μm C18(2)



*ZORBAX is a registered trademark of Agilent Technologies. Dikma Technologies Inc. is not affiliated with the above company.

*SymmetryShield and XBridge are trademarks of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.


*Gemini and Luna are registered trademarks of Phenomenex. Dikma Technologies Inc. is not affiliated with the above company.

*Hypersil is a registered trademark of Thermo Scientific. Dikma Technologies Inc. is not affiliated with the above company.


Multiple Injections of Antibiotics on Spursil™ C18 Column

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Ceftazidime
 2. Cefadroxil
 3. Cefuroxime
 4. Cefazoline
 5. Cefaclor
 6. Cephalexin


1st injection

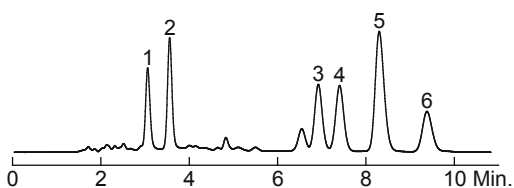

After 500 injections

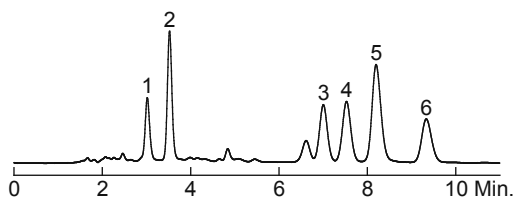


After 1,000 injections

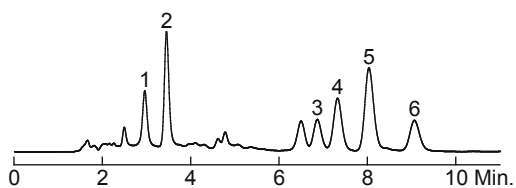


Multiple Injections of Antibiotics on Spursil™ C18-EP Column

Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Ceftazidime
 2. Cefadroxil
 3. Cephalexin
 4. Cefradine
 5. Cefazoline
 6. Cefoxitin


1st injection

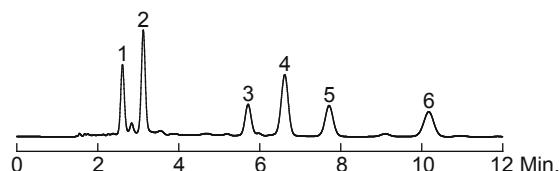

After 500 injections

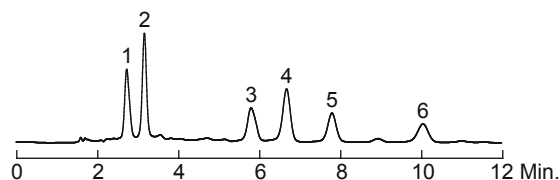

After 1,000 injections

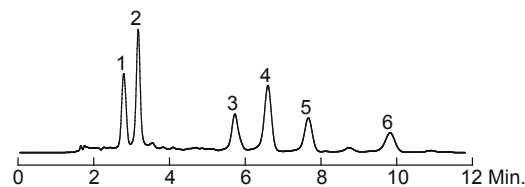

Separation of Cephalosporin Antibiotics at Phosphate Buffer Mobile Phase Conditions*

Column: Listed on chromatograms

Dimension: 150 x 4.6 mm

Mobile Phase: MeOH:25 mM phosphate buffer (pH 3) = 25:75


Flow Rate: 1.0 mL/min

Temperature: Ambient


Detection: UV 230 nm

Sample: 1. Cefadroxil 4. Cephalexin
 2. Ceftazidime 5. Cefazoline
 3. Cefaclor 6. Cefradine


**Dikma
Spursil™ 5 μm C18 (Cat#82001)**

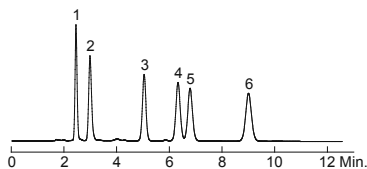


**Dikma
Spursil™ 5 μm C18-EP (Cat#82101)**

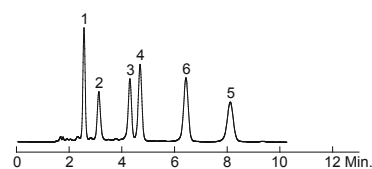


**Waters
SymmetryShield 5 μm RP18**




**Waters
XBridge 5 μm C18**




**Waters
Symmetry 5 μm C18**




**Agilent
ZORBAX 5 μm Bonus-RP**




**Agilent
ZORBAX Eclipse 5 μm XDB-C18**




**GL Science
Inertsil 5 μm ODS-3**




**Phenomenex
Gemini 5 μm C18**

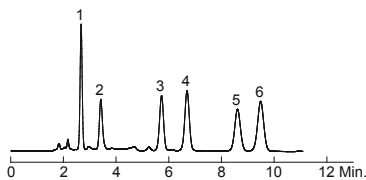


**Phenomenex
Luna 5 μm C18(2)**

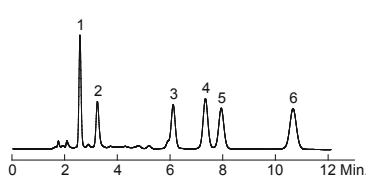


**Eka Chemicals AB
Kromasil 5 μm C18**

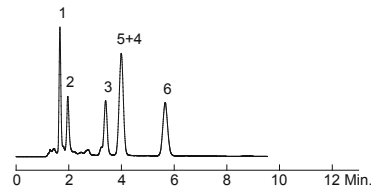


**Thermo Scientific
Hypersil 5 μm BDS C18**



**Beckman Coulter
Ultrasphere 5 μm C18**




**Separation Methods Technologies
OD-5-100 5 μm C18**




*The comparative data presented here may not be representative for all applications.

Separation of Cephalosporin Antibiotics at Acetate Buffer Mobile Phase Conditions

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:100 mM acetate buffer = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Ceftazidime 4. Cefoxitin
 2. Cefadroxil 5. Cefaclor
 3. Cefuroxime 6. Cefradine

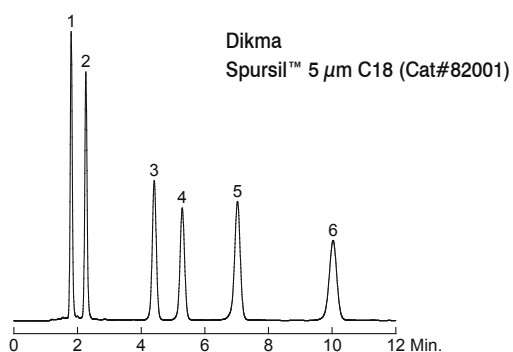


Mobile Phase: MeOH:100 mM acetate buffer = 20:80
 Flow Rate: 1.0 mL/min
 Detection: UV 254 nm
 Sample: 1. Ceftazidime 4. Cefradine
 2. Cephalexin 5. Cefoxitin
 3. Cefaclor

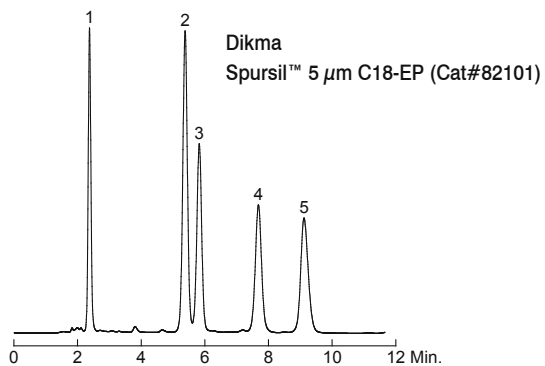


Separation of Cephalosporin Antibiotics at TFA Mobile Phase Conditions

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Ceftazidime 5. Cefaclor
 2. Cefadroxil 6. Cephalexin
 3. Cefuroxime 7. Cefradine
 4. Cefazoline

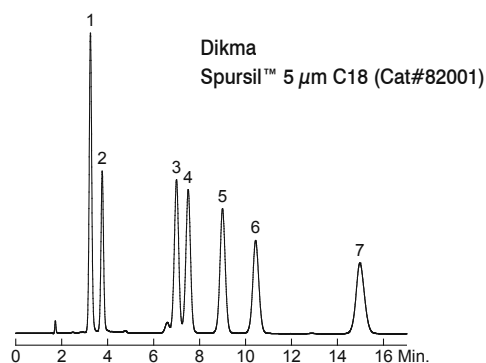



Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Ceftazidime 4. Cefradine
 2. Cefadroxil 5. Cefazoline
 3. Cephalexin 6. Cefoxitin

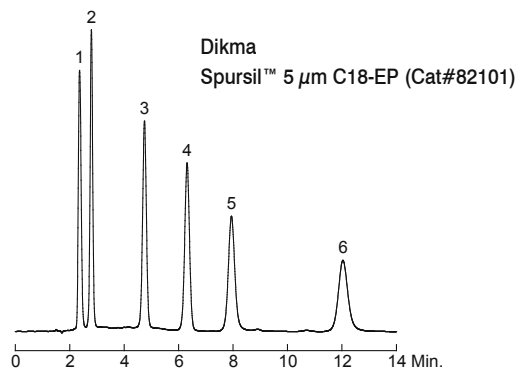

HPLC Columns



Separation of TCAs and Benzos

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Doxepin
 2. Alprazolam
 3. Diazepam
 4. Trimipramine
 5. Triazolam
 6. Clomipramine
 7. Oxazepam
 8. Clonazepam

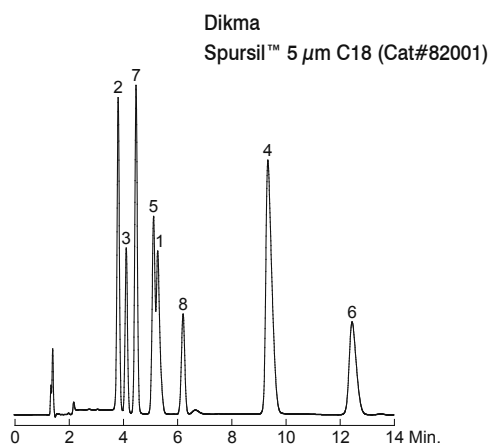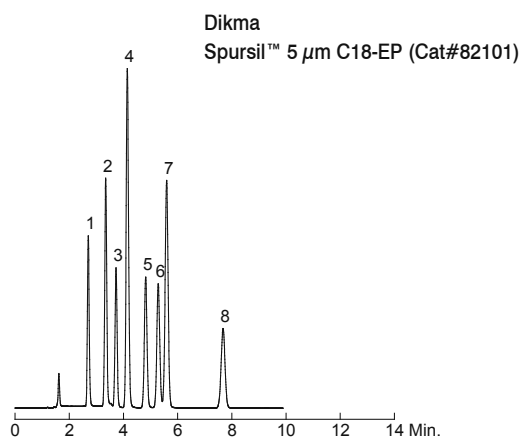

Separation of Nucleotides in 100% Aqueous Conditions


Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 50 mM K₂HPO₄, pH 6
 Flow Rate: 0.7 mL/min
 Temperature: Ambient
 Detection: UV 260 nm
 Sample: 1. CTP
 2. CMP
 3. GTP
 4. GDP
 5. GMP
 6. ATP
 7. ADP
 8. AMP

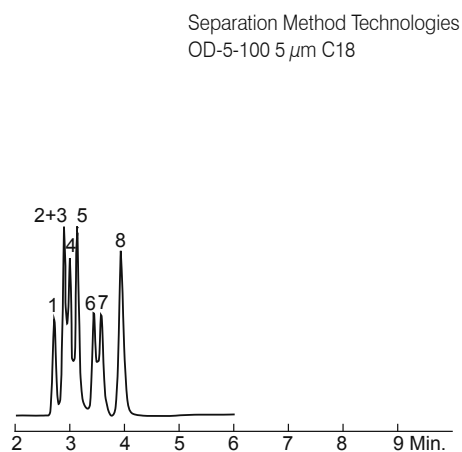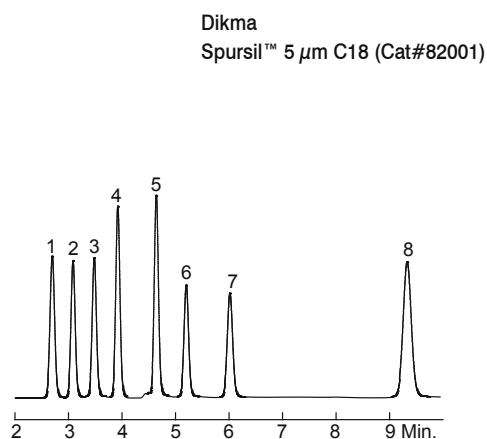


Sander Test*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:20 mM phosphate buffer (pH 7) = 80:20
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uracil
 2. Toluene
 3. Ethylbenzene
 4. Amitriptyline
 5. Quinizarin


Dikma
 Spursil™ 5 µm C18 (Cat#82001)

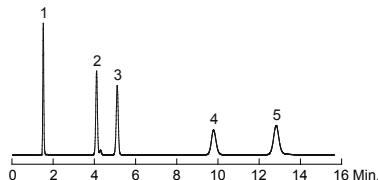


Dikma
 Spursil™ 5 µm C18-EP (Cat#82101)

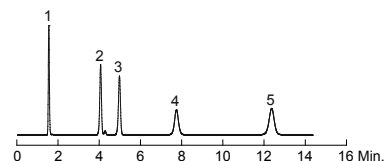


Agilent
 ZORBAX 5 µm Bonus-RP

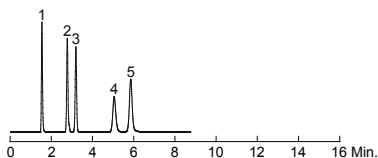


Agilent
 5 µm HC-C18

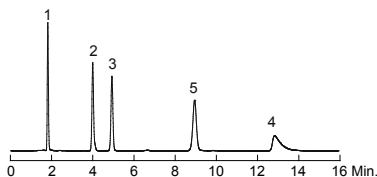


Agilent
 ZORBAX Eclipse 5 µm XDB-C18

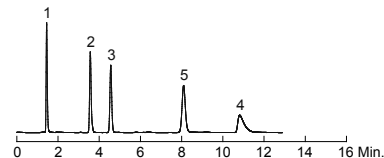


Waters
 XBridge 5 µm C18

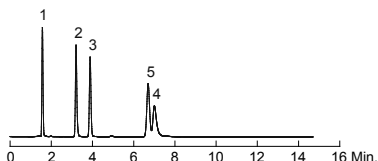


Waters
 Symmetry 5 µm C18

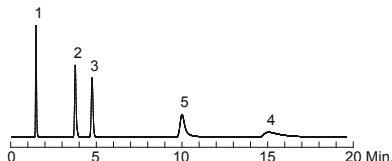


Waters
 SymmetryShield 5 µm RP18

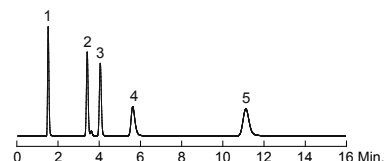


Phenomenex
 Gemini 5 µm C18

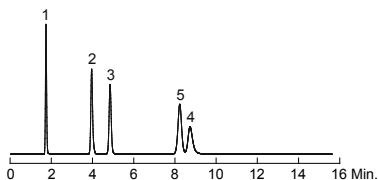


Phenomenex
 Luna 5 µm C18(2)

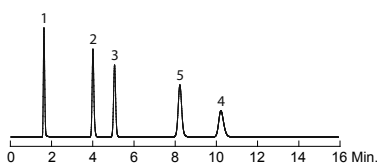


Eka Chemicals AB
 Kromasil 5 µm C18

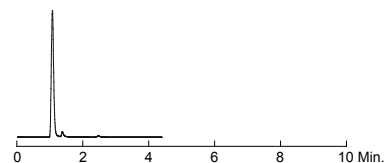


Thermo Scientific
 Hypersil 5 µm BDS C18

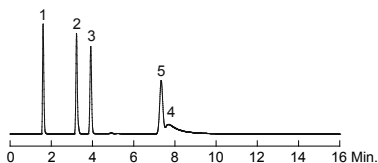

Beckman Coulter
 Ultrasphere 5 µm C18

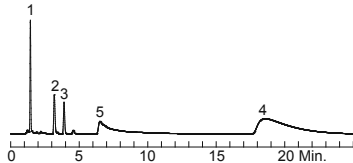

Separation Methods Technologies
 OD-5-100 5 µm C18

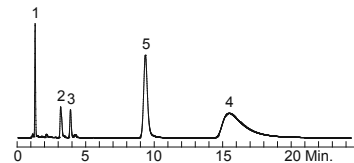


*The comparative data presented here may not be representative for all applications.

HPLC Columns


Phenols*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 55:45
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Phenol 5. 4-Chlorophenol
 2. 2-Nitrophenol 6. 4-Chloro-3-methylphenol
 3. 4-Nitrophenol 7. 2,4-Dichlorophenol
 4. 2-Chlorophenol 8. 2,4,6-Trichlorophenol


Dikma
Spursil™ 5 μm C18 (Cat#82001)

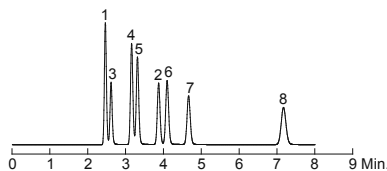


Dikma
Spursil™ 5 μm C18-EP (Cat#82101)

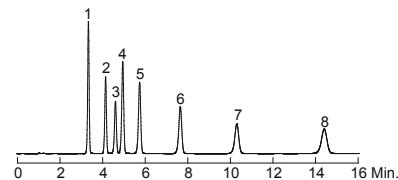


Agilent
ZORBAX 5 μm Bonus-RP

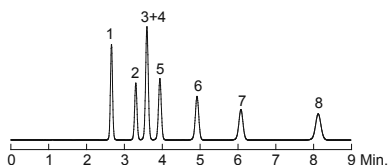


Agilent
ZORBAX 5 μm SB-C18

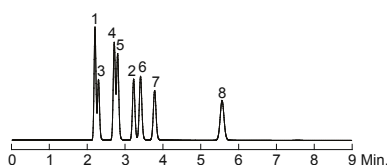


Agilent
ZORBAX Eclipse 5 μm XDB-C18

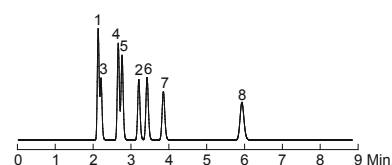


Waters
SymmetryShield 5 μm RP18

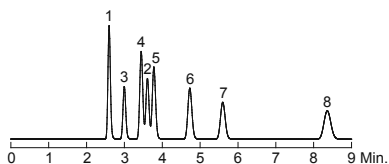


Waters
XBridge 5 μm C18

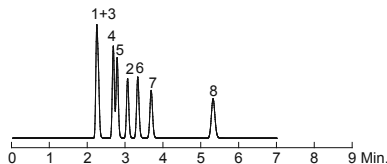


GL Science
Inertsil 5 μm ODS-3

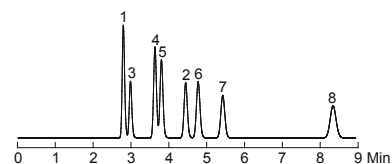


Phenomenex
Gemini 5 μm C18

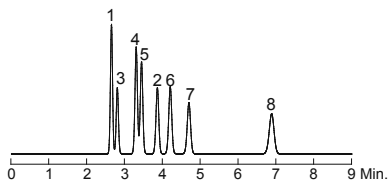


Phenomenex
Luna 5 μm C18(2)

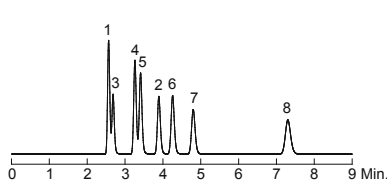


Eka Chemicals AB
Kromasil 5 μm C18

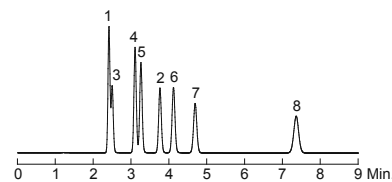


Thermo Scientific
Hypersil 5 μm BDS C18

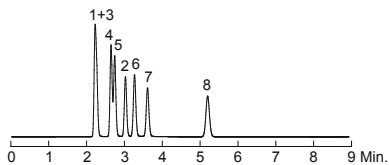

Beckman Coulter
Ultrasphere 5 μm C18

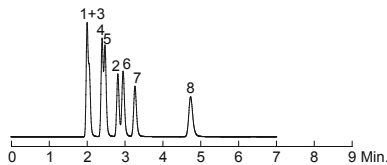

Separation Methods Technologies
OD-5-100 5 μm C18

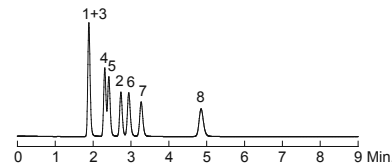


*The comparative data presented here may not be representative for all applications.


Pyridine / Phenol*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:H₂O = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Pyridine
 2. Phenol


Dikma
 Spursil™ 5 μm C18 (Cat#82001)

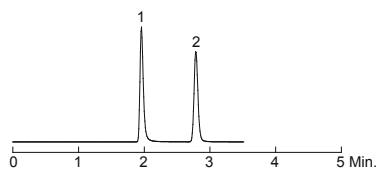


Dikma
 Spursil™ 5 μm C18-EP (Cat#82101)

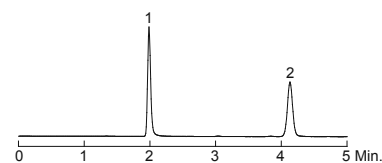


Waters
 XBridge 5 μm C18




Waters
 SymmetryShield 5 μm C18




GL Science
 Inertsil 5 μm ODS-3

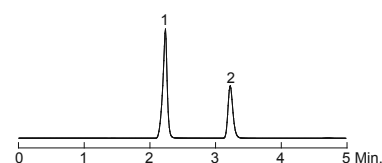


Agilent
 ZORBAX 5 μm Bonus-RP

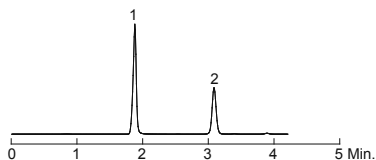


Agilent
 ZORBAX 5 μm SB-C18

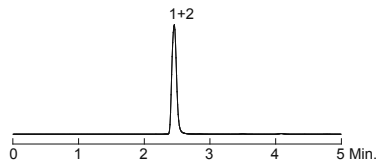


Agilent
 ZORBAX Eclipse 5 μm XDB-C18

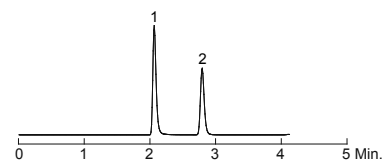


Phenomenex
 Gemini 5 μm C18

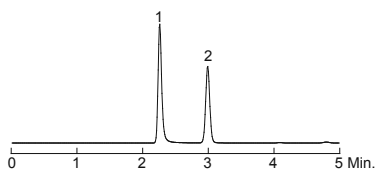


Phenomenex
 Luna 5 μm C18(2)

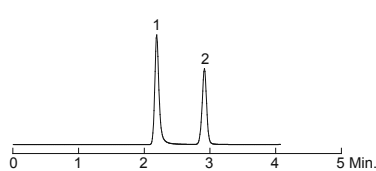


Eka Chemicals AB
 Kromasil 5 μm C18

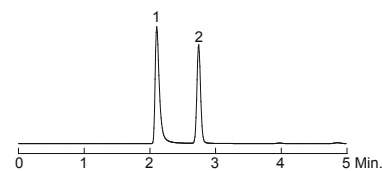


Thermo Scientific
 Hypersil 5 μm BDS C18



Beckman Coulter
 Ultrasphere 5 μm C18



Separation Methods Technologies
 OD-5-100 5 μm C18

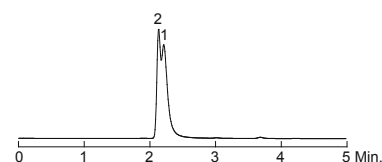


*The comparative data presented here may not be representative for all applications.


Catecholamines*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: 20 mM KH₂PO₄, pH 7
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample:
 1. Norepinephrine
 2. Epinephrine
 3. Dopamine


Dikma
Spursil™ 5 μm C18 (Cat#82001)

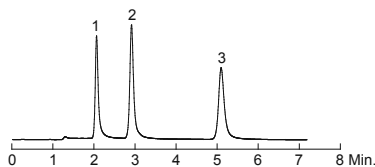


Dikma
Spursil™ 5 μm C18-EP (Cat#82101)

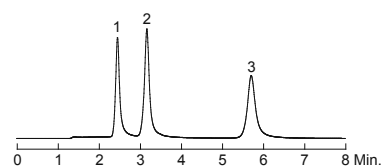


Waters
XBridge 5 μm C18




Waters
Symmetry 5 μm C18




Waters
SymmetryShield 5 μm RP18




Agilent
ZORBAX 5 μm SB-C18




Agilent
ZORBAX 5 μm Bonus-RP




GL Science
Inertsil 5 μm ODS-3




Phenomenex
Gemini 5 μm C18




Phenomenex
Luna 5 μm C18(2)




Eka Chemicals AB
Kromasil 5 μm C18




Thermo Scientific
Hypersil 5 μm BDS C18



Beckman Coulter
Ultrasphere 5 μm C18



Separation Methods Technologies
OD-5-100 5 μm C18

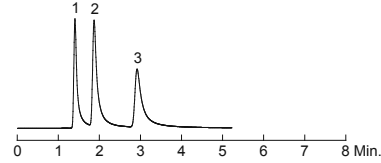


*The comparative data presented here may not be representative for all applications.


Catechols and Resorcinols*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample: 1. Resorcinol 5. 2,5-Dimethylresorcinol
 2. Catechol 6. 3-Methylcatechol
 3. 2-Methylresorcinol 7. 4-Nitrocatechol
 4. 4-Methylcatechol


Dikma
 Spursil™ 5 μm C18 (Cat#82001)




Dikma
 Spursil™ 5 μm C18-EP (Cat#82101)

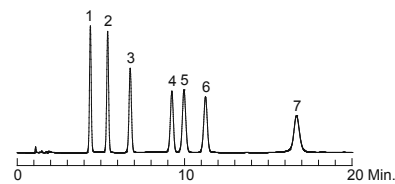


Waters
 XBridge 5 μm C18




Waters
 SymmetryShield 5 μm RP18




GL Science
 Inertsil 5 μm ODS-3




Agilent
 ZORBAX 5 μm Bonus-RP

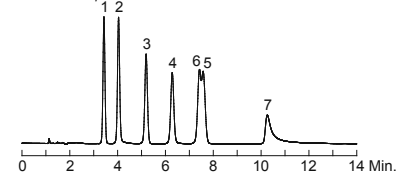


Agilent
 5 μm HC-C18

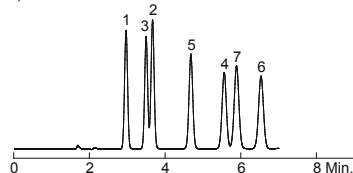


Agilent
 5 μm TC-C18

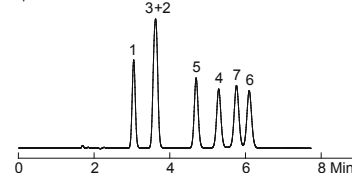


Phenomenex
 Gemini 5 μm C18




Phenomenex
 Luna 5 μm C18(2)




Eka Chemicals AB
 Kromasil 5 μm C18




Thermo Scientific
 Hypersil 5 μm BDS C18

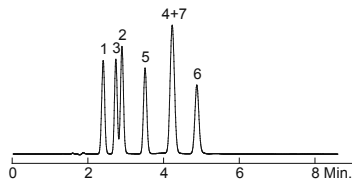

Beckman Coulter
 Ultrasphere 5 μm C18

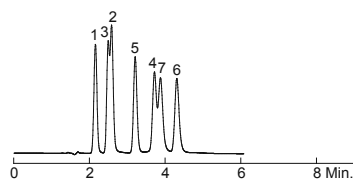

Separation Methods Technologies
 OD-5-100 5 μm C18

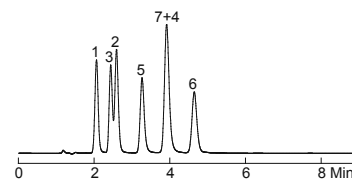


*The comparative data presented here may not be representative for all applications.


TCAs at High pH*

Column: Listed on chromatograms
 Dimension: 150 x 4.6 mm
 Mobile Phase: MeOH:5 mM NH₄HCO₃ (pH 10) = 80:20
 Flow Rate: 1.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Doxepin 5. Trimipramine
 2. Nordoxepin 6. Clomipramine
 3. Imipramine 7. Nortriptyline
 4. Amitriptyline 8. Protriptyline


Dikma
Spursil™ 5 μm C18 (Cat#82001)

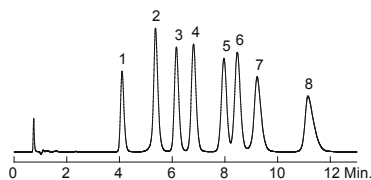


Dikma
Spursil™ 5 μm C18-EP (Cat#82101)

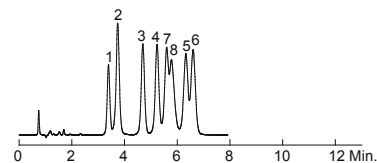


Waters
XBridge 5 μm C18

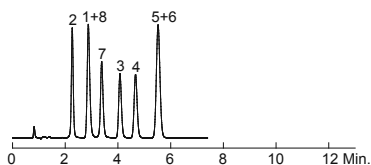


Waters
SymmetryShield 5 μm RP18

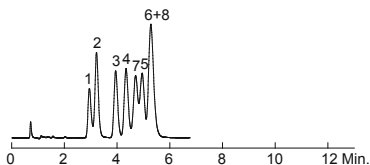


GL Science
Inertsil 5 μm ODS-3

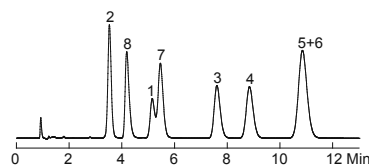


Agilent
5 μm HC-C18

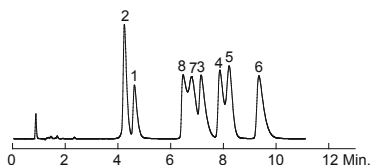


Agilent
5 μm TC-C18

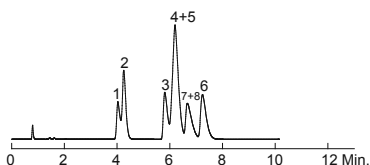


Agilent
ZORBAX 5 μm Bonus-RP

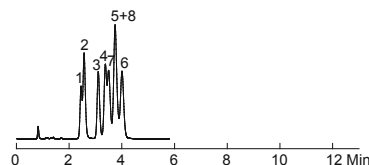


Phenomenex
Gemini 5 μm C18




Phenomenex
Luna 5 μm C18(2)

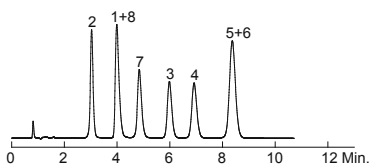


Eka Chemicals AB
Kromasil 5 μm C18

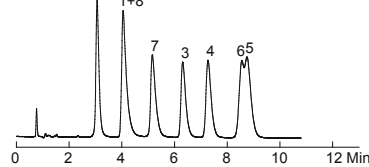


Thermo Scientific
Hypersil 5 μm BDS C18

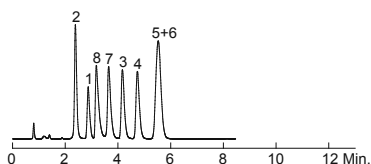

Beckman Coulter
Ultrasphere 5 μm C18

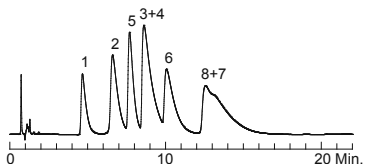

Separation Methods Technologies
OD-5-100 5 μm C18

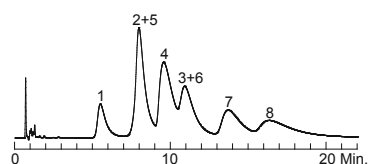

*The comparative data presented here may not be representative for all applications.

Spursil™ Ordering Information

3 µm Microbore Columns (2.1 mm)

Guard Cartridge, 2/pk

Phases	30 x 2.1	Price	50 x 2.1	Price	100 x 2.1	Price	150 x 2.1	Price	250 x 2.1	Price	10 x 2.1	Price
Spursil™ C18	82030	\$353	82004	\$373	82012	\$542	82013	\$592	82015	\$621	6701	\$149
Spursil™ C18-EP	82130	353	82104	373	82112	542	82113	592	82115	621	6702	149

3 µm Analytical Columns (3.0 mm)

Phases	30 x 3.0	Price	50 x 3.0	Price	100 x 3.0	Price	150 x 3.0	Price	250 x 3.0	Price	10 x 2.1	Price
Spursil™ C18	82029	\$353	82021	\$373	82022	\$542	82023	\$592	82024	\$621	6701	\$149
Spursil™ C18-EP	82129	353	82121	373	82122	542	82123	592	82124	621	6702	149

3 µm Analytical Columns (4.6 mm)

Phases	30 x 4.6	Price	50 x 4.6	Price	100 x 4.6	Price	150 x 4.6	Price	250 x 4.6	Price	10 x 4.0	Price
Spursil™ C18	82031	\$353	82016	\$373	82017	\$542	82018	\$592	82020	\$621	6801	\$149
Spursil™ C18-EP	82131	353	82116	373	82117	542	82118	592	82120	621	6802	149

5 µm Microbore Columns (2.1 mm)

Phases	30 x 2.1	Price	50 x 2.1	Price	100 x 2.1	Price	150 x 2.1	Price	250 x 2.1	Price	10 x 2.1	Price
Spursil™ C18	82033	\$343	82003	\$363	82007	\$527	82002	\$577	82009	\$606	6703	\$149
Spursil™ C18-EP	82133	343	82103	363	82107	527	82102	577	82109	606	6704	149

5 µm Analytical Columns (3.0 mm)

Phases	30 x 3.0	Price	50 x 3.0	Price	100 x 3.0	Price	150 x 3.0	Price	250 x 3.0	Price	10 x 2.1	Price
Spursil™ C18	82032	\$343	82025	\$363	82026	\$527	82027	\$577	82028	\$606	6703	\$149
Spursil™ C18-EP	82132	343	82125	363	82126	527	82127	577	82128	606	6704	149

5 µm Analytical Columns (4.6 mm)

Phases	30 x 4.6	Price	50 x 4.6	Price	100 x 4.6	Price	150 x 4.6	Price	250 x 4.6	Price	10 x 4.0	Price
Spursil™ C18	82034	\$343	82010	\$363	82011	\$527	82001	\$577	82006	\$606	6803	\$149
Spursil™ C18-EP	82134	343	82110	363	82111	527	82101	577	82106	606	6804	149

EasyGuard™ Guard Holder: Cat#6220, Price: \$99

5 µm and 10 µm Semi-preparative Columns

Guard Cartridge, 2/pk

Phases	Particle Size (µm)	250 x 4.6		250 x 10.0		150 x 21.2		250 x 21.2		10 x 10.0		10 x 21.2	
		Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
Spursil™ C18	5	82006	\$606	82038	\$1,359	82045	\$2,759	82039	\$2,959	6705	\$195	6706	\$311
Spursil™ C18-EP	5	82106	606	82138	1,359	82145	2,759	82139	2,959	6707	195	6708	311
Spursil™ C18	10	82035	403	82036	1,159	82046	2,359	82037	2,559	6709	195	6710	311
Spursil™ C18-EP	10	82135	403	82136	1,159	82146	2,359	82137	2,559	6711	195	6712	311

10 mm Guard Holder: Cat#6221, Price: \$199, 21.2 mm Guard Holder: Cat#6222, Price: \$299

10 µm Packing Materials

Phases	Particle Size (µm)	100 G		1 KG	
		Cat. No.	Price	Cat. No.	Price
Spursil™ C18	10	85201	Inquire	85202	Inquire
Spursil™ C18-EP	10	85301	Inquire	85302	Inquire

Features of Bio-Bond™ Columns


- Designed to analyze and purify proteins, peptides and biomolecules
- Available with C18, C8 and C4 bonded phases
- Direct scale-up to preparative material
- Outstanding reproducibility, efficiency and column lifetime

Bio-Bond™ columns with 300 Å pore silica gel are suitable for analysis of proteins, peptides and biological samples. Meticulous care is given to the quality control of surface smoothness, particle shape, pore structure and pore consistency to ensure uniformity of particle structure and enhanced mechanical strength. A low fine percentage from damaged silica particles strengthens the column bed, leading to low backpressure and enhanced column performance and lifetime. Ultra low active silanol and metal content make perfect symmetrical peaks and avoid protein absorption, thereby ensuring detectable activity for protein sensitive to metal.


Bio-Bond™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Purity (%)	Phase density (µmol/m ²)	Carbon loading (%)	pH range	Endcapping
C18	3, 5, 10	300	100	> 99.999	3.7	8	2 - 8	Yes
C8	3, 5, 10	300	100	> 99.999	4.5	5	2 - 8	Yes
C4	3, 5, 10	300	100	> 99.999	4.4	3	2 - 8	Yes


Insulin Genetic Variant

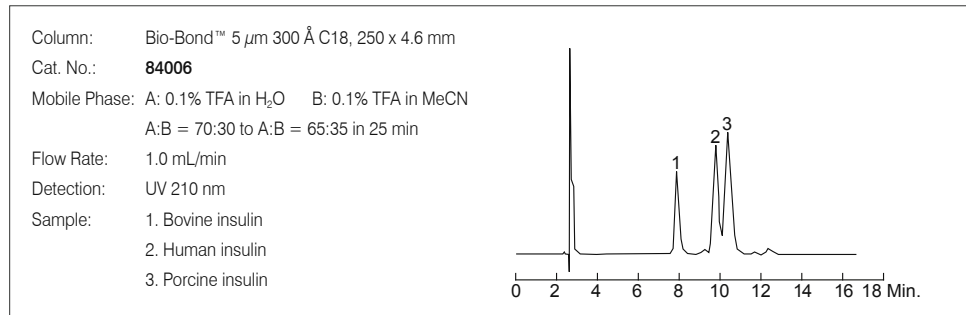

Chemotactic Peptide

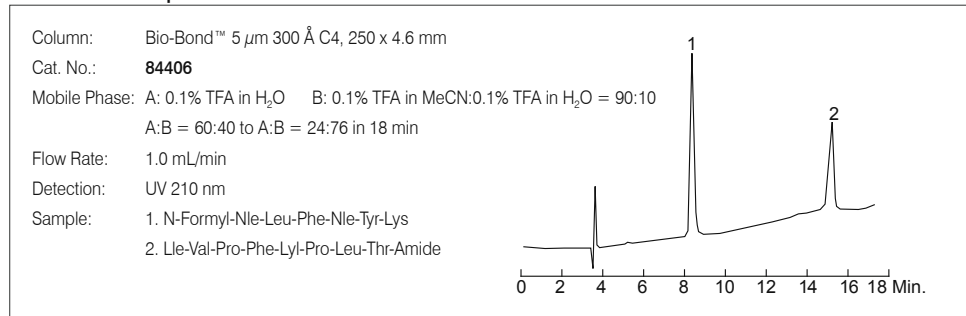

Proteins

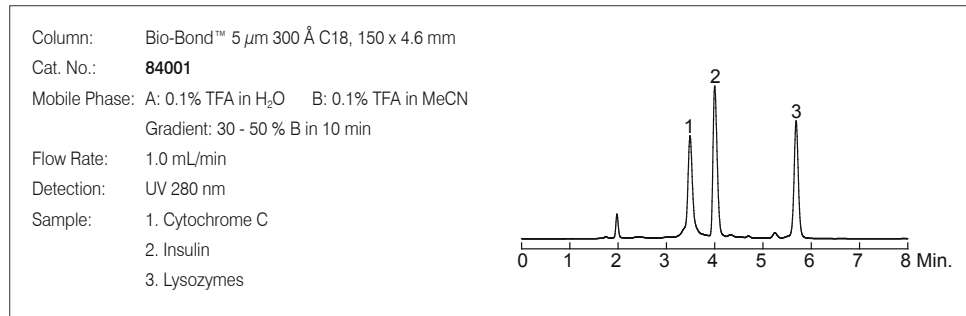

Bio-Bond™ Ordering Information

3 μm Analytical Columns

Phases	50 x 2.1	Price	150 x 2.1	Price	50 x 4.6	Price	150 x 4.6	Price	250 x 4.6	Price	10 x 2.1	Price	10 x 4.0	Price
Bio-Bond™ C18	84004	\$373	84013	\$592	84016	\$373	84018	\$592	84020	\$621	6901	\$149	6951	\$149
Bio-Bond™ C8	84104	373	84113	592	84116	373	84118	592	84120	621	6902	149	6952	149
Bio-Bond™ C4	84404	373	84413	592	84416	373	84418	592	84420	621	6905	149	6955	149

5 μm Analytical Columns

Phases	50 x 2.1	Price	150 x 2.1	Price	50 x 4.6	Price	150 x 4.6	Price	250 x 4.6	Price	10 x 2.1	Price	10 x 4.0	Price
Bio-Bond™ C18	84003	\$363	84002	\$577	84010	\$363	84001	\$577	84006	\$606	6903	\$149	6953	\$149
Bio-Bond™ C8	84103	363	84102	577	84110	363	84101	577	84106	606	6904	149	6954	149
Bio-Bond™ C4	84403	363	84402	577	84410	363	84401	577	84406	606	6906	149	6956	149

EasyGuard™ Holder: Cat#6220

5 μm and 10 μm Semi-preparative Columns

Phases	Particle Size (μm)	250 x 4.6		250 x 10.0		150 x 21.2		250 x 21.2		10 x 10.0		10 x 21.2	
		Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
Bio-Bond™ C18	5	84006	\$606	84038	\$1,359	84045	\$2,759	84039	\$2,959	6907	\$195	6908	\$311
Bio-Bond™ C8	5	84106	606	84138	1,359	84145	2,759	84139	2,959	6909	195	6910	311
Bio-Bond™ C4	5	84406	606	84438	1,359	84445	2,759	84439	2,959	6911	195	6912	311
Bio-Bond™ C18	10	84035	403	84036	1,159	84046	2,359	84037	2,559	6913	195	6914	311
Bio-Bond™ C8	10	84135	403	84136	1,159	84146	2,359	84137	2,559	6915	195	6916	311
Bio-Bond™ C4	10	84435	403	84436	1,159	84446	2,359	84437	2,559	6917	195	6918	311

10 mm EasyGuard™ Holder: Cat#6221, Price: \$199, 21.2 mm EasyGuard™ Holder: Cat#6222, Price: \$299

Features of Platisil™ Columns


- Unique bonding technology prevents the phase collapse, and allows stable retention in highly aqueous mobile phases
- Unique selectivity, excellent peak shape
- Enhanced retention of polar compounds
- High loadability
- pH range 1 - 11
- Reduced silanol interactions and improved peak shape for basic analytes

Platisil™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Purity (%)	Impurities (mg/kg)	Carbon loading (%)	pH range	Endcapping
C18	5	100	440	> 99.999	< 10	15	1 - 11	Yes


Cold Medicine

Column: Platisil™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **99501**
 Mobile Phase: MeOH:MeCN:1% sodium dodecyl sulfate:
 acetic acid = 30:35:30:0.3
 Flow Rate: 1.0 mL/min
 Detection: UV 265 nm
 Temperature: Ambient
 Sample: 1. Pseudoephedrine hydrochloride
 2. Naphazoline hydrochloride
 3. Chlorpheniramine
 4. Dextromethorphan hydrobromide

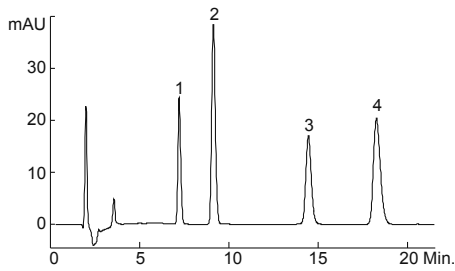

The Active Ingredients of Rhubarb

Column: Platisil™ 5 µm C18, 250 x 4.6 mm
 Cat. No.: **99503**
 Mobile Phase: MeOH:0.1% phosphoric acid = 80:20
 Flow Rate: 1.0 mL/min
 Detection: UV 254 nm
 Temperature: 30 °C
 Sample: 1. Aloe emodin
 2. Rhein
 3. Emodin
 4. Chrysophanol
 5. Physcion

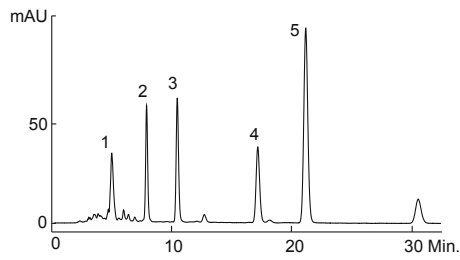

Platisil™ Ordering Information

5 µm Analytical Columns

Phase	150 x 4.6	Price	250 x 4.6	Price
Platisil™ C18	99501	\$519	99503	\$545

Features of EasyGuard™ Columns

- Universal design to match any brand column
- A variety of optional bonded phase material
- Does not affect the analytical column resolution
- Long lifetime column cartridges, high performance and low price

Balance

Guard columns provide protection against contamination with minimal impact on column efficiency. The column diameter determines both the sample loadability and column efficiency. A small diameter will decrease the column lifetime, but a large diameter will adversely affect column resolution. EasyGuard™ columns effectively protect the analytical column without adversely affecting the resolution or column lifetime.

Simple to Use

- Flexibility to move PEEK fittings
- Matches any brand analytical column
- Low dead volume connection
- Rugged 316 stainless steel column holder


EasyGuard™ Kit (1 holder and 2 cartridges)

Description	10 x 2.1 mm	Price	10 x 4.0 mm	Price
C18	6231	\$158	6201	\$158
C8	6232	158	6202	158
Phenyl	6233	158	6203	158
CN	6234	158	6204	158
NH ₂	6235	158	6205	158
Silica	6236	158	6206	158



EasyGuard™ Replacement Cartridges (5/pk)

Description	10 x 2.1 mm	Price	10 x 4.0 mm	Price
C18	6241	\$147	6211	\$147
C8	6242	147	6212	147
Phenyl	6243	147	6213	147
CN	6244	147	6214	147
NH ₂	6245	147	6215	147
Silica	6246	147	6216	147



EasyGuard™ Guard Column Accessories

Description	Qty	Cat. No.	Price
EasyGuard™ Holder Assembly	1/pk	6220	\$99
PEEK Fingertight Fitting (Machined Version)	5/pk	90412	55

Easy-Lok™ Coupler **New!**

When the EasyGuard™ guard column connects to a 250 mm analytical column, it can not fit in certain ovens (such as Agilent 1200) because the length is not long enough. The Easy-Lok™ coupler resolves this issue by removing the pre-tightened connecting pipe by wrench before using.

Description	Qty	Cat. No.	Price
Easy-Lok™ Coupler	1/pk	6132	\$59
Tip for Easy-Lok™ Coupler, PEEK	2/pk	6133	49



Preparative Chromatography

Dikma prep materials are designed to provide fast separation with superior performance in suitable for the most demanding preparative applications. The stationary phases created by combining advanced bonding technologies with high surface area ultra-pure silica deliver superior resolution and loadability, extended column lifetime and excellent stability and reproducibility. With Dikma prep column you can load more samples and obtain a larger amount of purified product in less time.



Features of Dikma Preparative Chromatography Packing Materials :

Excellent Mechanical Stability

By optimizing pore volume, pore diameter, particle size structure, Dikma preparative chromatography packing materials maintain their physical and chemical integrity through repeated packing and unpacking cycles.

During the mechanical strength test, the same batch for Dikma Inspire™ 10 μm materials was packed, tested for column pressure, and then unpacked material. This process is repeated for 10 times in a 250 x 4.6 mm column at a pressure of 2,000 psi. The result of the pressure test as shown below did not significantly change.

The second test proves as well the mechanical strength of Dikma packing materials. The data illustrated clearly indicates a linear correlation between column pressure and packing pressure, which indicates that Dikma packing materials have strong mechanical stability.

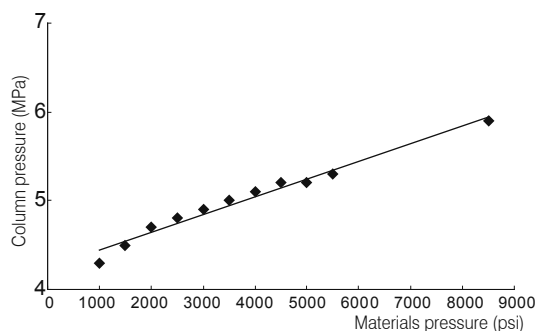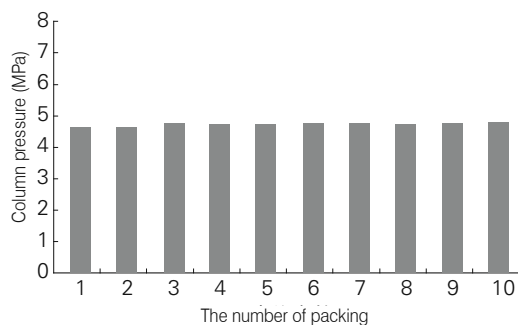




Quick and Easy Transition from Analytical to Prep

Dikma Technologies Inc. offers the same line of packing materials, although the particles are different with no change in selectivity and retention characteristics, to support rapid scale-up from analytical to preparative scale, making it more convenient for method development.

Scale up from analytical to prep is easily achieved without loss of performance. High-tech packing procedures in combination with the State-of-the-Art Dikma bonded phases ensure similar chromatographic performance regardless of dimension. This eliminates the need of additional time-consuming method development. Dikma offers columns in 3, 5 and 10 μm particle sizes that make it easy to scale-up. The data demonstrates easy linear scale-up of natural products from 3 μm and 5 μm analytical columns to a 10 μm preparative column.


Linear Scale-up

Column: Inspire™ C18, 250 x 4.6 mm
Mobile Phase: MeCN:H₂O = 70:30
Flow Rate: 1.0 mL/min
Temperature: 30 °C
Detection: UV 220 nm
Sample: 1. Capsaicin 2. Dihydrocapsaicin



Linear Scale-up with LSF=1000

Mobile Phase: *n*-hexane:isopropanol = 80:20
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Toluene 2. 4-Nitrobenzyl alcohol 3. 2-Nitrobenzyl alcohol







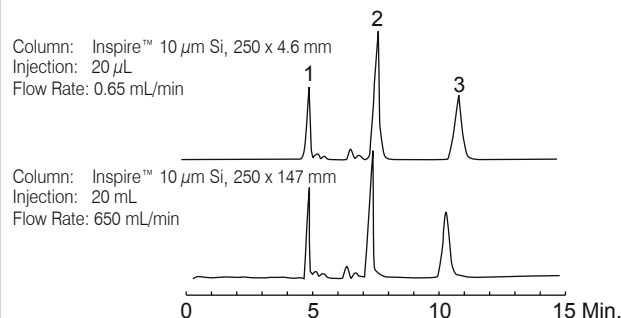


Maximum Loadability

The loadability is an important parameter for preparative chromatography as packing materials with high loading capacity and good separation efficiency can undoubtedly improve the overall yield. Dikma uses a proprietary technique to bond more alkyl groups to silica surface to increase the loadability of the packing material.

Dikma prep offers maximum loadability, which results in improved laboratory productivity by delivering more purified material per run time. Superior mass loading capabilities translate into less preparative runs for a given amount of pure material, resulting in faster purification and increased throughput.

Column: Inspire™ 10 µm C18, 250 x 21.2 mm
 Cat. No.: 81037
 Mobile Phase: MeOH:H₂O = 70:30
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Methyl benzoate
 2. Ethyl benzoate

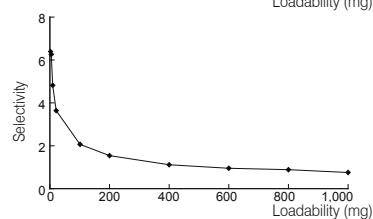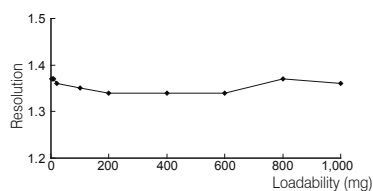


Increasing loadability did not reduce the resolution of compounds 1 and 2


Column: Listed on chromatograms
 Dimension: 250 x 4.6 mm
 Mobile Phase: MeOH:H₂O = 70:30
 Flow Rate: 20 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Methyl benzoate
 2. Ethyl benzoate

0.1 mg


Dikma Inspire™ 10 µm C18 (Cat#81035)



Kromasil* 10 µm C18




DAISOGEL* 10 µm C18-AP




20 mg


Dikma Inspire™ 10 µm C18 (Cat#81035)



Kromasil 10 µm C18




DAISOGEL 10 µm C18-AP




50 mg


Dikma Inspire™ 10 µm C18 (Cat#81035)



Kromasil 10 µm C18



DAISOGEL 10 µm C18-AP



*Kromasil is a registered trademark of Eka Chemicals AB. Dikma Technologies Inc. is not affiliated with the above company.


*DAISOGEL is a registered trademark of DAISO Co., LTD.. Dikma Technologies Inc. is not affiliated with the above company.

Preparative Chromatography

Outstanding Chemical Stability

Silica-based materials may be hydrolyzed or dissolved in the low pH or high pH, leading to loss of stationary phase and rapidly decreasing column efficiency. Dikma preparative chromatography packing materials have excellent stability in these extreme pH conditions. We continuously flushed a Dikma Inspire™ C18 column for more than 1440 hours at pH 1 and pH 11 respectively, and then recorded and calculated the retention time, asymmetry and capacity factor (as shown below). The experimental data show the Dikma Inspire™ C18 column can maintain outstanding tolerance and stability under extreme pH conditions.

Column: Inspire™ 10 μ m C18, 150 x 4.6 mm
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample:
 1. Uracil
 2. Pyridine
 3. Phenol
 4. Benzene

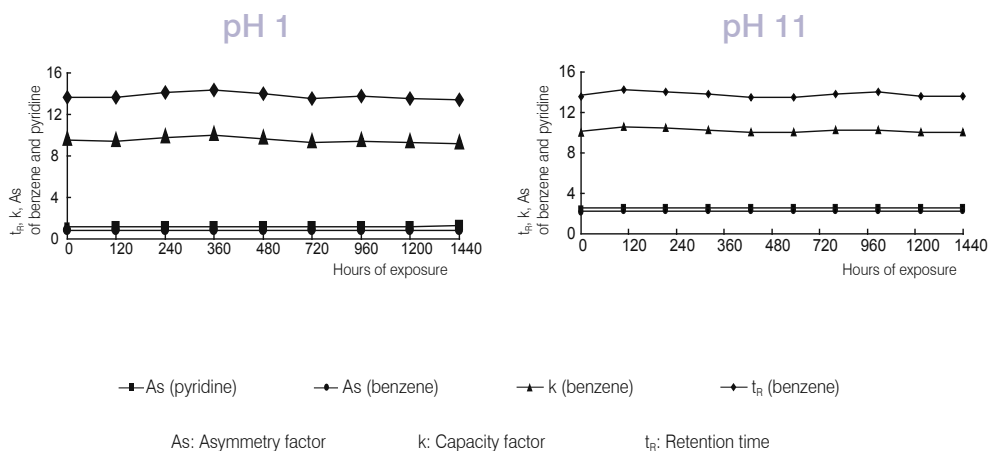

Flush solution (pH 1)

Mobile Phase: 1% TFA in MeCN:1% TFA in H₂O = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient

Flush solution (pH 11)




Mobile Phase: MeCN:20 mM phosphate buffer = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient

Ultimate Performance

Large-scale purification process consumes a large amount of solvents and increases production costs. Fast separation without compromising resolution can reduce solvent use and production costs.




Separation of Basic Compounds*

Column: Listed on chromatograms
 Dimension: 250 x 4.6 mm
 Mobile Phase: MeOH:5 mM NaHCO₃ (pH 10) = 70:30
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Norclozapine
 2. Verapamil
 3. Diphenhydramine

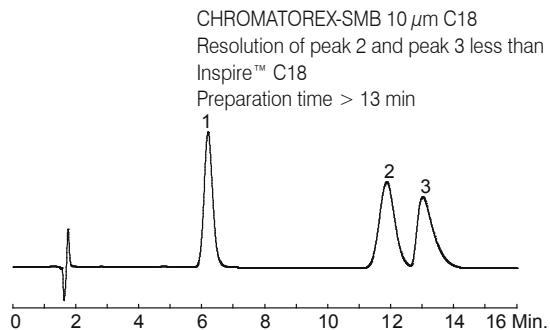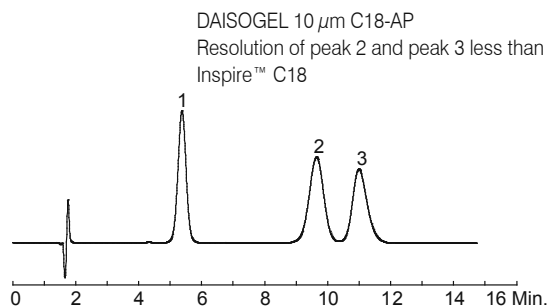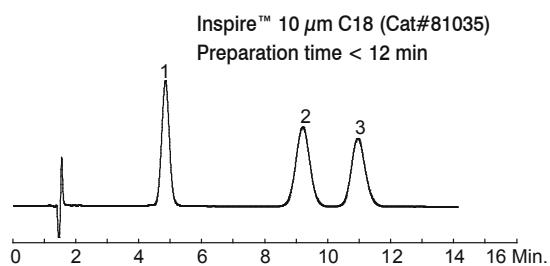

Separation of Acidic Compounds

Column: Listed on chromatograms
 Dimension: 250 x 4.6 mm
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Homovanillic acid
 2. *o*-Hydroxyhippuric acid
 3. Sorbic acid
 4. Salicylic acid
 5. Nalidixic acid

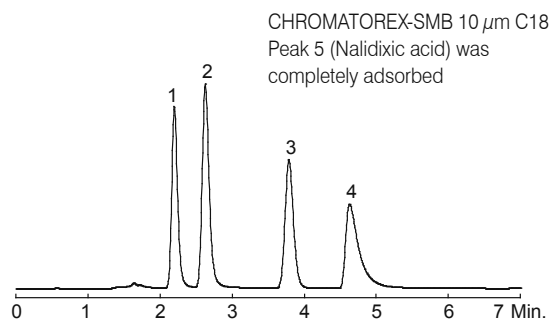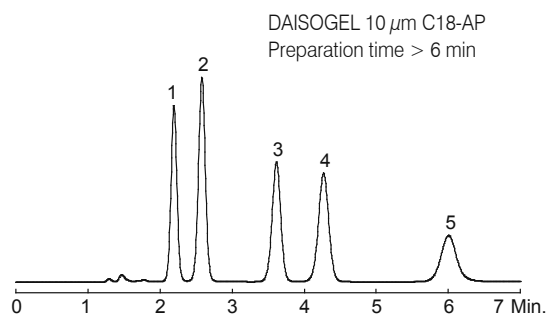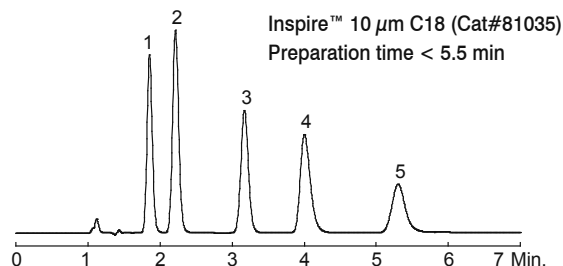

*DAISOGEL is a registered trademark of DAISO Co., LTD.. Dikma Technologies Inc. is not affiliated with the above company.

*CHROMATOREX is a registered trademark of Fuji Silysia Chemical Ltd.. Dikma Technologies Inc. is not affiliated with the above company.





Preparative Chromatography

Unparalleled Performance

Dikma preparative chromatography packing materials are promoted by Dikma Technologies Inc. with independent intellectual property rights. Dikma adopts ultrapure spherical silica with a larger specific surface area and patented chemical bonding technology to ensure high resolution and shortened separation time, thereby increasing the loadability while saving solvent, and improving yield.

Separation of Basic Compounds*

Column: Listed on chromatograms
Dimension: 250 x 4.6 mm
Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 30:70
Flow Rate: 1.0 mL/min
Temperature: 30 °C
Detection: UV 220 nm
Sample: 1. Nadolol
2. Pindolol
3. Metoprolol
4. Labetolol
5. Propranolol

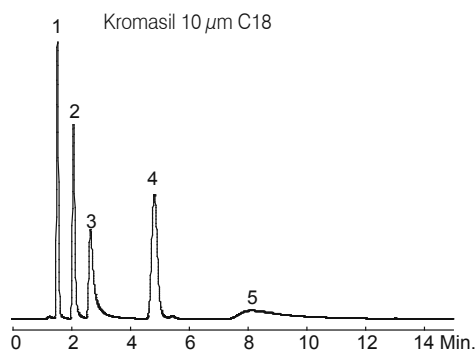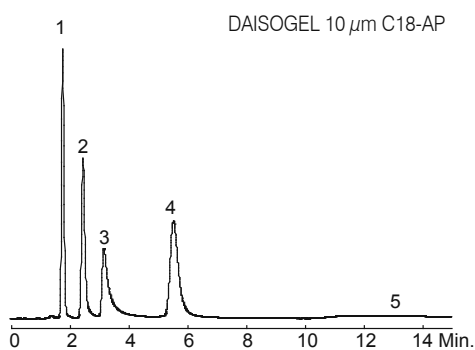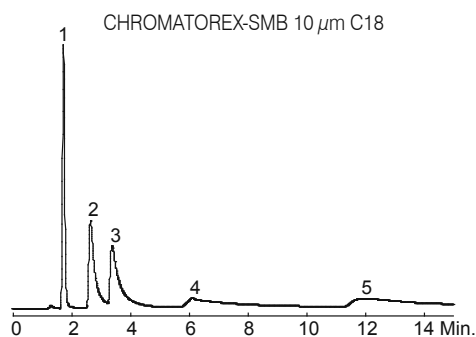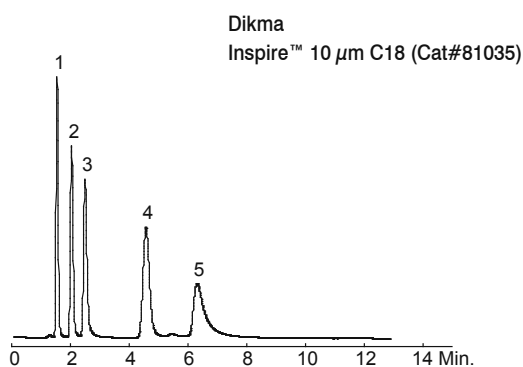

*DAISOGEL is a registered trademark of DAISO Co., LTD.. Dikma Technologies Inc. is not affiliated with the above company.

*CHROMATOREX is a registered trademark of Fuji Silysia Chemical Ltd.. Dikma Technologies Inc. is not affiliated with the above company.

*Kromasil is a registered trademark of Eka Chemicals AB. Dikma Technologies Inc. is not affiliated with the above company.

Features of Inspire™ Semi-preparative and Preparative Columns

- Rapid separations with outstanding resolution, high loadability
- Wide applications, suitable for separation of acidic / neutral / basic compounds
- Support linear scale-up, from analytical to preparative scale
- High mechanical strength, long column lifetime

Inspire™ material meets the most stringent requirements from analytical to preparative scale in the pharmaceutical industry. High surface area and carbon load are the keys to success. These features meet preparative chromatography resolution, and loadability requirements in the pharmaceutical production.



Inspire™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Carbon loading (%)	pH range	Endcapping
C18	5, 10	100	440	27	1 - 11	Yes
C8	5, 10	100	440	17	1 - 11	Yes
Diol	5, 10	100	440	7.5	2 - 8	No

Inspire™ Ordering Information

Phases	Particle 250 x 4.6		250 x 10.0		150 x 21.2		250 x 21.2		Guard Cartridge 2/pk				Bulk Materials				
	(µm)	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	10 x 10.0	10 x 21.2	100 G	1 KG	Cat. No.	Price	Cat. No.	Price
Inspire™ C18	5	81006	\$587	81038	\$1,291	81045	\$2,691	81039	\$2,891	6505	\$195	6506	\$311	-	-	-	-
Inspire™ C8	5	81106	587	81138	1,291	81145	2,691	81139	2,891	6507	195	6508	311	-	-	-	-
Inspire™ Diol	5	81247	587	81238	1,291	81245	2,691	81239	2,891	6509	195	6510	311	-	-	-	-
Inspire™ C18	10	81035	383	81036	1,092	81046	2,291	81037	2,491	6511	195	6512	311	85001	Inquire	85002	Inquire
Inspire™ C8	10	81135	383	81136	1,092	81146	2,291	81137	2,491	6513	195	6514	311	85101	Inquire	85102	Inquire
Inspire™ Diol	10	81235	383	81236	1,092	81246	2,291	81237	2,491	6515	195	6516	311	85021	Inquire	85022	Inquire

Features of Spursil™ Semi-preparative and Preparative Columns

- Surfaces modified with polar groups, stable retention in highly aqueous mobile phase conditions
- Enhanced retention for hydrophilic and polar compounds
- Support linear scale-up, from analytical to preparative scale
- High mechanical strength, long column lifetime

Spursil™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Carbon loading (%)	pH range	Endcapping
C18	5, 10	100	440	25	1.5 - 10	Yes
C18-EP	5, 10	100	440	24	1.5 - 10	Yes

Spursil™ Ordering Information

Phases	Particle 250 x 4.6		250 x 10.0		150 x 21.2		250 x 21.2		Guard Cartridge 2/pk				Bulk Materials				
	(µm)	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	10 x 10.0	10 x 21.2	100 G	1 KG	Cat. No.	Price	Cat. No.	Price
Spursil™ C18	5	82006	\$606	82038	\$1,359	82045	\$2,759	82039	\$2,959	6705	\$195	6706	\$311	-	-	-	-
Spursil™ C18-EP	5	82106	606	82138	1,359	82145	2,759	82139	2,959	6707	195	6708	311	-	-	-	-
Spursil™ C18	10	82035	403	82036	1,159	82046	2,359	82037	2,559	6709	195	6710	311	85201	Inquire	85202	Inquire
Spursil™ C18-EP	10	82135	403	82136	1,159	82146	2,359	82137	2,559	6711	195	6712	311	85301	Inquire	85302	Inquire

Preparative Chromatography

Features of Luster™ Semi-preparative and Preparative Columns

- Support linear scale-up, from analytical to preparative scale
- Economical packing
- High separation capacity and loadability
- Long column lifetime
- Excellent reproducibility
- High performance at a reasonable price

Luster™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Carbon loading (%)	pH range	Endcapping
C18	5, 10	110	320	20	2 - 9	Yes
C8	5, 10	110	320	12	2 - 9	Yes
Diol	5, 10	110	320	5	2 - 8	No
Silica	5, 10	110	320	-	-	No

Luster™ Ordering Information

Phases	Particle 250 x 4.6 (µm)		250 x 10.0		150 x 21.2		250 x 21.2		Guard Cartridge 2/pk				Bulk Materials			
	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	10 x 10.0	10 x 21.2	100 G	1 KG	Cat. No.	Price	Cat. No.	Price
Luster™ C18	5	83046 \$528	83047 \$1,161	83051 \$2,401	83048 \$2,601	6409 \$195	6410 \$311	-	-	-	-	-	-	-	-	-
Luster™ C8	5	83146 528	83147 1,161	83151 2,401	83148 2,601	6411 195	6412 311	-	-	-	-	-	-	-	-	-
Luster™ Diol	5	83246 528	83247 1,161	83251 2,401	83248 2,601	6413 195	6414 311	-	-	-	-	-	-	-	-	-
Luster™ Silica	5	83346 528	83347 1,161	83351 2,401	83348 2,601	6415 195	6416 311	-	-	-	-	-	-	-	-	-
Luster™ C18	10	83035 345	83036 983	83045 2,041	83037 2,241	6401 195	6402 311	85601	Inquire	85602	Inquire	-	-	-	-	-
Luster™ C8	10	83135 345	83136 983	83145 2,041	83137 2,241	6403 195	6404 311	85631	Inquire	85632	Inquire	-	-	-	-	-
Luster™ Diol	10	83235 345	83236 983	83245 2,041	83237 2,241	6405 195	6406 311	85621	Inquire	85622	Inquire	-	-	-	-	-
Luster™ Silica	10	83335 345	83336 983	83345 2,041	83337 2,241	6407 195	6408 311	85611	Inquire	85612	Inquire	-	-	-	-	-

Features of Bio-Bond™ Semi-preparative and Preparative Columns

- Designed to analyze and purify proteins, peptides and biomolecules
- Uniformity of particle structure
- Perfect endcapping
- Support linear scale-up, from analytical to preparative scale

Bio-Bond™ Material Characteristics

Bonded phase	Particle size (µm)	Pore size (Å)	Surface area (m ² /g)	Carbon loading (%)	pH range	Endcapping
C18	5, 10	300	100	8	2 - 8	Yes
C8	5, 10	300	100	5	2 - 8	Yes
C4	5, 10	300	100	3	2 - 8	Yes

Bio-Bond™ Ordering Information

Phases	Particle 250 x 4.6 (µm)		250 x 10.0		150 x 21.2		250 x 21.2		Guard Cartridge 2/pk				Bulk Materials			
	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	10 x 10.0	10 x 21.2	100 G	1 KG	Cat. No.	Price	Cat. No.	Price
Bio-Bond™ C18	5	84006 \$606	84038 \$1,359	84045 \$2,759	84039 \$2,959	6907 \$195	6908 \$311	-	-	-	-	-	-	-	-	-
Bio-Bond™ C8	5	84106 606	84138 1,359	84145 2,759	84139 2,959	6909 195	6910 311	-	-	-	-	-	-	-	-	-
Bio-Bond™ C4	5	84406 606	84438 1,359	84445 2,759	84439 2,959	6911 195	6912 311	-	-	-	-	-	-	-	-	-
Bio-Bond™ C18	10	84035 403	84036 1,159	84046 2,359	84037 2,559	6913 195	6914 311	85701	Inquire	85702	Inquire	-	-	-	-	-
Bio-Bond™ C8	10	84135 403	84136 1,159	84146 2,359	84137 2,559	6915 195	6916 311	85731	Inquire	85732	Inquire	-	-	-	-	-
Bio-Bond™ C4	10	84435 403	84436 1,159	84446 2,359	84437 2,559	6917 195	6918 311	85741	Inquire	85742	Inquire	-	-	-	-	-

10 mm EasyGuard™ Holder, Cat# 6221 Price: \$199, 21.2 mm EasyGuard™ Holder, Cat# 6222, Price: 299

GC Columns

GC Column Selection	64
Structures, Properties, Polarities and Uses for DM Columns	64
Column Phase Cross Reference	65
GC Guard Columns	66
Guard Columns / Transfer Lines	66
Ordering Information	66
DikmaCap™ (DM) Capillary Columns	67
DM-1 / DM-1MS.....	67
DM-5 / DM-5MS.....	68
DM-5MS / LB	69
DM-1HT / DM-5HT	70
DM-35 / DM-35MS.....	71
DM-1701	72
DM-17 / DM-17MS.....	73
DM-200 / DM-200MS.....	74
DM-225	75
DM-Wax	76
DM-InertWax	77
DM-FFAP	78
DM-2330	79
DM-2560	80
DM-PLOT	81
DM-PONA.....	87
DM-TCEP	88
DM Series SimDist Metal	89
DM-2887 / DM-2887 Metal	90
DM-BDTG Metal	91
DM-Volatile Amine.....	92
DM-5 Amine.....	93
DM-35 Amine.....	94
DM-Wax Amine	95
DM-624 / DM-624MS.....	96
DM-AQUA.....	97
DM-TVOC.....	98
DM-PAH	99
DM-FAMEWAX.....	100




DikmaCap™ (DM)

Structures, Properties, Polarities and Uses for DM Columns

DM-1 / DM-1MS / DM-1HT

100% Dimethyl polysiloxane




Polarity: Non-polar

Application: Solvents, natural gases, petroleum products, etc.

DM-5 / DM-5MS / DM-5HT

5% Diphenyl
95% Dimethyl polysiloxane




Polarity: Slightly polar

Application: Flavors, aromatic hydrocarbons, environmental compounds, etc.

DM-5MS / LB

5% Diphenyl
95% Phenyl arylene dimethyl polysiloxane




Polarity: Slightly polar

Application: Semi-volatile / volatile compounds, phenols, aromatic hydrocarbons, PCBs

DM-624 / DM-624MS

6% Cyanopropylphenyl
94% Dimethyl polysiloxane




Polarity: Slightly polar

Application: Insecticides, alcohols, volatile organic compounds

DM-35 / DM-35MS

35% Diphenyl
65% Dimethyl polysiloxane




Polarity: Intermediately polar

Application: Pesticides, PCBs, herbicides

DM-1701

14% Cyanopropylphenyl
86% Dimethyl polysiloxane




Polarity: Intermediately polar

Application: Alcohols, oxygenates, PCBs

DM-17 / DM-17MS

50% Diphenyl
50% Dimethyl polysiloxane




Polarity: Intermediately polar

Application: Triglycerides, steroids, PAEs

DM-200

100% Trifluoropropylmethyl polysiloxane




Polarity: Intermediately polar, special selectivity for compounds containing lone pair electron groups

Application: Solvents, alcohols, etc.

DM-225

50% Cyanopropylmethyl
50% Phenylmethyl polysiloxane




Polarity: Polar

Application: Adipic acid monomethyl ester, sugars, FAMES

DM-2330

90% Biscyanopropyl
10% Cyanopropylphenyl polysiloxane




Polarity: Polar

Application: *cis* / *trans* FAMES, dioxins, rosin acids

DM-Wax / DM-InertWax

Polyethylene glycol



Polarity: Polar

Application: FAMES, flavors, solvents, aromatic hydrocarbons

Column Phase Cross Reference

DikmaCap™	Phase	Agilent	SGE	Restek	Supelco
DM-1	100% Dimethyl polysiloxane	HP-1, DB-1, CP-Sil 5 CB	BP-1	Rtx-1, MXT-1	SPB-1
DM-1HT	100% Dimethyl polysiloxane	DB-1ht, VF-1ht	-	Rxi-1HT	-
DM-1MS	100% Dimethyl polysiloxane (low bleed)	HP-1, HP-1ms, DB-1, DB-1ms, Ultra 1, VF-1ms, CP-Sil 5 CB Low Bleed / MS	BP-1	Rxi-1MS	SPB-1, Equity-1
DM-5	5% Diphenyl 95% Dimethyl polysiloxane	HP-5, DB-5, CP-Sil 8 CB	BP-5	Rtx-5, MXT-5	SPB-5
DM-5HT	5% Diphenyl 95% Dimethyl polysiloxane	DB-5ht, VF-5ht	-	Rxi-5HT	-
DM-5MS	5% Diphenyl 95% Dimethyl polysiloxane (low bleed)	HP-5, HP-5ms, DB-5, Ultra 2, CP-Sil 8 CB	BP-5	Rxi-5MS	SPB-5, Equity-5
DM-5MS / LB	5% Diphenyl 95% Phenyl arylene dimethyl polysiloxane (low bleed)	DB-5ms, DB-5ms UI, VF-5ms, CP-Sil 8 CB Low Bleed / MS	BPX-5	Rxi-5Sil MS	SLB-5MS
DM-35	35% Diphenyl 65% Dimethyl polysiloxane	HP-35, DB-35	BPX-35, BPX-608	Rtx-35	SPB-35, SPB-608
DM-35MS	35% Diphenyl 65% Dimethyl arylene polysiloxane	DB-35ms, VF-35ms	BP-35	Rxi-35Sil MS	-
DM-1701	14% Cyanopropylphenyl 86% Dimethyl polysiloxane	HP-1701, PAS-1701, DB-1701, CP-Sil 19 CB, VF-1701ms	BP-10	Rtx-1701	SPB-1701
DM-17	50% Diphenyl 50% Dimethyl polysiloxane	HP-50+, HP-17, DB-17, DB-608, CP-Sil 24 CB	-	Rxi-17	SPB-50
DM-17MS	50% Diphenyl 50% Dimethyl arylene polysiloxane	HP-17, DB-17, DB-17ms, CP-Sil 24 CB, VF-17ms	BPX-50	Rxi-17Sil MS	-
DM-200	100% Trifluoropropylmethyl polysiloxane	DB-210, DB-200, VF-200ms	-	Rtx-200	-
DM-200MS	100% Trifluoropropylmethyl polysiloxane (low bleed)	VF-200ms	-	Rtx-200MS	-
DM-225	50% Cyanopropylmethyl 50% Phenylmethyl polysiloxane	HP-225, DB-225, CP-Sil 43 CB	BP-225	Rtx-225	SPB-225
DM-Wax	Polyethylene glycol	HP-INNOWax, CP-Wax 52 CB, VF-WAXms	-	Stabilwax	Supelcowax 10
DM-InertWax	Polyethylene glycol	HP-Wax, DB-Wax, CP-Wax 52 CB	BP-20	Rtx-Wax	-
DM-FFAP	Polyethylene glycol	HP-FFAP, DB-FFAP, CP-Wax 58 CB	BP-21	Stabilwax-DA	Nukol
DM-2330	90% Biscyanopropyl 10% Cyanopropylphenyl polysiloxane	-	BPX-70	Rt-2330	SP-2330, SP-2331, SP-2380
DM-2560	Biscyanopropyl polysiloxane	HP-88, CP-Sil 88	-	Rt-2560	SP-2560
DM-PLOT Alumina	Aluminum oxide	GS-Alumina, HP-PLOT S, CP-Al ₂ O ₃ PLOT	-	-	-
DM-PLOT Alumina / Na ₂ SO ₄	Aluminum oxide Na ₂ SO ₄ deactivation	GS-Alumina, HP-PLOT S, CP-Al ₂ O ₃ / Na ₂ SO ₄ PLOT	-	Rt-Alumina BOND / Na ₂ SO ₄	Alumina Sulfate PLOT
DM-PLOT Alumina / KCl	Aluminum oxide KCl deactivation	GS-Alumina / KCl, HP-PLOT Al ₂ O ₃ / KCl, CP-Al ₂ O ₃ / KCl PLOT	-	Rt-Alumina BOND / KCl	Alumina Chloride PLOT
DM-PLOT CFC	-	-	-	Rt-Alumina BOND / CFC	-
DM-PLOT MS 5A	Molecular sieve 5A	GS-Molsieve, HP-PLOT Molesieve, CP-PoraSieve 5A	-	Rt-Msieve 5A	Molsieve 5A
DM-PLOT Q	100% Divinylbenzene	CP-PoraPLOT Q, CP-PoraBond Q	-	Rt-Q-BOND	Supel-Q PLOT
DM-PLOT QS	Porous divinyl benzene homopolymer	GS-Q	-	Rt-QS-BOND	-
DM-PLOT S	Divinylbenzene 4-vinylpyridine	CP-PoraPLOT S	-	Rt-S-BOND	-
DM-PLOT U	Divinylbenzene ethylene glycol / dimethylacrylate	HP-PLOT U, CP-PoraPLOT U, CP-PoraBond U	-	Rt-U-BOND	-
DM-624	6% Cyanopropylphenyl 94% Dimethyl polysiloxane	HP-1301, HP-624, DB-1301, DB-624, CP-1301, VF-624ms, VF-1301ms	BP-624	Rtx-1301, Rtx-624	SPB-1301
DM-624MS	6% Cyanopropylphenyl 94% Dimethyl arylene polysiloxane	HP-624, DB-624, VF-624ms	BP-624	Rxi-624Sil MS	-
DM-FAMEWAX	Polyethylene glycol	-	-	FAMEWAX	Omegawax
DM-5 Amine	5% Diphenyl 95% Dimethyl polysiloxane	CP-Sil 8 CB	-	Rtx-5 Amine	-
DM-35 Amine	35% Diphenyl 65% Dimethyl polysiloxane	-	-	Rtx-35 Amine	-
DM-Wax Amine	Polyethylene glycol	CAM, CP-Wax 51	-	Stabilwax-DB	Carbowax Amine
DM-TVOC	100% Dimethyl polysiloxane	-	-	-	-
DM-PONA	100% Dimethyl polysiloxane	HP-PONA, DB-Petro, CP-Sil PONA CB	BP1-PONA	Rtx-DHA	Petrocol DH
DM-TCEP	1,2,3-tris[2-cyanoethoxy]propane	CP-TCEP	-	Rt-TCEP	TCEP
DM-2887 DM-2887 Metal	100% Dimethyl polysiloxane	DB-2887	-	Rtx-2887	Petrocol 2887, Petrocol EX2887
DM-AQUA	25% Phenyl 75% Methyl polysiloxane	-	-	-	-
DM-1HT SimDist Metal	100% Dimethyl polysiloxane	DB-HT Sim Dis, CP-SimDist	-	MXT-1HT SimDist	-
DM-1 SimDist Metal	-	CP-SimDist	-	MXT-1HT SimDist	-
DM-500 SimDist Metal	Carborane siloxane polymer	-	-	MXT-500 SimDist	-
DM-BDTG Metal	-	-	-	MXT-Biodiesel TG	-
DM-Volatile Amine	-	CP-VolAmine	-	Rtx-Volatile Amine	-
DM-PAH	50% Methyl 50% Phenyl polysiloxane	-	-	-	-

GC Guard Columns

Guard Columns / Transfer Lines (Intermediate Polarity Deactivated)

- Use in a wide variety of applications
- Allow most common solvents

Ordering Information

ID (mm)	OD (mm)	MAOT (°C)	5 m		5 m (6/pk)		10 m		30 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.05	0.363 ± 0.012	325	7001	\$115						
0.10	0.363 ± 0.012	325	7002	130						
0.15	0.363 ± 0.012	325	7003	130						
0.18	0.37 ± 0.04	325	7004	87						
0.25	0.37 ± 0.04	325	7005	64	7061	\$345	7015	\$115	7064	\$336
0.28	0.37 ± 0.04	325	7006	64						
0.32	0.45 ± 0.04	325	7007	73	7062	390	7017	130	7065	385
0.45	0.69 ± 0.04	325	7008	94						
0.53	0.69 ± 0.05	325	7009	94	7063	503	7019	175	7066	511

Guard Columns / Transfer Lines (Polar Deactivated)

- Provide optimum wettability for polar compounds
- Minimize peak splitting and peak tailing when using polar solvents such as water or methanol
- Polyethylene glycol deactivation used for DM-Wax, DM-225 and DM-2330

Ordering Information

ID (mm)	OD (mm)	MAOT (°C)	5 m		10 m		30 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.37 ± 0.04	280	7011	\$64	7014	\$115	7010	\$336
0.32	0.45 ± 0.04	280	7012	73	7016	130	7020	385
0.53	0.69 ± 0.05	280	7013	94	7018	175	7030	511

Guard Columns / Transfer Lines (Water Resistant Deactivated)

- High-density surface deactivation and excellent water resistance
- Use for purge / trap system, headspace injection, gas concentration analysis and hydrated sample test
- Inertness and water resistance tube connection

Ordering Information

ID (mm)	OD (mm)	MAOT (°C)	5 m		5 m (6/pk)		10 m		30 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.05	0.363 ± 0.012	325	7021	\$115						
0.10	0.363 ± 0.012	325	7022	130						
0.15	0.363 ± 0.012	325	7023	130						
0.18	0.37 ± 0.04	325	7024	87						
0.25	0.37 ± 0.04	325	7025	64	7031	\$345	7034	\$130	7037	\$385
0.32	0.45 ± 0.04	325	7027	73	7032	390	7035	147	7038	427
0.53	0.69 ± 0.05	325	7029	94	7033	503	7036	196	7039	560

Guard Columns / Transfer Lines (Base Deactivated)

- Excellent inertness for basic compounds
- Use for DM-5 Amine, DM-35 Amine, DM-Wax Amine, DM-Volatile Amine
- Batch test with basic compounds

Ordering Information

ID (mm)	OD (mm)	MAOT (°C)	5 m		5 m (6/pk)	
			Cat. No.	Price	Cat. No.	Price
0.25	0.37 ± 0.04	315	7041	\$73	7044	\$390
0.32	0.45 ± 0.04	315	7042	80	7045	428
0.53	0.69 ± 0.05	315	7043	101	7046	540

DM-1 / DM-1MS

- 100% Dimethyl polysiloxane
- General purpose column of non-polar phase
- Long lifetime
- Temperature range: -60 °C to 350 °C
- Bonded and cross-linked phase, solvent rinsable
- DM-1MS is a low bleed column, use for MSDs
- Similar to DB-1, SPB-1, HP-1, etc.
- Equivalent to USP G1, G2, G38 phases

DM-1MS column exhibits ultra-low bleed that has excellent inertness for active compounds and improves detection performance for MSDs, ECDs and NPDs.

Application Chromatogram

Sample / Compound	Page
Air Sample TO-14	154
Citronella Java Oils	205
Fatty Acids (Free)	200
Flavor Volatiles	203
Fragrance	206
Gasoline Aromatics	180
Hydrocarbons, C7-C42	179
Oxygenates MTBE	175
Petroleum Oxygenates	175
Sulfide	176
Sulfur in Gasoline	176
Solvents	193, 195, 197
Sulfur in Naphtha	176
USP Solvents	192

DM-1 Ordering Information

ID (mm)	df (µm)	MAOT (°C)	15 m		30 m		50 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.10	-60 to 330 / 350			7119	\$450				
	0.25	-60 to 330 / 350			7121	435	7172	\$785	7122	\$775
	0.50	-60 to 330 / 350			7123	435	7174	785	7124	775
	1.00	-60 to 330 / 340			7125	435	7176	785	7126	775
0.32	0.25	-60 to 330 / 350			7131	470	7182	850	7132	840
	0.50	-60 to 330 / 350			7133	470	7184	850	7134	840
	1.00	-60 to 320 / 340			7135	470	7186	850	7136	840
	1.50	-60 to 310 / 330			7137	470			7138	840
	3.00	-60 to 280 / 300			7141	470			7142	840
	4.00	-60 to 280 / 300			7143	495				
0.53	0.50	-60 to 310 / 330			7147	530			7148	870
	1.00	-60 to 310 / 330	7109	\$295	7149	530			7150	885
	1.50	-60 to 310 / 330	7110	295	7151	530			7152	885
	3.00	-60 to 270 / 290	7112	295	7155	530			7156	885
	5.00	-60 to 270 / 290	7113	310	7157	530			7158	870
	7.00	-60 to 270 / 290			7159	530			7160	870

DM-1MS Ordering Information

ID (mm)	df (µm)	MAOT (°C)	30 m	
			Cat. No.	Price
0.25	0.25	-60 to 330 / 350	8121	\$490
0.32	0.25	-60 to 330 / 350	8131	515

DM-5 / DM-5MS

DM-5 / DM-5MS

- Bonded and cross-linked 5% diphenyl / 95% dimethyl polysiloxane
- General purpose column with low polarity phase
- Temperature range: -60 °C to 350 °C
- Solvent rinsable
- DM-5MS is a low bleed column, use for MSDs
- Similar to DB-5, SPB-5, HP-5, etc.
- Equivalent to USP G27, G36 phases

DM-5 column has a slightly higher polarity compared to DM-1, resulting in a better selectivity for aromatic compounds. DM-5 column exhibits excellent reproducibility, high column efficiency, and low bleed.

DM-5MS column exhibits ultra-low bleed with excellent inertness for active compounds and improves detection performance for MSDs, ECDs and NPDs.

Application Chromatogram

Sample / Compound	Page
Alcohols	187
Basic Drugs (Underivatized)	208
Benzidine / Phenol (EPA 604 / 605)	161
Butyl Tins	165
Chlorinated Hydrocarbons (EPA 612)	160
Food Packaging Volatiles	206
Glycols / Alcohols	187
Nitrogen-Containing Herbicides	163
Organochlorine Pesticides	162, 164
PAEs	167
PAHs (EPA 610)	157
Solvents	199
Steroids, Anabolic	210

DM-5 Ordering Information

ID (mm)	df (µm)	MAOT (°C)*	15 m		30 m		50 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.10	-60 to 330 / 350			7219	\$450				
	0.25	-60 to 330 / 350			7221	435	7272	\$785	7222	\$775
	0.50	-60 to 330 / 350			7223	435	7274	785	7224	775
	1.00	-60 to 320 / 340			7225	435	7276	785	7226	775
0.32	0.25	-60 to 330 / 350			7231	470	7282	850	7232	840
	0.50	-60 to 330 / 350			7233	470	7284	850	7234	840
	1.00	-60 to 330 / 350			7235	470	7286	850	7236	840
	1.50	-60 to 310 / 330			7237	470			7238	840
	3.00	-60 to 280 / 300			7241	470			7242	840
0.53	0.50	-60 to 310 / 330			7247	530			7248	870
	1.00	-60 to 310 / 330	7209	\$295	7249	530				
	1.50	-60 to 310 / 330	7210	295	7251	530				
	3.00	-60 to 270 / 290	7212	295	7255	530				
	5.00	-60 to 270 / 290	7213	310	7257	530	7298	885	7258	885

DM-5MS Ordering Information

ID (mm)	df (µm)	MAOT (°C)*	30 m		50 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.10	-60 to 330 / 350	8219	\$490			8220	\$780
	0.25	-60 to 330 / 350	8221	490	8272	\$790	8222	780
	0.50	-60 to 330 / 350	8223	490				
0.32	0.10	-60 to 330 / 350	8229	520			8230	845
	0.25	-60 to 330 / 350	8231	515	8282	855	8232	845
	0.50	-60 to 330 / 350	8233	260				

*The listed temperature limits are for 15 m and 30 m columns. Longer columns may have lower temperature limits.

DM-5MS / LB


- Cross-linked 5% diphenyl / 95% phenyl arylene dimethyl polysiloxane
- Very low bleed
- Improves the resolution between Benzo[b]fluoranthene and Benzo[k]fluoranthene
- Similar to DB-5MS

DM-5MS / LB (low bleed) column is coated with a 5% diphenyl / 95% phenyl arylene dimethyl polysiloxane phase, which can inhibit the formation of ring-shaped fragments of siloxane skeleton, thereby reducing column bleed and increasing the thermal stability. The stationary phase has better stability; and will not exhibit oxidative degradation when there is trace oxygen in the carrier gas.

DM-5MS / LB column is similar to DM-5MS. The DM-5MS / LB has good sensitivity and peak symmetry for strong polar and basic compounds. We recommend DM-5MS / LB column for analysis of semi-volatile compounds such as PAHs and PCBs.

Application Chromatogram

Sample / Compound	Page
Phenols	158
PAHs (EPA 610)	156
Semi-volatile Organic Compounds (EPA 8270)	159
Volatile Organic Compounds	158

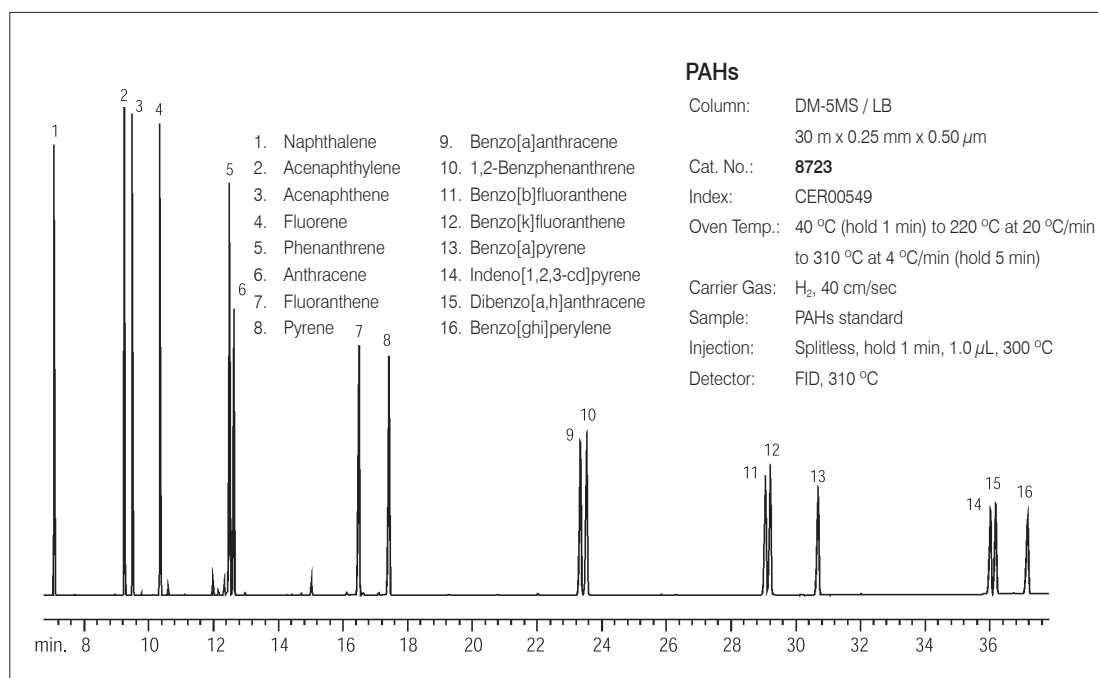

DM-5MS / LB Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m Cat. No.	Price
0.25	0.10	-60 to 330 / 350	8719	\$500
	0.25	-60 to 330 / 350	8721	490
	0.50	-60 to 330 / 350	8723	490
0.32	0.10	-60 to 330 / 350	8729	520
	0.25	-60 to 330 / 350	8731	515
	0.50	-60 to 330 / 350	8733	515

DM-1HT / DM-5HT

DM-1HT

- 100% Dimethyl polysiloxane
- High temperature resistant application
- Temperature range: -60 °C to 400 °C

DM-1HT Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	15 m		30 m	
			Cat. No.	Price	Cat. No.	Price
0.25	0.10	-60 to 400	8841	\$335	8842	\$545
	0.25	-60 to 400			8843	545
0.32	0.10	-60 to 400	8844	365	8845	585
	0.25	-60 to 400			8846	585
0.53	0.15	-60 to 400			8847	640

*Column is capable of going up to 430 °C, but it will reduce column lifetime.

DM-5HT

- Low polarity phase, bonded and cross-linked 5% diphenyl / 95% dimethyl polysiloxane
- 40% longer lifetime from designed fused silica tubing
- High temperature resistant application
- Temperature range: -60 °C to 400 °C
- Similar to DB-5ht, VF-5ht


DM-5HT Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	15 m		30 m	
			Cat. No.	Price	Cat. No.	Price
0.25	0.10	-60 to 400	8848	\$335	8849	\$545
	0.25	-60 to 400			8850	545
0.32	0.10	-60 to 400	8851	365	8852	585
	0.25	-60 to 400			8853	585
0.53	0.15	-60 to 400			8854	640

*Column is capable of going up to 430 °C, but it will reduce column lifetime.

Bleed Profiles of DM-5HT

Column: DM-5HT
30 m x 0.25 mm x 0.10 μm
Cat. No.: **8849**
Index: CGN1144
Carrier Gas: He, 38 cm/sec
Oven Temp.: 110 °C (hold 8 min) to 380 °C (hold 10 min)
at 30 °C/min to 400 °C (hold 10 min) at 30 °C/min
Detector: FID, 400 °C
Injection: Split, 250 °C, 1.0 μL
Instrument: HP5890 GC

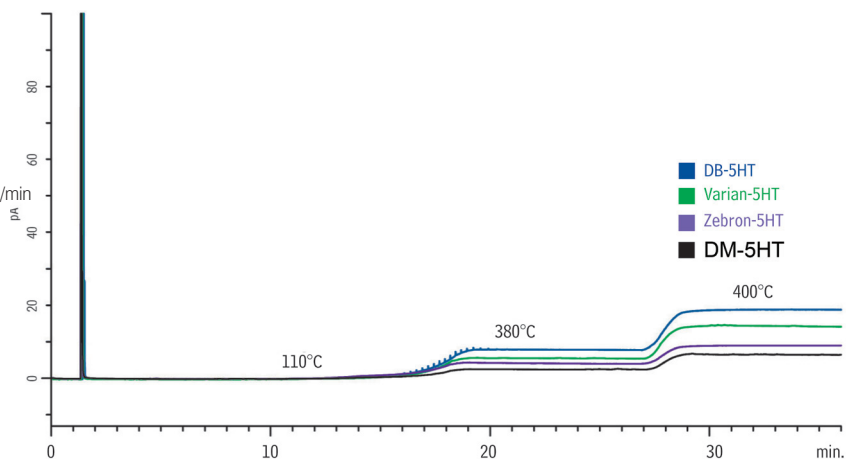


DM-35

- Bonded and cross-linked 35% diphenyl / 65% dimethyl polysiloxane
- General purpose column of mid-polarity phase for pesticides, herbicides, pharmaceuticals, sterols, etc.
- Temperature range: 40 °C to 320 °C
- Solvent rinsable
- Similar to DB-35, SPB-35, HP-35, SPB-608, etc.
- Equivalent to USP G42 phase

DM-35MS

- Bonded and cross-linked 35% diphenyl / 65% dimethyl arylene polysiloxane
- Special selectivity and excellent inertness for substituted polar compounds
- Temperature range: 50 °C to 360 °C
- Ultra-low bleed for MSDs and ECDs analysis
- Similar to DB-35ms, VF-35ms, BP-35

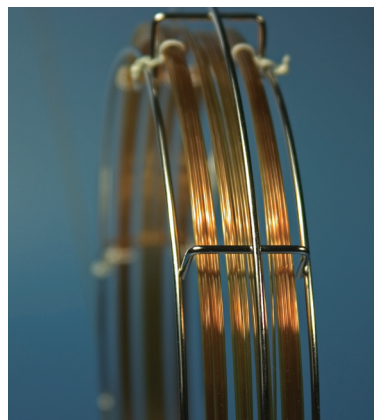**Application Chromatogram**

Sample / Compound	Page
Acidic / Neutral Drugs (Underivatized)	209
Basic Drugs (Underivatized)	208
Chlorinated Hydrocarbons (EPA 612)	160
Chlorophenoxyacid Herbicides (EPA 615)	165
Endocrine Disruptors Butyl Tins (Hexyl Derivatives)	167
Nitrogen-Containing Herbicides	163
Organochlorine Pesticides (EPA 8081)	164
Organophosphorus Pesticides	162

DM-35 Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	15 m		30 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 320			7921	\$435	7922	\$775
	0.50	40 to 310			7923	435	7924	775
0.32	0.25	40 to 320			7931	470	7932	840
	0.50	40 to 310			7933	470	7934	840
0.53	1.00	40 to 290	7910	\$295	7951	530		

DM-35MS Ordering Information

ID (mm)	df (μm)	MAOT (°C)	30 m	
			Cat. No.	Price
0.25	0.25	50 to 340 / 360	8101	\$490
0.32	0.25	50 to 340 / 360	8102	515

*The listed temperature limits are for 15 m and 30 m columns. Longer columns may have lower temperature limits.

DM-1701

DM-1701

- Cross-linked 14% cyanopropylphenyl / 86% dimethyl polysiloxane
- General purpose column of mid-polarity phase
- Temperature range: -20 °C to 280 °C
- Bonded and cross-linked phase, solvent rinsable
- Similar to DB-1701, HP-1701, SPB-1701
- Equivalent to USP G46 phase

DM-1701 is one of the most popular stationary phases. The mix of cyano and phenyl functional groups increases polarity and offers a different elution order compared to DM-1 or DM-5 column. DM-1701 column exhibits low bleed, high inertness and thermal stability because the polymer is characterized, and can be used for ECDs, NPDs and MSDs.

Application Chromatogram

Sample / Compound	Page
Acrylic Esters	191
Formaldehyde	189
Fragrance	206
Organochlorine Pesticides (EPA 8081)	164
Styrene Impurities	191

DM-1701 Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	15 m		30 m		50 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	-20 to 280			7321	\$435			7322	\$775
	0.50	-20 to 270 / 280			7325	435			7326	775
	1.00	-20 to 260 / 280			7323	435			7324	775
0.32	0.25	-20 to 280			7331	470	7382	\$850	7332	840
	0.50	-20 to 270 / 280			7335	480			7336	840
	1.00	-20 to 260 / 280			7333	470	7384	850	7334	840
0.53	0.50	-20 to 260 / 270			7347	530			7348	870
	1.00	-20 to 250 / 270	7310	\$295	7351	530			7352	885
	1.50	-20 to 240 / 260			7353	530			7354	870
	3.00	-20 to 230 / 250			7355	530			7356	870

*The listed temperature limits are for 15 m and 30 m columns. Longer columns may have lower temperature limits.

DM-17

- Bonded and cross-linked 50% diphenyl / 50% dimethyl polysiloxane
- General purpose column of mid-polarity phase for pesticides, herbicides, sterols, etc.
- Temperature range: 40 °C to 320 °C
- Solvent rinsable
- Similar to DB-17, HP-17, HP-50+, etc

DM-17MS

- Bonded and cross-linked 50% diphenyl / 50% dimethyl arylene polysiloxane
- Excellent inertness and selectivity for active environmental compounds
- Temperature range: 40 °C to 360 °C
- Ultra-low bleed
- Similar to DB-17ms, VF-17ms, BPX-50
- Equivalent to USP G3 phase

Application Chromatogram

Sample / Compound	Page
BHA / BHT	206
Chlorophenoxyacid Herbicides (EPA 515.1)	165
Organochlorine Pesticides (EPA 8081)	164
PAEs (EPA 8060)	160
Phenols (EPA 604)	161
Triazine Herbicides (EPA 619)	165

DM-17 Ordering Information

ID (mm)	df (µm)	MAOT (°C)*	15 m		30 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 280 / 320			7421	\$435	7422	\$775
	0.50	40 to 280 / 320			7423	435	7424	775
0.32	0.25	40 to 280 / 320			7431	470	7432	840
	0.50	40 to 280 / 320			7433	470	7434	840
0.53	1.00	40 to 280 / 320	7410	\$295	7451	530		

DM-17MS Ordering Information

ID (mm)	df (µm)	MAOT (°C)*	15 m		30 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 340 / 360	8831	\$330	8832	\$530	8833	\$905
0.32	0.25	40 to 340 / 360	8834	350	8835	570		

*The listed temperature limits are for 15 m and 30 m columns. Longer columns may have lower temperature limits.

DM-200 / DM-200MS

DM-200 / DM-200MS

- 100% Trifluoropropylmethyl polysiloxane
- General purpose column of mid-polarity phase
- Temperature range: -20 °C to 340 °C
- Bonded and cross-linked phase, solvent rinsable
- Similar to DB-200, DB-210, etc.
- Equivalent to USP G6 phase

Interaction between trifluoropropylmethyl phase and molecules with lone pair electrons or electron-rich molecules is easier, due to electrophilicity of the fluorine. DM-200 column has accomplished many difficult separations that are not possible on other bonded stationary phases, such as PH, CN and WAX phase. The trifluoropropyl stationary phase can change elution orders of compounds. The DM-200 column can make a qualitative analysis of phenols, nitrosamines, organochlorine pesticides, and chlorhydrocarbons and chlorophenoxy herbicides in coordination with the DM-5 column.

DM-200 column offers low bleed, superb inertness, and excellent thermal stability, even with sensitive detectors, such as ECDs, NPDs and MSDs.

Application Chromatogram

Sample / Compound	Page
Aromatics (Benzene / Toluene / Xylene)	181
Basic Drugs	208
Chlorinated Hydrocarbons (EPA 612)	160
Explosives	167
Glycols	187
Nitrosamines	161
PAHs (EPA 610)	157
Silanes	191
Solvents	194, 196, 198
USP Solvents	192
VOCs in Water (EPA 551.1)	166

DM-200 Ordering Information

ID (mm)	df (µm)	MAOT (°C)*	15 m		30 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	-20 to 320 / 340			8321	\$470	8322	\$775
	0.50	-20 to 310 / 330			8323	470	8324	775
	1.00	-20 to 290 / 310			8325	470	8326	775
0.32	0.25	-20 to 320 / 340			8331	495	8332	840
	0.50	-20 to 310 / 330			8333	495	8334	840
	1.00	-20 to 290 / 310			8335	495	8336	840
	1.50	-20 to 280 / 300			8337	495	8338	840
0.53	0.50	-20 to 300 / 320			8347	555	8348	905
	1.00	-20 to 290 / 310	8310	\$345	8351	555	8352	965
	1.50	-20 to 280 / 300			8353	555	8354	905
	3.00	-20 to 260 / 280			8355	555	8356	905

DM-200 MS Ordering Information

ID (mm)	df (µm)	MAOT (°C)	30 m	
			Cat. No.	Price
0.25	0.25	-20 to 320 / 340	8103	\$490
0.32	0.25	-20 to 320 / 340	8104	515

*The listed temperature limits are for 15 m and 30 m columns. Longer columns may have lower temperature limits.

DM-225

- Cross-linked 50% cyanopropylmethyl / 50% phenylmethyl polysiloxane
- General purpose column of polar phase, for FAMES, carbohydrates, sterols and flavor compounds
- Temperature range: 40 °C to 240 °C
- Similar to DB-225, HP-225
- Equivalent to USP G7, G19 phases

The stationary phase of DM-225 is less polar than that of WAX column containing polyethylene glycol, but can be used for many of the same applications.

In most cases, the cyanopropyl siloxane polymer is not fully compatible with a Carbowax deactivation layer. DM-225 polymer has solved this problem because of the unique polymer synthesis technology and proprietary siloxane deactivation technology, and provides a 20 °C thermal stability advantage over other "225" columns.

Application Chromatogram

Sample / Compound	Page
Neutral Sterols	207
Sugars (Alditol Acetates)	207

DM-225 Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	15 m		30 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 220 / 240			8421	\$435	8422	\$775
	0.50	40 to 220 / 240			8423	435	8424	775
0.32	0.25	40 to 220 / 240			8431	470	8432	840
	0.50	40 to 220 / 240			8433	470	8434	840
0.53	1.00	40 to 200 / 220	8410	\$305	8451	530		

*The listed temperature limits are for 15 m and 30 m columns. Longer columns may have lower temperature limits.

DM-Wax

DM-Wax

- Bonded and cross-linked polyethylene glycol
- General purpose column of polar phase
- Resistant to oxidation
- Temperature range: 40 °C to 260 °C
- Solvent rinsable
- Similar to HP-INNOWax, CP-WAX 52 CB, etc.
- Equivalent to USP G14, G15, G16, G20 and G39 phases

DM-Wax vs. DM-InertWax

Column	Features	Benefits
DM-Wax	<ul style="list-style-type: none"> • Wide chemical compatibility (acidic, basic and neutral samples) • Low bleed at elevated temperatures • High inertness • High stability and ruggedness 	<ul style="list-style-type: none"> • General purpose column • Best choice for MS use
DM-InertWax	<ul style="list-style-type: none"> • Wide operating temperature range • Lowest operating temperature limit • Best inertness 	<ul style="list-style-type: none"> • Analyze low boiling point analytes

Application Chromatogram

Sample / Compound	Page
Aldehydes	189
Alcohols	186
Alcohols / Aldehydes	188
Amines / Alcohols / Chlorides	185
Aromatics	181, 182
Concentrated Liquors	204
Esters	190
Flavor Volatiles	203
Glycols	187
Ketones	189
Solvents	194, 196, 198
Styrene Impurities	191
Peppermint Oil	205
Petroleum Oxygenates	174
PUFA (Animal Source)	201

DM-Wax Ordering Information


ID (mm)	df (µm)	MAOT (°C)	15 m		30 m		50 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 250 / 260			7521	\$450	7572	\$810	7522	\$790
	0.50	40 to 250 / 260			7523	450	7574	810	7524	790
0.32	0.25	40 to 250 / 260			7531	480	7582	880	7532	870
	0.50	40 to 250 / 260			7533	480	7584	435	7534	860
	1.00	40 to 250 / 260			7535	480			7536	860
0.53	0.50	40 to 250 / 260			7547	545			7548	885
	1.00	40 to 250 / 260	7510	\$310	7551	545	7592	900	7552	885
	2.00	40 to 220 / 230	7511	315	7553	545				

DM-InertWax

- Bonded and cross-linked polyethylene glycol
- General purpose column of polar phase for analysis of solvents, such as FAMES, BTEX, and flavor volatiles
- Temperature range: 20 °C to 250 °C
- Similar to DB-Wax, HP-Wax, etc.
- Equivalent to USP G14, G15, G16, G20 and G39 phases

Application Chromatogram

Sample / Compound	Page
Aldehydes	188
FAMES	201

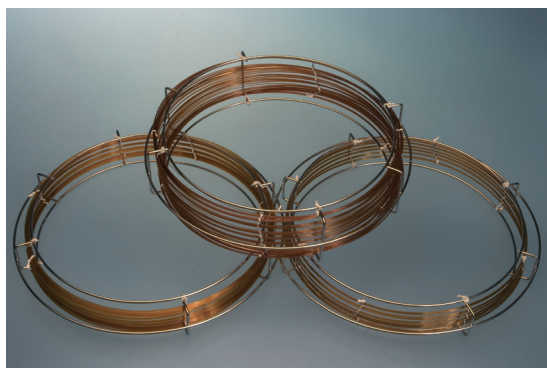

DM-InertWax Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	30 m		60 m	
			Cat. No.	Price	Cat. No.	Price
0.25	0.25	20 to 250	8521	\$450	8522	\$790
	0.50	20 to 250	8523	450	8524	790
0.32	0.25	20 to 250	8531	480	8532	860
	0.50	20 to 250	8533	480	8534	860
0.53	1.00	20 to 240 / 250	8551	545	8552	885

*The listed temperature limits are for 30 m columns. Longer columns may have lower temperature limits.

DM-FFAP


DM-FFAP

- Nitroterephthalic acid modified polyethylene glycol
- Designed for analysis of underivatized free acids
- Resistant to oxidation
- Temperature range: 40 °C to 250 °C
- Similar to DB-FFAP, HP-FFAP, Nukol, etc.
- Equivalent to USP G25, G35 phases

DM-FFAP column is used to analyze acidic compounds including phenol, derivatized or underivatized free acids, organic acids, flavor compounds and solvents.

Application Chromatogram

Sample / Compound	Page
Alcoholic Standard: Acids and Esters	204
Fatty Acids (Free)	200

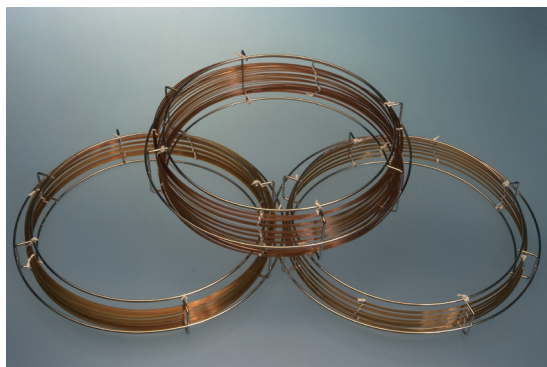

DM-FFAP Ordering Information

ID (mm)	df (µm)	MAOT (°C)	15 m		30 m		50 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 250			7621	\$440	7672	\$785	7622	\$775
	0.50	40 to 250			7623	440	7673	785	7624	775
0.32	0.25	40 to 250			7631	480	7682	850	7632	840
	0.50	40 to 250			7633	480	7684	850	7634	840
	1.00	40 to 250			7635	480			7636	840
0.53	0.50	40 to 240 / 250			7647	540			7648	920
	1.00	40 to 240 / 250	7610	\$315	7651	540	7692	1,010	7652	960
	1.50	40 to 220 / 230	7611	325	7653	540				

DM-2330

- 90% Biscyanopropyl / 10% phenylcyanopropyl polysiloxane
- General purpose highly polar phase for *cis* / *trans* FAMES and dioxin isomers
- Temperature range: 0 °C to 275 °C
- Similar to SP-2330, SP-2331, SP-2380, etc.
- Equivalent to USP G8 and G48 phases

DM-2330 is one of the most polar capillary column stationary phases. This column offers high selectivity for *cis* / *trans* isomers with conjugated double bonds due to cyano groups on both sides of the polymer backbone.

In order to overcome the poor column efficiencies, high bleed and short column lifetime of highly polar columns, we have developed an advanced surface treatment technology that is compatible with the DM-2330 phase. Our improved polymer exhibits better column efficiency and lower bleed.

Since the stationary phase of DM-2330 is not bonded, it should not be solvent rinsed.

Application Chromatogram

Sample / Compound	Page
Dioxins	155
PUFA (Animal Source)	201
Sugers (Alditol Acetate)	207

DM-2330 Ordering Information

ID (mm)	df (μm)	MAOT (°C)*	30 m		60 m	
			Cat. No.	Price	Cat. No.	Price
0.25	0.10	0 to 260 / 275	8621	\$450	8622	\$810
	0.20	0 to 260 / 275	8623	450	8624	810
0.32	0.10	0 to 260 / 275	8631	490	8632	855
	0.20	0 to 260 / 275	8633	490	8634	855

*The listed temperature limits are for 30 m columns. Longer columns may have lower temperature limits.


DM-2560

DM-2560

- Biscyanopropyl polysiloxane
- Specially designed for *cis* / *trans* FAMES
- Temperature range: 20 °C to 250 °C
- Similar to SP-2560, HP-88, Silar 10C, CP-Sil 88 FAME, and CP-Sil 88
- Since the stationary phase of DM-2560 is not bonded, it should not be solvent rinsed

Application Chromatogram

Sample / Compound	Page
FAMES (<i>cis</i> / <i>trans</i> Isomers)	200

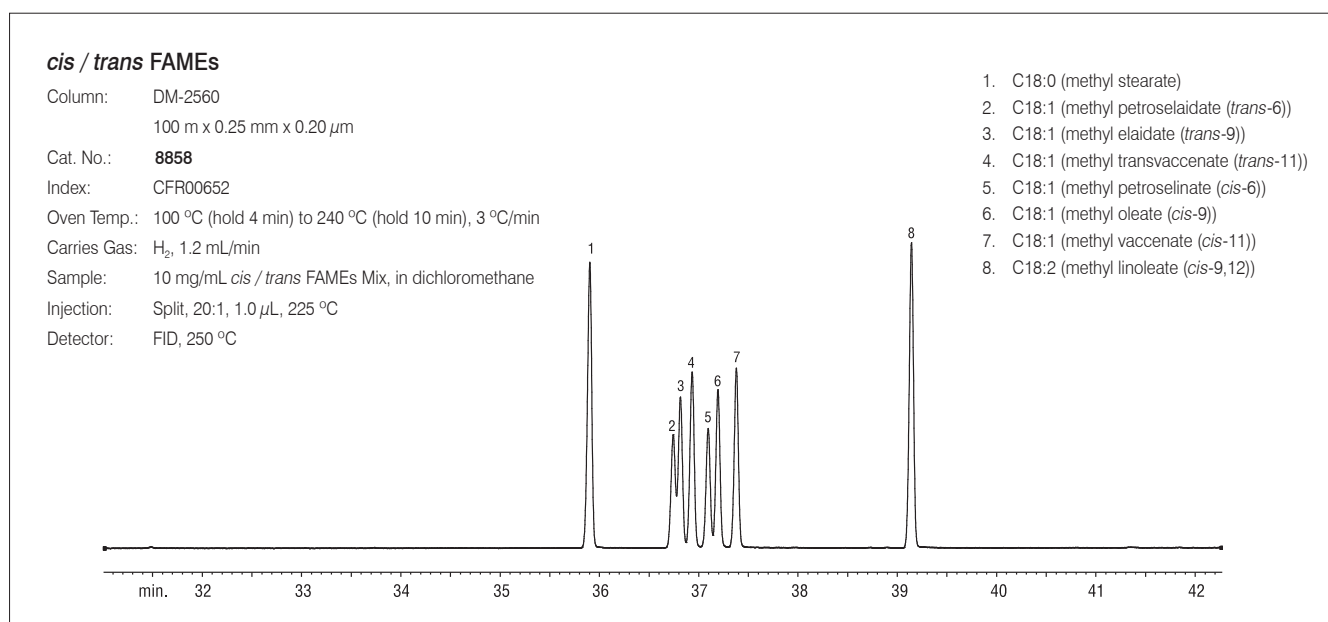

DM-2560 Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	100 m	
			Cat. No.	Price
0.25	0.20	20 to 250	8858	\$1,275

Column Phase Cross Reference

DikmaCap™	Phase	Agilent	Restek	Supelco
DM-PLOT Alumina	Aluminum oxide	GS-Alumina, HP-PLOT S, CP-Al ₂ O ₃ PLOT	-	-
DM-PLOT Alumina / Na ₂ SO ₄	Aluminum oxide Na ₂ SO ₄ deactivation	GS-Alumina, HP-PLOT S, CP-Al ₂ O ₃ / Na ₂ SO ₄ PLOT	Rt-Alumina BOND / Na ₂ SO ₄ Alumina Sulfate PLOT	
DM-PLOT Alumina / KCl	Aluminum oxide KCl deactivation	GS-Alumina / KCl, HP-PLOT Al ₂ O ₃ / KCl, CP-Al ₂ O ₃ / KCl PLOT	Rt-Alumina BOND / KCl	Alumina Chloride PLOT
DM-PLOT CFC			Rt-Alumina BOND / CFC	
DM-PLOT MS 5A	Molecular sieve 5A	HP-PLOT Molesieve, CP-Molesieve 5A	Rt-Msieve 5A	Molsieve 5A
DM-PLOT Q	100% DVB	CP-PoraPLOT Q, CP-PoraBond Q	Rt-Q-BOND	Supel-Q PLOT
DM-PLOT QS	Porous DVB homopolymer	GS-Q	Rt-QS-BOND	-
DM-PLOT S	DVB 4-vinylpyridine	CP-PoraPLOT S	Rt-S-BOND	-
DM-PLOT U	DVB ethylene glycol / dimethylacrylate	HP-PLOT U, CP-PoraPLOT U, CP-PoraBond U	Rt-U-BOND	

DM-PLOT Alumina (Al₂O₃)

- Retention index for unsaturated hydrocarbons is higher than that of alkane hydrocarbon. Selectivity of DM-PLOT Alumina column is tested using retention indices for unsaturated hydrocarbons.
- Dikma has developed a special procedure to reduce the activity of alumina to the lowest level. The column sensitivity for unsaturated compounds (such as alkenes, alkynes and dienes) is also verified to ensure a linear and quantitative chromatographic analysis for these compounds.
- Every DM-PLOT Alumina column is tested with a hydrocarbon standard to ensure proper phase thickness and inertness.
- Strong bonding avoids particle generation.
- The phase can be regenerated by water flushing after contamination.



Selectivity

Selectivity of DM-PLOT Alumina columns are measured using retention indices for acetylene and propadiene. The retention property is higher with increasing compounds unsaturation and decreasing volatility.

For saturated substances, the volatility decides the retention strength of compounds. The volatility is stronger with less retention index. All alkane isomers have weaker retention strengths and stronger volatility compared with *n*-alkanes containing same number of carbon atoms. Similarly, the volatility is decreased and retention index is increased as the number of carbon atoms is increased.

For unsaturated hydrocarbons, the retention index is decided by the degree of unsaturation (polarity). Retention properties are higher with stronger degree of unsaturation. In general, hydrocarbons with a higher degree of unsaturation have higher polarity due to the π -electrons.

Table 1 The Retention Index and Sensitivity of DM-PLOT Alumina to Unsaturated Hydrocarbons

	Ethylene	Acetylene	Propylene	Allene
Retention Index	255	421	372	407
Ratio of Peak Height	0.65	0.72	0.84	0.54

Sensitivity

A reasonable deactivation treatment can reduce the activity of alumina phase to the lowest level and improves the selectivity of column. The inertness of alumina phase ensures a linear response which is the base of quantitative analysis. Dikma has developed special deactivated procedures to DM-PLOT Alumina to ensure high inertness and linear response to unsaturated and saturated hydrocarbons. The sensitivity of DM-PLOT Alumina is four times more than that of other PLOT columns on the market (see Table 1).

Reproducibility

Every DM-PLOT Alumina column is tested with gas standard (C1-C4) to confirm proper phase thickness and deactivation degree, ensuring maximum reproducibility.

Application Chromatogram

Sample / Compound	Page
1,3-Butadiene Purity	172
Hydrocarbons	173
Propylene Purity	171
Refinery Gas	172


DM-PLOT Alumina / Na₂SO₄

DM-PLOT Alumina / Na₂SO₄

- Butanes (impurities in acetylene / propadiene) elute before acetylene / propadiene
- Best separation for butene isomers (impurities in butene streams)
- Propylene elutes after cyclopropane (impurity in propylene)
- Similar to GS-Alumina, HP-PLOT S, Alumina Sulfate PLOT, AT-Alumina, and CP-Al₂O₃ / Na₂SO₄ PLOT

Application Chromatogram

Sample / Compound	Page
Refinery Gas	170

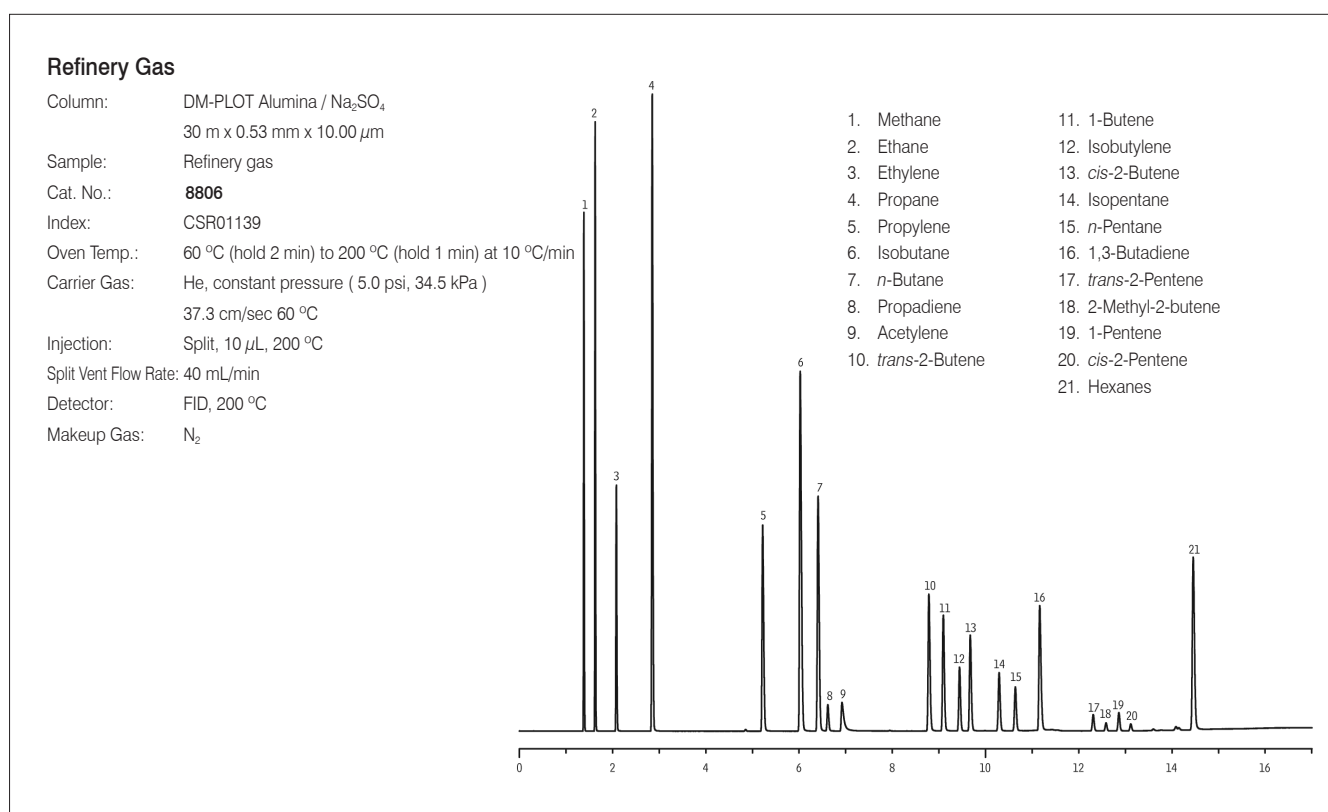

DM-PLOT Alumina / Na₂SO₄ Ordering Information


ID (mm)	df (μm)	MAOT (°C)	30 m		50 m	
			Cat. No.	Price	Cat. No.	Price
0.25	4.00	to 200	8860	\$620		
0.32	5.00	to 200	8804	620	8805	\$1,005
0.53	10.00	to 200	8806	600	8807	990

DM-PLOT Alumina / KCl

- C4 hydrocarbons (impurities in butane / isobutane) elute after acetylene
- 1,3-Butadiene elutes after methyl acetylene (impurity in 1,3-butadiene)
- Similar to GS-Alumina / KCl and CP-Al₂O₃ / KCl PLOT

Application Chromatogram

Sample / Compound	Page
Butane Lighter Fluid	170

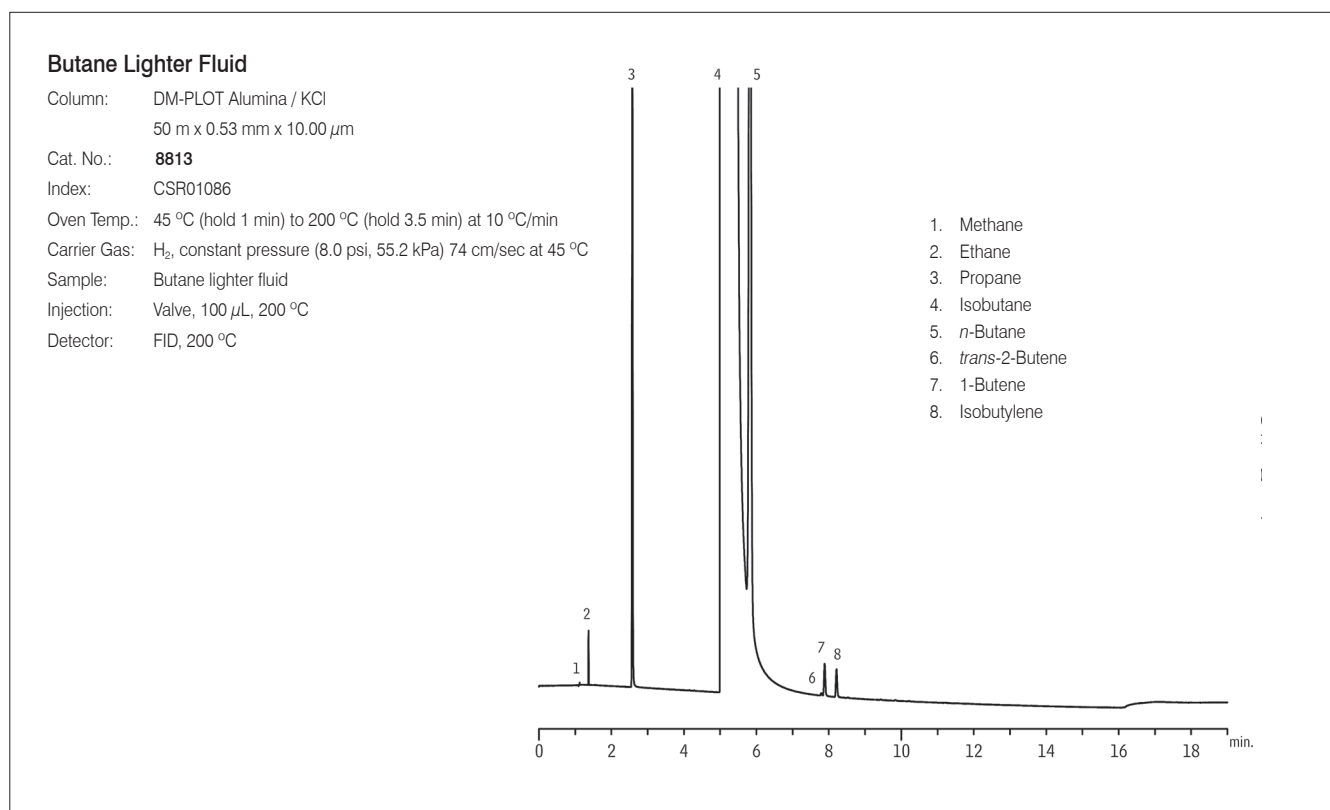

DM-PLOT Alumina / KCl Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m		50 m	
			Cat. No.	Price	Cat. No.	Price
0.25	4.00	to 200	8861	\$620		
0.32	5.00	to 200	8808	620	8809	\$1,005
0.53	10.00	to 200	8811	600	8813	990

DM-PLOT MS 5A

DM-PLOT MS 5A


- Separation for permanent gases
- 100% Stationary phase bonded without particles loss

DM-PLOT MS 5A column is used for separation of Ar / O₂ and other permanent gases. Special procedures ensure high column efficiency and integrity of the porous layer coating. This column has special selectivity to certain compounds by controlling the pore size of particles. Additionally, our special immobilization process ensures that the stationary phase particles adheres to the tubing.

The advanced molecular sieve DM-PLOT MS 5A column can separate Ar / O₂ and H₂ / He at or above ambient temperature. This column is also an ideal choice for separation of permanent gases in refined or natural gases.

Application Chromatogram

Sample / Compound	Page
Permanent Gases	168, 169

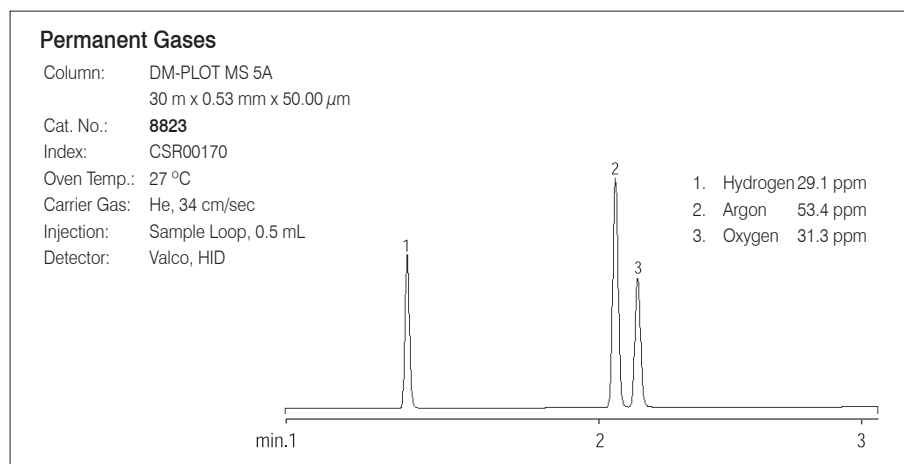

DM-PLOT MS 5A Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m	
			Cat. No.	Price
0.32	30.00	to 300	8822	\$555
0.53	50	to 300	8823	640

DM-PLOT Q / QS / S / U

- Separation for gases and volatile organic compounds
- 100% Stationary phase bonded without particles loss

We have developed a unique polymer synthesis technology and coating process for the manufacture of porous polymer PLOT columns. The selectivity of stationary phase is similar to the phase of Porapak and HayeSep.

The porous polymer PLOT column is not sensitive to water, so this column can be used for analysis of water-containing samples.

The polarity and selectivity of the stationary phase is changed by incorporating polar groups on PS / DVB. The non-polar phase of DM-PLOT Q column is DVB. DM-PLOT S is the mid-polarity PLOT column with high 4-vinyl pyridine on DVB.

The stationary phase of DM-PLOT QS is porous divinylbenzene homopolymer, which has a polarity between DM-PLOT Q and DM-PLOT S due to intermediate polarity PLOT column incorporation of low 4-vinyl pyridine. This column is used for separation of ethane, ethylene and acetylene to baseline.

DM-PLOT U is a polar PLOT column incorporating divinylbenzene ethylene glycol / dimethylacrylate, and can be used for the analysis of polar and non-polar compounds.

All PLOT columns have wide application range. PLOT columns can analyze permanent gases below room temperature. Inorganic gases such as CO₂, hydrocarbons and polar and non-polar solvents can be easily separated on PLOT columns.

Application Chromatogram

Sample / Compound	Page
Alcohols	186
Hydrocarbon Gases	171, 172, 173
Hydrocarbons	172
Natural Gas #2	170
Polar Solvents	199
Permanent Gases	168, 169

DM-PLOT Q / QS / S / U Ordering Information

	ID (mm)	df (μm)	MAOT (°C)	30 m	
				Cat. No.	Price
DM-PLOT Q	0.25	8.00	to 280 / 300	8866	\$580
	0.32	10.00	to 280 / 300	8818	585
	0.53	20.00	to 280 / 300	8816	640
DM-PLOT QS	0.25	8.00	to 250	8867	580
	0.32	10.00	to 250	8828	550
	0.53	20.00	to 250	8830	600
DM-PLOT S	0.25	8.00	to 250	8868	580
	0.32	10.00	to 250	8810	585
	0.53	20.00	to 250	8812	640
DM-PLOT U	0.25	8.00	to 190	8869	580
	0.32	10.00	to 190	8824	595
	0.53	20.00	to 190	8826	640

DM-PLOT CFC

DM-PLOT CFC


- Improved inertness for halogenated compounds
- Highly selective alumina-based column
- High retention and capacity for CFCs
- Specially designed for CFCs separation

Aluminum oxide is an ideal adsorbent for retaining halogenated compounds especially CFCs (Freon products). It has high selectivity for separating CFC isomers at above ambient temperatures.

DM-PLOT CFC column can reduce the reactivity of alumina due to the deactivation process. Even though there is still some residual mono- or di-substituted CFCs, the majority of these compounds can be accurately quantified in impurity analysis.

Application Chromatogram

Sample / Compound	Page
Impurity Analysis of 1,1,1,2-Tetrafluoroethane	170

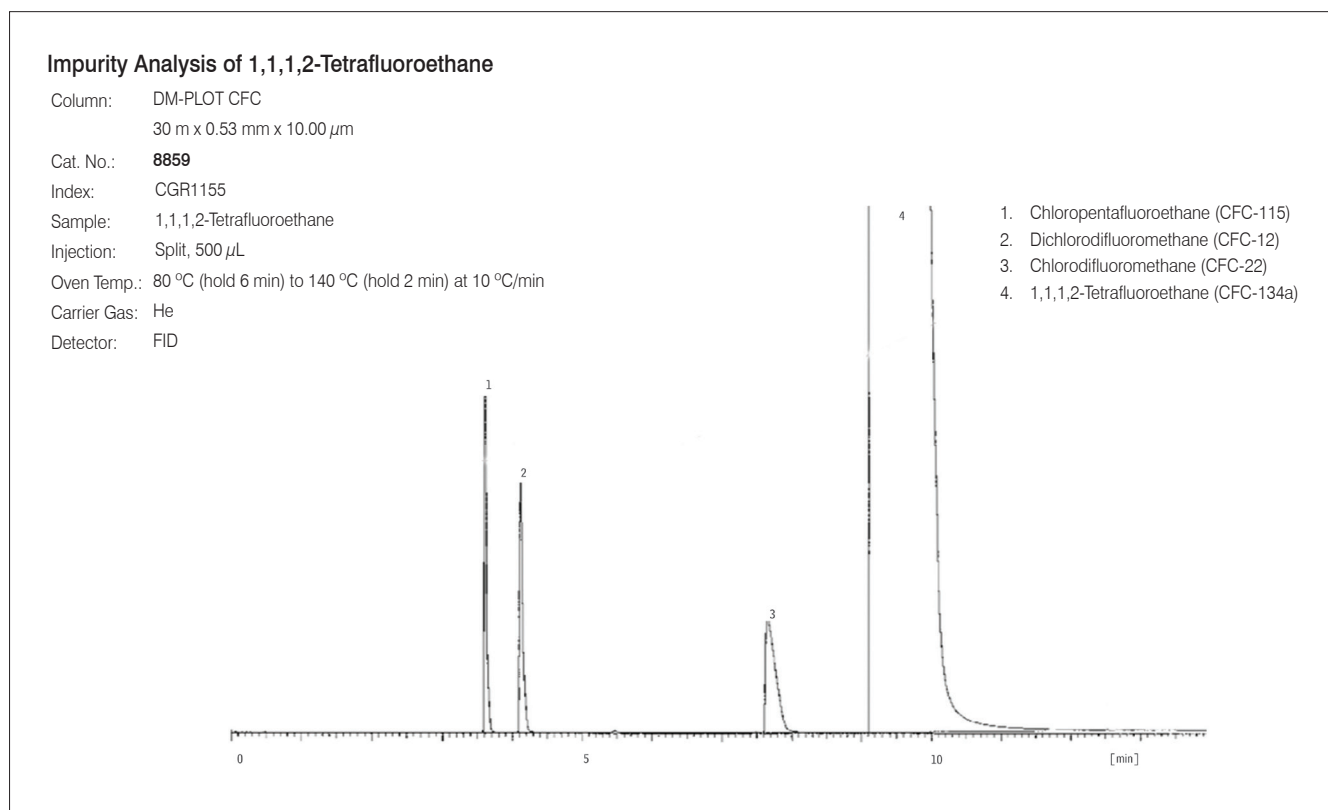

DM-PLOT CFC Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m Cat. No.	Price
0.53	10.00	to 200	8859	\$600

DM-PONA

- 100% Dimethyl polysiloxane
- Non-polar phase
- Specially designed for analysis of complex hydrocarbon compounds
- Exceeds ASTM and CGSB method guidelines
- Temperature range: -60 °C to 340 °C
- Similar to Petrocol DH, DB-petro and HP-PONA
- Solvent rinsable

DM-PONA is a non-polar column for analysis of complex hydrocarbon compounds. Our rigorous QC method exceeds the ASTM method guidelines for resolution and retention time.

Application Chromatogram

Sample / Compound	Page
Detailed Hydrocarbons Analysis	179

Detailed Hydrocarbons Analysis

Column: DM-PONA

100 m x 0.25 mm x 0.50 μ m

Cat. No.: 7805

Index: CSR00209

Oven Temp.: 35 °C (hold 13 min) to 45 °C (hold 15 min) at 10 °C/min to 60 °C (hold 15 min) at 1 °C/min to 200 °C (hold 5 min) at 1.9 °C/min


Carrier Gas: He, 24 cm/sec, 35 °C

Sample: Unleaded gasolines, 0.5 μ L

Injection: Split, 100:1, 250 °C

Detector: FID, 4 x 10⁻¹² AFS, 250 °C

1. Propane	10. <i>n</i> -Heptane	19. <i>n</i> -Nonane
2. Isobutane / Methanol	11. Toluene	20. 1,3,5-Trimethylbenzene
3. <i>n</i> -Butane	12. 2,3-Dimethylhexane	21. 1,2,4-Trimethylbenzene
4. <i>iso</i> -Pentane	13. <i>n</i> -Octane	22. <i>n</i> -Decane
5. <i>n</i> -Pentane	14. Ethylbenzene	23. <i>n</i> -Undecane
6. 3-Methylpentane	15. <i>m</i> -Xylene	24. Naphthalene
7. <i>n</i> -Hexane	16. <i>p</i> -Xylene	25. <i>n</i> -Dodecane
8. Benzene	17. 2,3-Dimethylheptane	26. 2-Methylnaphthalene
9. 2-Methylhexane	18. <i>o</i> -Xylene	27. <i>n</i> -Tridecane

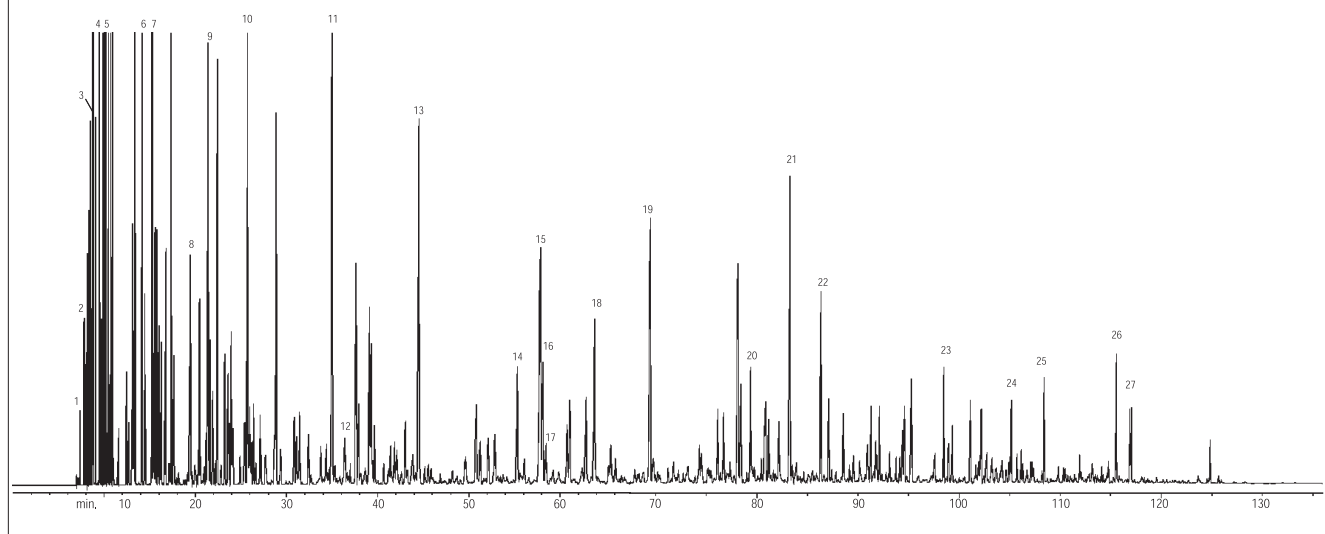

DM-PONA Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	50 m		100 m	
			Cat. No.	Price	Cat. No.	Price
0.20	0.50	-60 to 300 / 340	7804	\$750		
0.25	0.50	-60 to 300 / 340			7805	\$875

DM-TCEP

DM-TCEP


- 1,2,3-*Tris*[2-cyanoethoxy]propane
- Highly polar phase
- General purpose column, ideal for aromatics and oxygenates in gasoline
- Temperature range: 0 °C to 135 °C
- Similar to CP-TCEP

Most gasolines contain aliphatic hydrocarbons up to C12. To separate aromatics and oxygenates in gasoline effectively, it is desirable to elute benzene after C11 and toluene after C12. The strong polar DM-TCEP stationary phase offers a retention index for benzene greater than 1,100 ppm and can separate alcohols and aromatics from the aliphatic constituents in gasoline.

DM-TCEP column has the same high polarity as packed columns, which is a column used for analysis of petroleum oxygenates listed in ASTM D4815 with higher efficiency.

Application Chromatogram

Sample / Compound	Page
Aromatics	181
Petroleum Oxygenates	174

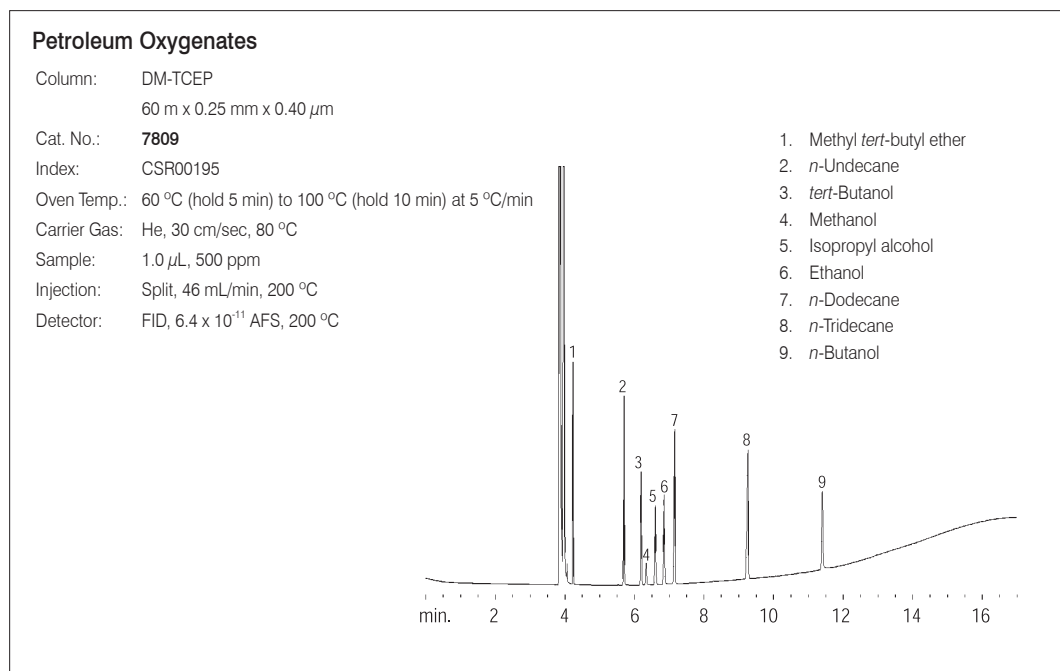

DM-TCEP Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	60 m	
			Cat. No.	Price
0.25	0.40	0 to 135	7809	\$780

DM-1HT SimDist Metal

- Special purpose column, ideal for high temperature simulated distillation
- Reliably meets all ASTM D6352, D7169, and D7500 specifications
- 100% Dimethyl polysiloxane phase
- Sulfinert-treated high elasticity stainless steel tubing
- Stable up to 450 °C

DM-1 HT SimDist Metal meets ASTM D6352, D7169 and D7500 specifications for high temperature simulated distillation. Highly robust phase provides an accurate retention time / boiling point curve, and exhibits excellent peak shape and low bleed even at 450 °C. DM-1HT SimDist Metal offers a higher maximum operating temperature compared with DM HT SimDist Metal (450 °C vs. 430 °C).

DM-1 / DM-500 SimDist Metal


- Special purpose column, ideal for high temperature simulated distillation
- DM-1 SimDist Metal phase offers true methyl silicone polarity
- DM-500 SimDist Metal phase is a carborane siloxane polymer
- Sulfinert-treated high elasticity stainless steel tubing
- Stable up to 430 °C

Application Chromatogram

Sample / Compound	Page
Bleed Profile	177
Hydrocarbons, C10-C44	178
Hydrocarbons, C30-C110	178
Hydrocarbons, C44-C100	177


Hydrocarbons, C44-C100

Column: DM-1HT SimDist Metal
5 m x 0.53 mm x 0.20 μ m
Cat. No.: 8871
Index: CSR01120
Oven Temp.: 40 °C to 430 °C at 100 °C/min
Carrier Gas: He
Sample: C10-C100, 1% in CS₂
Injection: PTV, 0.2 μ L
Flow Rate: 20 mL/min
Detector: FID, 430 °C

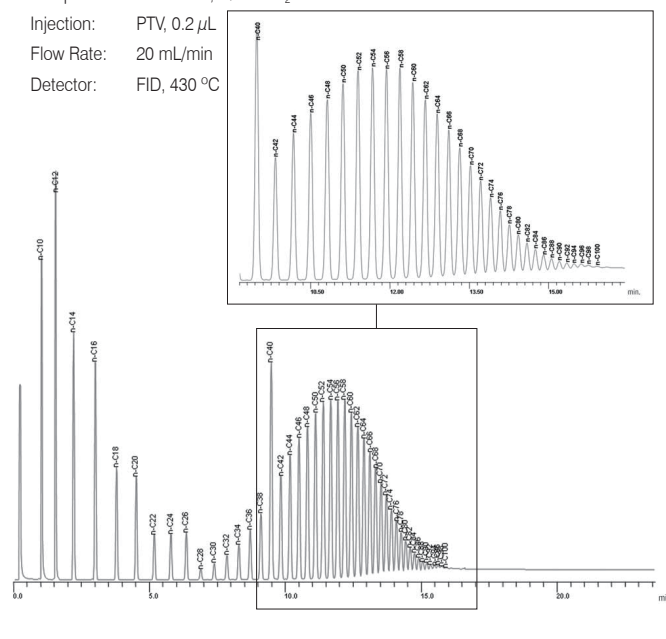

DM Series SimDist Metal (Sulfinert Treated Stainless Steel) Ordering Information

Phase	ID (mm)	df (μ m)	MAOT (°C)	5 m		6 m	
				Cat. No.	Price	Cat. No.	Price
DM-1HT SimDist Metal	0.53	0.10	-60 to 450	8870	\$280		
						8871	280
DM-1 SimDist Metal	0.53	0.15	-60 to 430			7838	\$310
DM-500 SimDist Metal	0.53	0.15	-60 to 430			7839	310



DM-2887 / DM-2887 Metal


DM-2887 / 2887 Metal

- 100% Dimethyl polysiloxane
- Special purpose column, ideal for simulated distillation
- Stable up to 360 °C
- Similar to DB-2887, Petrocol EX2887

DM-2887 column's stationary phase, film thickness, and dimension have been optimized to exceed the asymmetry factor and resolution requirements specified in ASTM method D2887. Each column is individually tested with hydrocarbon mixtures to guarantee low bleed and reproducibility.

Application Chromatogram

Sample / Compound	Page
Simulated Distillation	178

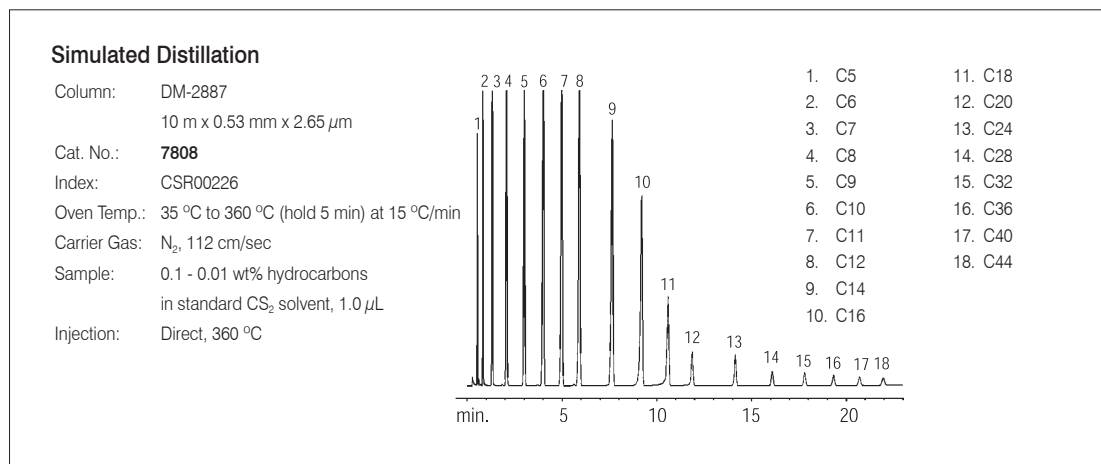

DM-2887 (Fused Silica) Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	10 m	
			Cat. No.	Price
0.53	2.65	-60 to 360	7808	\$220

DM-2887 Metal (Sulfinit-Treated Stainless Steel) Ordering Information


ID (mm)	df (μ m)	MAOT (°C)	10 m	
			Cat. No.	Price
0.53	2.65	-60 to 400	7810	\$225

DM-BDTG Metal

- For biological diesel oil analysis
- Reduces analysis time and optimizes mono-, di- and triglyceride peaks
- Stable up to 430 °C
- Integra-Gap built-in retention gap eliminates column coupling completely

Application Chromatogram

Sample / Compound	Page
Glycerin in Biodiesel (ASTM D6584)	177

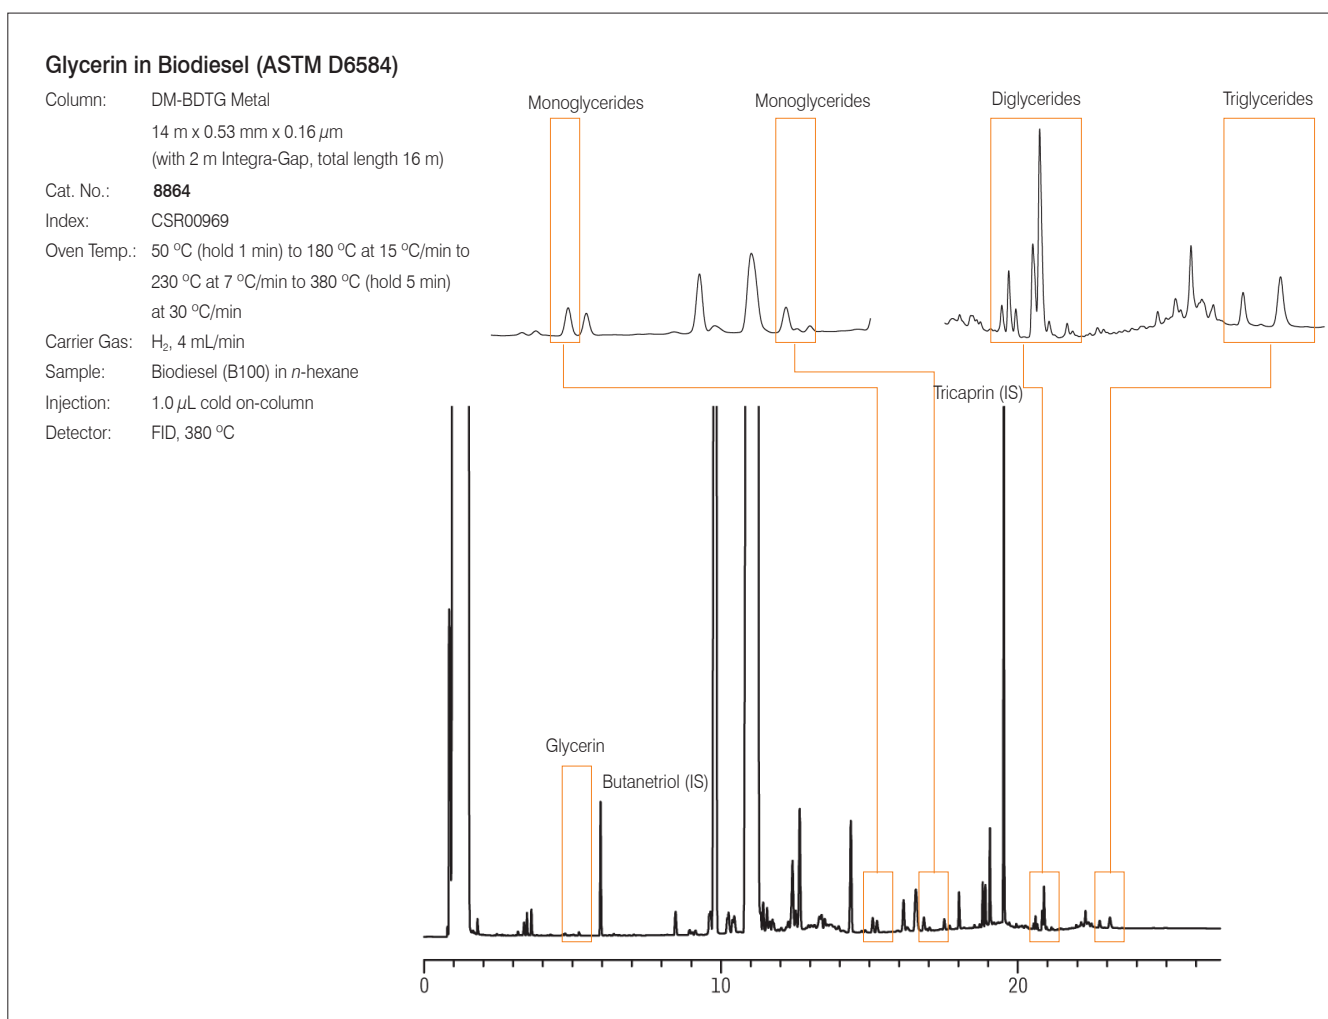

DM-BDTG Metal Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	Length	Cat. No.	Price
0.53	0.16	-60 to 380 / 430	14 m with 2 m Integra-Gap (total length 16 m)	8864	\$505

DM-Volatile Amine

DM-Volatile Amine


- Special selectivity for baseline resolution of all volatile amines
- Excellent inertness assures sensitivity and accuracy for volatile amines such as free ammonia
- Highly robust phase allows repeated water injections, increases longer column lifetime
- Direct replacement for CP-Volatile, thick-film CP-Sil 8

The DM-Volatile Amine column was optimized for the separation of volatile amines even when the sample contains high percentages of water. The unique base deactivation creates an exceptionally inert surface for these sensitive compounds, resulting in highly symmetric peaks which allow low detection limits.

Both 30 m and 60 m columns are available to ensure the separation for most of amine samples. Due to the high temperature stability up to 290 °C, it ensures elution of amines up to C16 and allows contaminations to be removed by "baking out" the column.

Application Chromatogram

Sample / Compound	Page
Short Chain Amines in Water	183

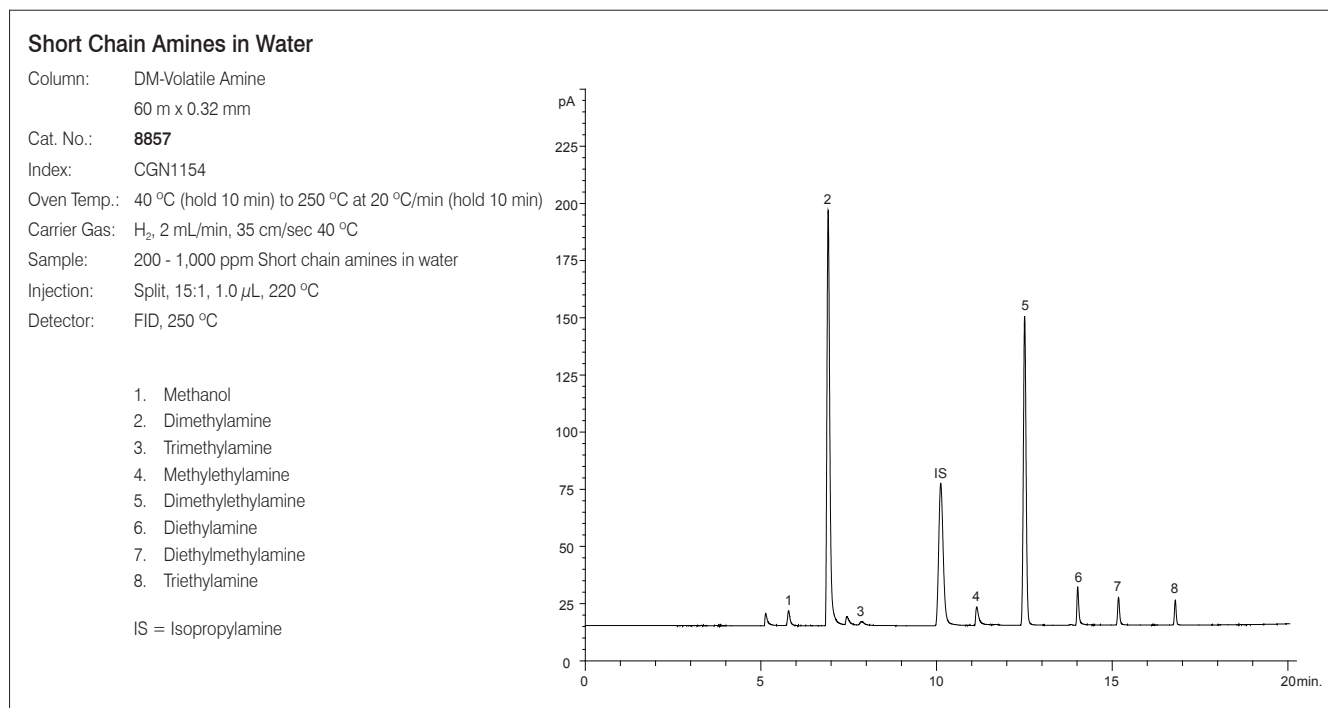

DM-Volatile Amine Ordering Information

ID (mm)	MAOT (°C)	30 m		60 m	
		Cat. No.	Price	Cat. No.	Price
0.32	-60 to 290	8856	\$540	8857	\$1,020

DM-5 Amine

- Bonded and cross-linked 5% diphenyl / 95% dimethyl polysiloxane
- Low polarity phase
- Specially designed for amines and other basic compounds
- Stable up to 315 °C
- Solvent rinsable
- Similar to PTA-5

Typical GC methods for analysis of basic compounds require derivatization to avoid peak tailing. The DM-5 Amine column has a special tubing surface which is chemically altered to reduce tailing of basic compounds, thereby eliminating the need for column priming.

The DM-5 Amine column is ideal for analysis of basic compounds including alkylamines, diamines, triamines, ethanolamines, nitrogen heterocyclic compounds, neutral compounds, and adsorptive compounds with oxygen groups susceptible to hydrogen bonding, or even weakly acidic compounds such as phenols.


Every DM-5 Amine column is tested to ensure that it meets the requirements for analyzing amines with low ppm levels, and to ensure low bleed at maximum operating temperature.

Application Chromatogram

Sample / Compound	Page
Amines / Phenols	185
Antihistamines	210
Ethylenediamines	184
Sympathomimetic Amines Drugs	209

Amines / Phenols

Column:	DM-5 Amine	
	30 m x 0.32 mm x 1.00 μ m	
Cat. No.:	7817	
Index:	CCR00301	
Oven Temp.:	120 °C to 220 °C at 10 °C/min	
Carrier Gas:	H ₂ , 38 cm/sec, 120 °C	
Sample:	Amines / phenols in water, 1.0 μ L, 22 ng	
Injection:	Split, 25:1, 305 °C	
Detector:	FID, 6.4 x 10 ⁻¹¹ AFS, 305 °C	
		1. Diethylamine
		2. Pyridine
		3. Morpholine
		4. Phenol
		5. Aniline
		6. 2-Chlorophenol
		7. Diethylenetriamine
		8. Octylamine
		9. 1-Methyl-2-pyrrolidinone
		10. 2-Nitrophenol
		11. 2,6-Dimethylaniline
		12. Nicotine
		13. 2-Nitroaniline

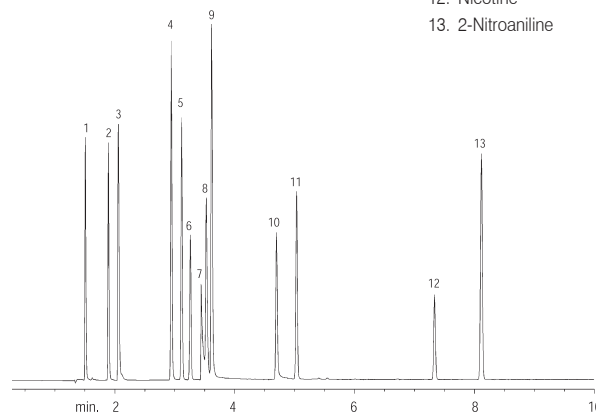

DM-5 Amine Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m	
			Cat. No.	Price
0.25	0.50	-60 to 300 / 315	7815	\$530
	1.00	-60 to 300 / 315	7816	530
0.32	1.00	-60 to 300 / 315	7817	560
	1.50	-60 to 290 / 305	7818	560
0.53	1.00	-60 to 290 / 305	7819	630
	3.00	-60 to 280 / 295	7820	630

DM-35 Amine

DM-35 Amine

- Bonded and cross-linked 35% diphenyl / 65% dimethyl polysiloxane
- Mid-polarity phase
- Base deactivated
- Specially designed for amines and other basic compounds
- Stable up to 220 °C
- Solvent rinsable

Typical GC methods for analysis of basic compounds require derivatization to avoid peak tailing. The DM-35 Amine column has a special tubing surface which is chemically altered to reduce tailing of basic compounds, thereby eliminating the need for column priming.

The DM-35 Amine column is ideal for analysis of basic compounds including alkylamines, diamines, triamines, ethanolamines, nitrogen heterocyclic compounds, neutral compounds and adsorptive compounds with oxygen groups susceptible to hydrogen bonding, or even weakly acidic compounds such as phenols.


Every DM-35 Amine column is tested to ensure that it meets the requirements for analyzing amines with low ppm levels, and to ensure low bleed at maximum operating temperature.

Application Chromatogram

Sample / Compound	Page
Cold Medicine	210
Ethanolamines	184
Primary Amines	183
Sympathomimetic Amines Drugs	209

Ethanolamines

Column:	DM-35 Amine
	30 m x 0.32 mm x 1.00 μ m
Cat. No.:	7823
Index:	CCR00585
Oven Temp.:	50 °C (hold 0.5 min) to 280 °C at 15 °C/min
Carrier Gas:	He, 40 cm/sec constant pressure
Sample:	500 μ g/mL Ethanolamine standard in water, 1.0 μ L
Injection:	Split, 10:1, 300 °C
Detector:	FID, 300 °C
	1. Monoethanolamine
	2. Diethanolamine
	3. Triethylene glycol monomethyl ether
	4. Triethanolamine

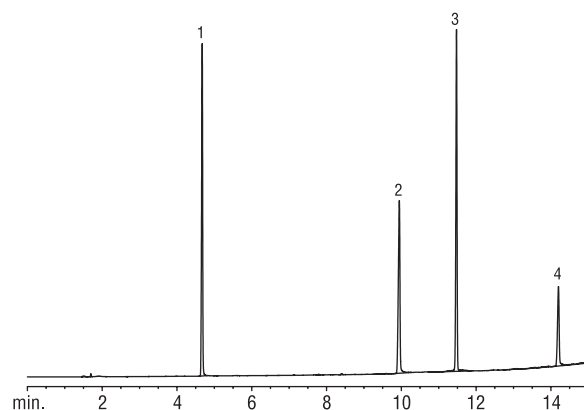

DM-35 Amine Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m	
			Cat. No.	Price
0.25	0.50	0 to 220	7821	\$530
	1.00	0 to 220	7822	530
0.32	1.00	0 to 220	7823	560
	1.50	0 to 220	7824	560
0.53	1.00	0 to 220	7825	630
	3.00	0 to 220	7826	630


DM-Wax Amine

- 100% polyethylene glycol
- Base deactivated
- Specially designed for amines and other basic compounds
- Does not require derivatization or column priming
- Stable up to 220 °C
- Similar to CAM, Carbowax Amine, CP-Wax 51

DM-Wax Amine column can reduce adsorption and improve sensitivity for many basic compounds without analyte derivatization or column priming. The DM-Wax Amine column can analyze alkylamines, diamines, triamines, ethanolamines and nitrogen heterocyclic compounds. We recommend use of DM-Wax Amine combined with DM-5 Amine columns when separating oxygenates because the DM-Wax Amine has weak adsorption of some compounds at less than ppm concentrations.

Application Chromatogram

Sample / Compound	Page
Amines (Low MW)	183
Hexamethylenediamine	184
Nitrosamines	185
Primary Amines (Low MW)	183

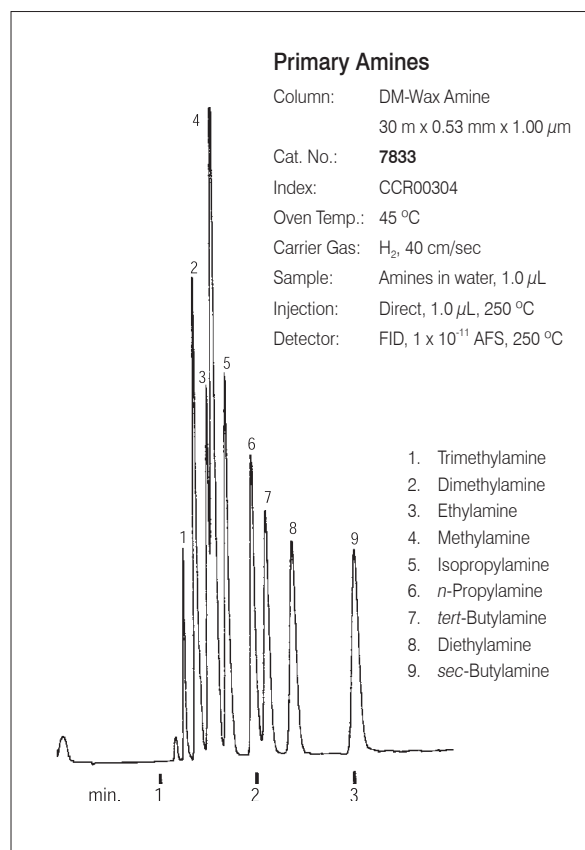

DM-Wax Amine Ordering Information

ID (mm)	df (μm)	MAOT (°C)	30 m		60 m	
			Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 210 / 220	7827	\$520		
	0.50	40 to 210 / 220	7828	520		
0.32	0.25	40 to 210 / 220	7829	565		
		40 to 210 / 220	7830	565		
	1.00	40 to 210 / 220	7832	565	7835	\$1,000
0.53	0.50	40 to 210 / 220	7837	650		
		40 to 210 / 220	7833	650	7836	\$1,110
	1.50	40 to 210 / 220	7834	660		

DM-624 / DM-624MS

DM-624


- 6% Cyanopropylphenyl / 94% dimethyl polysiloxane
- Recommended in US EPA methods for volatile organic pollutants
- Ideal for analyzing residual solvents in drugs
- Stable up to 240 °C
- Solvent rinsable
- Similar to HP-1301, HP-624, DB-1301, DB-624, etc.
- Equivalent to USP G43 phase

DM-624MS

- 6% Cyanopropylphenyl / 94% dimethyl arylene polysiloxane
- High inertness and low bleed
- Highly selective for residual solvents
- Stable up to 320 °C
- Similar to DB-624, HP-624, VF-624 ms, etc.

Application Chromatogram

Sample / Compound	Page
EP Class 1 and Class 2 Solvents	211
Organic Volatile Impurities	211
Primary, Secondary and Tertiary Amines	212
Residual Solvents	212
VOCs	155

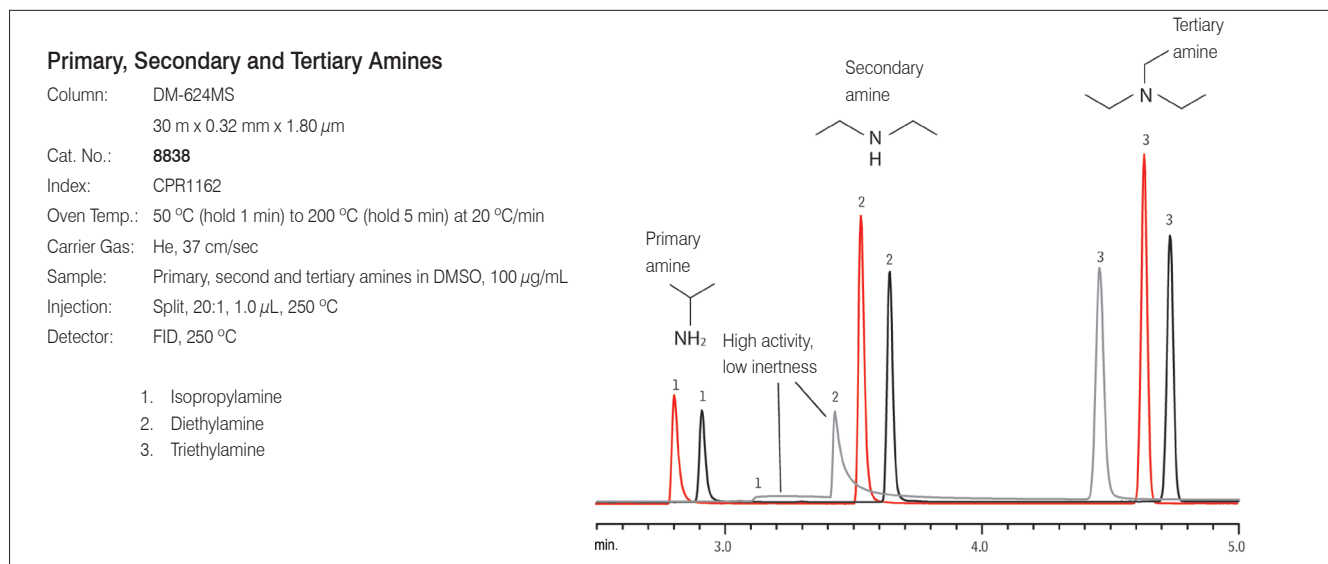

DM-624 Ordering Information

ID (mm)	df (μm)	MAOT (°C)	30 m		60 m		75 m		105 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.25	1.40	-20 to 240	7721	\$480	7722	\$790				
0.32	1.80	-20 to 240	7731	510	7732	860				
0.53	3.00	-20 to 240	7751	545			7752	\$1,055	7753	\$1,145

DM-624MS Ordering Information

ID (mm)	df (μm)	MAOT (°C)	20 m		30 m		60 m	
			Cat. No.	Price	Cat. No.	Price	Cat. No.	Price
0.18	1.00	-20 to 300 / 320	8836	\$405				
0.25	1.40	-20 to 300 / 320			8837	\$500		
0.32	1.80	-20 to 300 / 320			8838	540	8839	\$900
0.53	3.00	-20 to 300 / 320			8840	615		

DM-AQUA

- 25% Phenyl / 75% methyl polysiloxane
- Specially designed for VOCs in water
- Chromatogram includes detection of 33 compounds
- Low bleed
- Bonded and cross-linked phase, solvent rinsable


Application Chromatogram

Sample / Compound	Page
VOCs in Water	166

AQUA

Column: DM-AQUA
60 m x 0.25 mm x 1.00 μ m
Cat. No.: 7801
Index: CCO04281
Oven Temp.: 40 °C to 200 °C at 4 °C/min
Carrier Gas: He, 25 cm/sec, 150 °C
Injection: Split, 1:100, 0.5 μ L
Detector: FID

1. Bromomethane	14. Tetrachloromethane	27. Tetrachloroethylene	40. 1,2,3-Trichloropropane
2. Chloroethane	15. 1,2-Dichloroethane	28. Chlorodibromomethane	41. Bromoben
3. Trichlorofluoromethane	16. Benzene	29. 1-Chlorohexane	42. <i>o</i> -Chlorotoluene
4. 1,1-Dichloroethylene	17. Benzotrifluoride	30. 1,2-Dibromoethane	43. <i>m</i> -Chlorotoluene
5. Dichloromethane	18. Trichloroethylene	31. Chlorobenzene	44. <i>p</i> -Chlorotoluene
6. <i>trans</i> -1,2-Dichloroethylene	19. 1,2-Dichloroethane	32. 1,1,1,2-Tetrachloroethane	45. 1,3-Dichlorobenzene
7. 1,1-Dichloroethane	20. Bromodichloromethane	33. Ethylbenzene	46. 1,4-Dichlorobenzene
8. 2,2-Dichloropropane	21. Dibromomethane	34. <i>m</i> -Xylene	47. 1,2-Dichlorobenzene
9. <i>cis</i> -1,2-Dichloroethylene	22. <i>cis</i> -1,3-Dichloropropene	35. <i>p</i> -Xylene	48. 1,2-Dibromo-3 -chloropropane
10. Chloroform	23. Toluene	36. <i>o</i> -Xylene	49. 1,2,4-Trichlorobenzene
11. Chlorobromomethane	24. <i>cis</i> -1,3-Dichloropropene	37. Bromoform	50. 1,1,2,3,4,4-Hexachloro -1,2-butadiene
12. 1,1,1-Trichloroethane	25. 1,1,2-Trichloroethane	38. 1,1,2,2-Tetrachloroethane	51. 1,2,3-Trichlorobenzene
13. 1,1-Dichloropropene	26. 1,3-Dichloropropene	39. 4-Bromofluorobenzene	

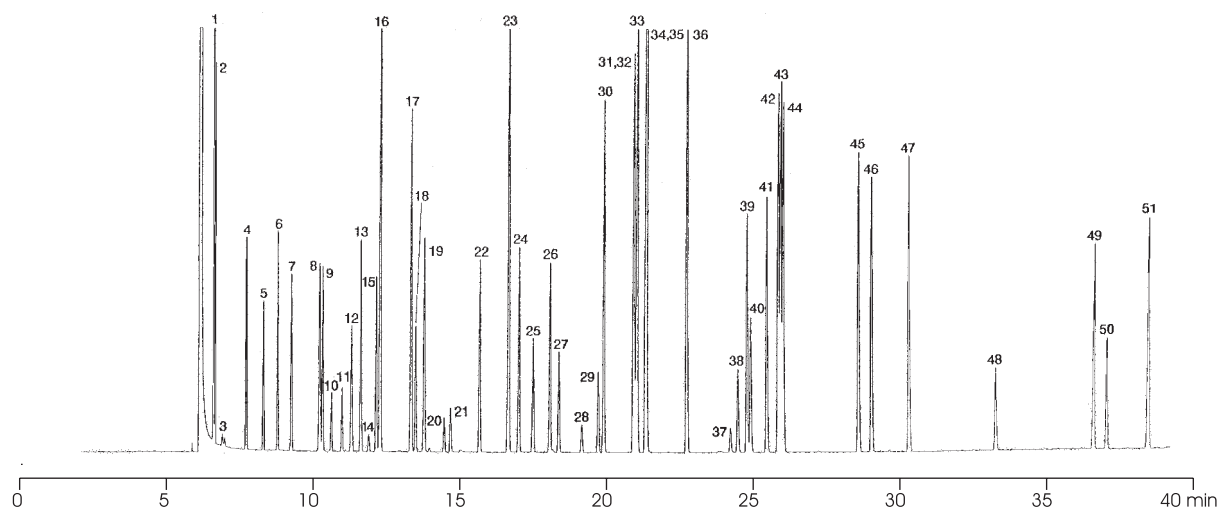

DM-AQUA Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	60 m	
			Cat. No.	Price
0.25	1.00	to 200 / 220	7801	\$1,420
0.32	1.40	to 200 / 220	7802	1,420


DM-TVOC

DM-TVOC

- 100% Dimethyl polysiloxane
- Specially designed for analysis of TVOCs
- Meets GB 50325-2001 specifications
- Low baseline noise when adopting programmed temperature
- Low bleed
- Bonded and cross-linked phase, solvent rinsable

Application Chromatogram

Sample / Compound	Page
TVOCs	154

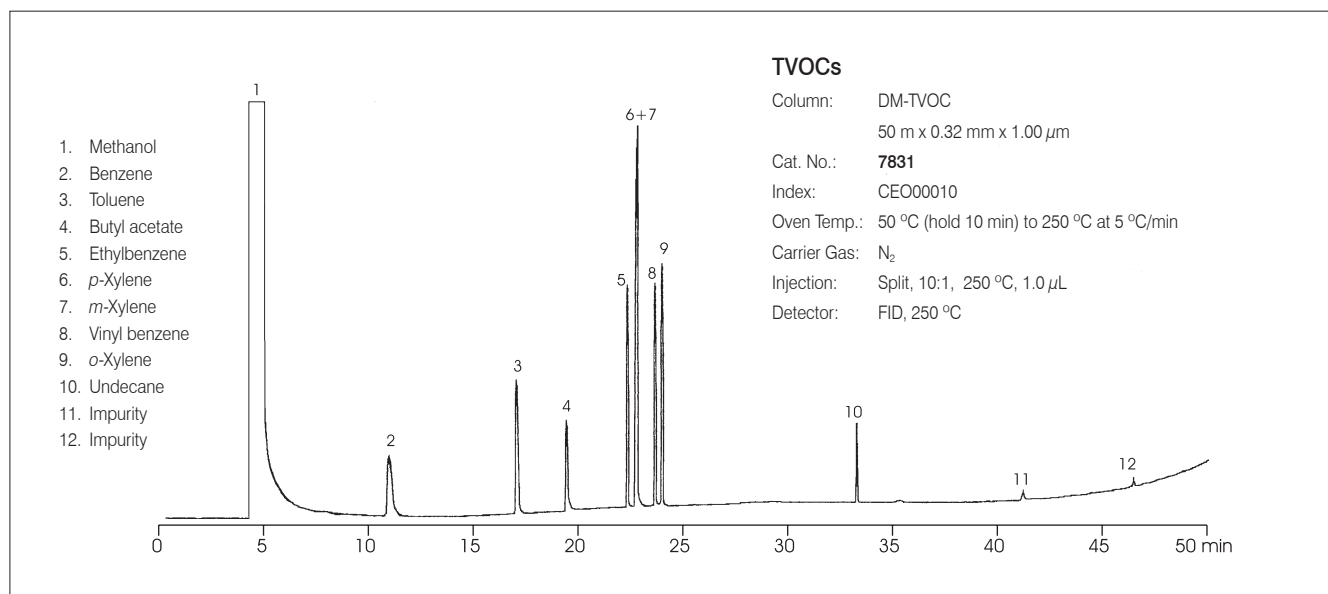

DM-TVOC Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	50 m Cat. No.	Price
0.32	1.00	to 300 / 320	7831	\$870

DM-PAH

- 50% Methyl / 50% phenyl polysiloxane
- Specially designed for analysis of PAHs
- Stable up to 360 °C
- Used for GC / MS and ECDs
- Bonded and cross-linked phase, solvent rinsable

The DM-PAH phase has excellent inertness and selectivity for PAHs. Equivalent to USP G43 phase, DM-PAH can separate EU-PAHs including fluoranthene.

Application Chromatogram

Sample / Compound	Page
PAHs	156

PAH-Mix 27

Column: DM-PAH

30 m x 0.25 mm x 0.25 μ m

Cat. No.: 8862

Index: CER1160

Oven Temp.: 65 °C (hold 0.5 min) to 220 °C at 15 °C/min
to 330 °C (hold 15 min), 4 °C/min

Carrier Gas: He, 2.0 mL/min


Sample: EPA 8310 PAHs in dichloromethane solution, 10 ppm

Injection: Splitless (hold 1.75 min), 0.5 μ L, 320 °C

Detector: FID, 320 °C

Makeup Gas: 75 mL/min

- | | |
|--------------------------|------------------------------|
| 1. Naphthalene | 15. Benzo[k]fluoranthene |
| 2. 2-Methylnaphthalene | 16. Benzo[j]fluoranthene |
| 3. 1-Methylnaphthalene | 17. Benzo[a]pyrene |
| 4. Acenaphthylene | 18. 3-Methylcholanthrene |
| 5. Acenaphthene | 19. Dibenzo[a,h]acridine |
| 6. Fluorene | 20. Dibenzo[a,i]acridine |
| 7. Phenanthrene | 21. Indeno[1,2,3-cd]pyrene |
| 8. Anthracene | 22. Dibenzo[a,h]anthracene |
| 9. Fluoranthene | 23. Benzo[ghi]perylene |
| 10. Pyrene | 24. 7H-Dibenzo[c,g]carbazole |
| 11. Benzo[a]anthracene | 25. Dibenzo[a,e]pyrene |
| 12. Chrysene | 26. Dibenzo[a,i]pyrene |
| 13. Triphenylene | 27. Dibenzo[a,h]pyrene |
| 14. Benzo[b]fluoranthene | |

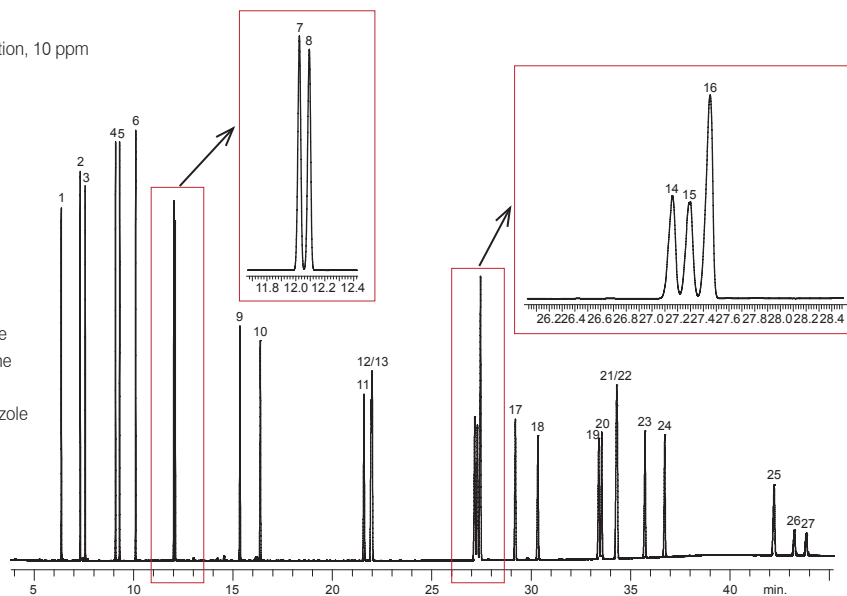

DM-PAH Ordering Information

ID (mm)	df (μ m)	MAOT (°C)*	30 m		60 m	
			Cat. No.	Price	Cat. No.	Price
0.25	0.25	40 to 340 / 360	8862	\$530	8863	\$905

*The listed temperature limits are for 30 m columns. Longer columns may have lower temperature limits.

DM-FAMEWAX


DM-FAMEWAX

- Polyethylene glycol
- Specially designed for analysis of FAMES
- Tested with a FAME mixture
- Stable up to 250 °C
- Similar to Omegawax

When DM-FAMEWAX is used for separation of unsaturated FAMES, the baseline resolution is achieved in less time.

Application Chromatogram

Sample / Compound	Page
FAMES (Black Currant Seed Oil)	202
FAMES (Flax Seed Oil)	202
FAMES (Marine Oil Standard)	202

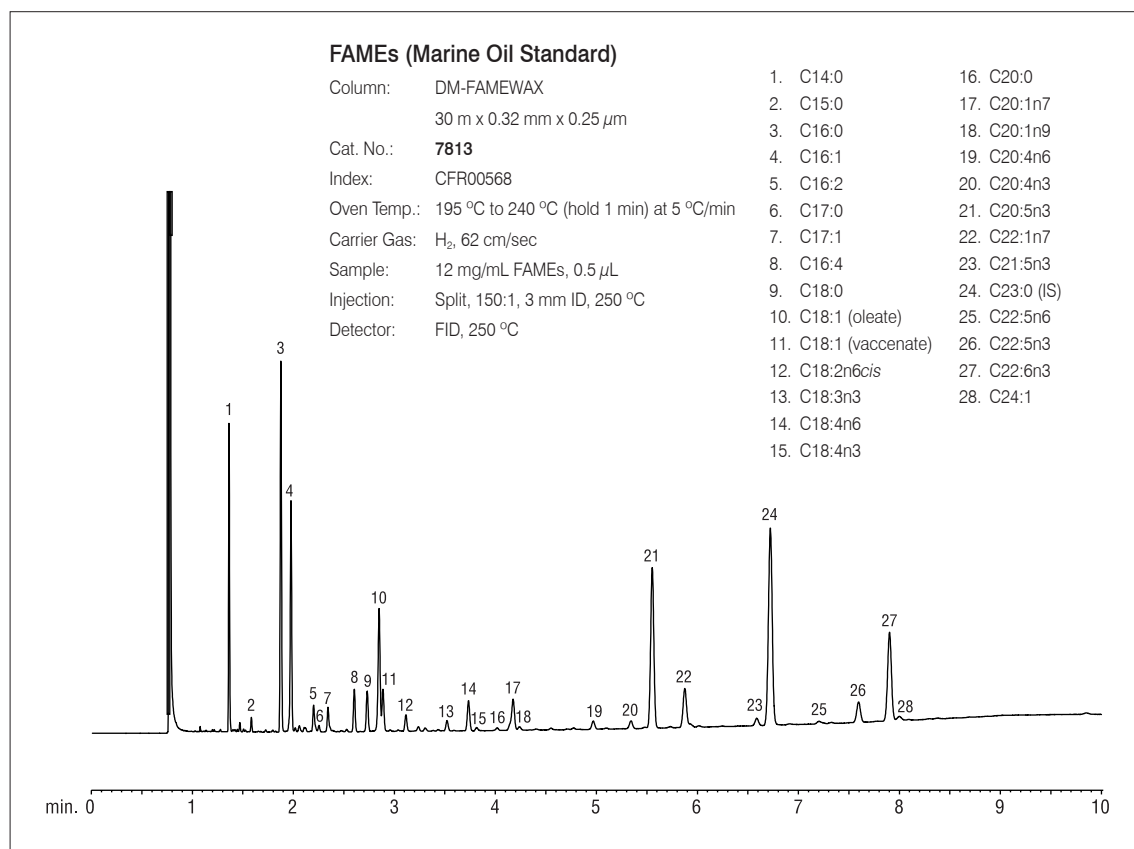

DM-FAMEWAX Ordering Information

ID (mm)	df (μ m)	MAOT (°C)	30 m	
			Cat. No.	Price
0.25	0.25	20 to 250	7811	\$460
0.32	0.25	20 to 250	7813	500
0.53	0.50	20 to 250	7814	555

Sample Preparation

ProElut™ SPE Cartridges	101
Introduction.....	102
Technical Reference	107
ProElut™ SPE Sorbents.....	109
ProElut™ QuEChERS	119
ProElut™ LLE+	123
ProMax™ Syringe Filters	124
Autosampler Vials	126
2 mL Autosampler Vials.....	126
Vial Rack.....	127



Introduction

The primary goal of solid phase extraction (SPE) with ProElut™ is the selective extraction of the components of interest from a complex sample or much larger sample volume prior to actual analysis (e.g. HPLC, GC). As SPE works on the principle of liquid chromatography, this is achieved by using strong but reversible interactions between the analyte and surface of the stationary phase. Typical interactions are hydrophobic (the Van der Waals force), polar (hydrogen bonding, dipole-dipole interaction) or ion exchange interactions. Interaction between the stationary phase and matrix should not occur. It is thus meaningful to carry out appropriate sample pre-treatment as this emphasizes the differences in chemical properties between the substance to be analyzed and matrix components so that these are then achieved by altering the pH or the ionic strength of the sample solution.

Under these conditions, the analyte is enriched as a narrow zone on the stationary phase. Subsequent to a washing step, which serves to remove possible adsorbed sample components, the actual selective elution of the analyte takes place.



ProElut™ SPE products are packed and assembled using custom designed equipment. Every part of ProElut™ manufacturing process is carefully monitored, we only accept products that meet our high quality standards.

SPE Principles and Techniques

SPE is a chromatographic technique first developed during the mid-1980s and is increasingly used for sample pre-treatment. The main objectives of SPE are removal of interfering matrix components and selective concentration and isolation of the analytes. This is done either by retaining the substance of interest and washing off everything else or by retaining the interfering substances and eluting the product of interest. Compared to traditional liquid / liquid extraction, SPE is more rapid, uses less solvent, eliminates emulsions, and can be automated. Additionally, a sample preparation task can often be solved more specifically by using SPE, since different interactions of the analyte with the adsorbent are possible, and methods can be optimized by adjusting chromatographic conditions. SPE offers a multitude of adsorbents for polar, hydrophobic and / or ionic interactions and has been widely used in medicine, food, environmental protection, commodity inspection, cosmetics and other fields.

The most popular SPE products are: Normal Phase, Reversed Phase, Ion Exchange Phase and Mix Mode. It is important to select the most suitable product for each application and sample.

Type	Reversed Phase	Normal Phase	Ion Exchange Phase	Mix Mode
Separation Mode	Reserved phase separation involves a polar (usually aqueous) or moderately polar sample matrix and a non-polar stationary phase. The analyte of interest is typically mid- to non-polar. C18 is the most common reversed phase packing	Normal phase SPE typically involves a mid- to non-polar sample matrix and a polar stationary phase. The analytes are polar compounds and the bonded phases are typically NH ₂ , PSA, polar adsorbent, silica, Florisil, and alumina, etc.	Ion exchange SPE can be used for compounds that are charged when in solution (usually aqueous, but sometimes organic). The primary retention mechanism of the compound is based on the electrostatic attraction of the charged functional group on the compound to the charged group that is bonded to the silica surface. In order for a compound to be retained by ion exchange from an aqueous solution, the pH of the sample matrix must be one at which both the compound of interest and the functional group on the bonded silica are charged The most common stationary phases are SAX and SCX	A mix of ion exchange and reserved phase retention mechanisms. This can be used for hydrophobic compounds (reversed phase) and compounds that are charged in solution (ion exchange). The most common stationary phases are PXC, PXA, etc.
Sample	Polar or hydrophobic compounds	Polar compounds	Compounds with charges	Compounds with charges, polar or hydrophobic compounds
Elution	Water or organic solvents	Non-polar solvents	Water or non-polar organic solvents	Water or organic solvents

Benefits of SPE

- Switch sample matrices to a form more compatible with chromatographic analyses
- Concentrate analytes for increased sensitivity
- Remove interference to simplify chromatography and improve quantitation
- Protect the analytical column from contaminants


Use SPE for Samples That

- Contain particulate matter that may cause system clogging and high back pressure
- Contain components that cause high background, misleading peaks, and / or poor sensitivity
- Require cleanup, trace enrichment / concentration, or purification
- Require sample matrix or solvent exchange

Choosing a SPE Product

1. *Characterize the sample.* Factors such as the analyte's polarity relative to the matrix, the presence of charged functional groups, solubility, molecular weight, etc., determine how strongly the analyte is retained by the packed bed.
2. *Select a retention strategy.* Two approaches are possible: retain interfering compounds while the analyte passes through, or retain the analyte while interfering compounds pass through. This second approach allows concentration of the sample during analyte elution.
3. *Select proper packing type and bed volume.* Choosing the packing material with the proper selectivity results in the cleanest extract with the highest recovery. Poor sample recovery often occurs when the packed bed dimensions are not optimized. Too large of a bed volume results in an incomplete elution while too small of a bed volume results in an incomplete retention. Due to the unknown composition of many samples, experimentation may be required to determine the optimum bed dimensions for an application. Start with an intermediate bed volume, such as 200 mg or 500 mg. If you observe complete retention, you may be able to use a smaller bed volume and elution volume. If you observe incomplete retention, you will need to use a larger bed volume and elution volume.
4. *Select suitable conditioning, wash, and elution solvents.* Consider the solvent strength relative to the packing material. The final conditioning solvent should be weak, so as not to act as an eluting solvent. Buffers should be used to control ionization of potentially charged compounds. Wash solvents should remove weakly retained interferences without being strong enough to elute the analyte. Elution solvents should be strong enough to completely elute an analyte in a small volume.

SPE Phase Selection

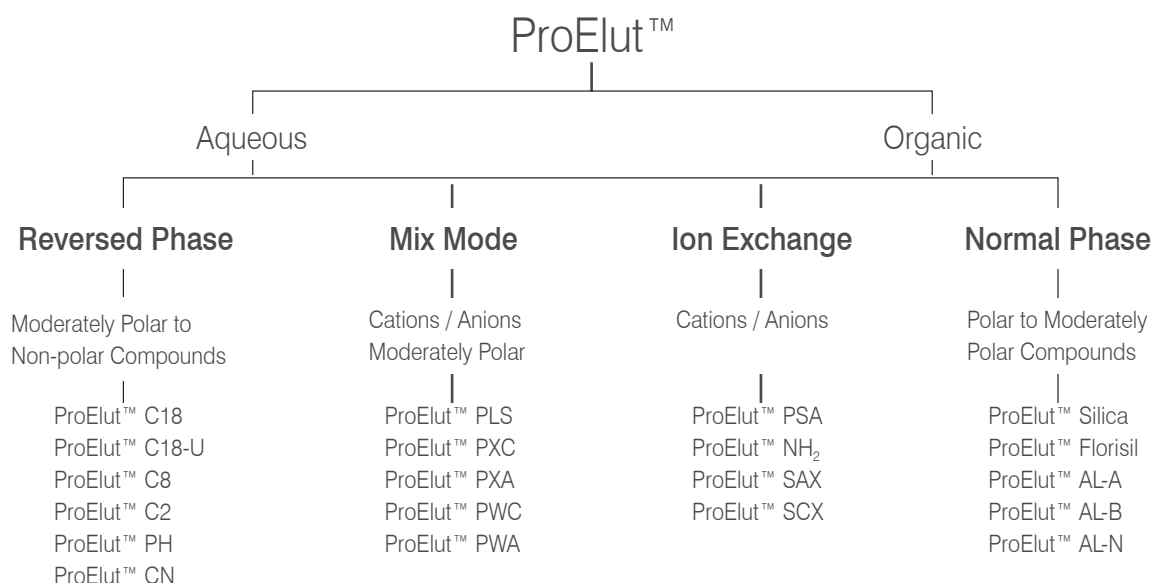

ProElut™ SPE

Common SPE Applications

- Pharmaceutical compounds and metabolites in biological fluids
- Drugs of abuse in biological fluids
- Environmental pollutants in drinking and waste water
- Pesticides and antibiotics in food / agricultural matrices
- Desalting of proteins and peptides
- Fractionation of lipids
- Water and fat soluble vitamins

General SPE Procedures

Reversed Phase

(extraction of hydrophobic or polar organic analytes from aqueous matrix)

A. Conditioning

Rinse tube with 3 - 5 mL of methanol follow by 3 - 5 mL of deionized water / buffer (do not allow tube to dry before next step).

B. Sample Application

Apply sample to the top of the tube and draw through the packing bed.

C. Tube Wash

Wash with 5 mL of a polar solvent if analyte is to be retained (deionized water, buffer or aqueous / organic mixtures are most often used).

D. Elution

Elute analyte into a collection tube with 1 - 5 mL of a non-polar solvent.

Normal Phase

(extraction of polar analytes from non-polar organic solvents)

A. Conditioning

Rinse tube with 3 - 5 mL of non-polar solvent.

B. Sample Application

Apply sample to the top of the tube and draw through the packing bed.

C. Tube Wash

Wash with 5 mL of a non-polar solvent if analyte is to be retained.

D. Elution

Elute analyte into a collection tube with 1 - 5 mL of a polar solvent.

Ion Exchange

(extraction of charged analytes from aqueous or non-polar organic samples)

A. Conditioning

Rinse tube with 3 - 5 mL of deionized water or low ionic strength buffer (10 mM).

B. Sample Application

Apply sample to the top of the tube and draw through the packing bed (ion exchange kinetics is slower than reverse or normal phase, so keep the flow slow).

C. Tube Wash

Wash with 5 mL of deionized water or low ionic strength buffer.

D. Elution

Elute analyte into a collection tube with 1 - 5 mL of buffer at high ionic strength (0.1 - 1 M) or modified pH (pH such that the analyte is uncharged).


Features of ProElut™ SPE

- Rapid sample preparation within minutes
- Higher recoveries without the formation of emulsion
- High precision of analytical results by use of disposable cartridges
- Saving of solvent and hence reduction in both materials costs and cost of disposal
- Possibilities for automating the entire process
- Optimized, validated and certified manufacturing

ProElut™ SPE Features and Benefits

ProElut™ SPE uses spherical silica with high purity and narrow particle size distribution as support. The spherical silica with fewer fines gives a more regular, stable and reproducible chromatography bed that gives a faster, more even flow rate for better separation. Fines cause back pressure increases that can result in clogging and can pass through filters and contaminate the final product. A narrower particle size distribution will give a more homogenous packing that will help in collecting more concentrated fractions and reducing solvent consumption to achieve higher recovery and reproducible results.

Figure 1. Comparison of Silica Shape and Particle Size Distribution

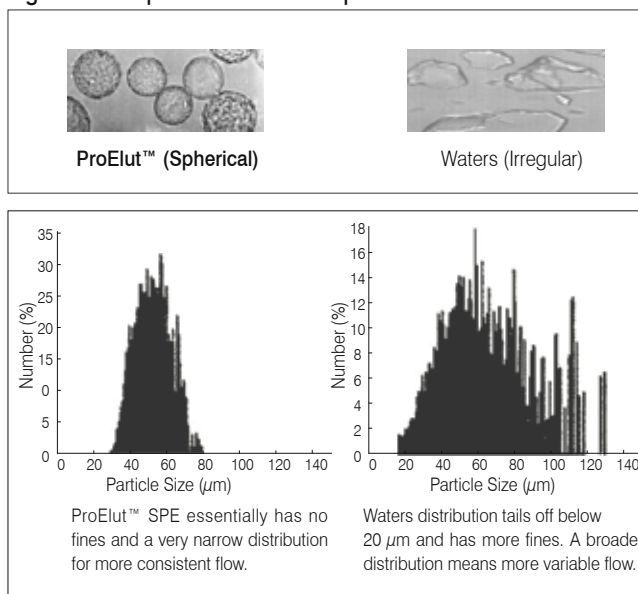


High Purity Silica Improves Recovery and Reproducibility

- ProElut™ packings are considerably lower in trace metals than the other materials
- High purity silica to enhance retention capacity of basic compounds
- Irregular silica, depending on its method of manufacturing, normally contains trace quantities of a variety of different metals, which in turn can affect the separation

Table 1. Metal Analysis of Base Silica (ppm)


Metal	Dikma ProElut™ High-purity Silica	Brand A Silica	Brand B Silica
Na	< 12	917	17
Al	< 12	276	57
Ca	< 12	< 12	< 12
Fe	< 12	64	23
Ti	< 12	< 12	130
Zr	< 12	48	38

Figure 2. Level of Organic Extractables from SPE Packing Materials as Measured by GC-FID*

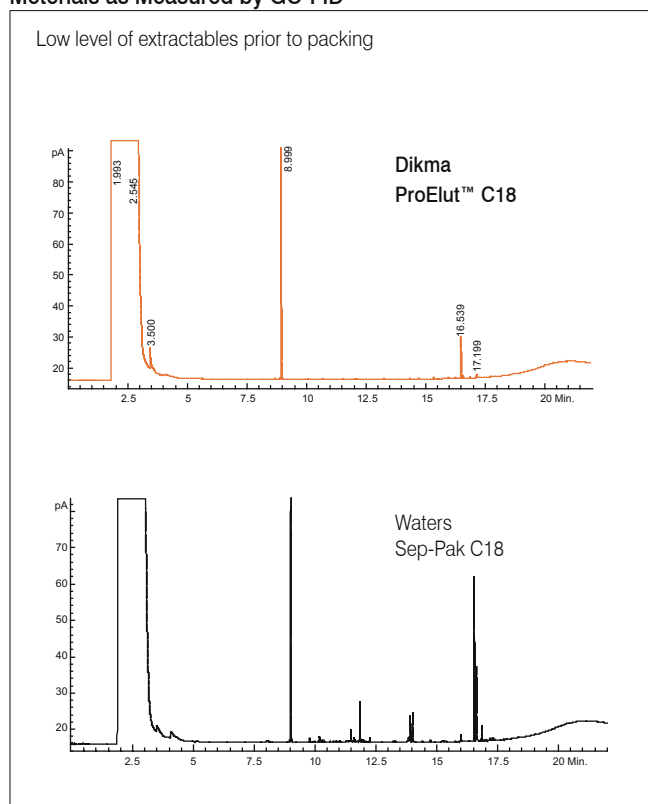

*Sep-Pak is a registered trademark of Waters Corporation. Dikma Technologies Inc. is not affiliated with the above company.

Figure 3. Level of Organic Extractables of Cartridge Tubes and Frits as Measured by GC-FID*

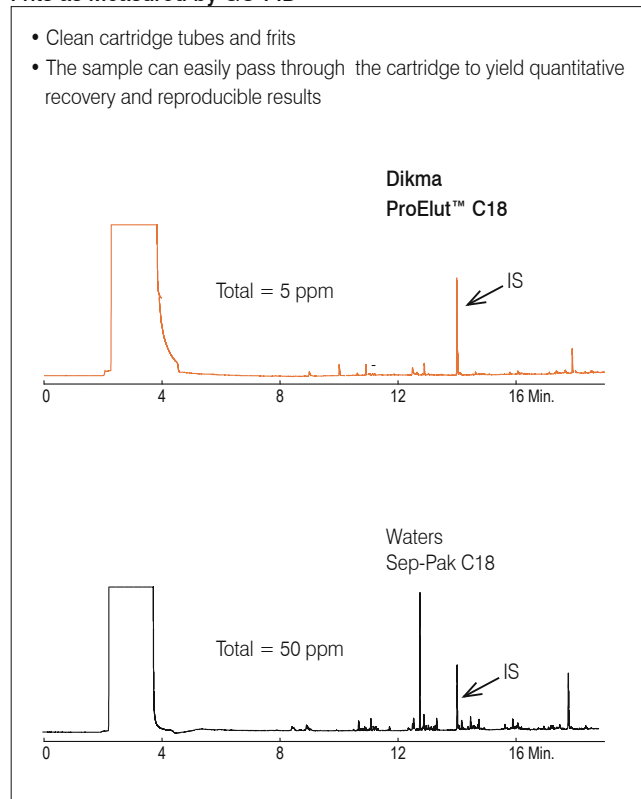

Sample Preparation

ProElut™ SPE

ProElut™ SPE

Sorbent Specifications

Sorbent Phase	Category	Base Material	Particle Size (µm)	Pore Size (Å)	Surface Area (m ² /g)	Bonded Functional Group	Carbon Loading	Endcapping
PLS	Reversed phase	PS-DVB	50	80	800	Hydrophilic / lipophilic	-	-
PWC	Reversed phase / weak cation exchange	PS-DVB	50	80	800	Hydrophilic / lipophilic, carboxylic acid	-	-
PWA	Reversed phase / weak anion exchange	PS-DVB	50	80	800	Hydrophilic / lipophilic, ethylene diamine	-	-
PXC	Reversed phase / strong cation exchange	PS-DVB	50	80	800	Hydrophilic / lipophilic, sulfonic acid	-	-
PXA	Reversed phase / strong anion exchange	PS-DVB	50	80	800	Hydrophilic / lipophilic, quaternary amine	-	-
C18	Reversed phase	Silica	50	60	500	Octadecyl	19%	Yes
C18-U	Reversed phase	Silica	50	60	500	Octadecyl, silanol	17%	No
C8	Reversed phase	Silica	50	60	500	Octyl	11%	Yes
C2	Reversed phase	Silica	50	60	500	Ethyl	5.6%	Yes
PH	Reversed phase	Silica	50	60	500	Phenyl	10%	Yes
CN	Normal / reversed phase	Silica	50	60	500	Cyanopropyl	8%	Yes
SCX	Strong cation exchange	Silica	50	60	500	Benzenesulfonic acid	10.9%	No
SAX	Strong anion exchange	Silica	50	60	500	Trimethylaminopropyl	8%	No
Silica	Normal phase	Silica	50	60	500	Silanol	-	No
NH ₂	Normal phase / weak anion exchange	Silica	50	60	500	Aminopropyl	5.5%	No
PSA	Normal phase / weak anion exchange	Silica	50	60	500	Ethylenediamino-N-propyl	8.5%	No
AL-A	Normal phase	Acidic alumina	125	-	200	Acidic alumina	-	-
AL-B	Normal phase	Basic alumina	125	-	200	Basic alumina	-	-
AL-N	Normal phase	Neutral alumina	125	-	200	Neutral alumina	-	-
Florisil	Normal phase	Magnesium	150 - 200	-	-	-	-	-
CARB	Nonbonded carbon phase	Carbon	120 - 400	-	100	-	-	-

Silica-based Sorbent	Reversed phase	Normal Phase	Weak Ion Exchange	Strong Ion Exchange
	C18 C18-U C8 C2 PH	Silica CN (can also be used as reversed phase)	NH ₂ PSA	SCX SAX
Polymer-based Sorbent	Universal Phase	Mix Mode*	Mix Mode**	
	PLS	PXC PXA	PWC PWA	
Other	Inorganic Material		Double Layer Sorbent	
	Al ₂ O ₃ (Acidic) Al ₂ O ₃ (Neutral) Al ₂ O ₃ (Basic) Florisil (Magnesium silicate) CARB (Graphitized carbon black) Na ₂ SO ₄		CARB / NH ₂ CARB / PSA SAX / PSA	

*Reversed phase and strong ion exchange

**Reversed phase and weak ion exchange

Brand Cross Reference

Dikma	Waters	Agilent	Supelco
ProElut™ PLS	Oasis HLB	Plexa	-
ProElut™ PXC	Oasis MCX	Plexa PCX	-
ProElut™ PXA	Oasis MAX	-	-
ProElut™ PWC	Oasis WCX	-	-
ProElut™ PWA	Oasis WAX	-	-
ProElut™ C18	Sep-pak C18	BondElut C18	ENVI-18, LC-18
ProElut™ C18-U	-	BondElut C18-OH	-
ProElut™ C8	Sep-pak C8	BondElut C8	-
ProElut™ C2	-	BondElut C2	-
ProElut™ PH	-	BondElut PH	LC-PH
ProElut™ CN	Sep-pak CN	BondElut CN	LC-CN
ProElut™ NH ₂	Sep-pak NH ₂	BondElut NH ₂	LC-NH ₂
ProElut™ PSA	-	BondElut PSA	-
ProElut™ Silica	Sep-pak Silica	BondElut Silica	LC-Silica
ProElut™ SCX	-	BondElut SCX	LC-SCX
ProElut™ SAX	-	BondElut SAX	LC-SAX

Technical Reference

A. Typical elution sequence of PLS, PXC, PXA, PWA and PWC

ProElut™ PLS (60 mg / 3 mL)

Suggested Method	Purpose
Condition / equilibrate 3 mL MeOH / 3 mL H ₂ O	Ready for use
Load sample solution 3 mL	The compounds of interest will be adsorbed by the sorbent
Wash 3 mL H ₂ O (5% MeOH)	To remove aqueous soluble materials and disruptors
Elution 3 mL MeOH	To get compounds of interest that previously adsorbed on the sorbent by non-polar interaction
Evaporate and reconstitute	For HPLC or GC analysis

ProElut™ PXC (60 mg / 3 mL)

Suggested Method	Purpose
Condition / equilibrate 3 mL MeOH / 3 mL H ₂ O	Ready for use
Load acidified sample solution 3 mL	Protonated basic compounds (under low pH) will approach sulfonic group by Coulomb force The neutral and acidic compounds will be adsorbed on the sorbent by non-polar interaction
Wash 1 3 mL 0.1 M HCl	To remove aqueous soluble materials and disruptors
Wash 2 3 mL MeOH	To remove compounds that adsorbed on the sorbent by non-polar interaction
Elution 3 mL MeOH (5% NH ₄ OH)	Neutralize the basic compounds that adsorbed on the sorbent by Coulomb force and carry them out
Evaporate and reconstitute	For HPLC or GC analysis

ProElut™ PXA (60 mg / 3 mL)

Suggested Method	Purpose
Condition / equilibrate 3 mL MeOH / 3 mL H ₂ O	Ready for use
Load sample solution 3 mL	Negative charged acidic compounds will approach quaternary amino group by Coulomb force The neutral and acidic compounds will be adsorbed on the sorbent by non-polar interaction
Wash 1 3 mL 5% NH ₄ OH	To remove aqueous soluble materials and disruptors, including salts and proteins The interaction between acid compounds and the quaternary amino group is reinforced
Wash 2 3 mL MeOH	To remove compounds that adsorbed on the sorbent by non-polar interaction
Elution 3 mL MeOH (2% HCOOH)	Neutralize the acidic compounds that adsorbed on the sorbent by Coulomb force and carry them out
Evaporate and reconstitute	For HPLC or GC analysis

ProElut™ SPE

ProElut™ PWC (60 mg / 3 mL)

Suggested Method	Purpose
Condition / equilibrate 3 mL MeOH / 3 mL 5% NH ₄ OH	Ready for use Add ammonia to make the carboxyl functional group negatively charged
Load sample solution 3 mL	Protonated strong basic compounds will approach carboxyl group by Coulomb force The neutral and weak- / mid- basic compounds will be absorbed on the sorbent by non-polar interaction
Wash 1 3 mL 5% NH ₄ OH	To remove aqueous soluble materials and disruptors, including salts and proteins The interaction between strong basic compounds and the carboxyl group is reinforced
Wash 2 3 mL MeOH	To remove compounds that adsorbed on the sorbent by non-polar interaction
Elution 3 mL MeOH (2% HCOOH)	To neutralize the carboxyl (negatively charged) so that the Coulomb force between analyte and functional group is cut off and therefore the strong basic compounds will be carried away by methanol
Evaporate and reconstitute	For HPLC or GC analysis

ProElut™ PWA (60 mg / 3 mL)

Suggested Method	Purpose
Condition / equilibrate 3 mL MeOH / 3 mL 2% HCOOH	Ready for use Add formic acid to make the piperazine functional group protonated
Load sample solution 3 mL	Negatively charged strong acidic compounds will approach sorbent functional group by Coulomb force The neutral and weak- / mid- basic compounds will be absorbed on the sorbent by non-polar interaction
Wash 1 3 mL 2% HCOOH	To remove aqueous soluble materials and disruptors, including salts and proteins The interaction between strong acidic compounds and the piperazine group is reinforced
Wash 2 3 mL MeOH	To remove compounds that adsorbed on the sorbent by non-polar interaction
Elution 3 mL MeOH (5% NH ₄ OH)	To neutralize the protonated functional group so that the Coulomb force between analyte and functional group is cut off and therefore the strong acidic compounds will be carried away by methanol
Evaporate and reconstitute	For HPLC or GC analysis

B. ProElut™ SPE Sorbents Weight Based on Sample Size

Bed Weight (mg)	Bed Capacity (mg)*	Minimum Elution Volume (μL)
50	2.5	125
100	5	250
150	7.5	375
200	10	500
500	25	1250
1000	50	2500

*This value depends on the analyte and sample matrix. As a rule of thumb, the bed capacity can be estimated with ~5% of the bed weight.

ProElut™ SPE Sorbents

Silica-based Sorbents

ProElut™ C18

ProElut™ C18 is the most broadly used SPE cartridge. It can be used to adsorb non-polar, slightly polar and mid-polar compounds. Polar materials such as salt cannot be retained on the sorbent, which makes ProElut™ C18 an excellent choice for desalting samples. In addition, non-polar and slightly polar disruptors in matrix such as fats, PAHs and phthalates can be retained by the sorbent, leaving ionic analytes eluted in the collector for reconstitution.

Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---C}_{18}\text{H}_{37} \\ \\ \text{CH}_3 \end{array}$
Endcapping	Yes
Carbon loading	19%
Retention mechanism	Reversed phase
Application	For reversed phase extraction of non-polar to moderately polar compounds, such as antibiotics, barbiturates, benzodiazepines, caffeine, drugs, dyes, essential oils, fat-soluble vitamins, fungicides, herbicides, pesticides, hydrocarbons, parabens, phenols, phthalate esters, steroids, surfactants, theophylline and water-soluble vitamins

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ C18 SPE Tubes				
50 mg	1 mL	100	63101	\$125
100 mg	1 mL	100	63102	125
200 mg	3 mL	50	63103	95
500 mg	3 mL	50	63104	115
500 mg	6 mL	30	63105	80
1 g	6 mL	30	63106	105
2 g	12 mL	20	63107	120
5 g	20 mL	20	63108	190
10 g	60 mL	10	63109	260
ProElut™ C18 Bulk Sorbents				
10 g		1	63181	Inquire
100 g		1	63182	Inquire
1 kg		1	63183	Inquire

ProElut™ C18-U

ProElut™ C18-U has a non-encapped octadecyl bonded phase that enables the silanols on the silica surface to be more active. However, the well-controlled silanol activity exhibits excellent selectivity towards polar compounds, especially amines such as tetracyclines.

Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å, Specific Surface Area: 500 m ² /g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---C}_{18}\text{H}_{37} \\ \\ \text{CH}_3 \\ \\ \text{---Si---OH} \\ \end{array}$
Endcapping	No
Carbon loading	17%
Retention mechanism	Reversed phase
Application	Similar to ProElut™ C18, but with enhanced retention for polar compounds

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ C18-U SPE Tubes				
50 mg	1 mL	100	63501	\$125
100 mg	1 mL	100	63502	125
200 mg	3 mL	50	63503	95
500 mg	3 mL	50	63504	115
500 mg	6 mL	30	63505	80
1 g	6 mL	30	63506	105
2 g	12 mL	20	63507	120
5 g	20 mL	20	63508	190
10 g	60 mL	10	63509	260
ProElut™ C18-U Bulk Sorbents				
10 g		1	63581	Inquire
100 g		1	63582	Inquire
1 kg		1	63583	Inquire

ProElut™ SPE

ProElut™ C8

ProElut™ C8 is very similar to the C18 phase, but has a shorter chain. This makes the phase less non-polar than C18, leaving non-polar compounds less retained by the sorbents. In this case, those compounds retained too strongly on the C18 can be effectively eluted if you choose the C8 phase. In addition, the C8 phase for polar interaction is somewhat higher than C18 because there is less coverage of the silica surface. However, this polar interaction is not the main characteristic of C8 phase.

Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---C}_8\text{H}_{17} \\ \\ \text{CH}_3 \end{array}$
Endcapping	Yes
Carbon loading	11%
Retention mechanism	Reversed phase
Application	For reversed phase extraction of non-polar to moderately polar compounds, such as antibiotics, barbiturates, benzodiazepines, caffeine, drugs, dyes, essential oils, fat-soluble vitamins, fungicides, herbicides, pesticides, hydrocarbons, parabens, phenols, phthalate esters, steroids, surfactants, theophylline, and water-soluble vitamins

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ C8 SPE Tubes				
100 mg	1 mL	100	63702	\$125
200 mg	3 mL	50	63703	95
500 mg	3 mL	50	63704	115
500 mg	6 mL	30	63705	80
1 g	6 mL	30	63706	105
2 g	12 mL	20	63707	120
5 g	20 mL	20	63708	190
10 g	60 mL	10	63709	260
ProElut™ C8 Bulk Sorbents				
10 g		1	63781	Inquire
100 g		1	63782	Inquire
1 kg		1	63783	Inquire

ProElut™ C2

ProElut™ C2 has the shortest carbon chain among non-polar silica-based phases. It provides the least retentive ability for non-polar compounds and somewhat higher polar interaction than C8 and C18 phases. The polarity of C2 is slightly lower than a cyano phase for polar interactions.


Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---C}_2\text{H}_5 \\ \\ \text{CH}_3 \end{array}$
Endcapping	Yes
Carbon loading	5.6%
Retention mechanism	Reversed phase
Application	Plasma, urine, aqueous samples

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ C2 SPE Tubes				
100 mg	1 mL	100	65602	\$125
500 mg	3 mL	50	65604	115
1 g	6 mL	30	65606	105
2 g	12 mL	20	65607	120
5 g	20 mL	20	65608	190
10 g	60 mL	10	65609	260
ProElut™ C2 Bulk Sorbents				
10 g		1	65681	Inquire
100 g		1	65682	Inquire
1 kg		1	65683	Inquire

ProElut™ PH

ProElut™ PH has a similar polarity as that of C8 phase. However, it shows different selectivity to other non-polar phases due to the presence of conjugated double bonds. In addition, the planar shape of benzene and its electron distribution make it much more retentive to aromatic compounds.


Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	
Endcapping	Yes
Carbon loading	10%
Retention mechanism	Reversed phase
Application	Volatiles in water: PAHs, PAEs, PCBs, pesticides, herbicides, phenols Biological fluids: blood, urine

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PH SPE Tubes				
100 mg	1 mL	100	63902	\$125
500 mg	3 mL	50	63904	115
1 g	6 mL	30	63906	105
2 g	12 mL	20	63907	120
5 g	20 mL	20	63908	190
10 g	60 mL	10	63909	260
ProElut™ PH Bulk Sorbents				
10 g		1	63981	Inquire
100 g		1	63982	Inquire
1 kg		1	63983	Inquire

ProElut™ CN

ProElut™ CN is a mid-polar phase SPE column. We recommend using it to extract samples for which analytes are irreversibly retained on C8 and C18 phases.


Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	
Endcapping	Yes
Carbon loading	8%
Retention mechanism	Reversed phase or normal phase
Application	Pesticides in water, metabolites

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ CN SPE Tubes				
100 mg	1 mL	100	63802	\$125
500 mg	3 mL	50	63804	115
1 g	6 mL	30	63806	105
2 g	12 mL	20	63807	120
5 g	20 mL	20	63808	190
10 g	60 mL	10	63809	260
ProElut™ CN Bulk Sorbents				
10 g		1	63881	Inquire
100 g		1	63882	Inquire
1 kg		1	63883	Inquire

ProElut™ Silica

ProElut™ Silica is the most polar SPE sorbent. It is very effective for separating compounds with similar structures and extracting polar compounds in non-polar solvents. In addition, the silica surface silanols have slight anion exchange properties that can be used to remove organic acids and phenols in extracts.

Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	
Endcapping	No
Carbon loading	-
Retention mechanism	Normal phase or weak anion exchange
Application	Extract polar compounds from non-polar matrix Remove polar hydrocarbons, organic acids, and phenols in extracts. Separate compounds with very similar structures (isomers)

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ Silica SPE Tubes				
100 mg	1 mL	100	63002	\$125
500 mg	3 mL	50	63004	115
1 g	6 mL	30	63006	105
ProElut™ Silica Bulk Sorbents				
10 g		1	63081	Inquire
100 g		1	63082	Inquire
1 kg		1	63083	Inquire

ProElut™ SPE

ProElut™ NH₂

ProElut™ NH₂ has both polar and weak anion exchange interactions. It can effectively absorb compounds with a polar functional group (-OH, -NH₂, -SH, etc.) by hydrogen bonding from non-polar solvents such as hexane. In addition, it has weaker anion exchange property than SAX (a quaternary amine sorbent that is always charged) and is therefore an excellent choice for retention of very strong anions that are always irreversibly adsorbed on a SAX sorbent, such as sulfonic acid.

Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---}(\text{CH}_2)_3\text{NH}_2 \\ \\ \text{CH}_3 \end{array}$
Endcapping	No
Carbon loading	5.5%
Retention mechanism	Normal phase or anion exchange
Application	Extract polar compounds from non-polar matrix Remove polar hydrocarbons, organic acids, and phenols in extracts Separate compounds with very similar structures (isomers)

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ NH₂ SPE Tubes				
100 mg	1 mL	100	63302	\$125
200 mg	3 mL	50	63303	95
500 mg	3 mL	50	63304	115
500 mg	6 mL	30	63305	80
1 g	6 mL	30	63306	105
2 g	12 mL	20	63307	120
5 g	20 mL	20	63308	190
10 g	60 mL	10	63361	260
ProElut™ NH₂ Bulk Sorbents				
10 g		1	63381	Inquire
100 g		1	63382	Inquire
1 kg		1	63383	Inquire

ProElut™ PSA

ProElut™ PSA sorbent contains two different amino groups, one primary and one secondary. It gives comparatively higher pK_a and ionic capacity relative to ProElut™ NH₂. The PSA sorbent is an excellent choice for extracting polar compounds from non-polar solvents. The compounds that are retained too strongly on a NH₂ sorbent can be effectively eluted on a PSA sorbent. In addition, the PSA functional group is a very effective bidentate ligand in chelation applications.

Base material	Spherical silica, Particle Size: 50 μm, Pore Size: 60 Å Specific Surface Area: 500 m ² /g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---}(\text{CH}_2)_3\text{NH}(\text{CH}_2)_2\text{NH}_2 \\ \\ \text{CH}_3 \end{array}$
Endcapping	No
Carbon loading	8.5%
Retention mechanism	Normal phase or weak anion exchange
Application	Extract polar compounds from non-polar matrix Remove polar hydrocarbons, organic acids, and phenols in extracts Separate compounds with very similar structures (isomers)

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PSA SPE Tubes				
100 mg	1 mL	100	63202	\$150
200 mg	3 mL	50	63203	115
500 mg	3 mL	50	63204	140
500 mg	6 mL	30	63205	115
1 g	6 mL	30	63206	160
2 g	12 mL	20	63207	188
5 g	20 mL	20	63208	223
10 g	60 mL	10	63209	307
ProElut™ PSA Bulk Sorbents				
10 g		1	63281	Inquire
100 g		1	63282	Inquire
1 kg		1	63283	Inquire

ProElut™ SCX

ProElut™ SCX sorbent has benzenesulfonic acid as a bonded functional group with a very low pK_a . The presence of the benzene ring in the functional group increases its potential for non-polar interaction. The two properties are quite useful in the absorption of cationic organic compounds from aqueous systems where non-polar compounds are seen.

Base material	Spherical silica, Particle Size: 50 μm , Pore Size: 60 \AA Specific Surface Area: 500 m^2/g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---}(\text{CH}_2)_3\text{C}_6\text{H}_4\text{SO}_3^-\text{H}^+ \\ \\ \text{CH}_3 \end{array}$
Endcapping	No
Carbon loading	10.9%
Retention mechanism	Strong cation exchange
Application	Basic compounds in aqueous solution

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ SCX SPE Tubes				
100 mg	1 mL	100	63602	\$150
500 mg	3 mL	50	63604	140
500 mg	6 mL	30	63606	115
2 g	12 mL	20	63607	147
5 g	20 mL	20	63608	211
10 g	60 mL	10	63609	271
ProElut™ SCX Bulk Sorbents				
10 g		1	63681	Inquire
100 g		1	63682	Inquire
1 kg		1	63683	Inquire

ProElut™ SAX

ProElut™ SAX sorbent has trimethylaminopropyl as a bonded functional group with a very high pK_a . The presence of the benzene ring in the functional group increases its potential for non-polar interaction. The two properties are quite useful in the absorption of anionic organic compounds from aqueous systems where non-polar compounds are seen.

Base material	Spherical silica, Particle Size: 50 μm , Pore Size: 60 \AA Specific Surface Area: 500 m^2/g
Functional group	$\begin{array}{c} \text{CH}_3 \\ \\ \text{---Si---}(\text{CH}_2)_3\text{N}^+(\text{CH}_3)_3 \\ \\ \text{CH}_3 \end{array} \text{Cl}^-$
Endcapping	No
Carbon loading	8%
Retention mechanism	Strong anion exchange
Application	Carboxylic acids in aqueous solution

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ SAX SPE Tubes				
100 mg	1 mL	100	63402	\$150
500 mg	3 mL	50	63404	140
500 mg	6 mL	30	63406	115
2 g	12 mL	20	63407	147
5 g	20 mL	20	63408	211
10 g	60 mL	10	63409	271
ProElut™ SAX Bulk Sorbents				
10 g		1	63481	Inquire
100 g		1	63482	Inquire
1 kg		1	63483	Inquire

ProElut™ SPE

Polymer-based Sorbents

ProElut™ PLS-Hydrophilic-Lipophilic-Balance Copolymer, Reversed Phase Sorbent

ProElut™ PLS is a hydrophilic polystyrene / divinylbenzene copolymer sorbent, designed to expand the SPE application fields and improve extraction efficiency. This sorbent contains the lipophilic divinylbenzene and the hydrophilic pyrrolidone. The hydrophilic-lipophilic balance is a reversed phase sorbent maintaining retention for non-polar and polar analytes. Compared to traditional silica-based reversed phase sorbent (C18), ProElut™ PLS features are as follows:

(1) Real Versatility

- High retention of hydrophilic compounds and lipophilic compounds
- Applications covering the non-polar, weakly polar, and polar compounds to overcome the C18 sorbent poor retention of polar compounds

(2) Higher Stability

- PLS is water-wettable
- Maintaining high retention and capacity after activation even if the SPE cartridge runs dry

(3) Wider pH Range

PLS is a polymer sorbent that can be used in the range of pH 0 - 14 while the silica-based sorbents can only be used in the range of pH 2 - 7.5.


(4) Higher Capacity

The PLS sorbent has greater capacity for more compounds. It reduces breakthrough potential and improves reproducibility.

(5) No Secondary Interaction


The residue silanols of silica-based sorbents can adsorb basic analytes resulting in low recovery. PLS is a polymer sorbent and there is no silanol activity leading to high recovery.

Structure of ProElut™ Polymer-based Sorbents

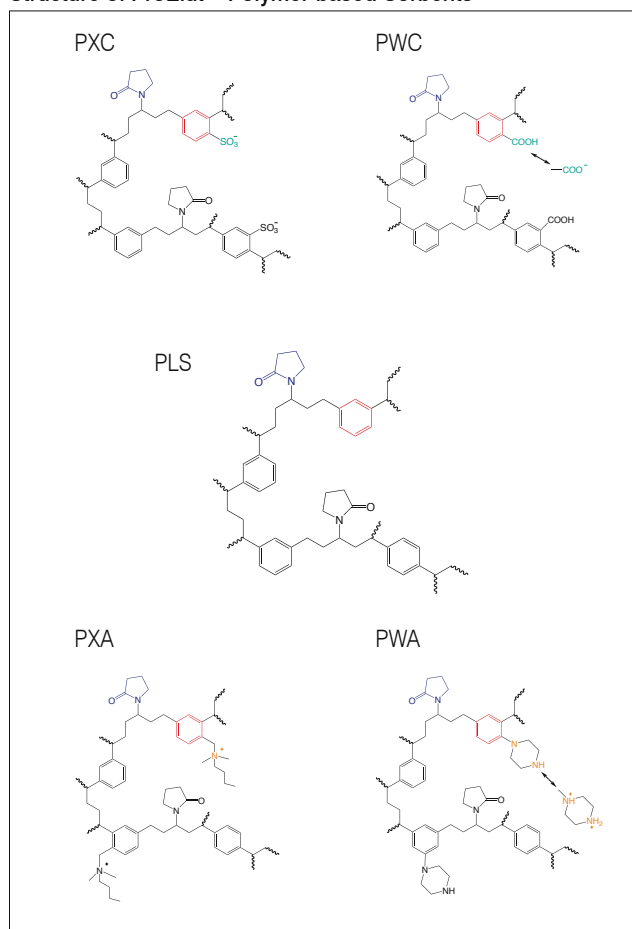

ProElut™ PLS

ProElut™ PLS is a highly cross-linked polystyrene-divinylbenzene (PS-DVB) copolymer with high surface area (800 m²/g) and high capacity. It is an excellent choice for extraction of polar analytes in aqueous solvents where traditional C18 and C8 sorbents are not advisable because they are not "wetttable". It is ideal in screening applications where a broad range of analytes can be extracted.


Base material	Porous, highly cross-linked, spherical PS-DVB, Particle Size: 50 μm, Pore Size: 80 Å, Specific Surface Area: 800 m ² /g
Functional group (Pyrrolidinone)	
Retention mechanism	Non-polar and polar interactions
Application	Pharmaceutical residues in animal tissue, such as tetracyclines, chloromycetin, sulfonamides, abamectin, macrolide antibiotics, nitrofurans, and pesticides in vegetables Environmental samples, such as PAHs, PAEs, phenols, and endocrine disruptors Biological samples, pharmaceuticals, and metabolites in plasma, serum, or urine

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PLS SPE Tubes				
30 mg	1 mL	100	68002	\$159
60 mg	1 mL	100	68011	184
60 mg	3 mL	50	68003	221
150 mg	6 mL	30	68004	136
200 mg	6 mL	30	68012	155
500 mg	6 mL	30	68005	195
500 mg	12 mL	20	68007	156
1 g	20 mL	20	68008	242
6 g	60 mL	10	68009	491

ProElut™ PXC

ProElut™ PXC is a highly cross-linked PS-DVB copolymer with sulfonic acid as the functional group. It has both non-polar and cation exchange interactions and is therefore an excellent choice for extraction of basic organic compounds.


Base material	Porous, highly cross-linked, spherical PS-DVB, Particle Size: 50 μm, Pore Size: 80 Å, Specific Surface Area: 800 m ² /g
Functional group (Sulfonic acid)	
Retention mechanism	Non-polar interaction and cation exchange
Application	Basic compounds, such as sulfonamides and clenbuterol Biological samples, pharmaceuticals, and metabolites in plasma, serum, or urine

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PXC SPE Tubes				
30 mg	1 mL	100	68202	\$143
60 mg	3 mL	50	68203	198
150 mg	6 mL	30	68204	122
200 mg	6 mL	30	68212	139
500 mg	12 mL	20	68207	140
1 g	20 mL	20	68208	218
6 g	60 mL	10	68209	442

ProElut™ PXA

ProElut™ PXA is a highly cross-linked PS-DVB copolymer with a quaternary amino as the functional group. It has both non-polar and anion exchange interactions and is therefore an excellent choice for extraction of acidic organic compounds, especially those containing carboxyl and phenolic hydroxyl.

Base material	Porous, highly cross-linked, spherical PS-DVB, Particle Size: 50 μm, Pore Size: 80 Å, Specific Surface Area: 800 m ² /g
Functional group (Quaternary amino)	
Retention mechanism	Non-polar interaction and anion exchange
Application	Compounds with groups as carboxyl and phenolic hydroxyl


Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PXA SPE Tubes				
30 mg	1 mL	100	68302	\$159
60 mg	3 mL	50	68303	221
150 mg	6 mL	30	68304	136
500 mg	12 mL	20	68307	156
1 g	20 mL	20	68308	242
6 g	60 mL	10	68309	491

ProElut™ SPE

ProElut™ PWC

ProElut™ PWC is a highly cross-linked PS-DVB copolymer with carboxyl as the functional group. It has both non-polar and weak cation exchange interactions and is therefore an excellent choice for extraction of strong basic compounds.


Base material	Porous, highly cross-linked, spherical PS-DVB, Particle Size: 50 μm , Pore Size: 80 \AA , Specific Surface Area: 800 m^2/g
Functional group (Carboxyl)	
Retention mechanism	Non-polar interaction and weak cation exchange
Application	Strong basic compounds, quaternary ammonium salts

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PWC SPE Tubes				
30 mg	1 mL	100	65711	\$159
60 mg	3 mL	50	65712	221
150 mg	6 mL	30	65713	136

ProElut™ PWA

ProElut™ PWA is a highly cross-linked PS-DVB copolymer with piperazine as the functional group. It has both non-polar and weak anion exchange interactions and is therefore an excellent choice for extraction of strong acidic compounds.

Base material	Porous, highly cross-linked, spherical PS-DVB, Particle Size: 50 μm , Pore Size: 80 \AA , Specific Surface Area: 800 m^2/g
Functional group (Piperazine)	
Retention mechanism	Non-polar interaction and weak anion exchange
Application	For purification of strong acidic compounds

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PWA SPE Tubes				
30 mg	1 mL	100	65811	\$159
60 mg	3 mL	50	65812	221
150 mg	6 mL	30	65813	136

Specific Sorbents

ProElut™ Florisil

Florisil is a highly selective adsorbent that has extensive utility in sample preparation, preparative and analytical chromatography. This sorbent is unique because it is comprised of extremely white, hard-powdered synthetic magnesium-silica gel.

Base material	Magnesium silicate, Particle Size: 150 - 200 μm
Functional group	MgSiO ₃
Retention mechanism	Polar interaction
Application	For extraction of drugs, dyes, herbicides, pesticides, nitrogen compounds, organic acids, phenols, steroids, PCBs, and PAHs

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ Florisil SPE Tubes				
100 mg	1 mL	100	65002	\$125
500 mg	3 mL	50	65004	115
500 mg	6 mL	30	65005	80
1 g	6 mL	30	65006	105
2 g	12 mL	20	65007	120
5 g	20 mL	20	65008	190
10 g	60 mL	10	65009	260
ProElut™ Florisil Bulk Sorbents				
10 g		1	65081	Inquire
100 g		1	65082	Inquire
1 kg		1	65083	Inquire

ProElut™ AL-A

Base material	Al ₂ O ₃ (Acidic), Particle Size: 125 μm
pH	4.5
Retention mechanism	Lewis acid, polar, and ion exchange interactions
Application	Polar and anionic compounds

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ AL-A SPE Tubes				
100 mg	1 mL	100	65102	\$125
500 mg	3 mL	50	65104	115
1 g	6 mL	30	65106	105
2 g	12 mL	20	65107	120
5 g	20 mL	20	65108	190
10 g	60 mL	10	65109	260
ProElut™ AL-A Bulk Sorbents				
10 g		1	65181	Inquire
100 g		1	65182	Inquire
1 kg		1	65183	Inquire

ProElut™ CARB

Base material	Graphitized carbon black, Particle Size: 120 - 400 μm
Application	In agriculture residues analysis, used to remove pigments in fruits and vegetables For purification of samples such as groundwater, fruits, and vegetables

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ CARB SPE Tubes				
250 mg	3 mL	50	65403	\$200
500 mg	6 mL	30	65405	210

ProElut™ AL-N

Base material	Al ₂ O ₃ (Neutral), Particle Size: 125 μm
pH	7.5
Retention mechanism	Lewis acid, polar, and ion exchange interactions
Application	Extract polar compounds from non-polar matrix Remove polar hydrocarbons, organic acids, and phenols in extracts. Separate compounds with very similar structures (isomers)

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ AL-N SPE Tubes				
100 mg	1 mL	100	65302	\$125
500 mg	3 mL	50	65304	115
1 g	6 mL	30	65306	105
2 g	12 mL	20	65307	120
5 g	20 mL	20	65308	190
10 g	60 mL	10	65309	260
ProElut™ AL-N Bulk Sorbents				
10 g		1	65381	Inquire
100 g		1	65382	Inquire
1 kg		1	65383	Inquire

ProElut™ AL-B

Base material	Al ₂ O ₃ (Basic), Particle Size: 125 μm
pH	10.0
Retention mechanism	Lewis acid, polar, and ion exchange interactions
Application	Polar and anionic compounds, amines

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ AL-B SPE Tubes				
100 mg	1 mL	100	65202	\$125
500 mg	3 mL	50	65204	115
1 g	6 mL	30	65206	105
2 g	12 mL	20	65207	120
5 g	20 mL	20	65208	190
10 g	60 mL	10	65209	260
ProElut™ AL-B Bulk Sorbents				
10 g		1	65281	Inquire
100 g		1	65282	Inquire
1 kg		1	65283	Inquire

ProElut™ CARB / NH₂

Base material	Packing of equivalent volume of CARB and amine (NH ₂)
Application	Widely used in analysis of pesticide residues (many different varieties) in foods To remove pigments, fatty acids, and phenols from analytes

Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ CARB / NH₂ SPE Tubes				
500 mg / 500 mg	6 mL	30	64105	\$240

ProElut™ SPE

ProElut™ GLASS SPE Tube

ProElut™ glass cartridges are designed for high-purity extraction as the inert glass body completely eliminates the pollution from plasticizers, such as phthalates. ProElut™ glass SPE tubes are standard size, with high quality sorbent and special purification frits, to assure stability and reproducibility.


Ordering Information

Mass	Volume	Qty	Cat. No.	Price
ProElut™ PLS GLASS SPE Tubes				
200 mg	6 mL	30	68012G	\$189
500 mg	6 mL	30	68005G	397
ProElut™ C18 GLASS SPE Tubes				
500 mg	6 mL	30	63105G	228
1 g	6 mL	30	63106G	302
ProElut™ Florisil GLASS SPE Tubes				
500 mg	6 mL	30	65005G	271
1 g	6 mL	30	65006G	302
ProElut™ PSA GLASS SPE Tubes				
500 mg	6 mL	30	63205G	200
1 g	6 mL	30	63206G	270
ProElut™ Silica GLASS SPE Tubes				
500 mg	6 mL	30	63005G	198
1 g	6 mL	30	63006G	254



ProElut™ QuEChERS Kits

In 2003, USDA scientists developed a groundbreaking sample preparation method for multi-pesticide residue analysis in a wide variety of food and agricultural products. The QuEChERS (pronounced "catchers") procedure entails a number of simple processing steps and is thus fast and easy to perform with little susceptibility to errors. QuEChERS provides high recoveries for a very broad scope of pesticides belonging to various chemical classes and delivers the final extract in acetonitrile, thereby giving full flexibility in the choice of the determinative analysis technique. Direct connection with liquid and gas chromatography is possible.

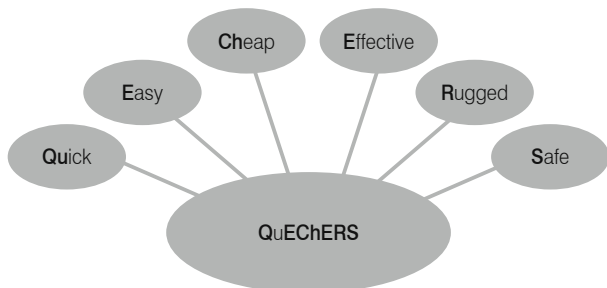

ProElut™ QuEChERS is an innovative sample preparation method for multi-pesticide residue analysis, standing for **Quick, Easy, Cheap, Effective, Rugged and Safe**. Now, QuEChERS has become a standard approach for the determination of pesticide residues in fruits and vegetables across the world. In addition, different fields have started to use this method. Application is developed in a number of different areas, such as meat, blood, wine, and even the antibiotics in soil, drugs, drug abuse, and other contaminants detected. Dikma ProElut™ QuEChERS kits contain extraction and clean-up kits which support AOAC Method 2007.01 and EN Method 15662.

Features of ProElut™ QuEChERS Kits

- Fast, simple sample preparation for multi-residue pesticide analysis
- Wide selection, support AOAC 2007.01 and EN 15662 methods
- Provide guidance to help you choose the right products
- Certified extraction salts and sorbents
- Individually sealed packages for enhanced protection and storage stability



Sample Preparation





ProElut™ QuEChERS

ProElut™ QuEChERS versus Traditional SPE

The ProElut™ QuEChERS method has almost the same analysis results as traditional SPE, with fewer analytical steps, lower solvent consumption, greater accuracy, wider applicability, and higher sample throughput.

	Traditional SPE	ProElut™ QuEChERS
Time to process 6 samples (min)	100 - 120	< 25
Solvent used (mL)	60 - 90	< 15
Steps	Complex	Simple
Evaporation	Yes	No
Glassware used	Yes	No
Apparatus used	More	Less
Application	Wide	Narrow
Recovery	High	Low (Part of compounds)

ProElut™ QuEChERS Steps

Step 1 Extraction		Step 2 Clean-up	
			
Weigh 10 g sample, add 10 mL acetonitrile, internal standard and shake for 1 min	Add extraction salts (buffer + Na ₂ SO ₄) to extraction sample and centrifuge for 5 min	Transfer supernatant to clean-up tube, shake for 30 sec and centrifuge for 5 min	Transfer cleaned extract to autosampler vial for analysis

Recommended Standard Operation Procedure for ProElut™ QuEChERS Kits

Original QuEChERS

Extraction

1. Add 10 mL MeCN to 10 g sample
2. Add internal standard
3. Add 4 g MgSO₄ and 1 g NaCl
4. Shake vigorously for 1 min
5. Centrifuge for 5 min

Dispersive SPE clean-up

6. Remove 1 mL of the upper layer
7. Add 25 mg PSA and 150 mg MgSO₄ to the 1 mL removed
8. Mix for 30 sec and centrifuge for 1 min

AOAC 2007.01

Extraction

1. Add 15 mL 1% HOAc in MeCN to 15 g of sample
2. Add internal standard
3. Add 6 g MgSO₄ and 1.5 g NaOAc
4. Shake vigorously for 1 min
5. Centrifuge for 5 min

Dispersive SPE clean-up

6. Remove 1 mL of the upper layer
7. Add 25 mg PSA and 150 mg MgSO₄ to the 1 mL removed
8. Mix for 30 sec and centrifuge for 1 min

EN 15662

Extraction

1. Add 10 mL MeCN to 10 g of sample
2. Add internal standard
3. Add 4 g MgSO₄ + 1 g NaCl + 1 g Na₃Citr·2H₂O + 0.5 g Na₃Citr·2H₂O (+ 0.6 mL 5 N NaOH for lemons, limes, etc.)
4. Shake vigorously for 1 min
5. Centrifuge for 5 min

Dispersive SPE clean-up

6. Remove 1 mL of the upper layer
7. Add 25 mg PSA and 150 mg MgSO₄ (add 2.5 or 7.5 mg GCB for matrices with a high content of carotenoids and chlorophyll)
8. Mix for 30 sec and centrifuge for 1 min





ProElut™ QuEChERS Kits Selection Guide

Step 1: Selected Extraction Salts Kit

Generally, we add solvent and buffer salts to the pulverized fruit or vegetable sample to extract the pesticides of interest into the organic layer. However, adding a food sample with a high percentage of water directly to the salts may create an exothermic reaction that can affect your analyte recoveries. With the separate packaging of ProElut™ QuEChERS extraction salts (pre-weighed, water free), you can add buffered extraction salt after adding solvent.

Method	Material	Qty	Cat. No.	Price
AOAC 2007.01	6 g MgSO ₄ , 1.5 g NaOAc with 50 mL Centrifuge Tube	50/pk	64520	\$168
EN 15662	4 g MgSO ₄ , 1 g NaCl, 1 g TSCD, 0.5 g DHS with 50 mL Centrifuge Tube	50/pk	64521	178

Step 2 : Selected Dispersive SPE Kit

	Sample Type	Method	2 mL Clean-up Tube	Price	15 mL Clean-up Tube	Price
	General fruits and vegetables Major interferences: organic acids, carbohydrates, phenols	AOAC	50 mg PSA 150 mg MgSO ₄ Cat#64501	\$123	400 mg PSA 1200 mg MgSO ₄ Cat#64502	\$118
		EN	25 mg PSA 150 mg MgSO ₄ Cat#64503	118	150 mg PSA 900 mg MgSO ₄ Cat#64504	113
	Fruits and vegetables with fats and waxes Major interferences: lipids, sterols, organic acids, carbohydrates, phenols	AOAC	50 mg PSA 50 mg C18 150 mg MgSO ₄ Cat#64505	128	400 mg PSA 400 mg C18 1200 mg MgSO ₄ Cat#64506	128
		EN	25 mg PSA 25 mg C18 150 mg MgSO ₄ Cat#64507	123	150 mg PSA 150 mg C18 900 mg MgSO ₄ Cat#64508	118
	Highly pigmented fruits and vegetables Major interferences: chlorophyll, carotenoids, organic acids, carbohydrates, phenols. Not for use with planar pesticides	AOAC	50 mg PSA 50 mg Carb 150 mg MgSO ₄ Cat#64509	172	400 mg PSA 400 mg Carb 1200 mg MgSO ₄ Cat#64510	215
		EN	25 mg PSA 7.5 mg Carb 150 mg MgSO ₄ Cat#64511	158	150 mg PSA 45 mg Carb 900 mg MgSO ₄ Cat#64512	143
	Fruits and vegetables with pigments and fats Major interferences: chlorophyll, carotenoids, lipids, organic acids, carbohydrates, phenols. Not for use with planar pesticides	AOAC	50 mg PSA 50 mg C18 50 mg Carb 150 mg MgSO ₄ Cat#64513	192	400 mg PSA 400 mg C18 400 mg Carb 1200 mg MgSO ₄ Cat#64514	238

Note: Sorbent listed in the table has been pre-weighed and placed in centrifuge tube

--PSA: Primary-secondary amine silica bonded sorbent

--C18: Octadecyl silica bonded sorbent

--Carb: Graphitized carbon black.

Tips: For different matrix food samples, we recommend an added amount of PSA and MgSO₄ as follows:

Fruits / Vegetables	Example	Recommended Minimum Usage Amount (mg/mL)			
		MgSO ₄	PSA	C18	Carb
High percentage of water	Lettuce, cucumber, grapes, apples	150 mg	25 mg		
High fat	Avocados, olives, peanuts, oil	150 mg	25 mg	25 mg	
High carotenoids and chlorophyll	Spinach, bean sprouts, artichokes, carrots	150 mg	25 mg		Low pigment: 2.5 mg High pigment: 10 mg

ProElut™ QuEChERS

Clean-up Kit Ordering Information

Material	Method	Qty	Cat. No.	Price
ProElut™ QuEChERS Clean-up Kit (2 mL)				
50 mg PSA / 150 mg MgSO ₄	AOAC	100/pk	64501	\$123
25 mg PSA / 150 mg MgSO ₄	EN	100/pk	64503	118
50 mg PSA / 50 mg C18 / 150 mg MgSO ₄	AOAC	100/pk	64505	128
25 mg PSA / 25 mg C18 / 150 mg MgSO ₄	EN	100/pk	64507	123
50 mg PSA / 50 mg Carb / 150 mg MgSO ₄	AOAC	100/pk	64509	172
25 mg PSA / 7.5 mg Carb / 150 mg MgSO ₄	EN	100/pk	64511	158
50 mg PSA / 50 mg C18 / 50 mg Carb / 150 mg MgSO ₄	AOAC	100/pk	64513	192
25 mg PSA / 2.5 mg Carb / 150 mg MgSO ₄	EN	100/pk	64515	158
ProElut™ QuEChERS Clean-up Kit (15 mL)				
400 mg PSA / 1200 mg MgSO ₄	AOAC	50/pk	64502	118
150 mg PSA / 900 mg MgSO ₄	EN	50/pk	64504	113
400 mg PSA / 400 mg C18 / 1200 mg MgSO ₄	AOAC	50/pk	64506	128
150 mg PSA / 150 mg C18 / 900 mg MgSO ₄	EN	50/pk	64508	118
400 mg PSA / 400 mg Carb / 1200 mg MgSO ₄	AOAC	50/pk	64510	215
150 mg PSA / 45 mg Carb / 900 mg MgSO ₄	EN	50/pk	64512	143
400 mg PSA / 400 mg C18 / 400 mg Carb / 1200 mg MgSO ₄	AOAC	50/pk	64514	238
150 mg PSA / 15 mg Carb / 900 mg MgSO ₄	EN	50/pk	64516	143

Extraction Kit Ordering Information

Material	Method	Qty	Cat. No.	Price
ProElut™ QuEChERS Extraction Kit (Extraction Salt + 50 mL Centrifuge Tube)				
6 g MgSO ₄ / 1.5 g NaOAc	AOAC	50/pk	64520	\$168
4 g MgSO ₄ / 1 g NaCl / 1 g TSCD / 0.5 g DHS	EN	50/pk	64521	178
ProElut™ QuEChERS Extraction Salts				
6 g MgSO ₄ / 1.5 g NaOAc	AOAC	50/pk	64520S	172
4 g MgSO ₄ / 1 g NaCl / 1 g TSCD / 0.5 g DHS	EN	50/pk	64521S	182



ProElut™ LLE+ (Liquid-Liquid Extraction)

Classical liquid-liquid extraction using a separation funnel is often associated with certain disadvantages such as formation of emulsion, poor phase separation, high solvent consumption, low degree of automation, and high personnel cost. However, liquid-liquid extraction is more efficient using ProElut™ LLE+ cartridges. The simple and excellent performance of ProElut™ LLE+ cartridges eliminates emulsions and therefore, results in higher recoveries and cleaner extractions.



How does ProElut™ LLE+ work?

The aqueous sample is applied to the ProElut™ LLE+ sorbent. The sample then distributes itself in the form of a thin film over the chemically inert matrix and thus acts as a stationary phase. Subsequently, elution takes place using organic solvents that are nonmiscible with water, e.g. diethyl ether, ethyl acetate or halogenated hydrocarbons. All the lipophilic substances are extracted from the aqueous into the organic phase. During this process the aqueous phase remains on the stationary phase. The eluate is free from emulsions and can be evaporated for further analysis.

Application of ProElut™ LLE+

ProElut™ LLE+ has been widely applied in the sample preparation of urine, whole blood, plasma, serum, gastric juice, liquor, amniotic fluid, and animal and plant tissue. Other applications are in the areas of environmental and residue analysis, e.g. the analysis of industrial and domestic wastewater.

Determination of Aromatic Amines Originating from Azo Dyes

1. Application

Determination of aromatic amines originating from azo dyes in textile products

2. Preparation

Cut samples into approximately 5 x 5 mm small pieces, and weigh out 1.0 g sample. Add 16 mL 70 ± 2 °C citrate buffer (0.06 M, pH 6) in a reactor, seal the reactor and shake it until the sample is immersed into the liquid. Keep the reactor in a thermostatic water bath for 30 min at 70 ± 2 °C. Add 3.0 mL sodium dithionite solution into the reactor, seal and shake immediately, then keep the reactor in thermostatic water bath for 30 min at 70 ± 2 °C, take it out, and cool it down to room temperature with warm water.

3. Final Extraction

Open the reactor and press the sample by a glass stick, then transfer the liquid to ProElut™ AZO (Cat#62551), let stand for 15 min. Wash the reactor 4 times with 20 mL diethyl ether, collect all solutions and transfer to ProElut™ AZO for extraction. Use a control flow rate, and collect the elution solution into a 250 mL flat bottom flask.

4. Concentration

The elution solution is concentrated in a vacuum to 1 mL at 35 °C. Dry the concentrated liquid by N₂, and dissolve the residue by 1 mL MeOH. Use HPLC or GC / MS to analyze.

5. GC / MS Method

Column: DM-5MS 30 m x 0.25 mm x 0.25 μm (Cat#8221)

Injection: Splitless, 250 °C

Sample: Aromatic amines, 1 μL

Carrier gas: He (> 99.999%)


Flow rate: 0.6 mL/min,

Temperature program: 50 °C (0.5 min) to 150 °C at 20 °C/min (hold 8 min) to 230 °C at

20 °C/min (hold 20 min) to 260 °C at 20 °C/min (hold 5 min)

MS Condition

Interface temperature: 270 °C, Scan range: 35 - 350 amu, Ionization: EI @ 70 eV

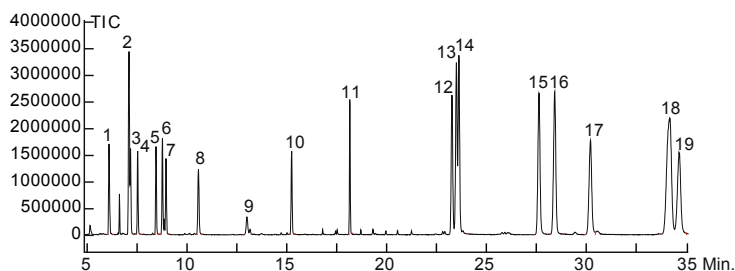

1. *o*-Toluidine
2. 2,4-Dimethylaniline
3. *o*-Anisidine
4. 4-Chloroaniline
5. 2-Methoxy-5-methylaniline
6. 2,4,5-Trimethylaniline
7. 4-Chloro-2-methylaniline
8. 2,4-Diaminotoluene
9. 2, 4-Diaminoanisole
10. 2-Aminonaphthalene
11. 4-Aminobiphenyl
12. 4,4'-Oxydianiline
13. Benzidine
14. 4,4'-Methylenedianiline
15. 3,3'-Dimethyl-4,4'-diaminodiphenylmethane
16. 3,3'-Dimethoxybenzidine
17. 4,4'-Thiodianiline
18. 3,3'-Dichlorobenzidine
19. 3,3'-Dimethoxybenzidine

Ordering Information

Max Sample Volume*	Qty	Cat. No.	Price
ProElut™ LLE+			
1 mL	100/pk	62502	\$210
3 mL	100/pk	62503	220
5 mL	100/pk	62504	230
10 mL	100/pk	62505	279
20 mL	100/pk	62506	290
Special Column for 24 Aromatic Amines Originating from Azo Dyes			
ProElut™ AZO	50/pk	62551	260
SS Rack 6-Ports for ProElut™ LLE+	1/pk	4802	129

*The recommended sample volumes must be adhered to: Solutions of smaller volume must be diluted to give indicated volumes.

ProElut™ Diatomaceous Earth Filter Aid

- Improves extraction efficiency
- Adsorbs moisture from samples

Diatomaceous earth is used as a filter aid to improve extraction efficiency of densely packed soils, such as clays. By mixing the sample with diatomaceous earth, recoveries can be improved and excess moisture can be absorbed.

Ordering Information

Description	Qty	Cat. No.	Price
Diatomite Filter Aid	800 g	62591	\$100

ProMax™ Syringe Filters



ProMax™ Syringe Filters

- Broad range of membrane types
- HPLC / GC sample and solvent filtration
- Standard Luer lock
- Ultra-clean polypropylene housing, low dissolution, for trace analysis
- Low residual volume
- Convenient, cost-effective

Particulates can damage expensive equipment, valves, columns and pumps. They can also lead to erratic analytical results. Pre-filtering samples prior to analysis is critical in preventing column and frit blockage, undue wear on valve seals, and abnormally high operating pressures.

ProMax™ syringe filters are designed for economical, rapid filtration of almost any solution prior to analysis. The housing attaches to any standard Luer lock syringe, so the sample can be pushed through the membrane under pressure. The resulting eluent is free from particulates and ready for use in HPLC, GC or other analytical techniques.

ProMax™ syringe filters are available in a broad range of pore sizes and membrane types. All are non-sterile. Filters made with 13 mm or 25 mm membranes are suitable for use with samples of 1 mL or greater. All filters are available in CA, NY, PVDF, PES, GF or PTFE membranes.

ProMax™ Syringe Filters Specifications

Diameter (mm)	4	13	25	33
Filter area (cm ²)	0.1	0.65	3.9	4.6
Mass Capacity (mL)	≤ 1	1 - 10	10 - 100	10 - 200
Residual volume (μL)	< 10	< 25	< 100	< 125
Max pressure (psig)	75	100	100	75
Max temperature (°C)	50	50	50	50
Material	Medical grade polypropylene; Standard Luer lock			

ProMax™ Filter Membrane Selection Guide

Membrane Type	Application
Cellulose Acetate (CA)	Hydrophilic membrane, uniform pore size, high porosity, small resistance, fast filtration rate, minimal adsorption. Mainly used to filter particles and bacteria in biological and water-soluble samples
Nylon (NY)	For general sample and solvent filtration. Nylon has inherent hydrophilic characteristics and works well with aqueous as well as most solvent-based samples. Nylon is excellent for most HPLC and GC sample and solvent preparations
Polysulfone and Polyvinylidene Difluoride (PVDF) - Not Sterilization	Hydrophobic membrane, exhibits very low protein binding. It can be used for general biological sample filtration. PVDF is especially useful in HPLC sample preparation and is highly resistant to most solvents. Polysulfone has very limited resistance to solvents and is generally used for aqueous-based biological samples. This membrane exhibits good flow rate characteristics
Polyethersulfone (PES)	PES hydrophilic membrane with fast flow, high-throughput characteristics, and ultra-low protein binding. It is ideally suited for use in life sciences applications. Recommended for filtering critical biological samples, tissue culture media, additives, and buffers. Ideal for hard-to-filter solutions. Use mainly with aqueous solutions
Polytetrafluoroethylene (PTFE)	An inherently hydrophobic membrane that is good for filtration of organic-based, highly acidic or basic sample and solvents. Widely used for chromatography, and for clarification of non-aqueous samples. Although this membrane is hydrophobic, it can be made hydrophilic by wetting the membrane with alcohol and then flushing with de-ionized water
Glass Fiber (GF)	For general sample and solvent filtration, pore size 10 μm, use for removing larger particulates or filtration of high viscosity sample. Compared with the standard membrane, GF pre-filters can provide higher throughput

Chemical Compatibility

Syringe Filter	Acetone	Acetonitrile	Glacial acetic acid	n-Butanol	Chloroform	1,4-Dioxan	N,N-Dimethylformamide	Dimethyl sulfoxide	Ethanol	Ethyl acetate	Ethyl ether	Freon TF	Hydrochloric acid (1N)	n-Hexane	Methanol	Dichloromethane	Methyl ethyl ketone	N-Methylpyrrolidone	Isopropyl alcohol	Sodium hydroxide (8N)	Tetrahydrofuran	THF / water (50 / 50)	Toluene	Water	
CA	NR	NR	R	R	NR	NR	NR	R	NR	R	NR	NR	R	R	NR	NR	NR	R	LR	NR	NR	NR	NR	R	
NY	R*	R	R	R	NR	R	R*	R*	R	R*	NR	R	R	R	R	NR	R*	R*	R	R	NR	LR	R*	R	
PVDF	R	NR	NR	R	NR	NR	LR	R	R	NR	NR	R	NR	R	R	NR	R	R	R	NR	R	R	R	R	
PES	LR	R	R	R	LR	LR	R	R	R	R	R	R	R	R	R	LR	R	R	-	-	LR	R	R	R	
PTFE	R*	R	R	R	R	R	R*	R	R*	R	R	R	R	R	R	R	R*	R*	R	LR	R	R	R*	R	
Membrane																									
NY	R	R	NR	R	NR	R	R	R	R	R	R	LR	NR	R	LR	NR	NR	R	R	R	R	R	R	NR	R
PTFE	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R	R

R = Resistant

LR = Limited Resistant

NR = NOT Resistant

*UV absorbance was set at 254 nm

ProMax™ Syringe Filter Ordering Information

Type	Porosity (µm)	Qty	4 mm		13 mm		25 mm	
			< 1 mL Sample Volume	Price	1 - 10 mL Sample Volume	Price	10 - 100 mL Sample Volume	Price
ProMax™ NY	0.22	100/pk	30021	\$115	37177	\$105	37184	\$125
	0.45	100/pk	30022	115	37180	105	37187	125
ProMax™ PTFE	0.22	100/pk	30023	115	37178	105	37185	125
	0.45	100/pk	30024	115	37182	105	37192	125
ProMax™ CA	0.22	100/pk	-	-	30009	105	30011	125
	0.45	100/pk	-	-	30010	105	30012	125
ProMax™ PVDF	0.22	100/pk	-	-	30013	105	30015	125
	0.45	100/pk	-	-	30014	105	30016	125
ProMax™ PES	0.22	100/pk	-	-	30017	105	30019	125
	0.45	100/pk	-	-	30018	105	30020	125



33 mm ProMax™ Syringe Filters

- Large membrane surface area for increased flow rate
- Lower operating pressure, easy for filtering
- Low retention volume
- Low dissolution, lower interference

Type	Porosity (µm)	Qty	33 mm	
			10 - 200 mL Sample Volume	Price
ProMax™ NY	0.22	50/pk	30026	\$84
	0.45	50/pk	30027	84
ProMax™ PTFE	0.22	50/pk	30028	84
	0.45	50/pk	30029	84

2-in-1 Filters

2-in-1 Filters have a two-layered filter in a single housing: the glass fiber pre-filter membrane (1 µm) removes larger particulates and the 0.45 µm membrane performs fine filtration. Compared with standard membrane, this combination can provide greater capacity, especially for filtering of dirty, viscous, or high concentration samples.

Type	Porosity (µm)	Qty	25 mm	
			10 - 100 mL Sample Volume	Price
ProMax™ GF / NY	0.45	100/pk	54839	\$210
ProMax™ GF / PTFE	0.45	100/pk	54840	210
ProMax™ GF / CA	0.45	100/pk	54838	210

2 mL Autosampler Vials

Dikma 2 mL Wide Opening Screw Thread Vials (12 x 32 mm, 9 mm)



- Superior thread design provides a more secure seal to the closure
- 40% larger neck opening versus standard opening screw top vials improve sample accessibility
- Uniformly flat bottom with insert for security
- Write-on patches with graduations at 0.5, 1.0, and 1.5 mL
- Pre-assembled cap and septa, convenient and direct use
- Compatible with most of HPLC / GC autosamplers

2 mL Screw Thread Vials

Desription	Qty	Cat. No.	Price
Clear	100/pk	5320	\$16
Clear, with label	100/pk	5321	18
Amber	100/pk	5322	20
Amber, with label	100/pk	5323	22

Screw Cap with Septa for 2 mL Screw Thread Vials

- Cap manufactured from polypropylene
- Pre-assembled caps and septa are convenient and minimize contamination from handling
- Choice of liner

Desription	Qty	Cat. No.	Price
Screw cap, blue, open top, with PTFE / Red rubber septa	100/pk	5324	\$18
Screw cap, blue, open top, with PTFE / White silicone septa	100/pk	5325	21
Screw cap, blue, open top, with PTFE / Silicone / PTFE septa	100/pk	5326	24
Screw cap, blue, open top, with Pre-slit PTFE / Silicone septa	100/pk	5327	25
Screw cap, blue, open top, with PTFE / ULB silicone septa	100/pk	5328	28
Screw cap, blue, open top, with Pre-slit PTFE / ULB silicone septa	100/pk	5329	29

Septum Selection Guide

Septum Material	Specification	Temperature
PTFE / Red Rubber	The most popular and economical choice for general gas chromatography applications. These septa are used primarily for routine analysis in gas chromatography. They offer moderate resealing ability, but are not recommended for multiple injections or storage of samples	-40 - 110 °C
PTFE / Silicone	Good for multiple injections or storage of samples due to its excellent resealing capabilities. The white silicone is soft and more easily punctured, and protects the needle in an autosampler accordingly	-60 - 200 °C
PTFE / Silicone Slit	Same as above, with an additional slit in the center providing easier needle puncture, especially for large diameter and blunt tip needles. However, this will result in evaporation of volatile organic solvents, and is thus not recommended for storage of samples	-60 - 200 °C
PTFE / Silicone / PTFE	Recommended for the most critical applications such as ultra trace analysis or where there is a longer period between injections or for internal standard methods	-60 - 200 °C
PTFE / ULB Silicone	Excellent chemical inertness and ultra-low bleed, the interference of a low baseline will make it much more suitable for highly sensitive detectors such as MSDs	-60 - 200 °C
PTFE / ULB Silicone Slit	Same as above, with an additional slit in the center providing easier needle puncture, especially for large diameter and blunt tip needles. However, this will result in evaporation of volatile organic solvents, and is thus not recommended for storage of samples	-60 - 200 °C

Dikma 2 mL Wide Opening Crimp Top Vials (12 x 32 mm, 11 mm)

- Write-on patches with graduations at 0.5, 1.0 and 1.5 mL
- Pre-assembled cap and septa, convenient and direct use
- Compatible with most of HPLC / GC autosamplers
- Uniformly flat bottom with inserts for security

2 mL Crimp Top Vials

Description	Qty	Cat. No.	Price
Clear	100/pk	3915	\$14
Clear, with label	100/pk	3916	16
Amber	100/pk	3917	18
Amber, with label	100/pk	3918	20



Aluminum Cap with Septa for Crimp Top Vials


Description	Qty	Cat. No.	Price
Aluminum cap 11 mm, with PTFE / Red rubber septa	100/pk	3919	\$12
Aluminum cap 11 mm, with PTFE / White silicone septa	100/pk	3920	18
Aluminum cap 11 mm, magnetic, with PTFE / White silicone septa for CTC autosamplers	100/pk	3921	22



Microvolume Inserts

For 2 mL Screw Thread Vials and 2 mL Crimp Top Vials


Description	Qty	Cat. No.	Price
100 μ L glass conical inserts, clear, 6 x 31 mm	100/pk	3972	\$38
100 μ L glass conical inserts, clear, 5.7 x 29 mm, with polyspring	100/pk	3973	80
300 μ L glass conical inserts, clear, 5.7 x 29 mm, with polyspring	100/pk	3974	60
350 μ L glass flat bottom inserts, clear, 6 x 31 mm	100/pk	52385	28



Vial Rack

For all 12 x 32 mm vials, can be cross-stacked

Description	Qty	Cat. No.	Price
Vial rack 12 mm PP 50 holes white	1/pk	52401A	\$24
Vial rack 12 mm PP 50 holes blue	1/pk	52401B	24




Compiled from our years of experience in chromatography, the application compendium contains HPLC, GC and SPE applications to help you find the solution you need.

A circular inset image showing a globe of the Earth with green foliage and water, symbolizing environmental science.

Environmental

A circular inset image showing a variety of fresh fruits and vegetables, including tomatoes, oranges, watermelon, and green beans, representing the food industry.

Food

A circular inset image showing several blue and red capsules and pills scattered on a light blue surface, representing the pharmaceutical industry.

Pharmaceutical

A circular inset image showing a blue DNA double helix structure with two human figures standing next to it, representing life science.

Life Science

A circular inset image showing an industrial refinery or petrochemical plant at night, with illuminated towers and structures.

Petrochemical

Applications and Index

HPLC Applications.....	130
Pharmaceutical.....	131
Food / Environmental	141
Life Science	149
Others	150
GC Applications.....	151
Environmental.....	154
Petrochemicals	168
Chemicals.....	183
Solvents	192
Food.....	200
Pharmaceutical.....	208
SPE Applications	213
Food.....	214
Environmental.....	229
Pharmaceutical.....	231
Others	232
Compound Index.....	233
Product Index	240

HPLC Applications Index

Industry Index

Pharmaceutical	131
Food / Environmental	141
Life Science	149
Others	150

Product Index

Bio-Bond™

Proteins	149
----------------	-----

Endeavorsil™

Acidic Compounds	141
Antiulcers	131
Antibacterials	132
Antifungals	141
Anti-inflammatories	133
β-Blockers at Low pH	134
β-Blockers at Neutral pH	134
Catecholamines	135
Parabens	145
Polar Acids	147
Steroids	150
TCAs at Low pH	140

Inspire™

Alkaloids	131
Antiulcers	132
Antibacterials	132
Antifungals	141
Antihistamines	133
Anti-inflammatories	133
Antioxidants	149
Benzoylurea and Bishydrazide Mixture	142
Caffeine Metabolites	142
Catecholamines	135
Cephalosporin Antibiotics	135, 136
Colorants	143
Derivatized Carbonyl Compounds	143
Flavonoids	138
Herbicides	143
Melamine	144
Organic Acids	144
Parabens	145
Penicillins	138
Polar Acids	146
Quinolones	139
Steroids	150
Sweeteners	147
TCAs and Benzos	139
TCAs at Low pH	140
Unsaturated Fatty Acids	148

Leapsil™

Antibacterials	132
Antifungals	141
Anti-inflammatories	133
β-Blockers at Low pH	134
β-Blockers at Neutral pH	134
Parabens	146
Polar Acids	147
Polar Bases	139
Water-Soluble Vitamins	140


Spursil™

Acidic Compounds	131
Benzoic Acid and Sorbic Acid in Milk	142
Benzoyl Peroxide in Wheat Flour	142
Catecholamines	135
Catechols and Resorcinols	143
Cephalosporin Antibiotics	136, 137
Flavonoids	138
Herbicides	144
Organic Acids	145
Phenols	146, 150
Sweeteners	147, 148
TCAs and Benzos	139

Acidic Compounds

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample:

1. L-Ascorbic acid
2. Acetaminophen
3. *p*-Aminobenzoic acid
4. Homovanillic acid
5. Acetylsalicylic acid
6. Sorbic acid
7. Benzoic acid

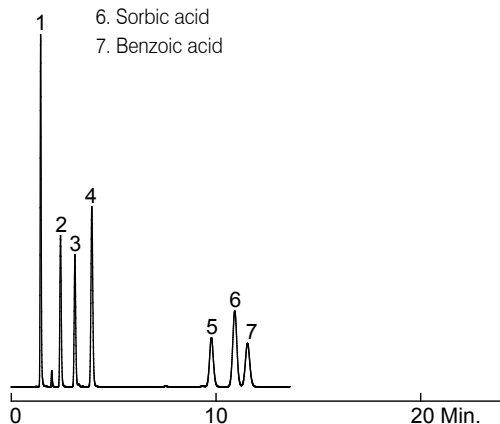


AN: S1167

Acidic Compounds

Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample:

1. L-Ascorbic acid
2. Acetaminophen
3. *p*-Aminobenzoic acid
4. Homovanillic acid
5. Acetylsalicylic acid
6. Sorbic acid
7. Benzoic acid

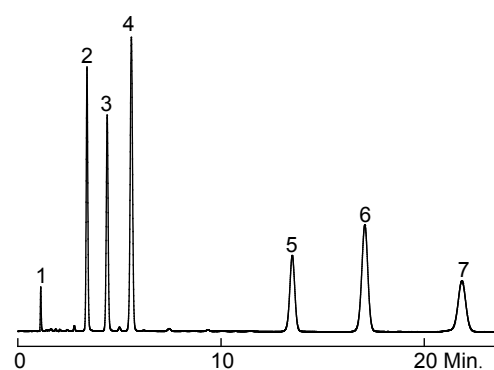


AN: S1168

Alkaloids

Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:20 mM KH₂PO₄ (pH 2.3) = 42:58
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample:

1. Theobromine
2. Quinine
3. Hydrastine
4. Berberine

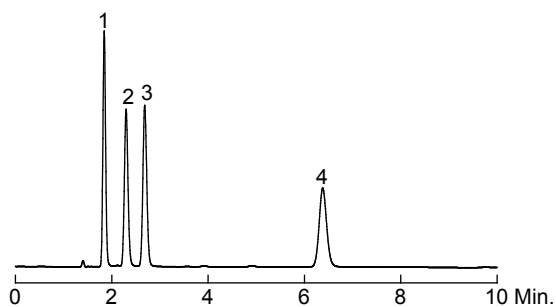


AN: I1101

Antiulcers

Column: Endeavorsil™ 1.8 μm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: MeOH:10 mM CH₃COONH₄ (pH 7) = 35:65
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample:


1. Famotidine
2. Ranitidine
3. Cimetidine
4. Nizatidine

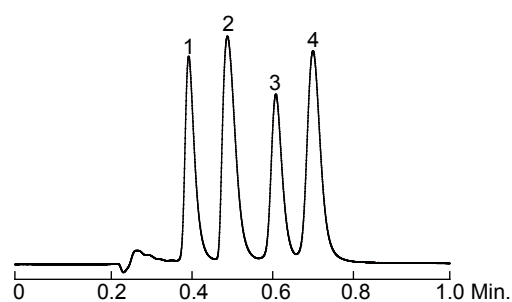

AN: E1101

Antulcers


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:10 mM CH₃COONH₄ (pH 7) = 35:65
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Famotidine
 2. Ranitidine
 3. Cimetidine
 4. Nizatidine

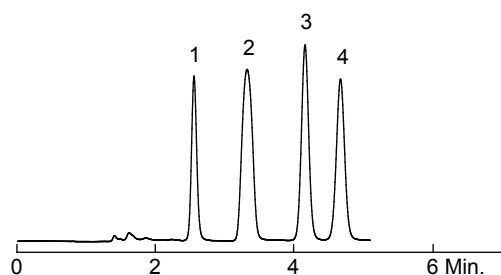

AN: I1102

Antibacterials


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Sulfanilamide 6. Sulfamethoxyipyridazine
 2. Carbadox 7. Furazolidone
 3. Sulfapyridine 8. Sulfamethoxazole
 4. Sulfamerazine 9. Sulfisoxazole
 5. Thiamphenicol 10. Oxolinic acid

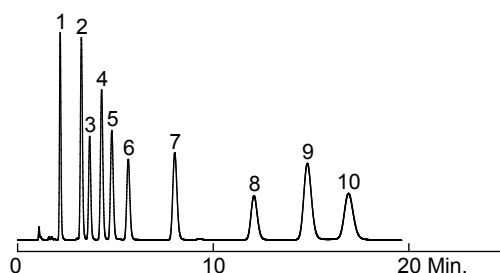

AN: I1103

Antibacterials


Column: Leapsil™ 2.7 μm C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Sulfanilamide
 2. Carbadox
 3. Sulfamerazine
 4. Sulfamethazine
 5. Sulfamethoxyipyridazine
 6. Furazolidone
 7. Sulfamethoxazole
 8. Sulfisoxazole
 9. Oxolinic acid
 10. Sulfadimethoxine

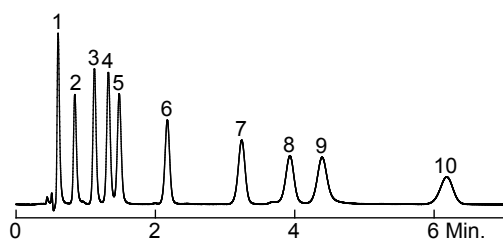

AN: L1112

Antibacterials


Column: Endeavorsil™ 1.8 μm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Sulfanilamide
 2. Carbadox
 3. Sulfamerazine
 4. Sulfamethoxyipyridazine
 5. Furazolidone
 6. Sulfamethoxazole
 7. Sulfisoxazole
 8. Oxolinic acid
 9. Sulfadimethoxine
 10. Sulfaquinoxaline

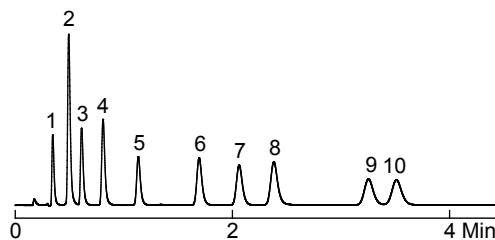

AN: E1102

Antihistamines


Column: Inspire™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:5 mM NH₄HCO₃ (pH 10) = 75:25
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Maleic acid
 2. Pheniramine
 3. Doxylamine
 4. Chlorpheniramine
 5. Brompheniramine
 6. Diphenhydramine

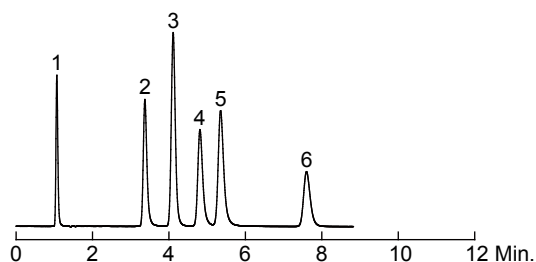

AN: I1104

Anti-inflammatories


Column: Inspire™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 55:45
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Phenacetin
 2. Tolmetin
 3. Ketoprofen
 4. Fenoprofen
 5. Flurbiprofen
 6. Diclofenac
 7. Ibuprofen

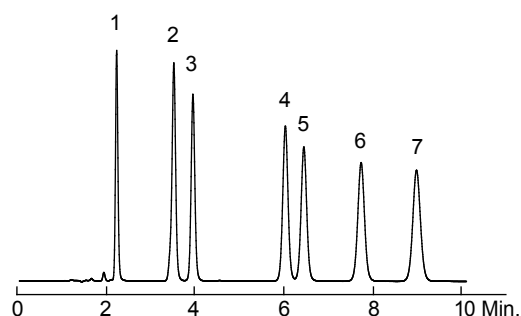

AN: I1105

Anti-inflammatories


Column: Endeavorsil™ 1.8 µm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 50:50
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Phenacetin
 2. Tolmetin
 3. Ketoprofen
 4. Fenoprofen
 5. Flurbiprofen
 6. Ibuprofen

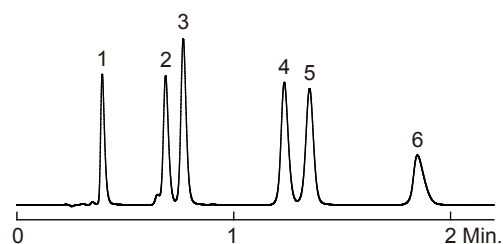

AN: E1103

Anti-inflammatories


Column: Leapsil™ 2.7 µm C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 50:50
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Phenacetin
 2. Tolmetin
 3. Ketoprofen
 4. Fenoprofen
 5. Flurbiprofen
 6. Ibuprofen

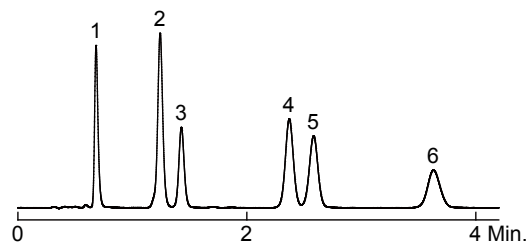

AN: L1102

β -Blockers at Low pH


Column: Endeavorsil™ 1.8 μ m C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 25:75
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Acebutolol
 4. Metoprolol
 5. Labetolol
 6. Propranolol
 7. Alprenolol

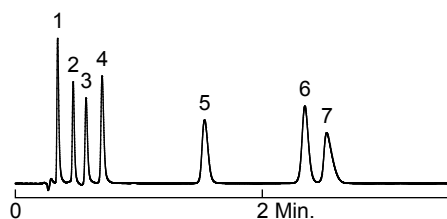

AN: E1104

β -Blockers at Low pH


Column: Leapsil™ 2.7 μ m C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 25:75
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Acebutolol
 4. Metoprolol
 5. Labetolol
 6. Propranolol

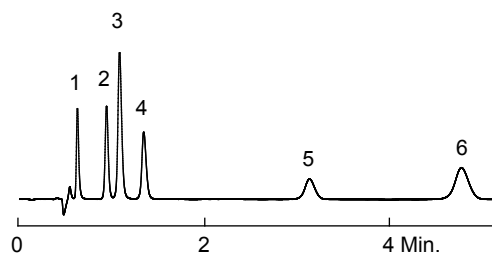

AN: L1103

β -Blockers at Neutral pH


Column: Endeavorsil™ 1.8 μ m C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 30:70
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Metoprolol
 4. Labetolol
 5. Propranolol

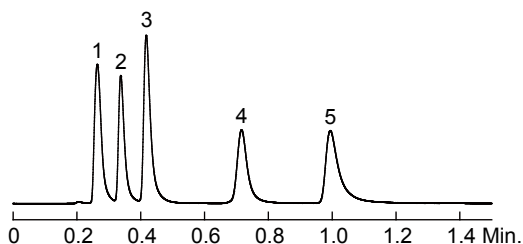

AN: E1105

β -Blockers at Neutral pH


Column: Leapsil™ 2.7 μ m C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: MeCN:20 mM phosphate buffer (pH 7) = 25:75
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Nadolol
 2. Pindolol
 3. Metoprolol
 4. Labetolol
 5. Propranolol

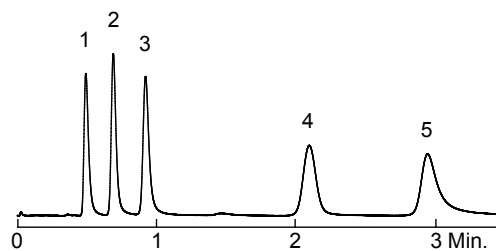

AN: L1104

Catecholamines


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 20 mM KH₂PO₄, pH 7
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample: 1. Norepinephrine
 2. Epinephrine
 3. Dopamine

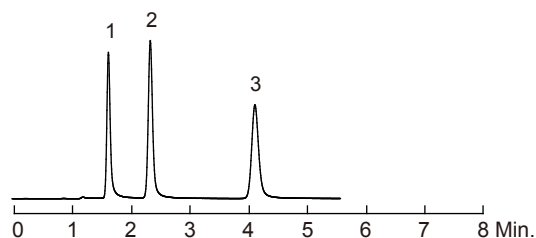

AN: I1106

Catecholamines


Column: Endeavorsil™ 1.8 μm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% TFA in H₂O
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample: 1. Norepinephrine
 2. Epinephrine
 3. Dopamine

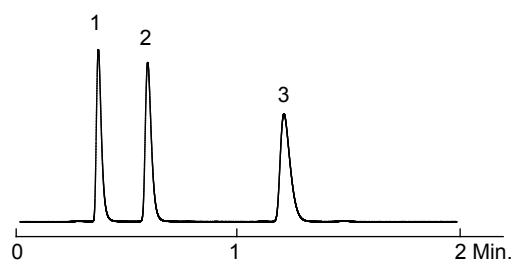

AN: E1106

Catecholamines


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: 20 mM KH₂PO₄, pH 7
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample: 1. Norepinephrine
 2. Epinephrine
 3. Dopamine

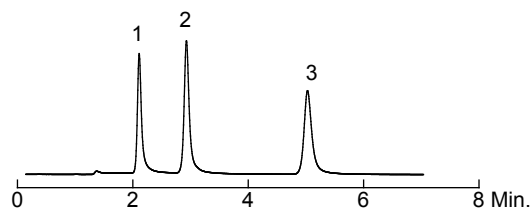

AN: S1152

Cephalosporin Antibiotics

Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Ceftazidime
 2. Cefadroxil
 3. Cefazoline
 4. Cefaclor
 5. Cephalexin
 6. Cefoxitin
 7. Cefradine

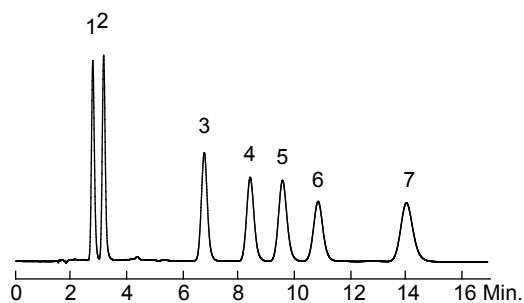


AN: I1123

Pharmaceutical

Cephalosporin Antibiotics


Column: Inspire™ 5 µm C18, 150 x 4.6 mm
Cat. No.: **81001**
Mobile Phase: MeOH:100 mM acetate buffer = 20:80
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Cefadroxil
2. Cefuroxime
3. Cefaclor
4. Cefoxitin
5. Cefradine

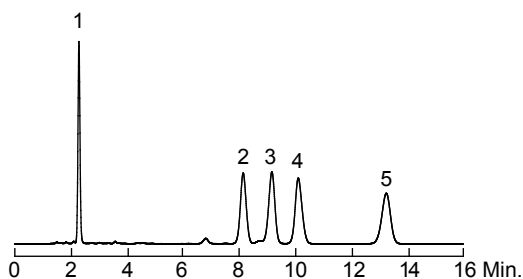

AN: I1107

Cephalosporin Antibiotics


Column: Inspire™ 5 µm C18, 150 x 4.6 mm
Cat. No.: **81001**
Mobile Phase: MeOH:25 mM phosphate buffer (pH 3) = 20:80
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 230 nm
Sample: 1. Cefadroxil
2. Ceftazidime
3. Cefaclor
4. Cephalixin
5. Cefazoline
6. Cefoxitin
7. Cefradine

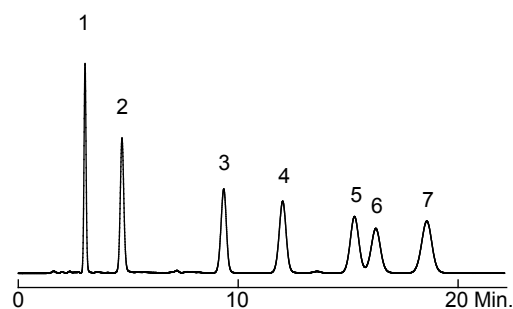

AN: I1108

Cephalosporin Antibiotics


Column: Spursil™ 5 µm C18, 150 x 4.6 mm
Cat. No.: **82001**
Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 230 nm
Sample: 1. Ceftazidime
2. Cefadroxil
3. Cefuroxime
4. Cefazoline
5. Cefaclor
6. Cephalixin
7. Cefradine

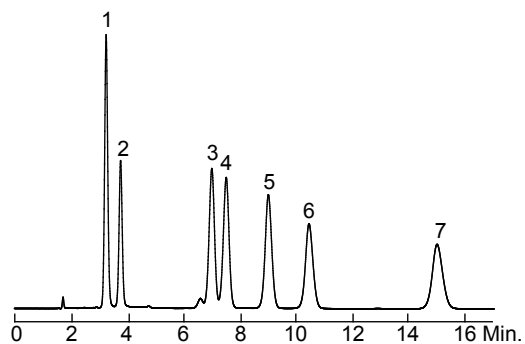

AN: I1127

Cephalosporin Antibiotics


Column: Spursil™ 5 µm C18, 150 x 4.6 mm
Cat. No.: **82001**
Mobile Phase: MeOH:100 mM acetate buffer = 20:80
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Ceftazidime
2. Cefadroxil
3. Cefuroxime
4. Cefoxitin
5. Cefaclor
6. Cefradine

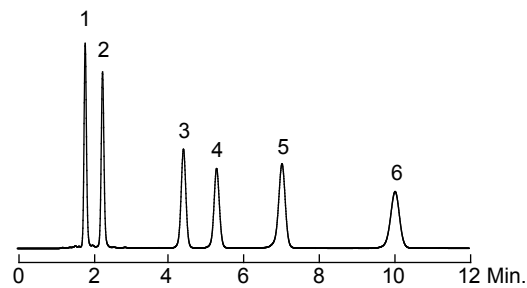

AN: E1113

Cephalosporin Antibiotics


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: MeOH:25 mM phosphate buffer (pH 3) = 25:75
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Cefadroxil
 2. Ceftazidime
 3. Cefaclor
 4. Cephalixin
 5. Cefazoline
 6. Cefradine

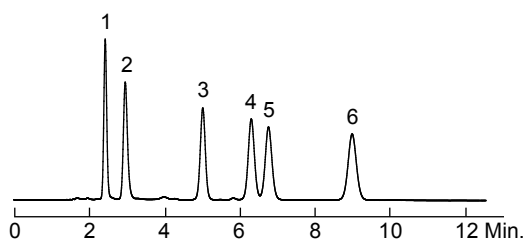

AN: S1170

Cephalosporin Antibiotics


Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeOH:0.1% TFA in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Ceftazidime
 2. Cefadroxil
 3. Cephalixin
 4. Cefradine
 5. Cefazoline
 6. Cefoxitin

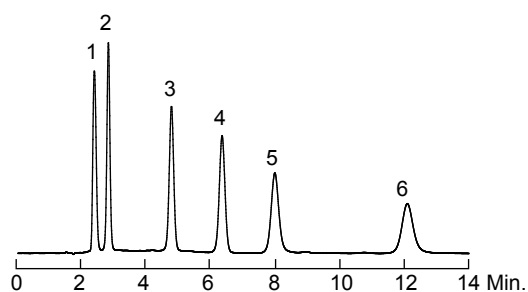

AN: S1171

Cephalosporin Antibiotics


Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeOH:100 mM acetate buffer = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Ceftazidime
 2. Cephalixin
 3. Cefaclor
 4. Cefradine
 5. Cefoxitin

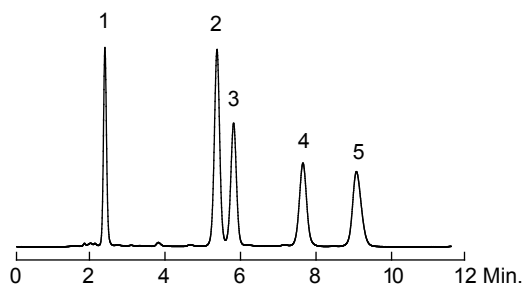

AN: S1172

Cephalosporin Antibiotics

Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeOH:25 mM phosphate buffer (pH 3) = 25:75
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 230 nm
 Sample: 1. Cefadroxil
 2. Ceftazidime
 3. Cefaclor
 4. Cephalixin
 5. Cefradine
 6. Cefazoline

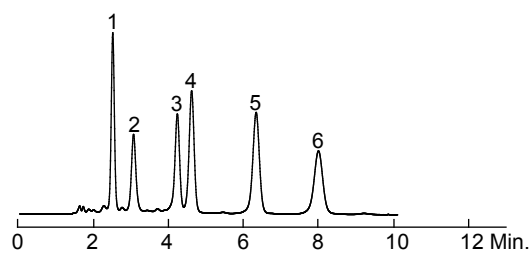


AN: S1173

Applications

Flavonoids


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeCN:0.085% H₃PO₄ = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Gallic acid
 2. Catechin
 3. Caffeic acid
 4. Vanillic acid
 5. *p*-Coumaric acid
 6. Quercitrin
 7. Myricetin

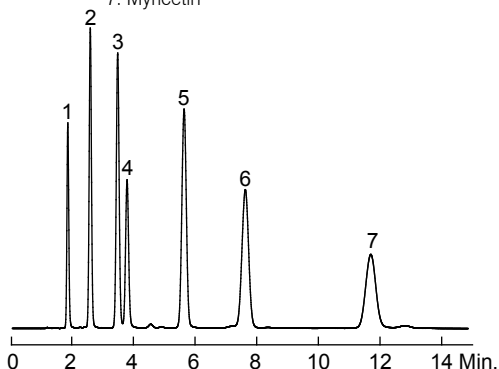

AN: I1109

Flavonoids


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: MeCN:0.085% H₃PO₄ = 20:80
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Gallic acid
 2. Catechin
 3. Caffeic acid
 4. Vanillic acid
 5. *p*-Coumaric acid
 6. Quercitrin
 7. Myricetin

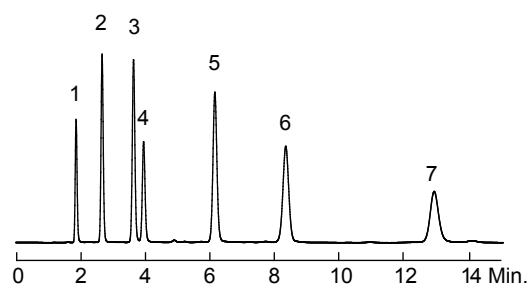

AN: S1154

Flavonoids


Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeCN:0.085% H₃PO₄ = 25:75
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Gallic acid
 2. Catechin
 3. Vanillic acid
 4. Caffeic acid
 5. *p*-Coumaric acid

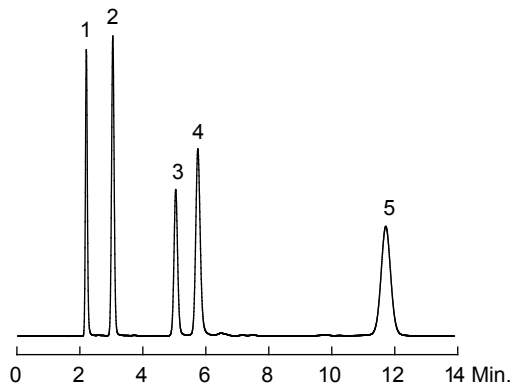

AN: S1169

Penicillins


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:25 mM KH₂PO₄ = 55:45
 Flow Rate: 0.5 mL/min
 Temperature: Ambient
 Detection: UV 220 nm
 Sample: 1. Amoxicillin
 2. Ampicillin
 3. Piperacillin
 4. Penicillin G
 5. Oxacillin
 6. Cloxacillin
 7. Dicloxacillin

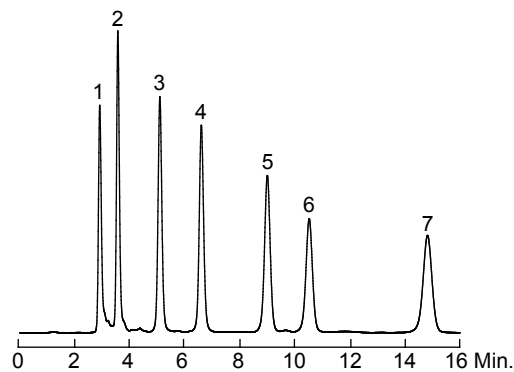

AN: I1125

Polar Bases

Column: Leapsil™ 2.7 μm C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 0.3 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Doxepin
 2. Protriptyline
 3. Nortriptyline
 4. Amitriptyline
 5. Trimipramine
 6. Clomipramine

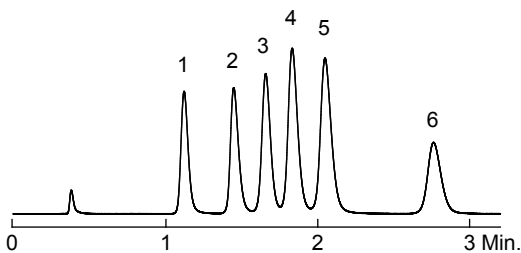


AN: L1105

Quinolones

Column: Inspire™ 5 μm C18, 250 x 4.6 mm
 Cat. No.: **81006**
 Mobile Phase A: MeOH
 Mobile Phase B: 0.2% H₃PO₄ in H₂O
 Flow Rate: 1.0 mL/min
 Temperature: 35 °C
 Detection: UV 254 nm
 Sample: 1. Marbofloxacin
 2. Ofloxacin
 3. Norfloxacin
 4. Enrofloxacin
 5. Ciprofloxacin
 6. Pazufloxacin
 7. Difloxacin
 8. Sarafloxacin
 9. Gatifloxacin
 10. Sparfloxacin
 11. Oxolinic acid
 12. Nalidixic acid
 13. Flumequine


t / min.	0	25	40	42	50
A / %	22	33	65	22	22
B / %	78	67	35	78	78

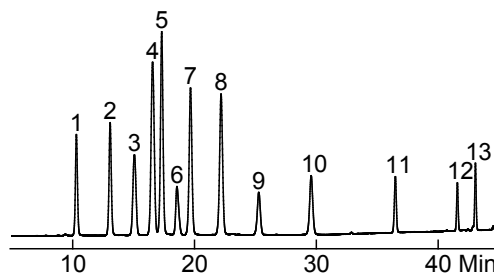

AN: I1124

TCAs and Benzos


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Nitrozepam
 2. Nordoxepin
 3. Alprazolam
 4. Diazepam
 5. Oxazepam
 6. Triazolam
 7. Nortriptyline
 8. Clonazepam
 9. Trimipramine

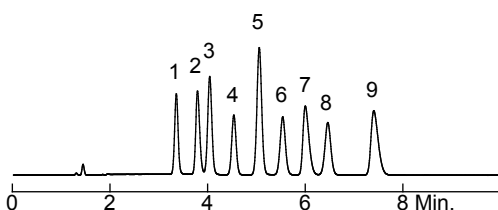

AN: I1112

TCAs and Benzos

Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Nitrozepam
 2. Estazolam
 3. Alprazolam
 4. Diazepam
 5. Triazolam
 6. Clonazepam
 7. Nortriptyline
 8. Amitriptyline
 9. Trimipramine

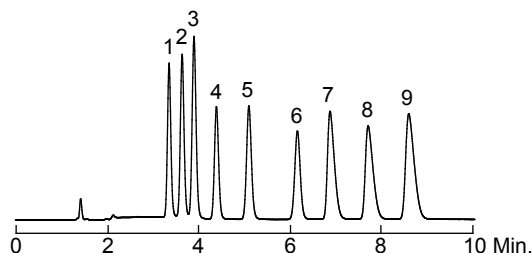


AN: S1155

Applications

Pharmaceutical

TCAs at Low pH


Column: Endeavorsil™ 1.8 μm C18, 50 x 2.1 mm
Cat. No.: **87002**
Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 35:65
Flow Rate: 0.5 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Doxepin
2. Desipramine
3. Nortriptyline
4. Amitriptyline
5. Trimipramine
6. Clomipramine

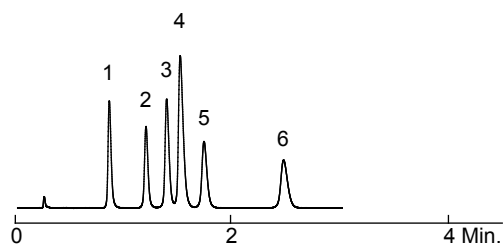

AN: E1107

TCAs at Low pH


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
Cat. No.: **81001**
Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Nordoxepin
2. Doxepin
3. Desipramine
4. Nortriptyline
5. Amitriptyline
6. Trimipramine
7. Clomipramine

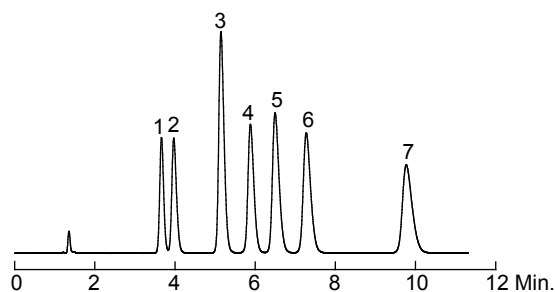

AN: I1126

Water-Soluble Vitamins


Column: Leapsil™ 2.7 μm C18, 50 x 2.1 mm
Cat. No.: **86004**
Mobile Phase: 10 mM HCOONH₄, pH 3
Flow Rate: 0.3 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Pyridoxamine
2. L-Ascorbic acid
3. Pyridoxal
4. Nicotinamide
5. Pyridoxol

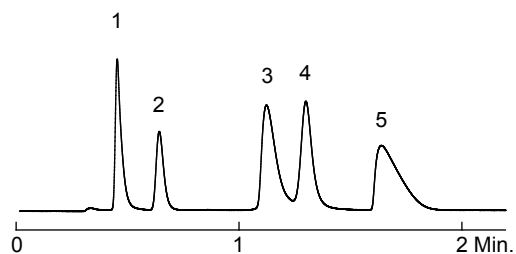

AN: L1106

Acidic Compounds


Column: Endeavorsil™ 1.8 µm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. L-Ascorbic acid
 2. *p*-Aminobenzoic acid
 3. Homovanillic acid
 4. Acetylsalicylic acid
 5. Sorbic acid
 6. Salicylic acid

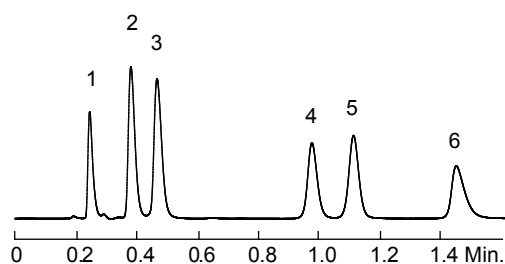

AN: E1108

Antifungals


Column: Inspire™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Acetylsalicylic acid
 3. Benzoic acid
 4. Salicylic acid

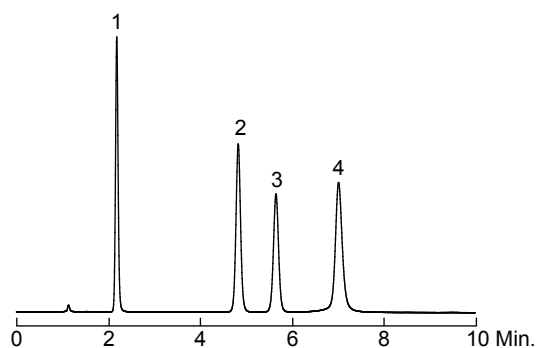

AN: I1114

Antifungals


Column: Endeavorsil™ 1.8 µm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 30:70
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Acetylsalicylic acid
 3. Benzoic acid
 4. Salicylic acid

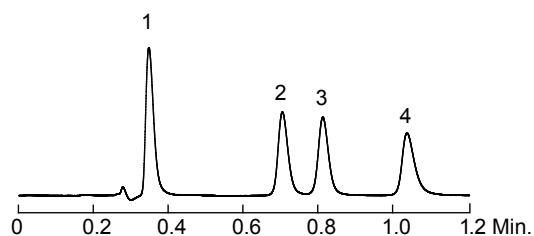

AN: E1109

Antifungals


Column: Leapsil™ 2.7 µm C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 30:70
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Acetylsalicylic acid
 3. Benzoic acid
 4. Salicylic acid

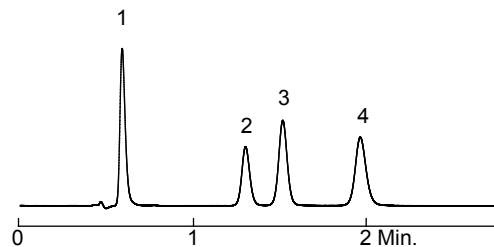

AN: L1110

Benzoic Acid and Sorbic Acid in milk


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82006**
 Mobile Phase: MeOH:phosphate buffer = 10:90
 Flow Rate: 1.2 mL/min
 Injection Volume: 10 μL
 Temperature: 40 °C
 Detection: UV 227 nm
 Sample: 1. Benzoic acid
 2. Sorbic acid

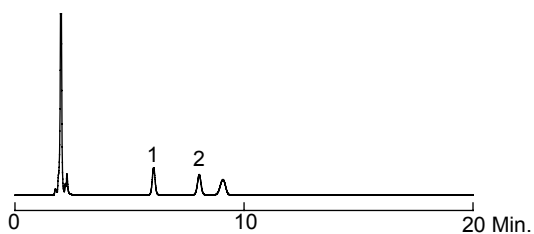

AN: S1156

Benzoyl Peroxide in Wheat Flour

Column: Spursil™ 5 μm C18, 250 x 4.6 mm
 Cat. No.: **82006**
 Mobile Phase: MeOH:20 mM acetate buffer = 10:90
 Flow Rate: 1.0 mL/min
 Injection Volume: 10 μL
 Temperature: 30 °C
 Detection: UV 230 nm
 Sample: 1. Benzoyl peroxide

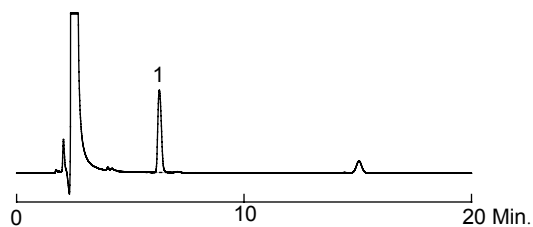


AN: S1157

Benzoylurea and Bishydrazide Mixture

Column: Inspire™ 5 μm C18, 250 x 4.6 mm
 Cat. No.: **81006**
 Mobile Phase A: MeOH
 Mobile Phase B: H₂O
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 248 nm
 Sample: 1. Methoxyfenozide
 2. Tebufenozide
 3. Diflubenzuron
 4. Chlorbenzuron
 5. Triflumuron
 6. Hexaflumuron
 7. Teflubenzuron
 8. Flufenoxuron
 9. Chlorfluazuron


t / min.	0	5	15	30	32	40
A / %	75	75	80	95	75	75
B / %	25	25	20	5	25	25

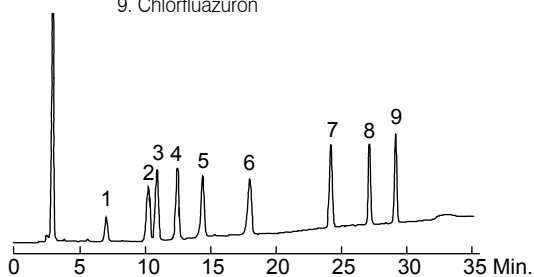

AN: I1115

Caffeine Metabolites


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:1% CH₃COOH in H₂O = 10:90
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Uric acid
 2. Xanthine
 3. 7-Methylxanthine
 4. 1-Methyluric acid
 5. 3-Methylxanthine
 6. 1,3-Dimethyluric acid
 7. Theobromine
 8. 1,7-Dimethylxanthine
 9. Theophylline

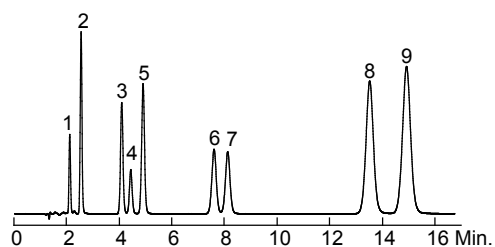

AN: I1123

Catechols and Resorcinols

Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 270 nm
 Sample: 1. Resorcinol
 2. Catechol
 3. 2-Methylresorcinol
 4. 4-Methylcatechol
 5. 2,5-Dimethylresorcinol
 6. 3-Methylcatechol
 7. 4-Nitrocatechol

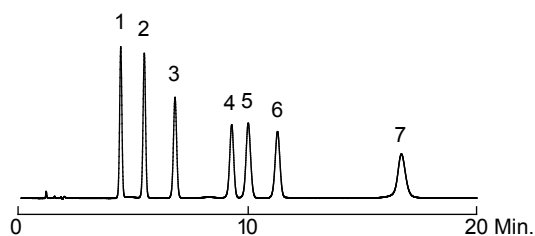


AN: S1158

Colorants

Column: Inspire™ 5 μm C18, 250 x 4.6 mm
 Cat. No.: **81006**
 Mobile Phase A: MeCN
 Mobile Phase B: 0.05 M CH₃COONH₄
 Flow Rate: 1.0 mL/min
 Temperature: 35 °C
 Detection: UV 254 nm
 Sample: 1. Tartrazine 10. Lissamine green B
 2. Amaranth 11. Brilliant blue
 3. Indigotin 12. Acid orange I
 4. Carmine 13. Erythrosine
 5. Brilliant black 14. Acid orange II
 6. Sunset yellow 15. Patent blue V
 7. Fancy red 16. Auramine
 8. Acid red 2G 17. Acid yellow 36
 9. Azorubine 18. Basic orange

t / min.	0	20	50	52	60
A / %	5	30	50	5	5
B / %	95	70	50	95	95

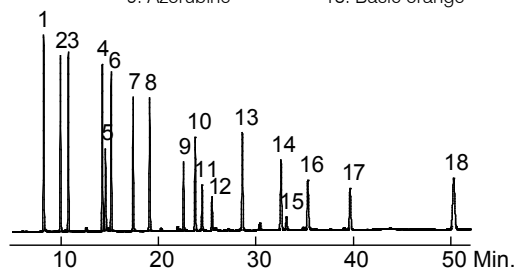


AN: I1117

Derivatized Carbonyl Compounds

Column: Inspire™ 5 μm C18, 250 x 4.6 mm
 Cat. No.: **81006**
 Mobile Phase A: MeOH
 Mobile Phase B: H₂O
 Flow Rate: 1.0 mL/min
 Temperature: 35 °C
 Detection: UV 360 nm
 Injection Volume: 20 μL
 Sample: 1. Formaldehyde-DNPH 9. Isovaleraldehyde-DNPH
 2. Acetaldehyde-DNPH 10. Valeraldehyde-DNPH
 3. Acrolein-DNPH 11. *o*-Tolualdehyde-DNPH
 4. Acetone-DNPH 12. *m*-Tolualdehyde-DNPH
 5. Propionaldehyde-DNPH 13. *p*-Tolualdehyde-DNPH
 6. Crotonaldehyde-DNPH 14. 2,5-Dimethylbenzaldehyde-DNPH
 7. Butyraldehyde-DNPH 15. Hexaldehyde-DNPH
 8. Benzaldehyde-DNPH


t / min.	0	35	40	41	50
A / %	70	80	80	70	70
B / %	30	20	20	30	30

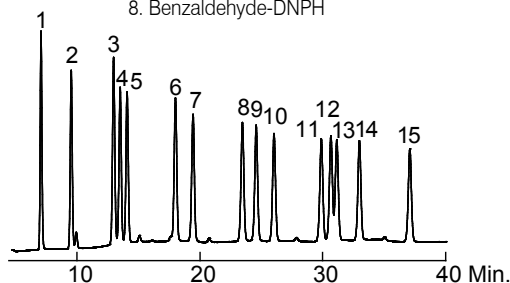

AN: I1118

Herbicides


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 40:60
 Flow Rate: 2.0 mL/min
 Temperature: Ambient
 Detection: UV 214 nm
 Sample: 1. Dalapon
 2. 2,4-D
 3. 2,4,5-T

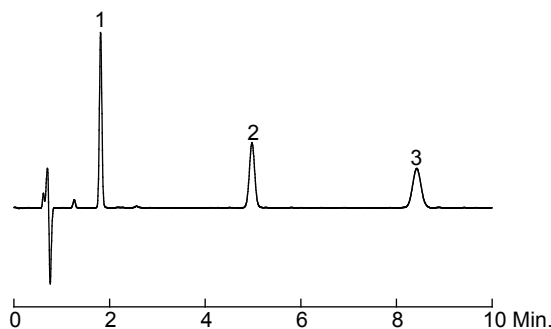

AN: I1119

Herbicides


Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: MeCN:H₂O = 60:40
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 214 nm
 Sample: 1. Fenuron
 2. Monuron
 3. Diuron
 4. Linuron

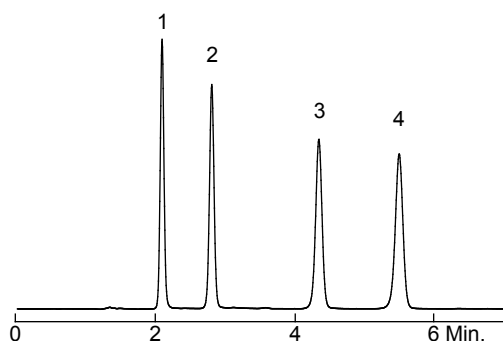

AN: S1159

Herbicides


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: MeCN:H₂O = 60:40
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 214 nm
 Sample: 1. Fenuron
 2. Monuron
 3. Diuron
 4. Linuron

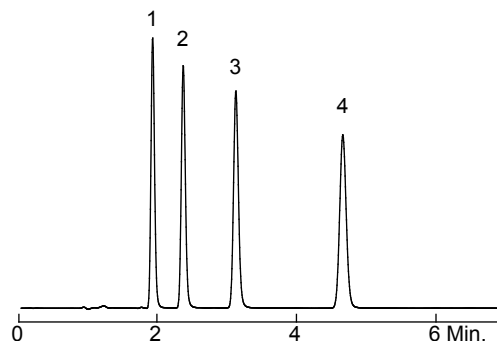

AN: S1160

Melamine


Column: Inspire™ 5 μm C18, 250 x 4.6 mm
 Cat. No.: **81006**
 Mobile Phase: MeCN:Buffer = 8:92
 Flow Rate: 1.0 mL/min
 Temperature: 30 °C
 Detection: UV 214 nm
 Sample: 1. Melamine

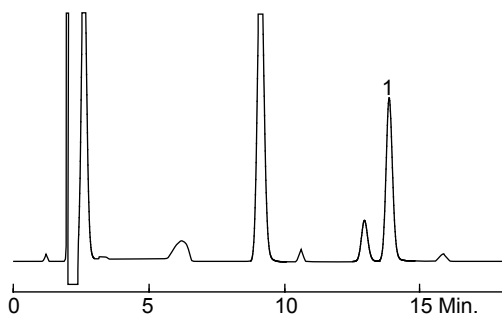

AN: I1110

Organic Acids


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 25 mM KH₂PO₄, pH 2.5
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Oxalic acid
 2. Tartaric acid
 3. Malic acid
 4. Lactic acid
 5. Acetic acid
 6. Citric acid
 7. Fumaric acid
 8. Succinic acid

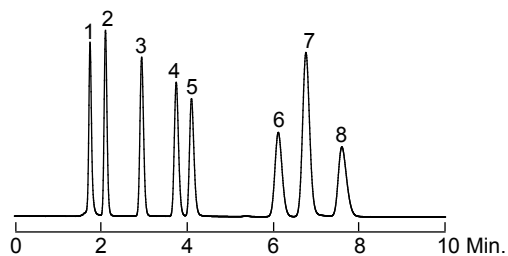

AN: I1112

Organic Acids


Column: Spursil™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: 25 mM KH₂PO₄, pH 2.5
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Oxalic acid
 2. Tartaric acid
 3. Malic acid
 4. Lactic acid
 5. Acetic acid
 6. Citric acid
 7. Fumaric acid
 8. Succinic acid

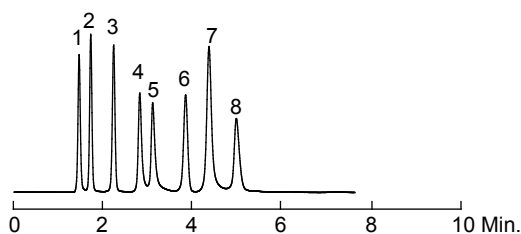

AN: S1161

Organic Acids


Column: Spursil™ 5 µm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: 25 mM KH₂PO₄, pH 2.5
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Oxalic acid
 2. Tartaric acid
 3. Malic acid
 4. Lactic acid
 5. Acetic acid
 6. Citric acid
 7. Succinic acid
 8. Fumaric acid

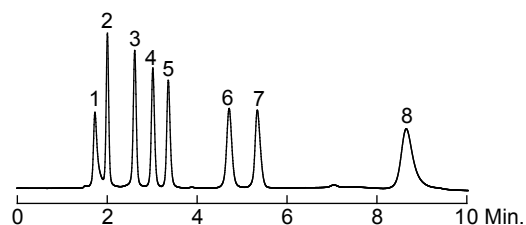

AN: S1162

Parabens


Column: Inspire™ 5 µm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeCN:20 mM K₂HPO₄ (pH 7) = 50:50
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 254 nm
 Sample: 1. Methyl paraben
 2. Ethyl paraben
 3. Propyl paraben
 4. Butyl paraben

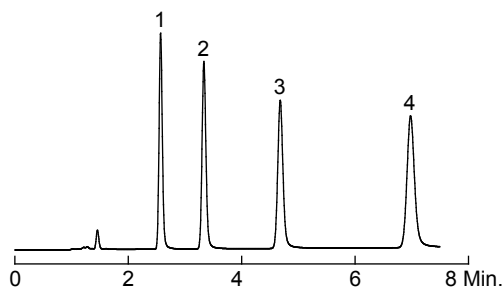

AN: I1113

Parabens

Column: Endeavorsil™ 1.8 µm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: MeCN:20 mM K₂HPO₄ (pH 7) = 50:50
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Methyl paraben
 2. Ethyl paraben
 3. Propyl paraben
 4. Butyl paraben

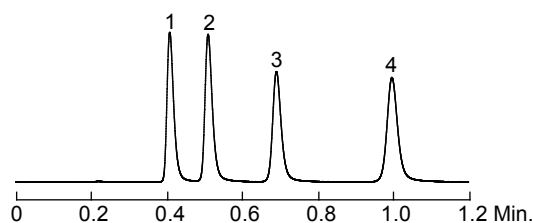


AN: E1110

Applications

Parabens


Column: Leapsil™ 2.7 μm C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: MeCN:20 mM K₂HPO₄ (pH 7) = 55:45
 Flow Rate: 0.3 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. Methyl paraben
 2. Ethyl paraben
 3. Propyl paraben
 4. Butyl paraben

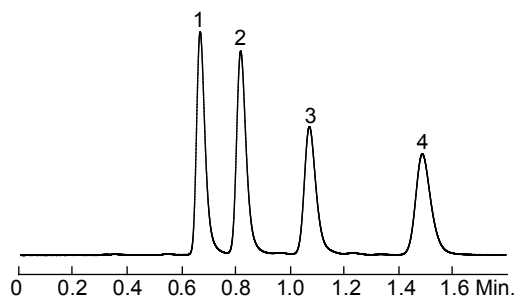

AN: L1108

Phenols


Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
 Cat. No.: **82101**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 55:45
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Phenol
 2. 2-Nitrophenol
 3. 4-Nitrophenol
 4. 2-Chlorophenol
 5. 4-Chlorophenol
 6. 4-Chloro-3-methylphenol
 7. 2,4-Dichlorophenol
 8. 2,4,6-Trichlorophenol

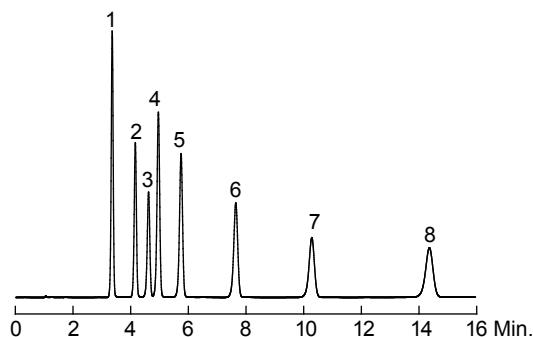

AN: S1163

Phenols


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 55:45
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 280 nm
 Sample: 1. Phenol
 2. 4-Nitrophenol
 3. 2-Chlorophenol
 4. 4-Chlorophenol
 5. 2-Nitrophenol
 6. 4-Chloro-3-methylphenol
 7. 2,4-Dichlorophenol
 8. 2,4,6-Trichlorophenol

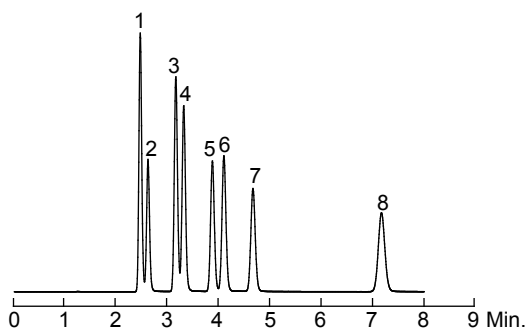

AN: S1174

Polar Acids


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 30:70
 Flow Rate: 0.3 mL/min
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Homovanillic acid
 3. Sorbic acid
 4. *p*-Nitrobenzoic acid
 5. *p*-Toluic acid

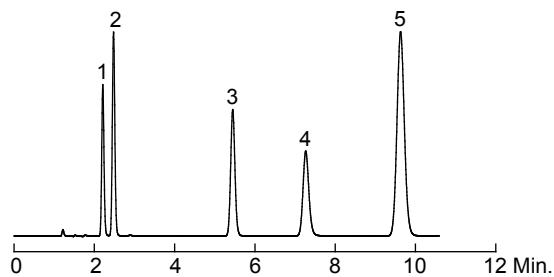

AN: I1125

Polar Acids


Column: Endeavorsil™ 1.8 μm C18, 50 x 2.1 mm
 Cat. No.: **87002**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 20:80
 Flow Rate: 0.5 mL/min
 Temperature: 30 °C
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Homovanillic acid
 3. Sorbic acid
 4. Salicylic acid
 5. *p*-Chlorobenzoic acid
 6. *p*-Nitrobenzoic acid

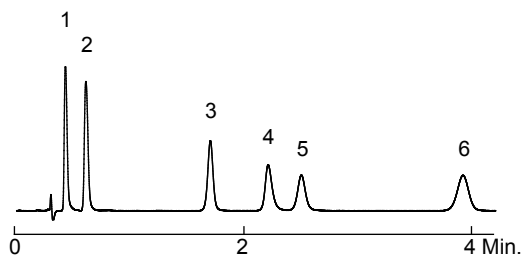

AN: E1111

Polar Acids


Column: Leapsil™ 2.7 μm C18, 50 x 2.1 mm
 Cat. No.: **86004**
 Mobile Phase: 0.1% HCOOH in MeCN:0.1% HCOOH in H₂O = 25:75
 Flow Rate: 0.3 mL/min
 Detection: UV 254 nm
 Sample: 1. *p*-Aminobenzoic acid
 2. Homovanillic acid
 3. Sorbic acid
 4. Salicylic acid
 5. *p*-Nitrobenzoic acid
 6. *p*-Toluic acid

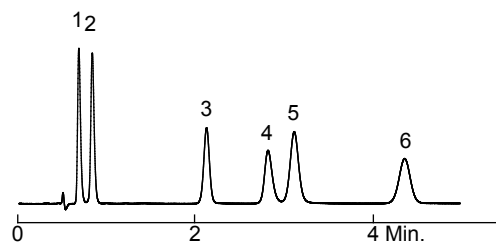

AN: L1109

Sweeteners


Column: Inspire™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **81001**
 Mobile Phase: MeOH:20 mM CH₃COONH₄ (pH 5) = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Acesulfame K
 2. Sodium saccharin
 3. Aspartame

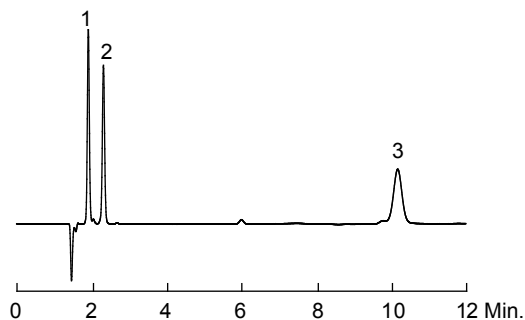

AN: I1120

Sweeteners


Column: Spursil™ 5 μm C18, 150 x 4.6 mm
 Cat. No.: **82001**
 Mobile Phase: MeOH:20 mM CH₃COONH₄ (pH 5) = 30:70
 Flow Rate: 1.0 mL/min
 Temperature: Ambient
 Detection: UV 210 nm
 Sample: 1. Acesulfame K
 2. Sodium saccharin
 3. Aspartame

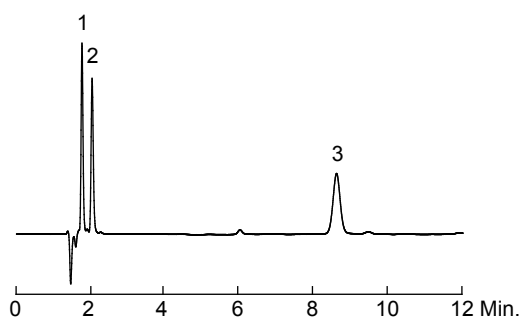

AN: S1164

Sweeteners


Column: Spursil™ 5 μm C18-EP, 150 x 4.6 mm
Cat. No.: **82101**
Mobile Phase: MeOH:20 mM CH₃COONH₄ (pH 5) = 30:70
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 210 nm
Sample: 1. Acesulfame K
2. Sodium saccharin
3. Aspartame

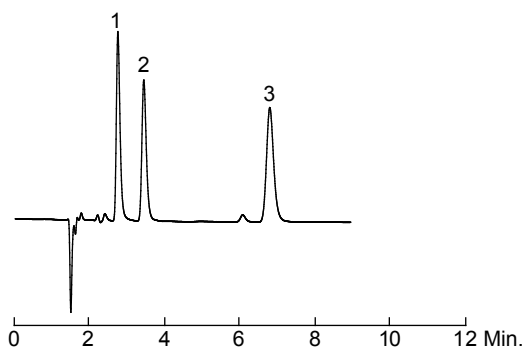

AN: S1165

Unsaturated Fatty Acids

Column: Inspire™ 5 μm C18, 150 x 4.6 mm
Cat. No.: **81001**
Mobile Phase: 0.1% TFA in MeCN:0.1% TFA in H₂O = 95:5
Flow Rate: 1.5 mL/min
Temperature: Ambient
Detection: UV 214 nm
Sample: 1. Linolenic acid
2. Linoleic acid
3. Oleic acid

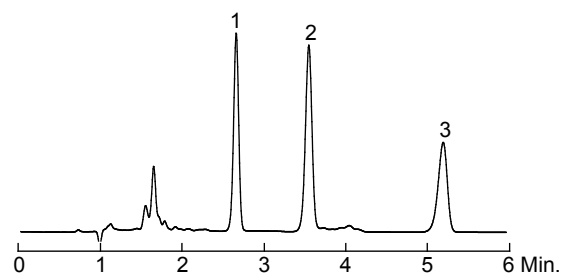

AN: I1121

Antioxidants

Column: Inspire™ 5 μm C18, 150 x 4.6 mm

Cat. No.: **81001**

Mobile Phase A: 5% CH₃COOH in H₂O

Mobile Phase B: MeCN:MeOH = 50:50

Flow Rate: 1.0 mL/min


Temperature: Ambient

Detection: UV 280 nm

Sample:

1. Propyl gallate	6. Ionox 100
2. TBHQ	7. Octyl gallate
3. THBP	8. BHT
4. NDGA	9. Lauryl gallate
5. BHA	

t / min.	0	10
A / %	50	0
B / %	50	100

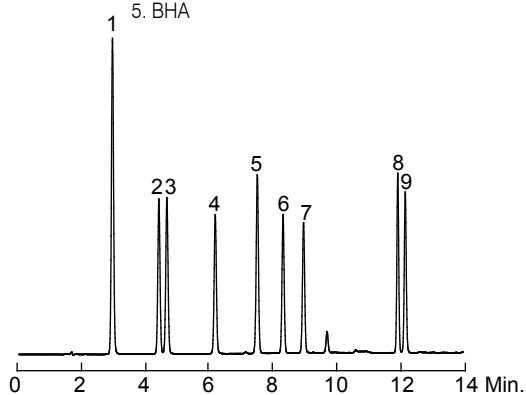

AN: I1122

Proteins

Column: Bio-Bond™ 5 μm C18, 150 x 4.6 mm

Cat. No.: **84001**

Mobile Phase A: 0.1% TFA in H₂O

Mobile Phase B: 0.1% TFA in MeCN


Flow Rate: 1.0 mL/min

Detection: UV 280 nm

Sample:

- Cytochrome C
- Insulin
- Lysozymes

t / min.	0	10
A / %	70	50
B / %	30	50

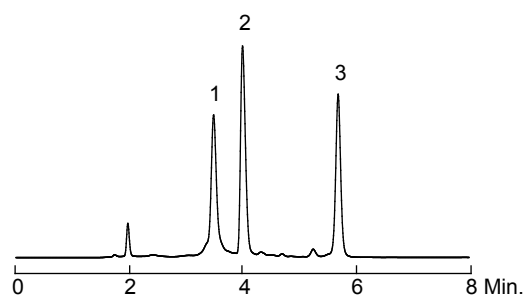


AN: B1101

Others

Phenols


Column: Spursil™ 5 µm C18-EP, 150 x 4.6 mm
Cat. No.: **82101**
Mobile Phase: MeCN:0.1% HCOOH in H₂O = 25:75
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 270 nm
Sample: 1. Phenol 6. 2,4-Dimethylphenol
2. 4-Nitrophenol 7. 4-Chloro-3-methylphenol
3. 2-Chlorophenol 8. 2,4-Dichlorophenol
4. 2,4-Dinitrophenol 9. 2,4,6-Trichlorophenol
5. 2-Nitrophenol 10. Pentachlorophenol

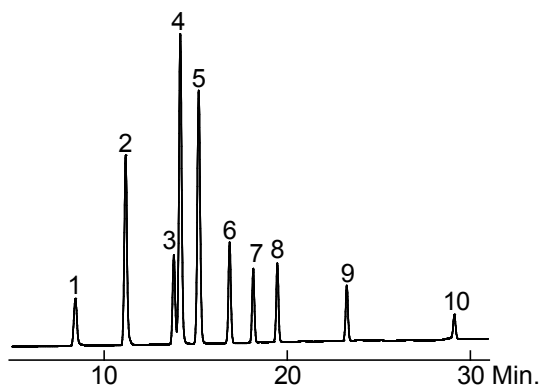

AN: S1166

Steroids


Column: Endeavorsil™ 1.8 µm C18, 50 x 2.1 mm
Cat. No.: **87002**
Mobile Phase: MeOH:H₂O = 50:50
Flow Rate: 0.5 mL/min
Temperature: 30 °C
Detection: UV 254 nm
Sample: 1. Prednisone
2. Prednisolone
3. Dexamethasone
4. Hydrocortisone 21-acetate
5. 11-α-Hydroxyprogesterone

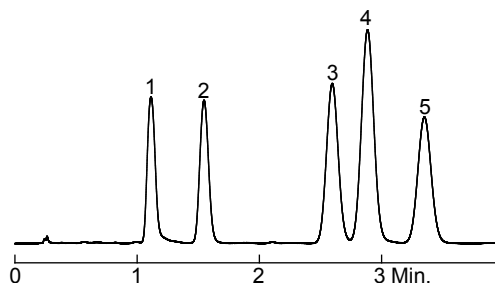

AN: E1112

Steroids

Column: Inspire™ 5 µm C18, 150 x 4.6 mm
Cat. No.: **81001**
Mobile Phase: MeOH:H₂O = 55:45
Flow Rate: 1.0 mL/min
Temperature: Ambient
Detection: UV 254 nm
Sample: 1. Prednisone 4. Dexamethasone
2. Cortisone 5. Hydrocortisone 21-acetate
3. Prednisolone 6. 11-α-Hydroxyprogesterone

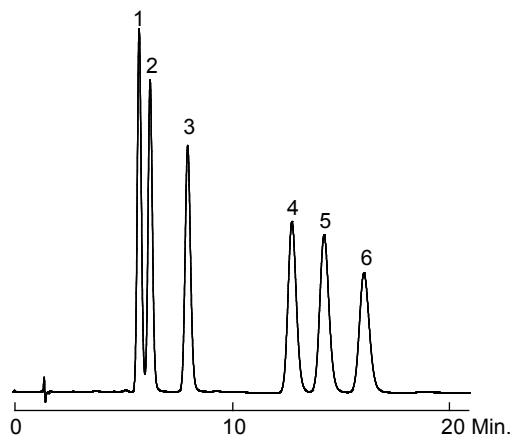

AN: I1123

Industry Index

Environmental.....	154
Petrochemicals.....	168
Chemicals	183
Solvents.....	192
Food	200
Pharmaceutical	208

Product Index

DM-1 / DM-1MS

Air Sample: TO-14.....	154
Citronella Java Oil	205
Fatty Acids (Free)	200
Flavor Volatiles	203
Fragrance	206
Gasoline Aromatics.....	180
Hydrocarbons, C7 - C42.....	179
Oxygenates MTBE	175
Petroleum Oxygenates.....	175
Solvents Mixture #1	193
Solvents Mixture #2	195
Solvents Mixture #3	197
Sulfide.....	176
Sulfur in Gasoline	176
Sulfur in Naphtha.....	176
USP Solvents.....	192

DM-5 / DM-5MS

Alcohols.....	187
Basic Drugs.....	208
Benzidines / Phenols (EPA 604 / 605).....	161
Butyl Tins	165
Chlorinated Hydrocarbons (EPA 612).....	160
Food Packaging Volatiles.....	206
Glycols / Alcohols.....	187
Nitrogen-Containing Herbicides	163
Organochlorine Pesticides	162
Organochlorine Pesticides (EPA 8081).....	164
PAHs (EPA 610).....	157
PAEs	167
Solvents.....	199
Steroids, Anabolic	210

DM-5 Amine

Amines / Phenols	185
Antihistamines	210
Ethylenediamines.....	184
Sympathomimetic Amines Drugs	209

DM-5MS / LB

PAHs (EPA 610).....	156
Phenols (EPA 528).....	158
Semi-volatile Organic Compounds.....	159
Volatile Organic Compounds (EPA 526).....	158

DM-17

BHA / BHT	206
Chlorophenoxyacid Herbicides (EPA 515.1).....	165
Organochlorine Pesticides (EPA 8081).....	164
PAEs (EPA 8060)	160
Phenols (EPA 604).....	161
Triazine Herbicides (EPA 619)	165

DM-1701

Acrylic Esters.....	191
Formaldehyde	189

GC Applications Index


Fragrance	206
Organochlorine Pesticides (EPA 8081)	164
Styrene Impurities.....	191
DM-35	
Acidic / Neutral Drugs	209
Basic Drugs.....	208
Chlorinated Hydrocarbons (EPA 612)	160
Chlorophenoxyacid Herbicides (EPA 615).....	165
Endocrine Disruptors Butyl Tins (Hexyl Derivatives)	167
Nitrogen-Containing Herbicides	163
Organochlorine Pesticides (EPA 8081)	164
Organophosphorus Pesticides (EPA 8140 / 8141 / 8141A).....	162
DM-35 Amine	
Cold Medicine	210
Ethanolamines.....	184
Primary Amines	183
Sympathomimetic Amines Drugs	209
DM-200	
Aromatics (Benzene / Toluene / Xylene)	181
Basic Drugs.....	208
Chlorinated Hydrocarbons (EPA 612)	160
Explosives	167
Glycols.....	187
Nitroamines	161
PAHs (EPA 610).....	157
Silanes.....	191
Solvents Mixture #1	194
Solvents Mixture #2	196
Solvents Mixture #3.....	198
USP Solvents.....	192
Volatile Organic Compounds in Water (EPA 551.1)	166
DM-225	
Neutral Sterols.....	207
Sugars (Alditol Acetates).....	207
DM-624 / DM-624MS	
EP Class 1 and Class 2 Solvents	211
Organic Volatile Impurities	211
Organic Volatile Impurities (USP 467)	211
Primary, Second and Tertiary Amines	212
Residual Solvents.....	212
Volatile Organic Compounds (EPA 524.2)	155
DM-2330	
Dioxins.....	155
PUFA (Animal Source)	201
Sugars (Alditol Acetates).....	207
DM-2560	
FAMEs (<i>cis</i> / <i>trans</i> Isomers)	200
DM-2887	
Simulated Distillation.....	178
DM-AQUA	
Volatile Organic Compounds in Water.....	166
DM-BDTG Metal	
Glycerin in Biodiesel (ASTM D6584)	177
DM-FAMEWAX	
FAMEs (Black Currant Seed Oil)	202
FAMEs (Flax Seed Oil)	202
FAMEs (Marine Oil Standard)	202
DM-FFAP	
Alcoholic Standard: Acids and Esters	204
Fatty Acids (Free)	200
DM-HT SimDist Metal	
Bleed Profile	177
Hydrocarbons, C10 - C44	178
Hydrocarbons, C30 - C110	178

Hydrocarbons, C44 - C100	177
DM-InertWax	
Aldehydes	188
FAMEs	201
DM-PAH	
PAHs	156
DM-PLOT Alumina	
1,3-Butadiene Purity	172
Hydrocarbons	173
Propylene Purity	171
Refinery Gas	172
DM-PLOT Alumina / KCl	
Butane Lighter Fluid	170
DM-PLOT Alumina / Na₂SO₄	
Refinery Gas	170
DM-PLOT CFC	
Impurity Analysis of 1,1,1,2-Tetrafluoroethane	170
DM-PLOT MS 5A	
Permanent Gases	168, 169
DM-PLOT Q	
Alcohols	186
Hydrocarbon Gases	171, 172, 173
Permanent Gases	168, 169
Polar Solvents	199
DM-PLOT QS	
Natural Gas #2	170
DM-PLOT S / DM-PLOT U	
Hydrocarbon Gases	172
Permanent Gases	169
Polar Solvents	199
DM-PONA	
Detailed Hydrocarbons Analysis	179
DM-TCEP	
Aromatics	181
Petroleum Oxygenates	174
DM-TVOC	
TVOCs	154
DM-Volatile Amine	
Short Chain Amines in Water	183
DM-Wax	
Alcohols	186
Alcohols / Aldehydes	188
Aldehydes	189
Amines / Alcohols / Chlorides	185
Aromatics	181, 182
Concentrated Liquors	204
Esters	190
Flavor Volatiles	203
Glycols	187
Ketones	189
Peppermint Oil	205
Petroleum Oxygenates	174
PUFA (Animal Source)	201
Solvents Mixture #1	194
Solvents Mixture #2	196
Solvents Mixture #3	198
Styrene Impurities	191
DM-Wax Amine	
Amines (Low MW)	183
Hexamethylenediamine	184
Nitrosamines	185
Primary Amines (Low MW)	183

Volatiles

TVOCs


Column: DM-TVOC, 50 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7831
 Index: CEO00010
 Carrier Gas: N₂
 Oven Temp.: 50 °C (hold 10 min) to 250 °C at 5 °C/min
 Injection: Split, 10:1, 250 °C 1 μ L
 Detector: FID, 250 °C

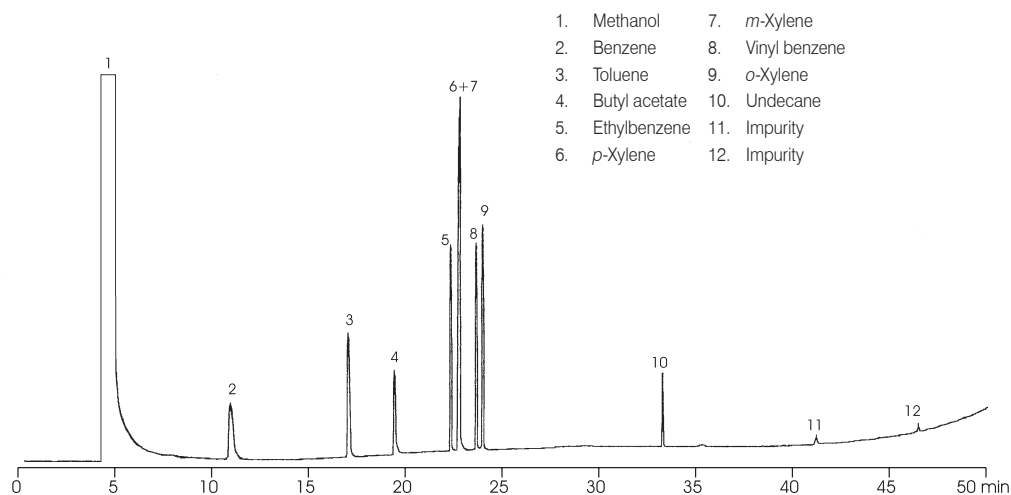

Air Sample: TO-14

Column: DM-1, 60 m x 0.32 mm x 3.00 μ m
 Cat. No.: 7142
 Index: CER00018
 Oven Temp.: 30 °C (hold 4 min) to 250 °C (hold 15 min) at 7 °C/min
 Carrier Gas: He, 21 cm/sec, 30 °C
 Detector: MS, 250 °C
 Ionization: EI
 Scan Range: 34-280 AMU
 Cryotrap Temp.: -160 °C
 Cryotrap Desorb Temp.: 150 °C


- | | | |
|---|---------------------------------------|-------------------------------|
| 1. Dichlorodifluoromethane | 14. Chloroform | 28. Ethylbenzene |
| 2. Chloromethane | 15. 1,2-Dichloroethane | 29. <i>m</i> -Xylene |
| 3. 1,2-Dichlorotetrafluoroethane | 16. 1,1,1-Trichloroethane | 30. <i>p</i> -Xylene |
| 4. Vinyl chloride | 17. Benzene | 31. Styrene |
| 5. Bromomethane | 18. Carbon tetrachloride | 32. <i>o</i> -Xylene |
| 6. Chloroethane | 19. 1,2-Dichloropropane | 33. 1,1,2,2-Tetrachloroethane |
| 7. Trichlorofluoromethane | 20. Trichloroethylene | 34. 4-Methyltoluene |
| 8. 1,1-Dichloroethene | 21. <i>cis</i> -1,3-Dichloropropene | 35. 1,3,5-Trimethylbenzene |
| 9. Methylene chloride | 22. <i>trans</i> -1,3-Dichloropropene | 36. 1,2,4-Trimethylbenzene |
| 10. 3-Chloropropene | 23. 1,1,2-Trichloroethane | 37. 1,3-Dichlorobenzene |
| 11. 1,1,2-Trichloro-1,2,2-trifluoroethane | 24. Toluene | 38. 1,4-Dichlorobenzene |
| 12. 1,1-Dichloroethane | 25. 1,2-Dibromoethane | 39. 1,2-Dichlorobenzene |
| 13. <i>cis</i> -1,2-Dichloroethene | 26. Tetrachloroethene | 40. 1,2,4-Trichlorobenzene |
| | 27. Chlorobenzene | 41. Hexachlorobutadiene |

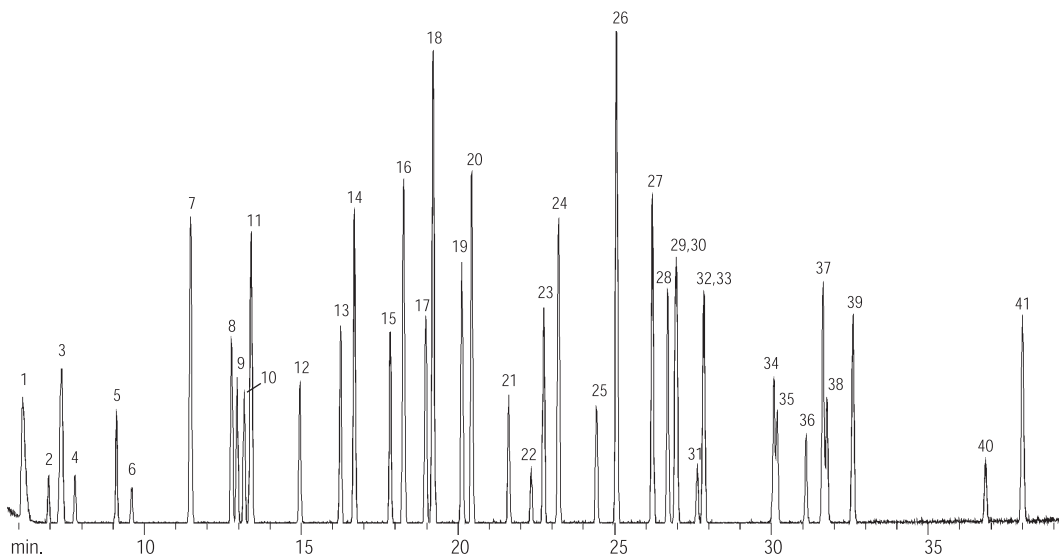

Volatile Organic Compounds (EPA 524.2)

Column: DM-624, 75 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7752
 Index: CER00011
 Oven Temp.: 35 $^{\circ}$ C (hold 8 min) to 220 $^{\circ}$ C (hold 3 min) at 10 $^{\circ}$ C/min
 Detector: MS, 250 $^{\circ}$ C
 Scan Range: 45 - 300 AMU
 Purging Time: 11 min
 Sorbent Tube: Tenax / Silica gel / Active carbon
 Desorb Temp.: 220 $^{\circ}$ C (hold 2 min), at 225 $^{\circ}$ C
 Desorb Speed.: 10 mL/min


1. Dichlorodifluoromethane
2. Chloromethane
3. Vinyl chloride
4. Bromomethane
5. Chloroethane
6. Trichlorofluoromethane
7. 1,1-Dichloroethene
8. Methylene chloride
9. *trans*-1,2-Dichloroethylene
10. 1,1-Dichloropropane
11. *cis*-1,2-Dichloroethylene

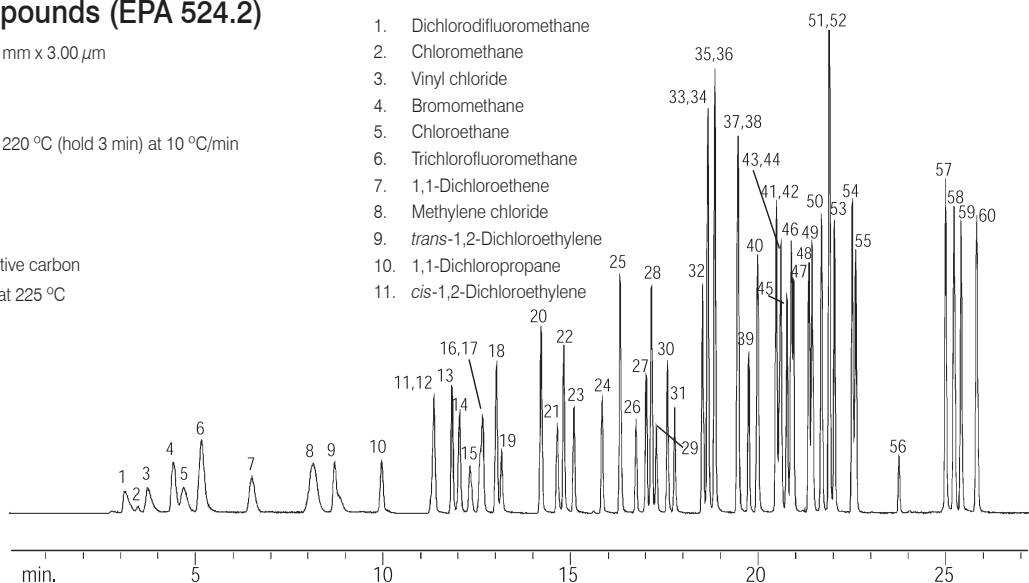

- | | | | | |
|---------------------------|---------------------------------------|-------------------------------|---------------------------------|---------------------------------|
| 12. 2,2-Dichloropropane | 23. Bromodichloromethane | 34. Ethylbenzene | 45. 2-Chlorotoluene | 55. 1,2-Dichlorobenzene |
| 13. Chlorobromomethane | 24. <i>cis</i> -1,3-Dichloropropene | 35. <i>m</i> -Xylene | 46. 1,3,5-Trimethylbenzene | 56. 1,2-Dibromo-3-chloropropane |
| 14. Chloroform | 25. Toluene | 36. <i>p</i> -Xylene | 47. 4-Chlorotoluene | 57. 1,2,4-Trichlorobenzene |
| 15. 1,1,1-Trichloroethane | 26. <i>trans</i> -1,3-Dichloropropene | 37. <i>o</i> -Xylene | 48. <i>tert</i> -Butylbenzene | 58. Hexachlorobutadiene |
| 16. Tetrachloromethane | 27. 1,1,2-Trichloroethane | 38. Styrol | 49. 1,2,4-Trimethylbenzene | 59. Naphthalene |
| 17. 1,1-Dichloropropene | 28. Tetrachloroethylene | 39. Bromoform | 50. <i>sec</i> -Butylbenzene | 60. 1,2,3-Trichlorobenzene |
| 18. Benzene | 29. 1,3-Dichloropropane | 40. Anisoxide | 51. 1,3-Dichlorobenzene | |
| 19. 1,2-Dichloroethane | 30. Dibromochloromethane | 41. Bromobenzene | 52. <i>p</i> -Isopropyl toluene | |
| 20. Trichloroethylene | 31. 1,2-Dibromoethane | 42. 1,1,2,2-Tetrachloroethane | 53. 1,4-Dichlorobenzene | |
| 21. 1,2-Dichloropropane | 32. Chlorobenzene | 43. 1,2,3-Trichloropropane | 54. <i>n</i> -Butylbenzene | |
| 22. Dibromomethane | 33. 1,1,1,2-Tetrachloroethane | 44. Propylbenzene | | |

Dioxins


Column: DM-2330, 60 m x 0.25 mm x 0.20 μ m
 Cat. No.: 8624
 Index: CER00108
 Oven Temp.: 200 $^{\circ}$ C (hold 1 min) to 250 $^{\circ}$ C (hold 15 min) at 8 $^{\circ}$ C/min,
 to 275 $^{\circ}$ C (hold 5 min) at 15 $^{\circ}$ C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Splitless, 275 $^{\circ}$ C
 Sample: TCDD isomers, 2.0 μ L
 Detector: ECD, 21 kHz full scale, 275 $^{\circ}$ C

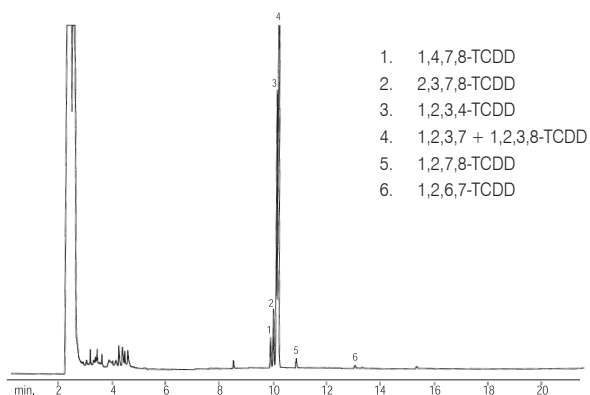

1. 1,4,7,8-TCDD
2. 2,3,7,8-TCDD
3. 1,2,3,4-TCDD
4. 1,2,3,7 + 1,2,3,8-TCDD
5. 1,2,7,8-TCDD
6. 1,2,6,7-TCDD

Dioxins

Column: DM-2330, 60 m x 0.32 mm x 0.20 μ m
 Cat. No.: 8634
 Index: CER00109
 Oven Temp.: 200 $^{\circ}$ C (hold 1 min) to 240 $^{\circ}$ C (hold 6 min) at 3 $^{\circ}$ C/min,
 to 275 $^{\circ}$ C (hold 30 min) at 15 $^{\circ}$ C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Cold on-column, 275 $^{\circ}$ C
 Sample: TCDD isomers, 1.5 μ L
 Detector: ECD, 5 kHz full scale, 275 $^{\circ}$ C

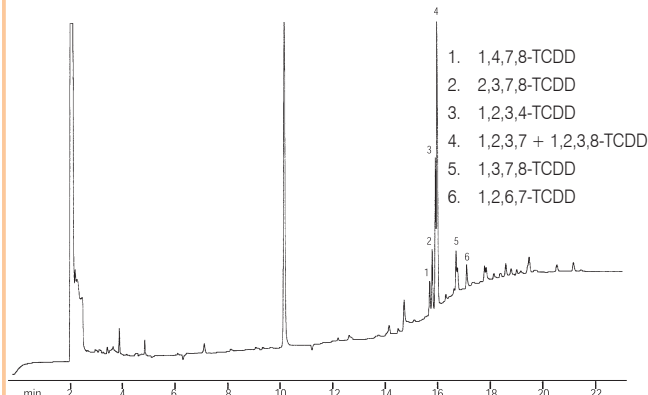


1. 1,4,7,8-TCDD
2. 2,3,7,8-TCDD
3. 1,2,3,4-TCDD
4. 1,2,3,7 + 1,2,3,8-TCDD
5. 1,3,7,8-TCDD
6. 1,2,6,7-TCDD

Semi-volatiles

PAHs

Column: DM-PAH, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: **8862**
 Index: CER1160
 Sample: EPA 8310 PAHs in dichloromethane solution, 10 ppm
 Oven Temp.: 65 $^{\circ}$ C (hold 0.5 min) to 220 $^{\circ}$ C at 15 $^{\circ}$ C/min,
 to 330 $^{\circ}$ C (hold 15 min) at 4 $^{\circ}$ C/min
 Carrier Gas: He, 2.0 mL/min
 Injection: Splitless (hold 1.75 min), 0.5 μ L, 320 $^{\circ}$ C
 Makeup Gas: 75 mL/min
 Detector: FID, 320 $^{\circ}$ C


- | | | |
|------------------------|--------------------------|------------------------------|
| 1. Naphthalene | 10. Pyrene | 19. Dibenzo[a,h]acridine |
| 2. 2-Methylnaphthalene | 11. Benzo[a]anthracene | 20. Dibenzo[a,i]acridine |
| 3. 1-Methylnaphthalene | 12. Chrysene | 21. Indeno[1,2,3-cd]pyrene |
| 4. Acenaphthylene | 13. Triphenylene | 22. Dibenzo[a,h]anthracene |
| 5. Acenaphthene | 14. Benzo[b]fluoranthene | 23. Benzo[ghi]perylene |
| 6. Fluorene | 15. Benzo[k]fluoranthene | 24. 7H-Dibenzo[c,g]carbazole |
| 7. Phenanthrene | 16. Benzo[j]fluoranthene | 25. Dibenzo[a,e]pyrene |
| 8. Anthracene | 17. Benzo[a]pyrene | 26. Dibenzo[a,i]pyrene |
| 9. Fluoranthene | 18. 3-Methylcholanthrene | 27. Dibenzo[a,h]pyrene |

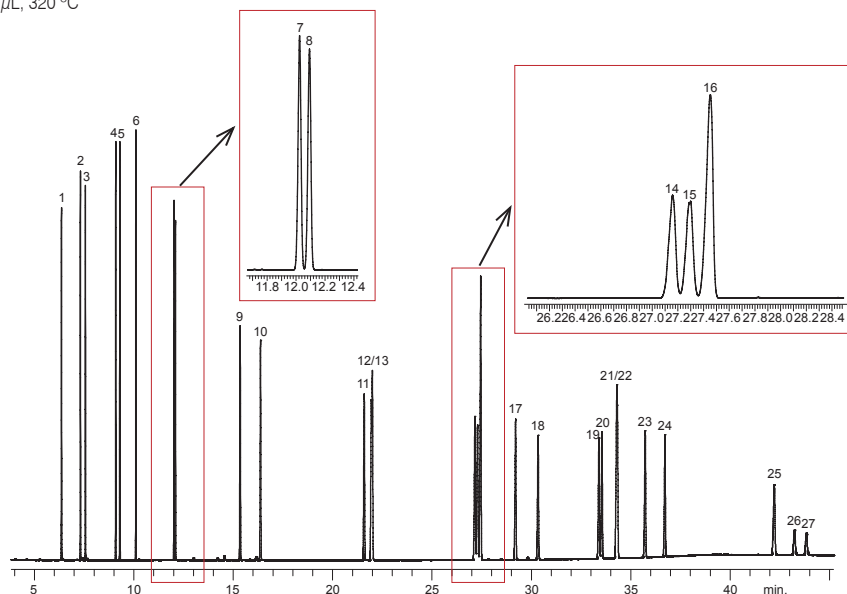

PAHs (EPA 610)

Column: DM-5 MS / LB, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: **8721**
 Index: CER00595
 Oven Temp.: 40 $^{\circ}$ C (hold 2 min) to 250 $^{\circ}$ C at 25 $^{\circ}$ C/min
 to 265 $^{\circ}$ C at 5 $^{\circ}$ C/min, to 300 $^{\circ}$ C (hold 4 min) at 25 $^{\circ}$ C/min
 Carrier Gas: H₂, 4 mL/min constant flow
 Injection: Splitless hold 2 min, 330 $^{\circ}$ C
 2 mm splitless inlet liner w / wool
 Sample: PAHs standard, 1.0 μ L, 50 μ g/mL
 Detector: FID, 350 $^{\circ}$ C


1. Naphthalene
2. Acenaphthylene
3. Acenaphthene
4. Fluorene
5. Phenanthrene
6. Anthracene
7. Fluoranthene
8. Pyrene
9. Benzo[a]anthracene
10. 1,2-Benzphenanthrene
11. Benzo[b]fluoranthene
12. Benzo[k]fluoranthene
13. Benzo[a]pyrene
14. Indeno[1,2,3-cd]pyrene
15. Dibenzo[a,h]anthracene
16. Benzo[ghi]perylene

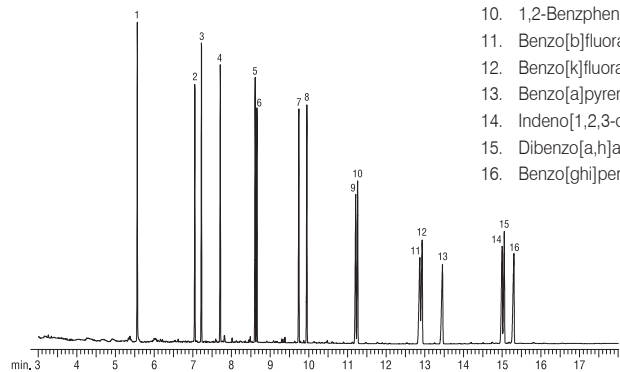

V.S.

PAHs (EPA 610)


Column: DM-5 MS / LB, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: **8723**
 Index: CER00549
 Oven Temp.: 40 $^{\circ}$ C (hold 1 min) to 200 $^{\circ}$ C at 20 $^{\circ}$ C/min
 to 310 $^{\circ}$ C (hold 5 min) at 4 $^{\circ}$ C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Splitless hold 1 min, 300 $^{\circ}$ C
 Sample: PAHs standard, 1.0 μ L, 20 ng/ μ L
 Detector: FID, 310 $^{\circ}$ C

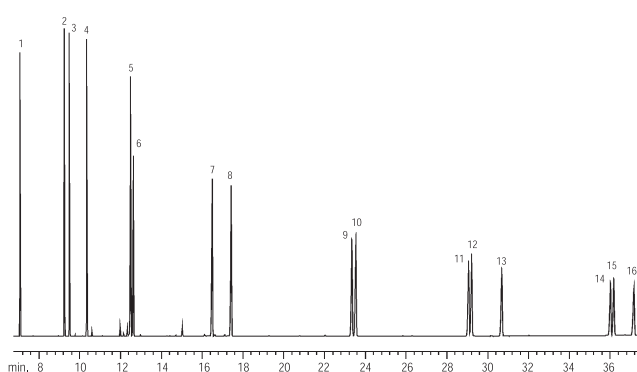

PAHs (EPA 610)

Column: DM-5, 30 m x 0.53 mm x 1.50 μ m
 Cat. No.: 7251
 Index: CER00043
 Oven Temp.: 4 °C (hold 6 min) to 300 °C (hold 15 min) at 10 °C/min
 Carrier Gas: H₂, 80 cm/sec
 Injection: Direct, 300 °C
 Sample: PAHs standard, 2.5 μ L
 Detector: FID, 8 x 10⁻¹¹ AFS, 300 °C


- | | |
|-------------------|----------------------------|
| 1. Naphthalene | 9. Benzo[a]anthracene |
| 2. Acenaphthylene | 10. 1,2-Benzphenanthrene |
| 3. Acenaphthene | 11. Benzo[b]fluoranthene |
| 4. Fluorene | 12. Benzo[k]fluoranthene |
| 5. Phenanthrene | 13. Benzo[a]pyrene |
| 6. Anthracene | 14. Indeno[1,2,3-cd]pyrene |
| 7. Fluoranthene | 15. Dibenzo[a,h]anthracene |
| 8. Pyrene | 16. Benzo[ghi]perylene |

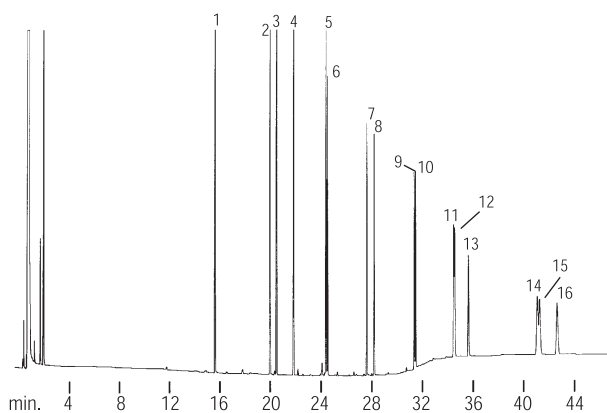

PAHs (EPA 610)


Column: DM-5, 30 m x 0.32 mm x 0.25 μ m
 Cat. No.: 7231
 Index: CER00376
 Oven Temp.: 35 °C (hold 4 min) to 325 °C at 10 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Direct, cold on-column
 Sample: PAHs standard, 0.5 μ L
 Detector: FID, 8 x 10⁻¹¹ AFS, 325 °C

- | | |
|-------------------|----------------------------|
| 1. Naphthalene | 9. Benzo[a]anthracene |
| 2. Acenaphthylene | 10. 1,2-Benzphenanthrene |
| 3. Acenaphthene | 11. Benzo[b]fluoranthene |
| 4. Fluorene | 12. Benzo[k]fluoranthene |
| 5. Phenanthrene | 13. Benzo[a]pyrene |
| 6. Anthracene | 14. Indeno[1,2,3-cd]pyrene |
| 7. Fluoranthene | 15. Dibenzo[a,h]anthracene |
| 8. Pyrene | 16. Benzo[ghi]perylene |

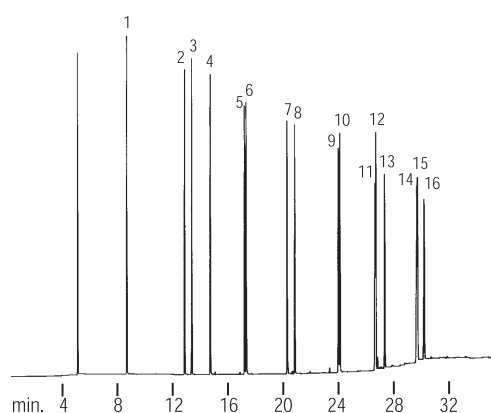

PAHs (EPA 610)

Column: DM-200, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 8321
 Index: CER00044
 Oven Temp.: 40 °C (hold 4 min) to 340 °C at 10 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 40:1, 340 °C
 Sample: PAHs standard, 1.2 μ L
 Detector: FID, 16 x 10⁻¹¹ AFS, 340 °C

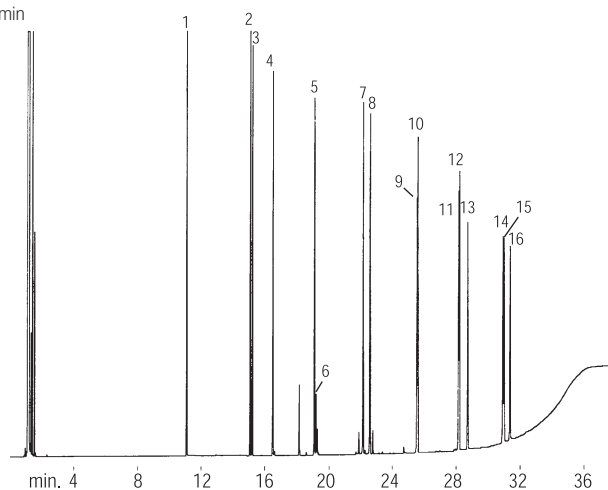


- | |
|----------------------------|
| 1. Naphthalene |
| 2. Acenaphthylene |
| 3. Acenaphthene |
| 4. Fluorene |
| 5. Phenanthrene |
| 6. Anthracene |
| 7. Fluoranthene |
| 8. Pyrene |
| 9. Benzo[a]anthracene |
| 10. 1,2-Benzphenanthrene |
| 11. Benzo[b]fluoranthene |
| 12. Benzo[k]fluoranthene |
| 13. Benzo[a]pyrene |
| 14. Indeno[1,2,3-cd]pyrene |
| 15. Dibenzo[a,h]anthracene |
| 16. Benzo[ghi]perylene |

Semi-volatiles

Volatile Organic Compounds (EPA 526)


Column: DM-5 MS / LB, 30 m x 0.25 mm x 0.25 μ m
Cat. No.: 8721
Index: CER00656
Oven Temp.: 50 °C (hold 1 min) to 200 °C (hold 5 min) at 20 °C/min,
to 310 °C (hold 3 min) at 30 °C/min
Carrier Gas: He, 0.8 mL/min
Injection: Splitless hold 0.3 min, 300 °C
Sample: EPA 526 mix, 1 μ L, 10 ppm
Transfer line Temp.: 280 °C
Tune: DFTPP
Solvent Delay: 5.5 min
Ionization: EI
Scan Range: 35 - 550 AMU
Detector: MS

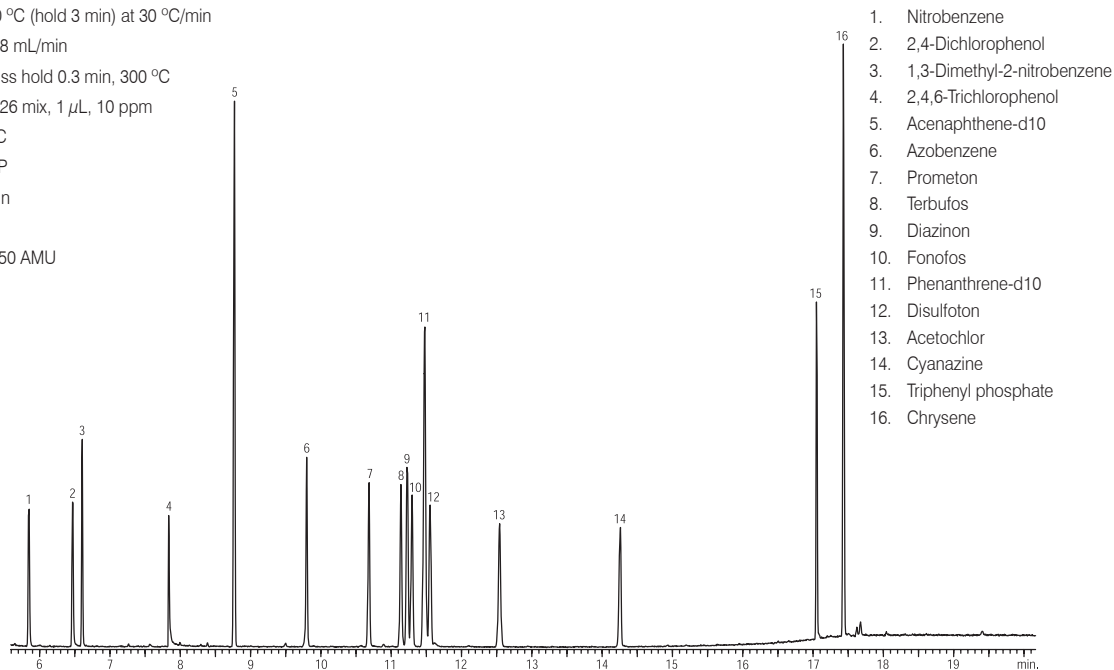

Applications

Phenols (EPA 528)

Column: DM-5 MS / LB, 30 m x 0.25 mm x 0.25 μ m
Cat. No.: 8721
Index: CER00664
Oven Temp.: 40 °C (hold 1 min) to 220 °C at 12 °C/min,
to 300 °C (hold 1 min) at 30 °C/min
Carrier Gas: He, 1.3 mL/min, constant flow
Injection: Splitless, 220 °C
Sample: EPA 528 mix, 1 μ L, 5 ppm
Transfer line Temp.: 280 °C
Tune: DFTPP
Solvent Delay: 5.5 min
Ionization: EI
Scan Range: 35 - 550 AMU
Detector: MS

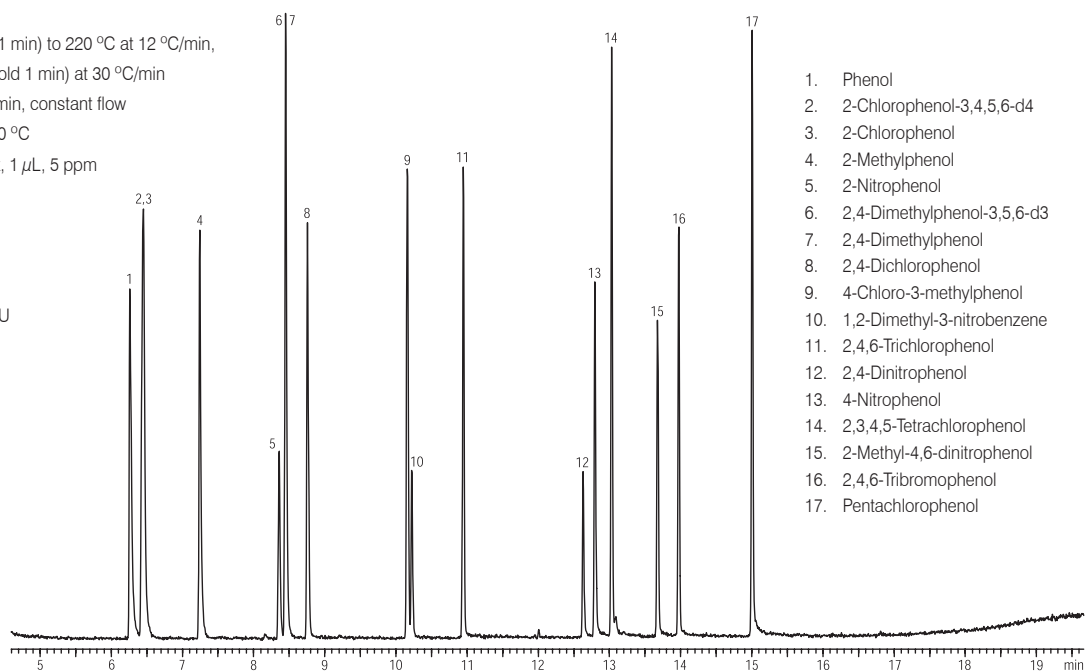

Semi-volatile Organic Compounds

Column: DM-5MS / LB, 30 m x 0.25 mm x 0.50 μ m

Cat. No.: 8723

Index: CER00532

Oven Temp.: 40 °C (hold 2 min) to 290 °C at 20 °C/min,
to 303 °C at 2 °C/min, to 330 °C (hold 1 min) at 6 °C/min

Carrier Gas: He, 1.0 mL/min, constant flow



Injection: Splitless, 300 °C

Sample: EPA 8270 standard, 80 ng

Scan Range: 35 - 550 AMU

Detector: MS, 280 °C


1. *N*-nitrosodimethylamine
2. Pyridine
3. Methyl methanesulfonate
4. 2-Fluorophenol
5. Ethyl methanesulfonate
6. Phenol-d6
7. Phenol
8. Aniline
9. *bis*(2-Chloroethyl)ether
10. 2-Chlorophenol-d4
11. 2-Chlorophenol
12. 1,3-Dichlorobenzene
13. 1,4-Dichlorobenzene-d4
14. 1,4-Dichlorobenzene
15. Benzyl alcohol
16. 1,2-Dichlorobenzene-d4
17. 1,2-Dichlorobenzene
18. 2-Methylphenol
19. *bis*(2-Chloroisopropyl)ether
20. 4-Methylphenol / 3-Methylphenol
21. *N*-Nitroso-*di-n*-propylamine
22. Acetophenone
23. Hexachloroethane
24. Nitrobenzene-d5
25. Nitrobenzene
26. Isophorone
27. 2,4-Dimethylphenol
28. 2-Nitrophenol
29. Benzoic acid
30. *bis*(2-Chloroethoxy)methane
31. 2,4-Dichlorophenol
32. 1,2,4-Trichlorobenzene
33. Naphthalene-d8
34. Naphthalene
35. 2,6-Dichlorophenol
36. 4-Chloroaniline
37. Hexachloropropene
38. Hexachlorobutadiene
39. 4-Chloro-3-methylphenol
40. Isosafrole
41. 2-Methylnaphthalene
42. 1-Methylnaphthalene
43. Hexachlorocyclopentadiene
44. 1,2,4,5-Tetrachlorobenzene
45. 2,4,6-Trichlorophenol
46. 2,4,5-Trichlorophenol
47. 2-Fluorobiphenyl
48. Safrole
49. 2-Chloronaphthalene
50. 2-Nitroaniline
51. 1,4-Naphthoquinone
52. Dimethylphthalate
53. 1,3-Dinitrobenzene
54. 2,6-Dinitrotoluene
55. Acenaphthylene
56. 3-Nitroaniline
57. Acenaphthene-d10
58. Acenaphthene
59. 2,4-Dinitrophenol
60. 4-Nitrophenol
61. Pentachlorobenzene
62. 2,4-Dinitrotoluene
63. Dibenzofuran
64. 2,3,4,6-Tetrachlorophenol
65. Diethyl phthalate
66. 4-Chlorophenyl phenyl ether
67. Fluorene
68. 4-Nitroaniline
69. 4,6-Dinitro-2-methylphenol
70. Diphenylamine
71. Azobenzene
72. 2,4,6-Tribromophenol
73. Phenacetin
74. 4-Bromophenyl phenyl ether
75. Hexachlorobenzene
76. Pentachlorophenol
77. Pentachloronitrobenzene
78. Dinoseb
79. Phenanthrene-d10
80. Phenanthrene
81. Anthracene
82. *di-n*-Butylphthalate
83. 4-Nitroquinoline-1-oxide
84. Isodrin
85. Fluoranthene
86. Benzidine
87. Pyrene
88. Aramite
89. *p*-Terphenyl-d14
90. Chlorbenzilate
91. Benzyl butyl phthalate
92. Kepone
93. *bis*(2-Ethylhexyl)phthalate
94. 3,3'-Dichlorobenzidine
95. Benzo[*a*]anthracene
96. Chrysene-d12
97. Chrysene
98. *di-n*-Octyl phthalate
99. Benzo[*b*]fluoranthene
100. Benzo[*k*]fluoranthene
101. Benzo[*a*]pyrene
102. Perylene-d12
103. 3-Methylcholanthrene
104. Indeno[1,2,3-*cd*]pyrene
105. Dibenzo[*a,h*]anthracene
106. Benzo[*ghi*]perylene

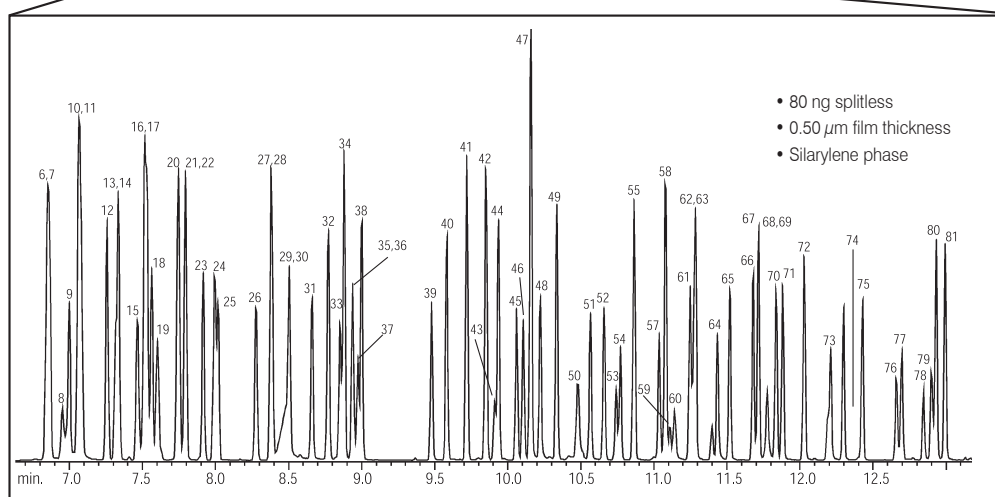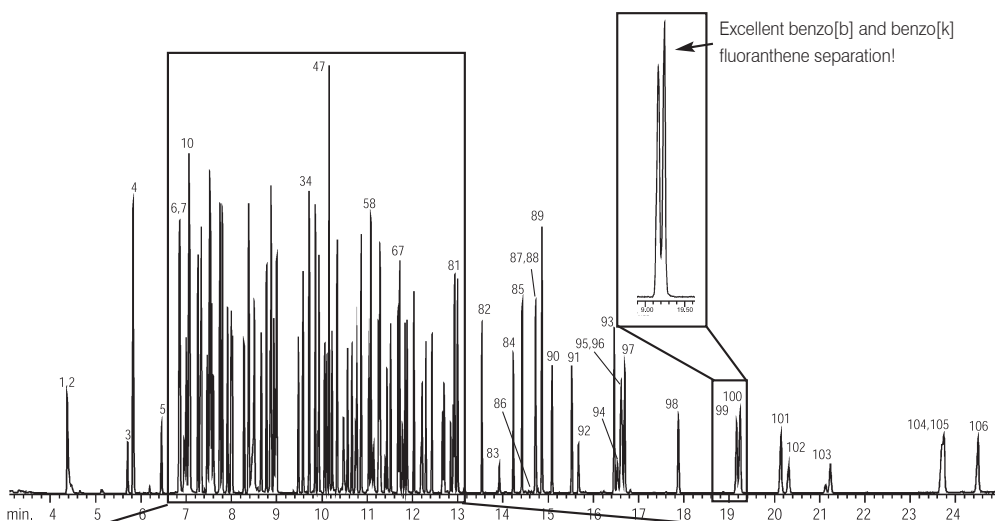

Pesticides

Chlorinated Hydrocarbons (EPA 612)


Column: DM-200, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 8347
 Index: CER00051
 Oven Temp.: 40 °C to 280 °C (hold 5 min) at 8 °C/min
 Carrier Gas: He, 40 cm/sec, 40 °C
 Injection: Direct, 275 °C
 Sample: Chlorinated hydrocarbons mix, 0.5 μ L
 Detector: 220 °C

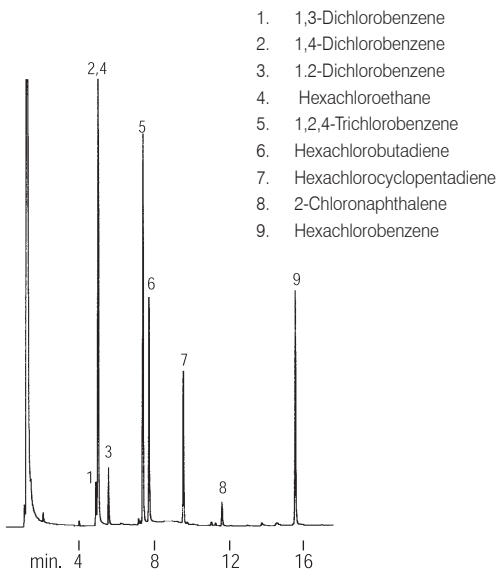

1. 1,3-Dichlorobenzene
2. 1,4-Dichlorobenzene
3. 1,2-Dichlorobenzene
4. Hexachloroethane
5. 1,2,4-Trichlorobenzene
6. Hexachlorobutadiene
7. Hexachlorocyclopentadiene
8. 2-Chloronaphthalene
9. Hexachlorobenzene

PAEs (EPA 8060)


Column: DM-17, 30 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7451
 Index: CER00037
 Oven Temp.: 100 °C to 275 °C (hold 10 min) at 15 °C/min
 Carrier Gas: He, 20 cm/sec
 Injection: Direct, 275 °C
 Sample: PAEs, 1.5 μ L, 60 μ g/mL
 Detector: FID, 64 x 10⁻¹¹ AFS, 275 °C

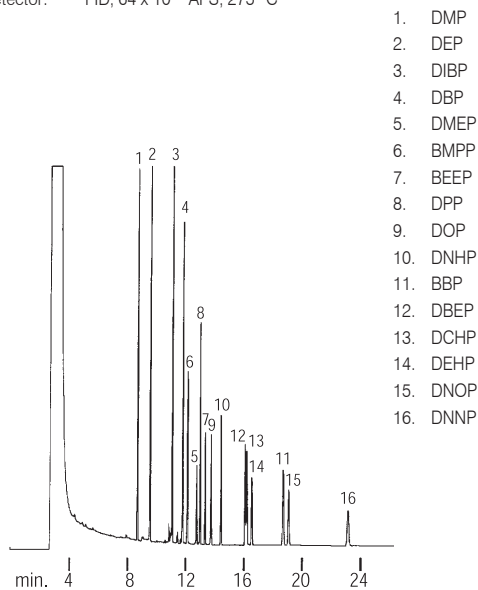

1. DMP
2. DEP
3. DIBP
4. DBP
5. DMEP
6. BMPP
7. BEEP
8. DPP
9. DOP
10. DNHP
11. BBP
12. DBEP
13. DCHP
14. DEHP
15. DNOP
16. DNNP

Chlorinated Hydrocarbons (EPA 612)


Column: DM-35, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7951
 Index: CER00052
 Oven Temp.: 40 °C to 250 °C (hold 5 min) at 8 °C/min
 Carrier Gas: He, 35 cm/sec, 40 °C
 Injection: Direct, 250 °C
 Sample: Chlorinated hydrocarbons, 0.1 μ L
 Detector: 300 °C

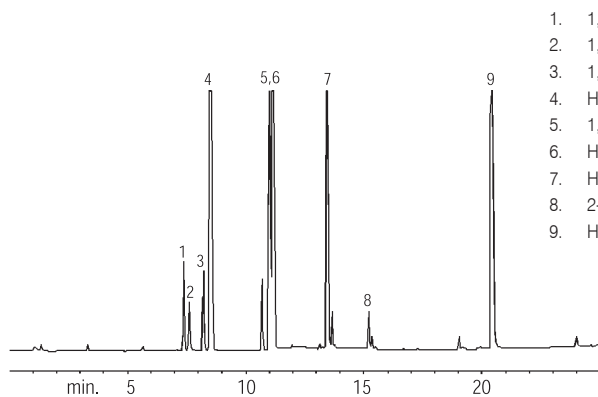

1. 1,3-Dichlorobenzene
2. 1,4-Dichlorobenzene
3. 1,2-Dichlorobenzene
4. Hexachloroethane
5. 1,2,4-Trichlorobenzene
6. Hexachlorobutadiene
7. Hexachlorocyclopentadiene
8. 2-Chloronaphthalene
9. Hexachlorobenzene


V.S.

Column: DM-5, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7247
 Index: CER00053
 Oven Temp.: 40 °C to 250 °C (hold 5 min) at 8 °C/min
 Carrier Gas: He, 35 cm/sec, 40 °C
 Injection: Direct, 250 °C
 Sample: Chlorinated hydrocarbons, 0.1 μ L
 Detector: 300 °C

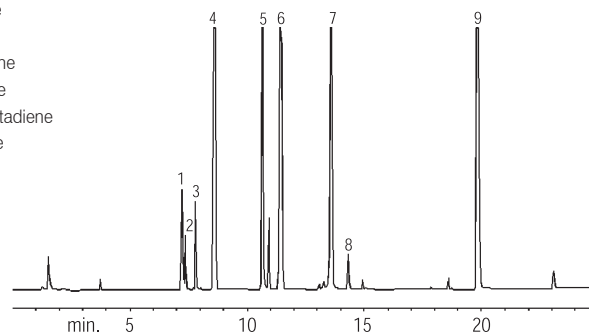


Phenols (EPA 604)

Column: DM-17, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7421
 Index: CER00029
 Oven Temp.: 50 °C (hold 10 min) to 250 °C (hold 15 min) at 15 °C/min
 Carrier Gas: He, 20 cm/sec
 Injection: Split, 40 cc/min, 280 °C
 Sample: Phenols mix, 1.0 μ L, 3 - 5 ng/ μ L
 Detector: FID, 32 x 10⁻¹¹ AFS, 280 °C

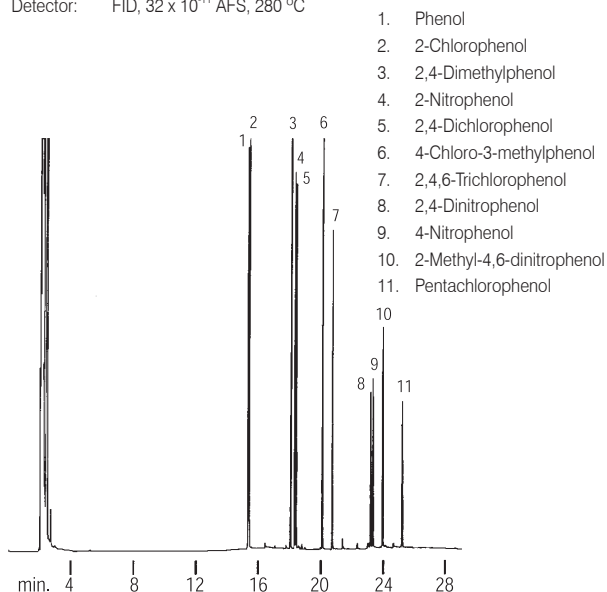

Nitrosamines

Column: DM-200, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 8347
 Index: CER00040
 Oven Temp.: 100 °C (hold 1 min) to 200 °C at 5 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 40 cc/min, 250 °C
 Sample: Nitrosamines mix, 1.0 μ L, 10 μ g/mL
 Detector: FID, 16 x 10⁻¹² AFS, 250 °C


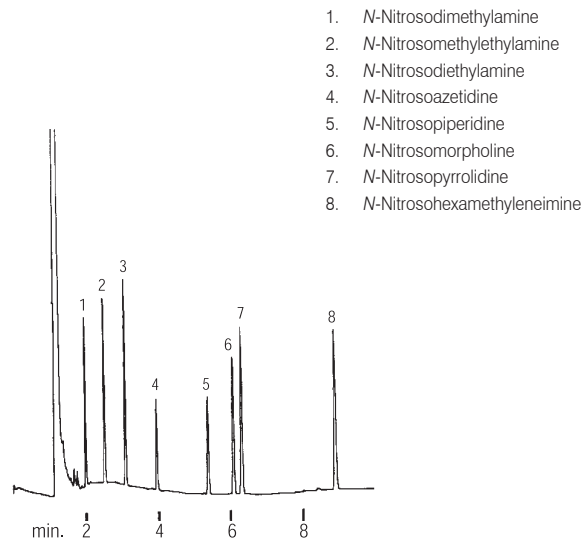


Benzidines / Phenols (EPA 604 / 605)

Column: DM-5, 30 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7235
 Index: CER00032
 Oven Temp.: 110 °C to 290 °C at 8 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 100:1, 310 °C
 Sample: Phenols / Benzidines mix, 1.5 μ L
 Detector: FID, 2 x 10⁻¹¹ AFS, 310 °C

V.S.


Column: DM-5, 30 m x 0.53 mm x 1.50 μ m
 Cat. No.: 7251
 Index: CER00033
 Oven Temp.: 40 °C (hold 6 min) to 300 °C (hold 15 min) at 10 °C/min
 Carrier Gas: H₂, 80 cm/sec
 Injection: Direct, 300 °C
 Sample: Phenols / Benzidines mix, 2.5 μ L
 Detector: FID, 8 x 10⁻¹¹ AFS, 300 °C

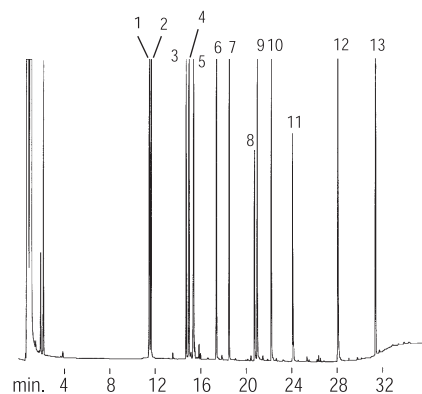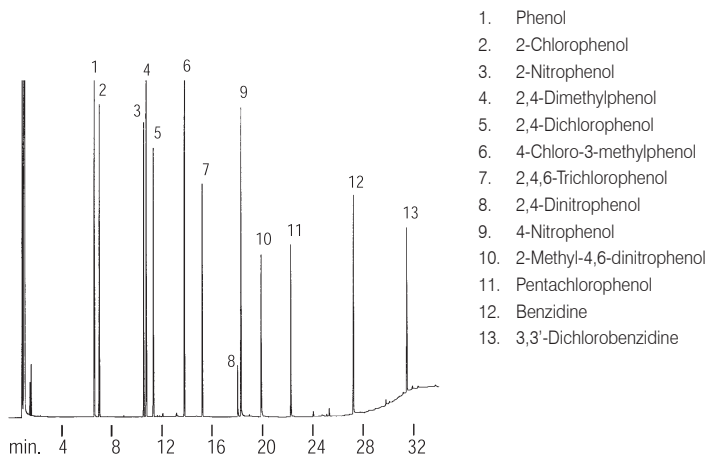

Pesticides

Organophosphorus Pesticides (EPA 8140 / 8141 / 8141A)

Column: DM-35, 30 m x 0.32 mm x 0.25 μ m
 Cat. No.: 7931
 Index: CER00696
 Oven Temp.: 100 °C to 180 °C (hold 2 min) at 10 °C/min to 300 °C at 18 °C/min
 Carrier Gas: He, 42 cm/sec constant flow, 60 °C
 Injection: 0.5 μ L, splitless (hold 5 min), 220 °C
 Detector: FPD, 280 °C

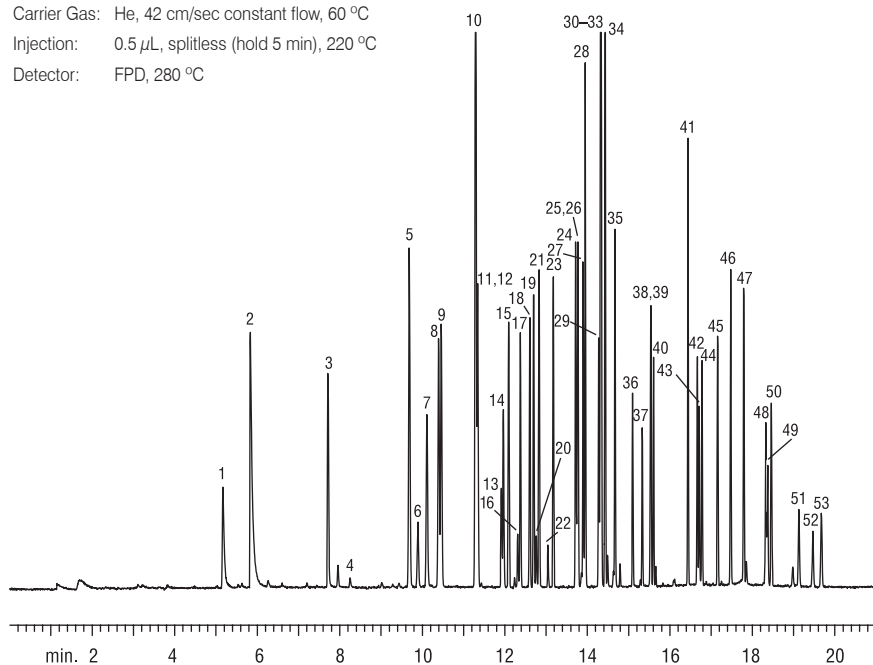


- | | |
|----------------------------|------------------------------------|
| 1. Dichlorvos | 29. Trichloronate |
| 2. Hexamethylphosphoramide | 30. Chlorpyrifos |
| 3. Mevinphos | 31. Fenitrothion |
| 4. Trichlorfon | 32. Merphos |
| 5. Tributyl phosphate | 33. Malathion |
| 6. Demeton-O | 34. Parathion-ethyl |
| 7. TEPP | 35. Fenthion |
| 8. Thionazin | 36. Chlorfenvinphos |
| 9. Ethoprop | 37. Crotoxyphos |
| 10. Sulfotepp | 38. Merphos oxone |
| 11. Naled | 39. Tokuthion |
| 12. Phorate | 40. Stirofos |
| 13. Dicrotophos | 41. Ethion |
| 14. Demeton-S | 42. Bolstar |
| 15. Terbufos | 43. Fensulfothion |
| 16. Monocrotophos | 44. Carbofenthothion |
| 17. Diazinon | 45. Famphur |
| 18. Fonophos | 46. Triphenyl phosphate |
| 19. Disulfoton | 47. EPN |
| 20. Dioxathion | 48. Phosmet |
| 21. Dimethoate | 49. Leptophos |
| 22. Phosphamidon isomer | 50. <i>tri-o</i> -Cresyl phosphate |
| 23. Dichlorofenthion | 51. Azinphos-methyl |
| 24. Chlorpyrifos methyl | 52. Azinphos-ethyl |
| 25. Phosphamidon | 53. Coumaphos |
| 26. Ronnel | |
| 27. Parathion-methyl | |
| 28. Aspon | |

Applications

Organochlorine Pesticides

Column: DM-5, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7221
 Index: CER00083
 Oven Temp.: 60 °C to 300 °C (hold 10 min) at 4 °C/min
 Carrier Gas: He, 30 cm/sec
 Injection: Splitless, 250 °C
 Sample: Pesticides mix, 2.0 μ L
 Detector: 320 °C


- | | | |
|-------------------------------------|--|---|
| 1. Etridiazole 50 pg/ μ L | 11. δ -BHC 20 pg/ μ L | 22. Endrin 30 pg/ μ L |
| 2. Chlorneb 1000 pg/ μ L | 12. Chlorothalonil 50 pg/ μ L | 23. Endosulfan II 30 pg/ μ L |
| 3. Propachlor 1000 pg/ μ L | 13. Heptachlor 20 pg/ μ L | 24. Chlorobenzilate 1000 pg/ μ L |
| 4. Trifluralin 50 pg/ μ L | 14. Aldrin 30 pg/ μ L | 25. 4,4'-DDD 50 pg/ μ L |
| 5. α -BHC 20 pg/ μ L | 15. DCPA 50 pg/ μ L | 26. Endrin aldehyde 50 pg/ μ L |
| 6. Hexachlorobenzene 10 pg/ μ L | 16. DCB 5000 pg/ μ L | 27. Endosulfan sulfate 30 pg/ μ L |
| 7. γ -BHC 30 pg/ μ L | 17. Heptachlor epoxide 30 pg/ μ L | 28. 4,4'-DDT 120 pg/ μ L |
| 8. β -BHC 20 pg/ μ L | 18. γ -Chlordane 30 pg/ μ L | 29. Methoxychlor 100 pg/ μ L |
| 9. PCNB 100 pg/ μ L | 19. Endosulfan I 30 pg/ μ L | 30. <i>cis</i> -Permethrin 1000 pg/ μ L |
| 10. PCNB (IS) 100 pg/ μ L | 20. α -Chlordane 30 pg/ μ L | 31. <i>trans</i> -Permethrin 1000 pg/ μ L |
| | 21. Dieldrin 40 pg/ μ L | |

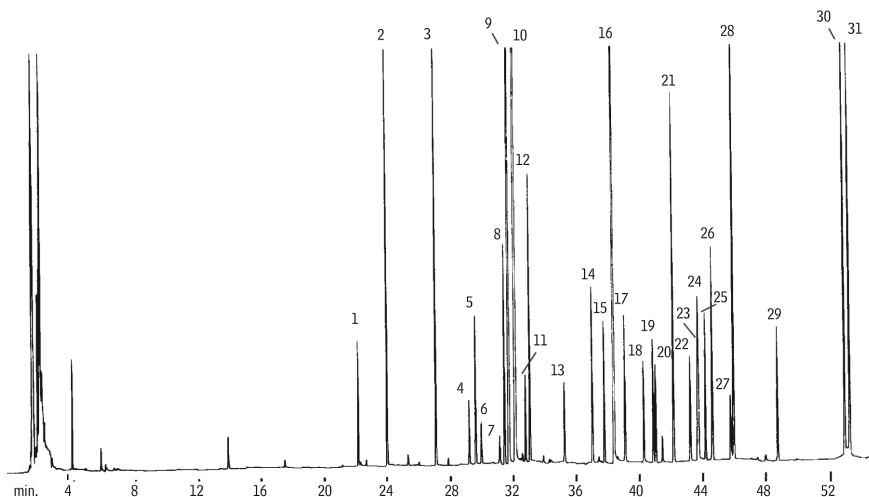

Nitrogen-Containing Herbicides

Column: DM-35, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7951
 Index: CER00088
 Oven Temp.: 60 °C (hold 1 min) to 290 °C (hold 5 min) at 15 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Direct, 290 °C
 Sample: Nitrogen-containing herbicides, 0.2 μ L
 Detector: FID, 16×10^{-11} AFS, 290 °C


- | | |
|---------------|----------------|
| 1. Eptam | 13. Simazine |
| 2. Sutan | 14. Terbacil |
| 3. Vernam | 15. Sencor |
| 4. Tillam | 16. Dual |
| 5. Ordram | 17. Paarlán |
| 6. Treflan | 18. Prowl |
| 7. Balan | 19. Bromacil |
| 8. Ro-Neet | 20. Oxadiazon |
| 9. Propachlor | 21. GOAL |
| 10. Tolban | 22. Hexazinone |
| 11. Propazine | |
| 12. Atrazine | |

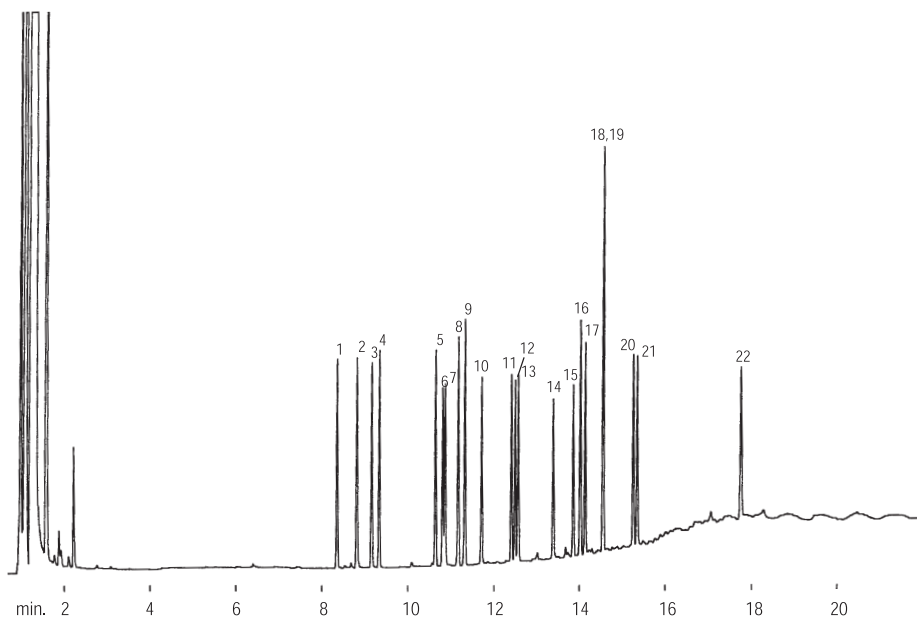

Nitrogen-Containing Herbicides

Column: DM-5, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7247
 Index: CER00087
 Oven Temp.: 60 °C (hold 1 min) to 290 °C (hold 5 min) at 15 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Direct, 290 °C
 Sample: Nitrogen-containing herbicides, 0.2 μ L
 Detector: FID, 16×10^{-11} AFS, 290 °C

- | | |
|---------------|----------------|
| 1. Eptam | 13. Tolban |
| 2. Sutan | 14. Terbacil |
| 3. Vernam | 15. Sencor |
| 4. Tillam | 16. Bromacil |
| 5. Ordram | 17. Dual |
| 6. Propachlor | 18. Paarlán |
| 7. Ro-Neet | 19. Prowl |
| 8. Treflan | 20. Oxadiazon |
| 9. Balan | 21. GOAL |
| 10. Simazine | 22. Hexazinone |
| 11. Atrazine | |
| 12. Propazine | |

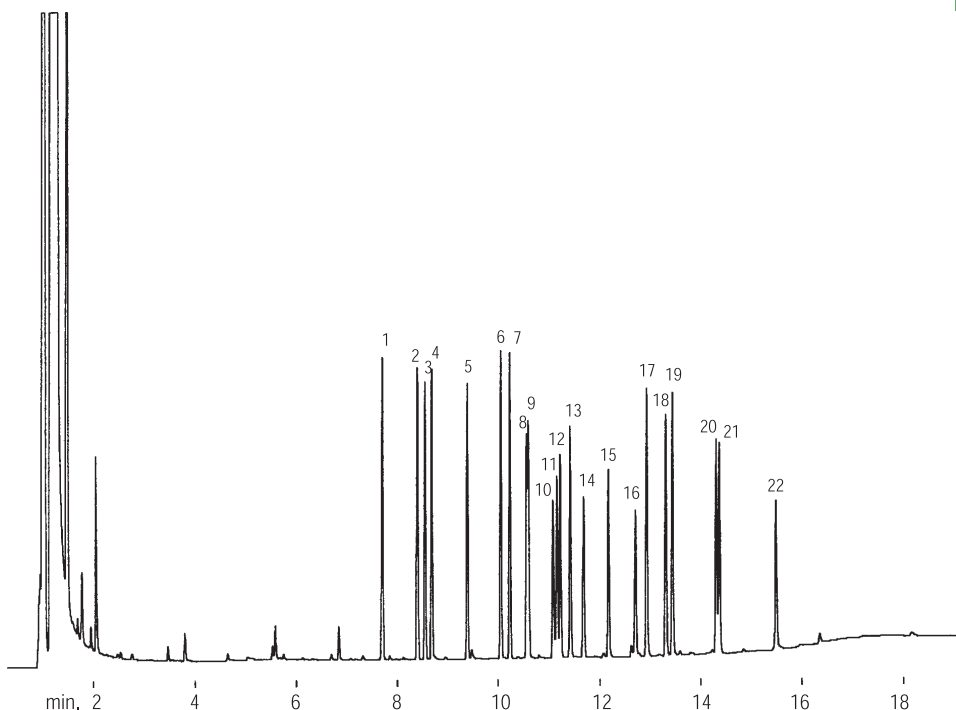


Applications

Pesticides

Organochlorine Pesticides (EPA 8081)


Column: DM-5, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7247
 Index: CER00408
 Oven Temp.: 150 °C (hold 5 min) to 275 °C (hold 5 min) at 4 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Direct, 200 °C
 Sample: Pesticides mix, 1.0 μ L, 80 - 800 ng/mL
 Detector: ECD, 5.12 x 10⁻¹¹ AFS, 275 °C

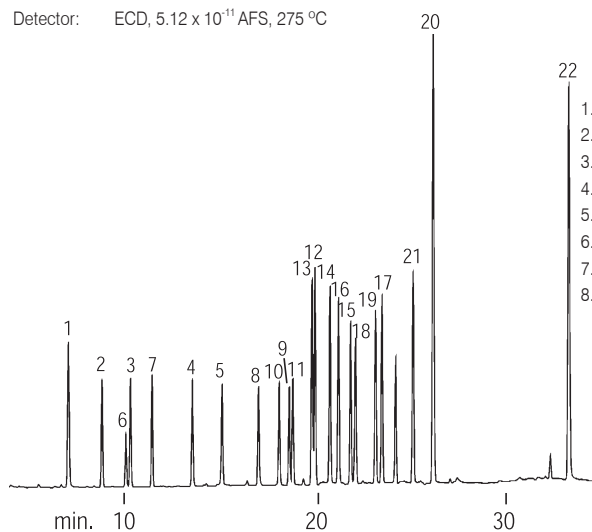

1. 2,4,5,6-Tetrachloro-*m*-xylene
2. α -BHC
3. γ -BHC
4. Heptachlor
5. Aldrin
6. β -BHC
7. δ -BHC
8. Heptachlor epoxide
9. Endosulfan I
10. γ -Chlordane
11. α -Chlordane
12. 4,4'-DDE
13. Dieldrin
14. Endrin
15. 4,4'-DDD
16. Endosulfan II
17. 4,4'-DDT
18. Endrin aldehyde
19. Endosulfan sulfate
20. Methoxychlor
21. Endrin ketone
22. Decachlorobiphenyl

Organochlorine Pesticides (EPA 8081)


Column: DM-1701, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7347
 Index: CER00409
 Oven Temp.: 150 °C (hold 5 min) to 275 °C (hold 5 min) at 4 °C/min
 Carrier Gas: He, 40 cm/sec, 150 °C
 Injection: Direct, 200 °C
 Sample: Organochlorine pesticides, 1.0 μ L, 80 - 800 ng/mL
 Detector: ECD, 5.12 x 10⁻¹⁰ AFS, 275 °C

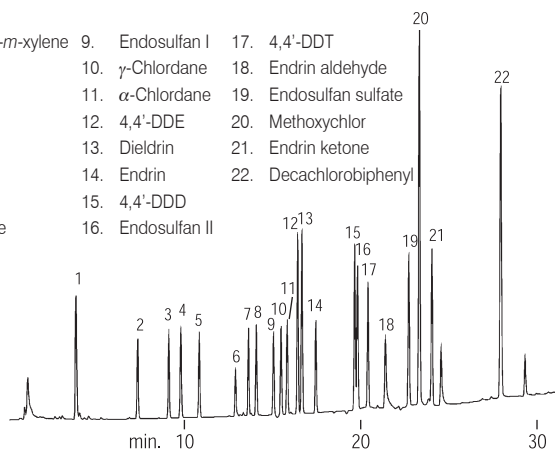

1. 2,4,5,6-Tetrachloro-*m*-xylene
2. α -BHC
3. γ -BHC
4. Heptachlor
5. Aldrin
6. β -BHC
7. δ -BHC
8. Heptachlor epoxide
9. Endosulfan I
10. γ -Chlordane
11. α -Chlordane
12. 4,4'-DDE
13. Dieldrin
14. Endrin
15. 4,4'-DDD
16. Endosulfan II
17. 4,4'-DDT
18. Endrin aldehyde
19. Endosulfan sulfate
20. Methoxychlor
21. Endrin ketone
22. Decachlorobiphenyl

Organochlorine Pesticides (EPA 8081)


Column: DM-17, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7451
 Index: CER00410
 Oven Temp.: 150 °C (hold 5 min) to 275 °C (hold 5 min) at 8 °C/min
 Carrier Gas: He, 40 cm/sec, 150 °C
 Injection: Direct, 200 °C
 Sample: Pesticides, 1.0 μ L
 Detector: ECD, 5.12 X 10⁻¹⁰ AFS, 275 °C

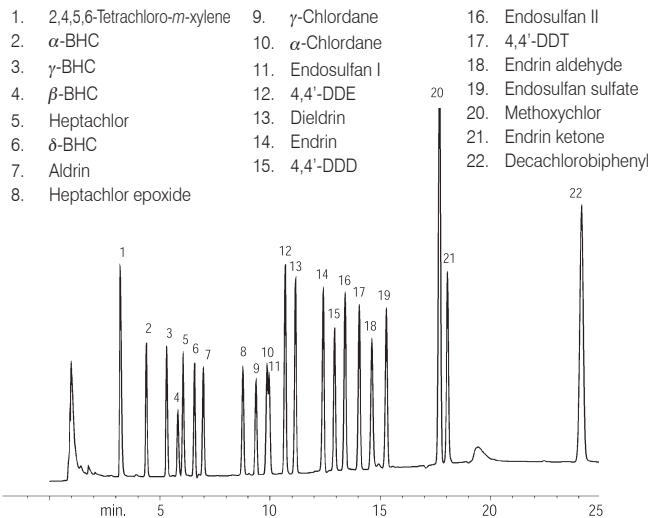

1. 2,4,5,6-Tetrachloro-*m*-xylene
2. α -BHC
3. γ -BHC
4. β -BHC
5. Heptachlor
6. δ -BHC
7. Aldrin
8. Heptachlor epoxide
9. γ -Chlordane
10. α -Chlordane
11. Endosulfan I
12. 4,4'-DDE
13. Dieldrin
14. Endrin
15. 4,4'-DDD
16. Endosulfan II
17. 4,4'-DDT
18. Endrin aldehyde
19. Endosulfan sulfate
20. Methoxychlor
21. Endrin ketone
22. Decachlorobiphenyl

Organochlorine Pesticides (EPA 8081)

Column: DM-35, 30 m x 0.32 mm x 0.50 μ m
 Cat. No.: 7933
 Index: CER00079
 Oven Temp.: 120 °C (hold 1 min) to 285 °C (hold 6 min) at 8.5 °C/min
 Carrier Gas: He, 2.1 mL/min, 120 °C
 Injection: Direct, 200 °C
 Detector: ECD 300 °C with anode purge

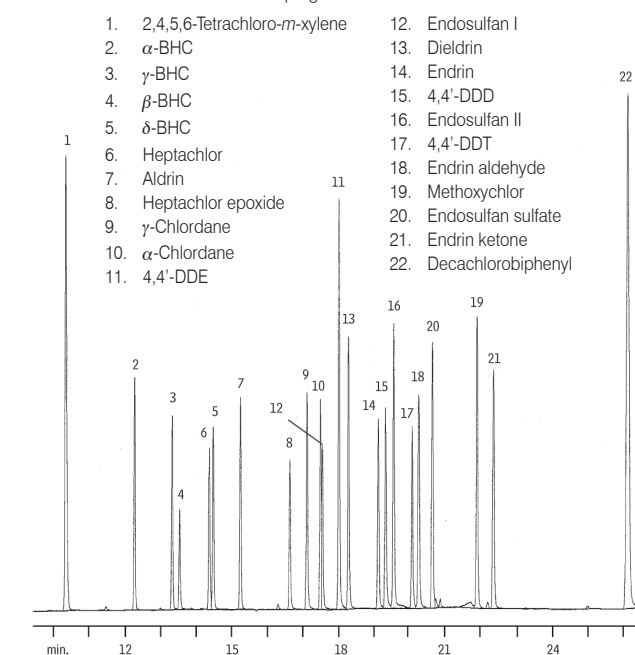


1. 2,4,5,6-Tetrachloro-*m*-xylene
2. α -BHC
3. γ -BHC
4. β -BHC
5. δ -BHC
6. Heptachlor
7. Aldrin
8. Heptachlor epoxide
9. γ -Chlordane
10. α -Chlordane
11. 4,4'-DDE
12. Endosulfan I
13. Dieldrin
14. Endrin
15. 4,4'-DDD
16. Endosulfan II
17. 4,4'-DDT
18. Endrin aldehyde
19. Methoxychlor
20. Endosulfan sulfate
21. Endrin ketone
22. Decachlorobiphenyl

Applications

Triazine Herbicides (EPA 619)

Column: DM-17, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7451
 Index: CER00058
 Oven Temp.: 150 °C to 250 °C (hold 5 min) at 4 °C/min
 Carrier Gas: He, 40 cm/sec, 150 °C
 Injection: Direct, 250 °C
 Sample: EPA Method 619 triazine herbicides, 0.5 μ L
 Detector: TSD, 275 °C


- | | |
|------------------|----------------|
| 1. Atraton | 7. Secbumeton |
| 2. Prometon | 8. Terbutryne |
| 3. Terbutylazine | 9. Ametryne |
| 4. Atrazine | 10. Simetryne |
| 5. Simazine | 11. Prometryne |
| 6. Propazine | |

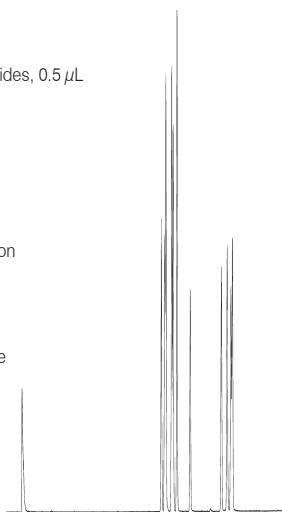

Butyl Tins

Column: DM-5, 30 m x 0.32 mm x 0.50 μ m
 Cat. No.: 7233
 Index: CER00047
 Oven Temp.: 100 °C (hold 1 min) to 285 °C at 10 °C/min
 Carrier Gas: He, 45 cm/sec
 Injection: 500 pg on-column direct, 250 °C
 Detector: FPD with 610 nm filter, 250 °C


1. Tetrapropyltin
2. Tetrabutyltin
3. Tributyltin
4. Dibutyltin
5. Tripropyltin
6. Monobutyltin

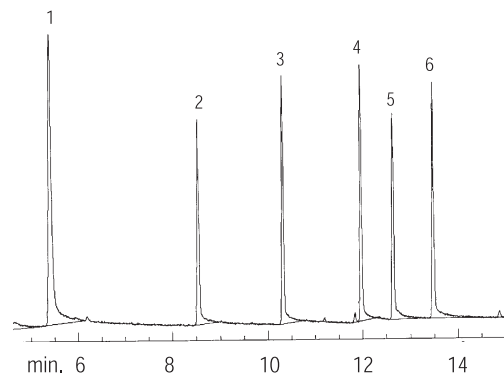

Chlorophenoxyacid Herbicides (EPA 515.1)

Column: DM-17, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: 7423
 Index: CER00093
 Oven Temp.: 50 °C (hold 0.75 min) to 84 °C at 4 °C/min,
 to 165 °C at 10 °C/min to 270 °C at 4 °C/min,
 to 300 °C (hold 6 min) at 20 °C/min
 Carrier Gas: He, 30 cm/sec constant flow, 50 °C
 Injection: Splitless, 0.75 min, 220 °C
 Sample: Chlorophenoxyacid herbicides, 2.0 μ L
 Detector: ECD, 320 °C


1. Dalapon methyl ester
2. 2,4-Dichlorophenylacetic acid methyl ester
3. Dicamba methyl ester
4. Dibromooctafluorobiphenyl methyl ester
5. 2,4-D methyl ester
6. Pentachlorophenol
7. 2,4,5-TP (silvex) methyl ester
8. 2,4,5-T methyl ester
9. Dinoseb methyl ester
10. 2,4-DB methyl ester
11. Picloram methyl ester

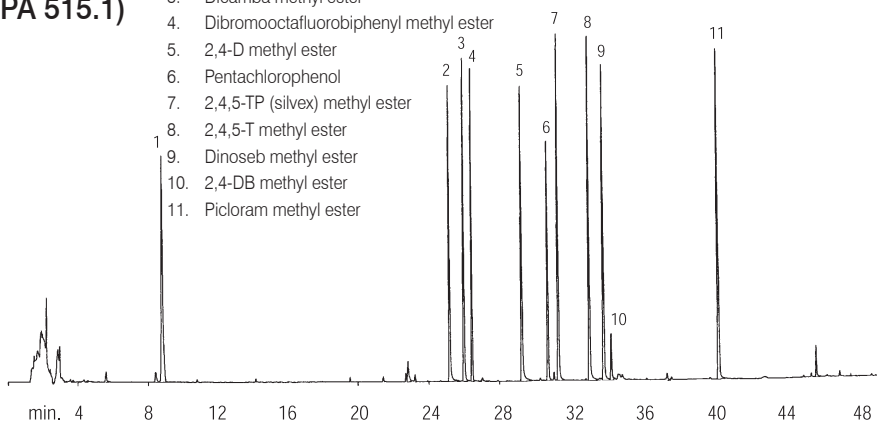

Chlorophenoxyacid Herbicides (EPA 615)

Column: DM-35, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7951
 Index: CER00094
 Oven Temp.: 60 °C to 150 °C (hold 5 min) at 8 °C/min,
 to 210 °C at 4 °C/min
 Carrier Gas: He, 35 cm/sec, 60 °C
 Injection: Direct, 250 °C
 Sample: Chlorophenoxyacid herbicides, 0.5 μ L
 Detector: ECD w / anode purge, 275 °C

1. Dalapon
2. DCAA (SS)
3. Dicamba
4. MCPP
5. MCPA
6. DBOB (IS)
7. Dichlorprop
8. 2,4-D
9. 2,4,5-TP
10. 2,4,5-T
11. Dinoseb
12. 2,4-DB

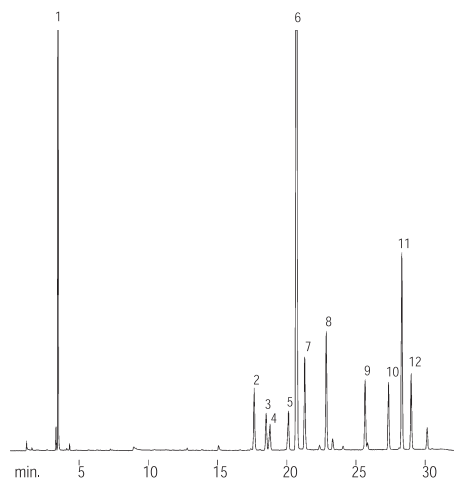


Applications

Drinking Water

Volatile Organic Compounds in Water (EPA 551.1)

Column: DM-200, 30 m x 0.25 mm x 1.00 μ m
 Cat. No.: 8325
 Index: CER00024
 Oven Temp.: 35 $^{\circ}$ C (hold 22 min) to 200 $^{\circ}$ C at 10 $^{\circ}$ C/min,
 Carrier Gas: He, 30 cm/sec, 50 $^{\circ}$ C
 Injection: 1 ng on-column, 200 $^{\circ}$ C
 Split Ratio: 10:1
 Detector: ECD, 20 kHz full scale, 290 $^{\circ}$ C

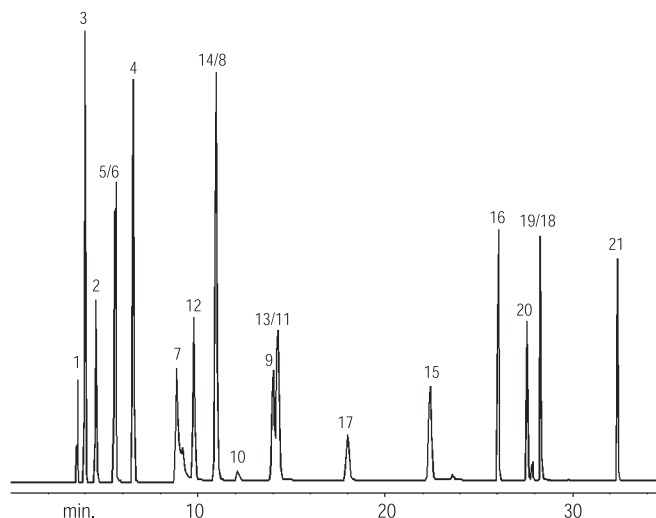


1. Chloroform
2. 1,1,1-Trichloroethane
3. Carbon tetrachloride
4. Trichloroacetonitrile
5. Trichloroethylene
6. Bromodichloromethane
7. Chloral hydrate
8. Dichloroacetonitrile
9. 1,1-Dichloro-2-propanone
10. 1,1,2-Trichloroethane
11. Chloropicrin
12. Dibromochloromethane
13. 1,2-Dibromoethane
14. Tetrachloroethylene
15. Bromochloroacetonitrile
16. 1,1,1-Trichloro-2-propanone
17. Bromoform
18. Dibromoacetonitrile
19. 1,2,3-Trichloropropane
20. 4-Bromofluorobenzene
21. 1,2-Dibromo-3-chloropropane

Volatile Organic Compounds in Water

Column: DM-AQUA, 60 m x 0.25 mm x 1.00 μ m
 Cat.No.: 7801
 Index: CEO04281
 Carrier Gas: He, 25 cm/sec, 150 $^{\circ}$ C
 Oven Temp.: 40 $^{\circ}$ C to 200 $^{\circ}$ C at 4 $^{\circ}$ C/min
 Injection: Split, 1:100, 0.5 μ L
 Detector: FID


- | | | | |
|---------------------------------------|---|-------------------------------|--|
| 1. Bromomethane | 16. 1,2-Dichloroethane | 29. 1-Chlorohexane | 43. <i>m</i> -Chlorotoluene |
| 2. Chloroethane | 17. Benzene | 30. 1,2-Dibromoethane | 44. <i>p</i> -Chlorotoluene |
| 3. Trichlorofluoromethane | 18. Benzotrifluoride | 31. Chlorobenzene | 45. 1,3-Dichlorobenzene |
| 4. 1,1-Dichloroethylene | 19. Trichloroethylene | 32. 1,1,1,2-Tetrachloroethane | 46. 1,4-Dichlorobenzene |
| 5. Dichloromethane | 20. 1,2-Dichloropropane | 33. Ethylbenzene | 47. 1,2-Dichlorobenzene |
| 6. <i>trans</i> -1,2-Dichloroethylene | 21. Bromodichloromethane | 34. <i>m</i> -Xylene | 48. 1,2-Dibromo-3-chloropropane |
| 7. 1,1-Dichloroethane | 22. Dibromomethane | 35. <i>p</i> -Xylene | 49. 1,2,4-Trichlorobenzene |
| 8. 2,2-Dichloropropane | 23. <i>cis</i> -1,3-Dichloropropylene | 36. <i>o</i> -Xylene | 50. 1,1,2,3,4,4-Hexachloro-1,2-butadiene |
| 9. <i>cis</i> -1,2-Dichloroethylene | 24. Toluene | 37. Bromoform | 51. 1,2,3-Trichlorobenzene |
| 10. Chloroform | 25. <i>trans</i> -1,3-Dichloropropylene | 38. 1,1,2,2-Tetrachloroethane | |
| 11. Bromochloromethane | 26. 1,1,2-Trichloroethane | 39. 4-Bromofluorobenzene | |
| 12. 1,1,1-Trichloroethane | 27. 1,3-Dichloropropane | 40. 1,2,3-Trichloropropane | |
| 13. 1,1-Dichloropropene | 28. Tetrachloroethylene | 41. Bromobenzene | |
| 14. Tetrachloromethane | 29. Dibromochloromethane | 42. <i>o</i> -Chlorotoluene | |

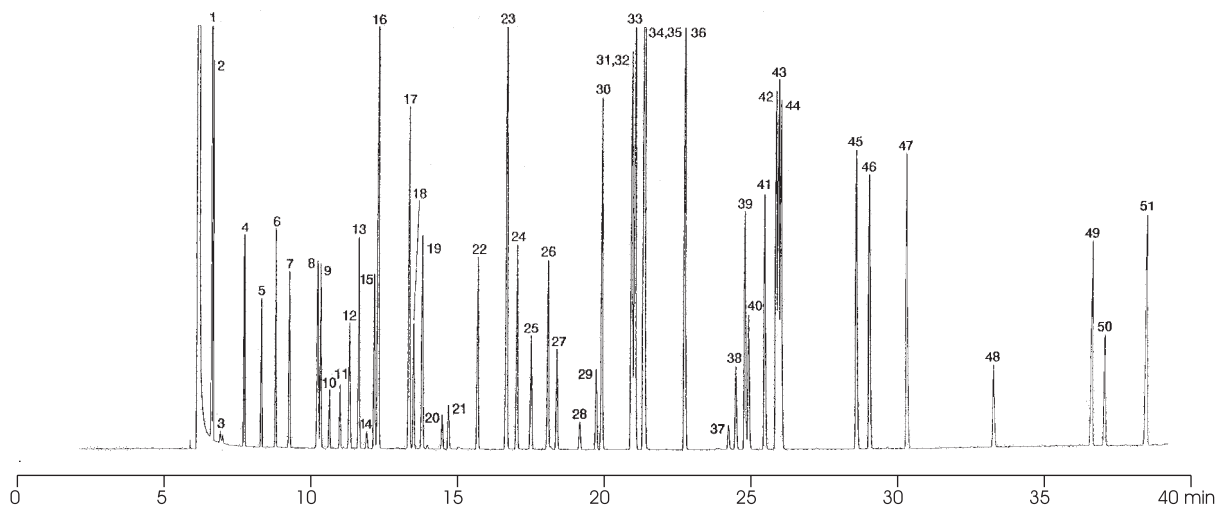

PAEs

Column: DM-5MS, 30 m x 0.25 mm x 0.50 μm
 Cat. No.: **8223**
 Index: CER00049
 Oven Temp.: 35 °C (hold 1 min) to 285 °C at 10 °C/min
 Pressure: 7.5 psi
 Injection: 100 pg on-column
 Detector: MS-SIM


1. Dimethyl phthalate
2. Diethyl phthalate
3. Isobutyl phthalate
4. Dibutyl phthalate
5. Dipentyl phthalate
6. Dihexyl phthalate
7. Benzyl ethyl phthalate
8. Diheptyl phthalate
9. 2-Ethylhexyl phthalate
10. Cyclohexyl phthalate
11. Dioctyl phthalate

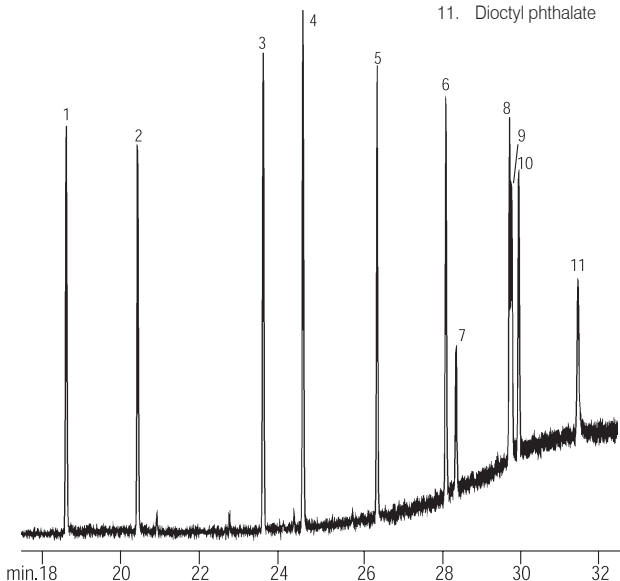

Endocrine Disruptors Butyl Tins (Hexyl Derivatives)

Column: DM-35, 30 m x 0.32 mm x 0.50 μm
 Cat. No.: **7933**
 Index: CER00048
 Oven Temp.: 100 °C (hold 1 min) to 285 °C at 10 °C/min
 Carrier Gas: He, 45 cm/sec
 Injection: 500 pg on-column, 250 °C
 Detector: FPD with 610 nm filter, 250 °C


1. Tetrapropyltin
2. Tetrabutyltin
3. Tributyltin
4. Dibutyltin
5. Tripentyltin
6. Monobutyltin

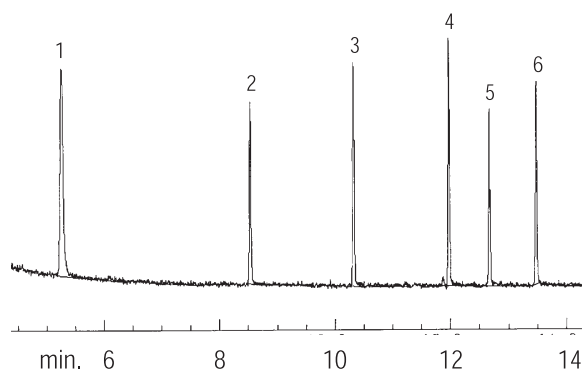

Explosives

Column: DM-200, 30 m x 0.25 mm x 0.25 μm
 Cat. No.: **8321**
 Index: CER00060
 Oven Temp.: 80 °C (hold 2 min) to 260 °C (hold 2 min) at 3 °C/min
 Carrier Gas: He, 20 cm/sec, 80 °C
 Injection: Splitless, hold 0.6 min, 280 °C
 Sample: Explosives, 1.0 μL
 Detector: MS, 300 °C

- | | |
|----------------------------|--------------------------------|
| 1. 2-Nitrotoluene | 14. 3,4-Dinitrotoluene |
| 2. 3-Nitrotoluene | 15. 3-Nitrobiphenyl |
| 3. 4-Nitrotoluene | 16. 2,4,6-Trinitrotoluene |
| 4. 2,3-Diaminotoluene | 17. 2,4,5-Trinitrotoluene |
| 5. 2,6-Diaminotoluene | 18. 4-Amino-2,6-dinitrotoluene |
| 6. 2,4-Diaminotoluene | 19. 2,3,4-Trinitrotoluene |
| 7. 1,4-Dinitrobenzene | 20. 1,3-Dinitronaphthalene |
| 8. 2,6-Dinitrotoluene | 21. 2,6-Diamino-4-nitrotoluene |
| 9. 2-Amino-6-nitrotoluene | 22. 2-Amino-4,6-dinitrotoluene |
| 10. 1,3-Dinitrobenzene | 23. 2,2'-Dinitrobiphenyl |
| 11. 2,4-Dinitrotoluene | |
| 12. 2-Amino-4-nitrotoluene | |
| 13. 2,3-Dinitrotoluene | |

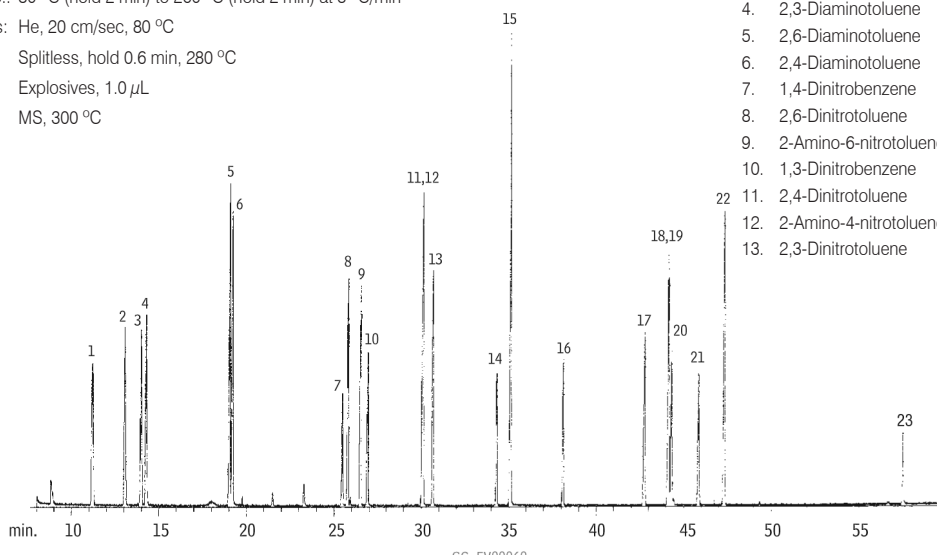

Petrochemicals

Permanent Gases

Column: DM-PLOT Q + DM-PLOT MS 5A,

A: 30 m x 0.53 mm x 20.00 μ m

B: 30 m x 0.32 mm x 30.00 μ m

Cat. No.: **8816 + 8822 = A + B**


Index: CSR00171

Carrier Gas: H₂, 8 psi

Injection: Split, 10:1, 20 μ L

Detector: TCD, 200 °C

1. Helium
2. Argon
3. Oxygen
4. Nitrogen
5. Methane
6. Carbon dioxide
7. Carbon monoxide

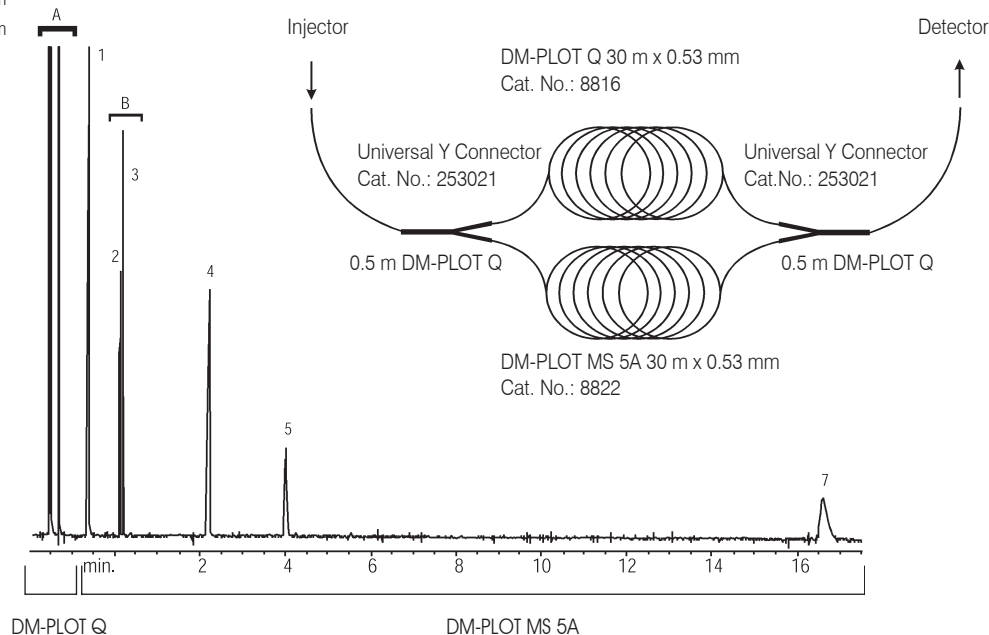

Applications

Permanent Gases

Column: DM-PLOT Q,
30 m x 0.32 mm x 10.00 μ m

Cat. No.: **8818**

Index: CSR00169

Oven Temp.: 30 °C


Carrier Gas: H₂, 38 cm/sec

Injection: Split, 40:1, 30 °C

Sample Concentration: 2 - 5 mol %, 30 μ L

Detector: TCD, 200 °C

1. Helium
2. Air
3. Carbon monoxide
4. Methane
5. Carbon dioxide

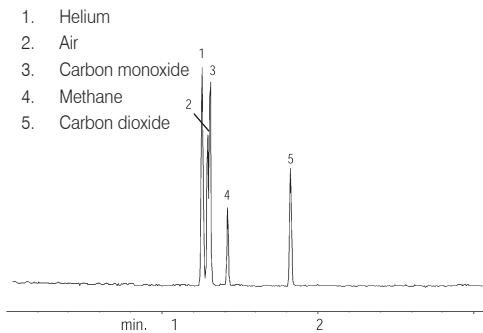

Permanent Gases

Column: DM-PLOT Q,
30 m x 0.32 mm x 10.00 μ m

Cat. No.: **8818**

Index: CSR00174L

Carrier Gas: H₂, 34 cm/sec


Injection Temp.: 15 °C

Split Ratio: 40:1

Sample Concentration: 2 - 5 mol %

Detector: TCD, 15 °C

1. Air
2. Carbon monoxide
3. Methane
4. Carbon dioxide

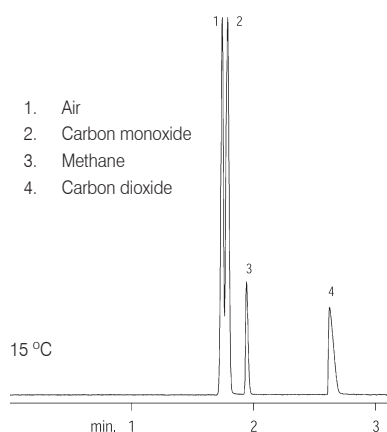

Permanent Gases

Column: DM-PLOT Q,
30 m x 0.32 mm x 10.00 μ m

Cat. No.: **8818**

Index: CSR00174R

Carrier Gas: H₂, 20 cm/sec


Injection Temp.: -40 °C

Split Ratio: 40:1

Sample Concentration: 2 - 5 mol %


Detector: TCD, -40 °C

1. Nitrogen
2. Oxygen
3. Argon

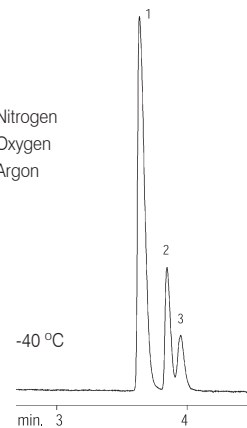

Permanent Gases


Column: DM-PLOT MS 5A, 30 m x 0.32 mm x 30.00 μ m
 Cat. No.: **8822**
 Index: CSR00165
 Oven Temp.: 70 $^{\circ}$ C
 Carrier Gas: H₂, 64 cm/sec
 Injection Temp.: Split, 70 $^{\circ}$ C
 Sample Concentration: 2 - 5 mol%, 20 μ L
 Detector: TCD, high sensitivity, 200 $^{\circ}$ C

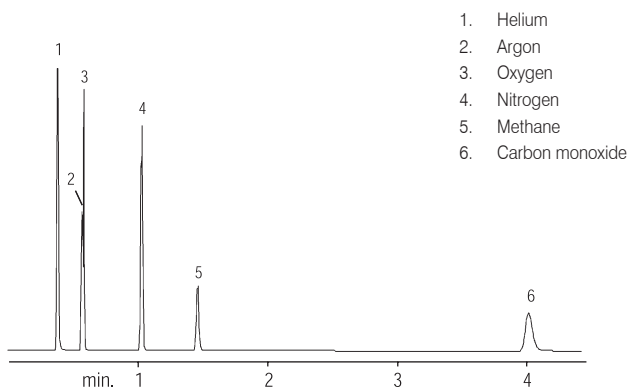

Permanent Gases




Column: DM-PLOT Q / DM-PLOT S / DM-PLOT U,
 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: **8818 / 8810 / 8824**
 Index: CSR00180
 Oven Temp.: 50 $^{\circ}$ C
 Carrier Gas: H₂
 Injection: Split, 20:1, 200 $^{\circ}$ C
 Sample: 1000 ppm (v/v) in He, 100 μ L
 Detector: FID, 200 $^{\circ}$ C

1. Methane
2. Ethylene
3. Ethane
4. Acetylene
5. Propylene
6. Propane

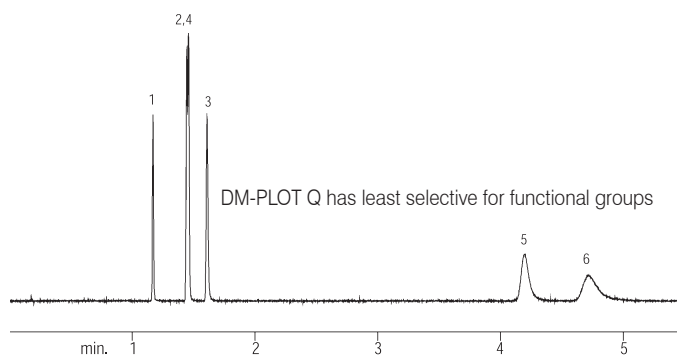

Permanent Gases

Column: DM-PLOT MS 5A, 30 m x 0.53 mm x 20.00 μ m
 Cat. No.: **8823**
 Index: CSR00170
 Oven Temp.: 27 $^{\circ}$ C
 Carrier Gas: He, 34 cm/sec
 Injection: Sample loop, 0.5 mL
 Detector: Valco HID

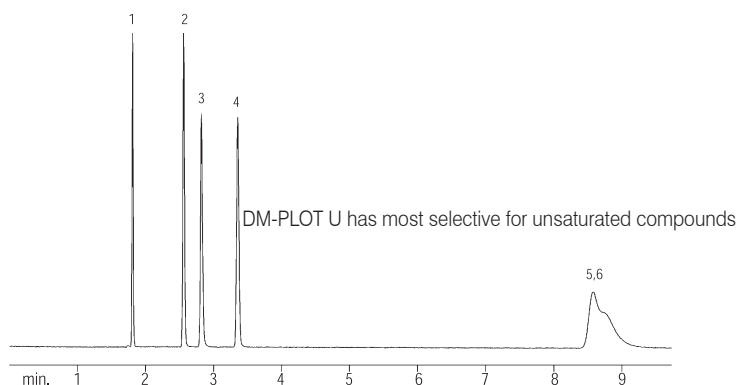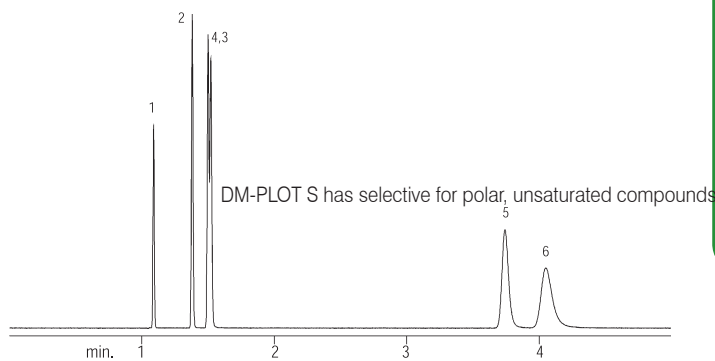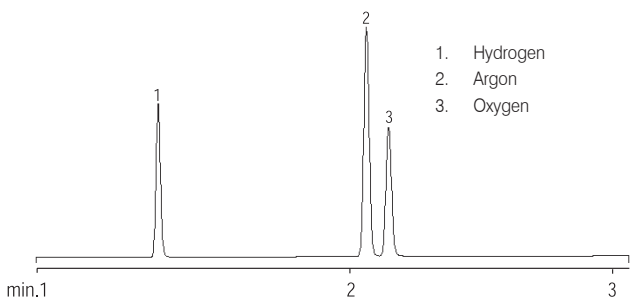

Applications

Petrochemicals

Refinery Gas

Column: DM-PLOT Alumina / Na₂SO₄,
30 m x 0.53 mm x 10.00 μm

Sample: Refinery gas

Cat. No.: **8806**

Index: CSR01139

Injection: Split, 10 μL, 200 °C

Split Vent Flow Rate: 40 mL/min


Oven Temp.: 60 °C (hold 2 min) to 200 °C (hold 1 min)
at 10 °C/min

Carrier Gas: He, constant pressure (5.0 psi, 34.5 kPa),
37.3 cm/sec, 60 °C

Detector: FID, 200 °C

Make up gas: N₂

1. Methane
2. Ethane
3. Ethylene
4. Propane
5. Propylene
6. Isobutane
7. *n*-Butane
8. Propadiene
9. Acetylene
10. *trans*-2-Butene
11. 1-Butene
12. Isobutylene
13. *cis*-2-Butene
14. Isopentane
15. *n*-Pentane
16. 1,3-Butadiene
17. *trans*-2-Pentene
18. 2-Methyl-2-butene
19. 1-Pentene
20. *cis*-2-Pentene
21. Hexanes

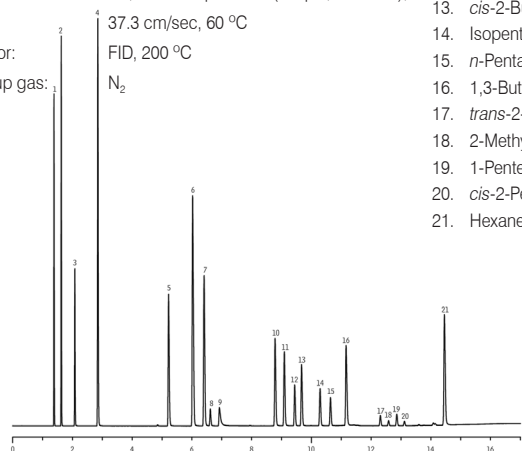

Impurity Analysis of 1,1,1,2-Tetrafluoroethane

Column: DM-PLOT CFC, 30 m x 0.53 mm x 10.00 μm

Cat. No.: **8859**

Index: CGR1155

Sample: 1,1,1,2-Tetrafluoroethane


Injection: Split, 500 μL

Oven Temp.: 80 °C (hold 6 min) to 140 °C (hold 2 min) at 10 °C/min

Carrier Gas: He

Detector: FID

1. Chloropentafluoroethane (CFC-115)
2. Dichlorodifluoromethane (CFC-12)
3. Chlorodifluoromethane (CFC-22)
4. 1,1,1,2-Tetrafluoroethane (CFC-134a)

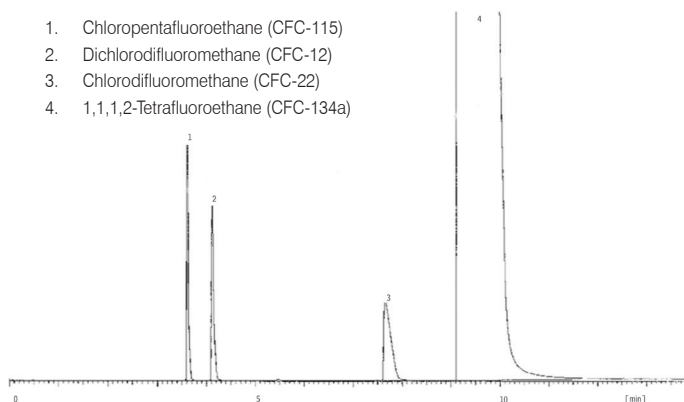

Natural Gas #2

Column: DM-PLOT QS, 30 m x 0.53 mm x 20.00 μm

Cat. No.: **8830**

Index: CSR01013

Oven Temp.: 40 °C (hold 2 min) to 225 °C (hold 5 min) at 20 °C/min


Carrier Gas: He, 5.7 mL/min

Injection: 20 μL split (split ratio 10:1), 240 °C

Sample: Natural gas mix (mol%)

Detector: FID, 240 °C

1. Methane
2. Ethane
3. Propane
4. Isobutane
5. *n*-Butane
6. Isopentane
7. *n*-Pentane
8. Hexanes / Hexenes

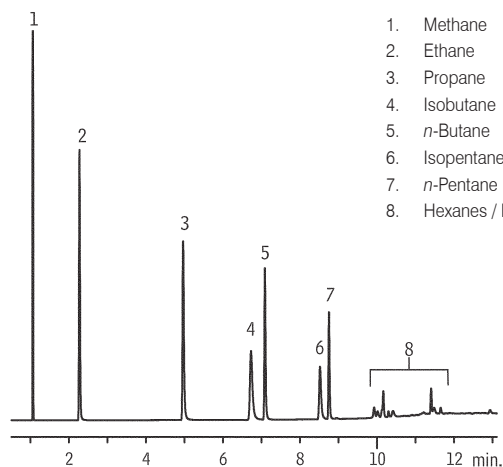

Butane Lighter Fluid

Column: DM-PLOT Alumina / KCl, 50 m x 0.53 mm x 10.00 μm

Cat. No.: **8813**

Index: CSR01086

Sample: Butane lighter fluid


Injection: Valve, 100 μL, 200 °C

Oven Temp.: 45 °C (hold 1 min) to 200 °C (hold 3.5 min) at 10 °C/min

Carrier Gas: H₂, constant pressure (8.0 psi, 55.2 kPa) 74 cm/sec 45 °C


Detector: FID, 200 °C

1. Methane
2. Ethane
3. Propane
4. Isobutane
5. *n*-Butane
6. *trans*-2-Butene
7. 1-Butene
8. Isobutylene

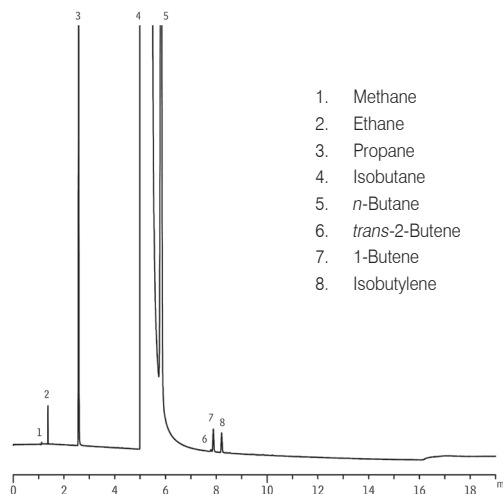


Propylene Purity

Column: DM-PLOT Alumina, 50 m x 0.53 mm x 6.00 μ m
 Cat. No.: 8801
 Index: CSR00185
 Oven Temp.: 40 °C (hold 3 min) to 120 °C (hold 5 min) at 10 °C/min
 Carrier Gas: He, 37.5 cm/sec, 80 °C
 Injection: Gas-tight syringe, 60 mL/min, 200 °C
 Sample: Hydrocarbons mix, 100 μ L
 Detector: FID, 1.28 x 10⁻¹⁰ AFS, 200 °C

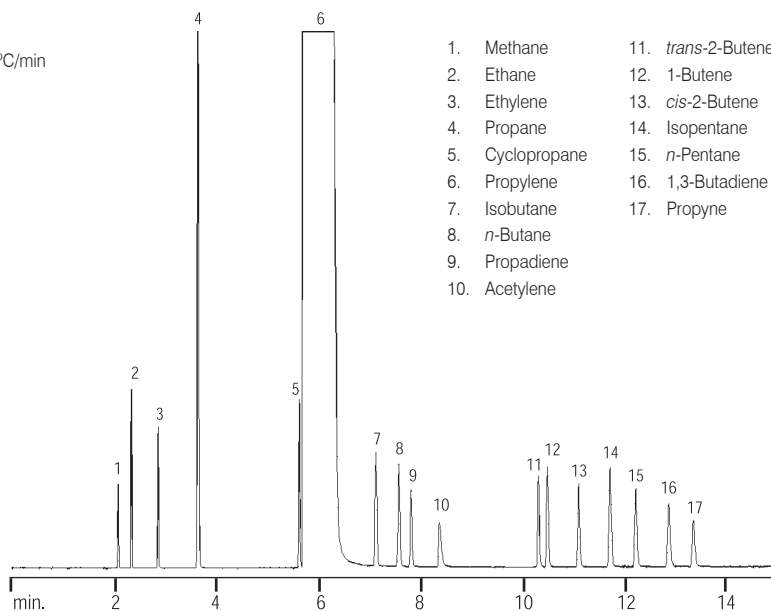

Hydrocarbon Gases

Column: DM-PLOT Q, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: 8818
 Index: CSR00521
 Oven Temp.: 40 °C to 240 °C (hold 10 min) at 8 °C/min
 Carrier Gas: He, 35 cm/sec, 40 °C
 Injection: Split, 20:1, 250 °C
 Head Pressure: 18.0 psi
 Column flow rate: 1.5 mL/min, 40 °C
 Sample: Hydrocarbon gases mix, 30 μ L
 Detector: FID, 240 °C

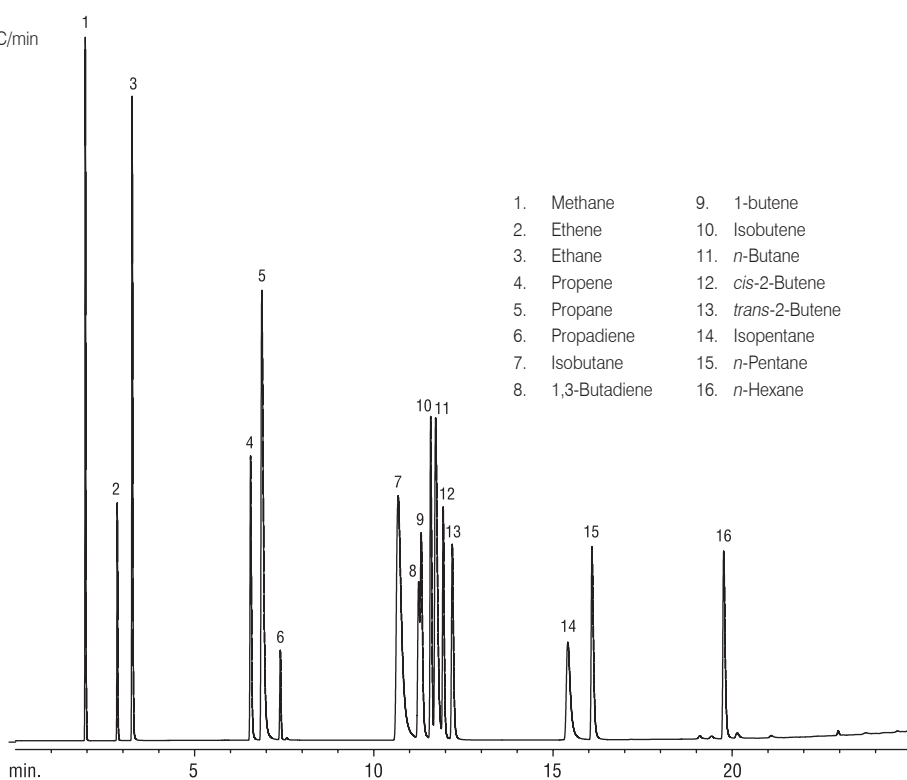


Applications

Petrochemicals

Hydrocarbon Gases

Column: DM-PLOT U, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: **8824**
 Index: CSR00177
 Oven Temp.: 50 °C to 190 °C at 10 °C/min
 Carrier Gas: He, 42 cm/sec, 80 °C
 Injection: Split, 300 μ L, 40 mL/min, 40:1, 250 °C
 Detector: FID, 1.28×10^{-10} AFS, 250 °C


1. Methane
2. Ethylene
3. Ethane
4. Acetylene
5. Propane
6. Propylene
7. Cyclopropane
8. Propadiene
9. Propyne
10. Isobutane
11. *n*-Butane
12. 1-Butene
13. *cis*-2-Butene
14. *trans*-2-Butene
15. 1,3-Butadiene
16. Isopentane
17. *n*-Pentane

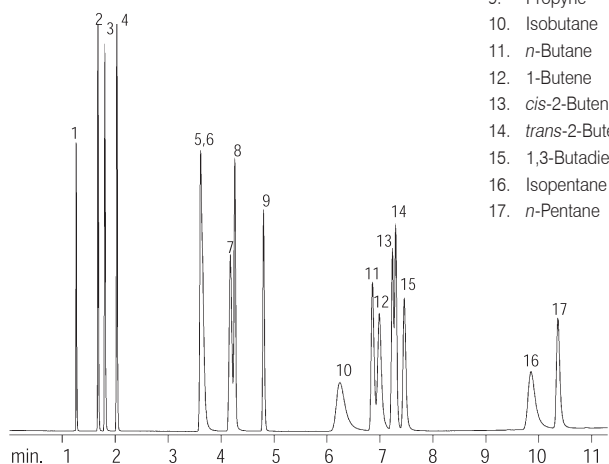

Hydrocarbon Gases

Column: DM-PLOT Q, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: **8818**
 Index: CSR00176
 Oven Temp.: 50 °C (hold 2 min) to 220 °C at 15 °C/min
 Carrier Gas: He, 42 cm/sec, 80 °C
 Injection: Split, 300 μ L, 40 mL/min, 40:1, 250 °C
 Detector: FID, 1.28×10^{-10} AFS, 250 °C

1. Methane
2. Ethylene
3. Acetylene
4. Ethane
5. Propylene
6. Propane
7. Cyclopropane
8. Propadiene
9. Propyne
10. Isobutane
11. 1,3-Butadiene
12. 1-Butene
13. *n*-Butane
14. *cis*-2-Butene
15. *trans*-2-Butene
16. Isopentane
17. *n*-Pentane

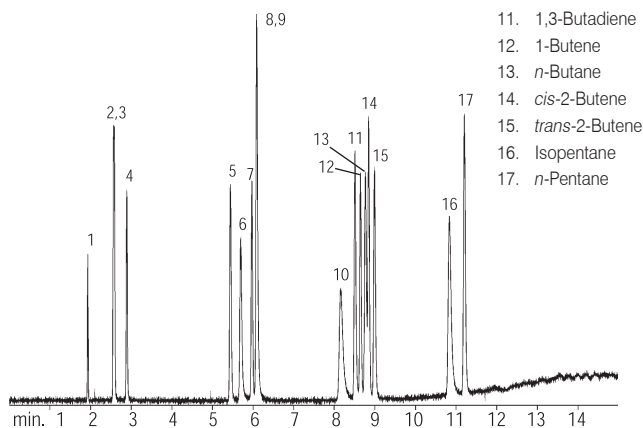


Applications

Refinery Gas

Column: DM-PLOT Alumina, 50 m x 0.53 mm x 6.00 μ m
 Cat. No.: **8801**
 Index: CSR00183
 Oven Temp.: 40 °C to 120 °C (hold 5 min) at 5 °C/min
 Carrier Gas: He, 37.5 cm/sec, 80 °C
 Injection: Split (gastight syringe) 60 mL/min, 200 °C
 Sample: Hydrocarbons mix, 100 μ L, 1,000 ppm
 Detector: FID, 1.28×10^{-10} AFS, 200 °C


1. Methane
2. Ethane
3. Ethylene
4. Propane
5. Cyclopropane
6. Propylene
7. Isobutane
8. *n*-Butane
9. Propadiene
10. Acetylene
11. *trans*-2-Butene
12. 1-Butene
13. *cis*-2-Butene
14. Isopentane
15. *n*-Pentane
16. 1,3-Butadiene
17. Propyne

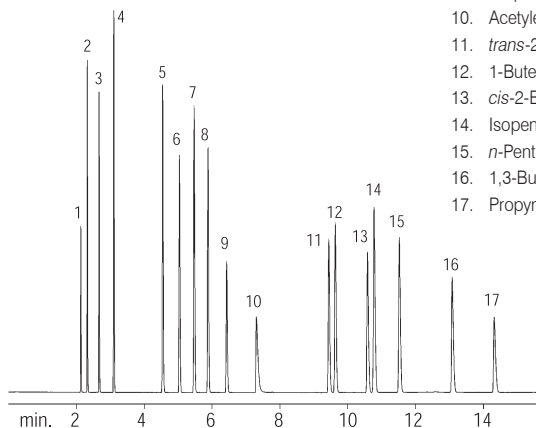

1,3-Butadiene Purity


Column: DM-PLOT Alumina, 50 m x 0.53 mm x 6.00 μ m
 Cat. No.: **8801**
 Index: CSR00186
 Oven Temp.: 80 °C
 Carrier Gas: He, 42 cm/sec, 80 °C
 Injection: Gastight syringe, 40 mL/min, 200 °C
 Sample: 99+% 1,3-Butadiene, 500 μ L
 Detector: FID, 1.28×10^{-10} AFS, 200 °C

1. Methane
2. Ethane
3. Propane
4. Isobutane
5. *n*-Butane
6. *trans*-2-Butene
7. 1-Butene
8. Isobutylene
9. *cis*-2-Butene
10. Isopentane
11. 1,3-Butadiene

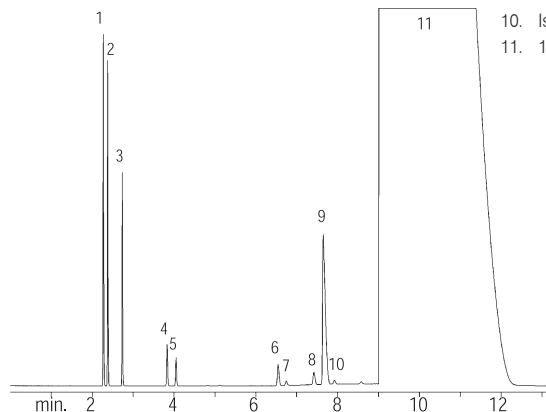


Hydrocarbons

Column: DM-PLOT Alumina, 50 m x 0.53 mm x 6.00 μ m
 Cat. No.: **8801**
 Index: CSR00551
 Oven Temp.: 80 °C
 Carrier Gas: He, 42 cm/sec, 80 °C
 Injection: Gastight syringe, 40 mL/min, 200 °C
 Sample: 200 μ L, 1,000 ppm
 Detector: FID, 1.28 x 10⁻¹⁰ AFS, 200 °C

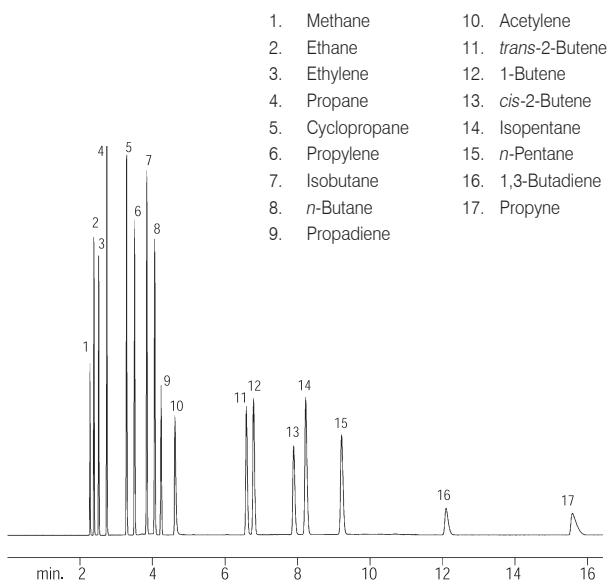


Hydrocarbon Gases

Column: DM-PLOT Q, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: **8818**
 Index: CSR00523
 Oven Temp.: 40 °C to 240 °C (hold 10 min) at 10 °C/min
 Carrier Gas: He, 35 cm/sec, 40 °C
 Head Pressure: 18.0 psi
 Column flow rate: 1.5 mL/min, 40 °C
 Injection: Split, 20:1, 250 °C
 Sample: Hydrocarbon gases mix, 30 μ L
 Detector: FID, 240 °C

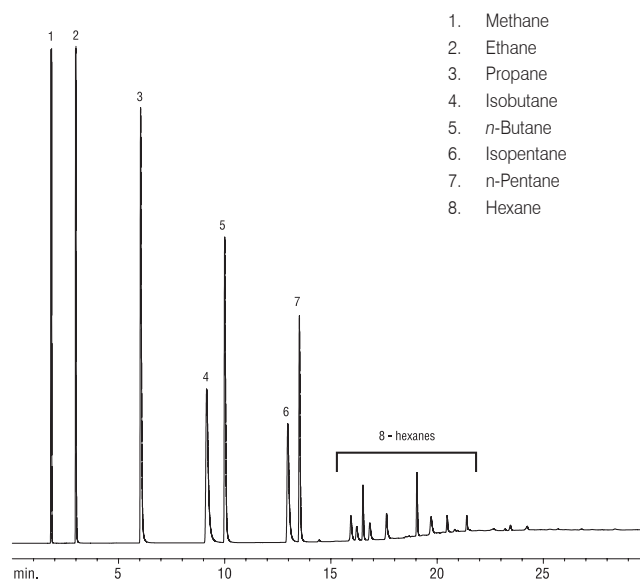

Hydrocarbon Gases

Column: DM-PLOT Q, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: **8818**
 Index: CSR00522
 Oven Temp.: 35 °C to 240 °C (hold 10 min) at 10 °C/min
 Carrier Gas: He, 35 cm/sec, 40 °C
 Head Pressure: 18.0 psi
 Column flow rate: 1.5 cc/min, 40 °C
 Injection: Split, 20:1, 250 °C
 Sample: Hydrocarbon gases mix, 30 μ L
 Detector: FID, 240 °C

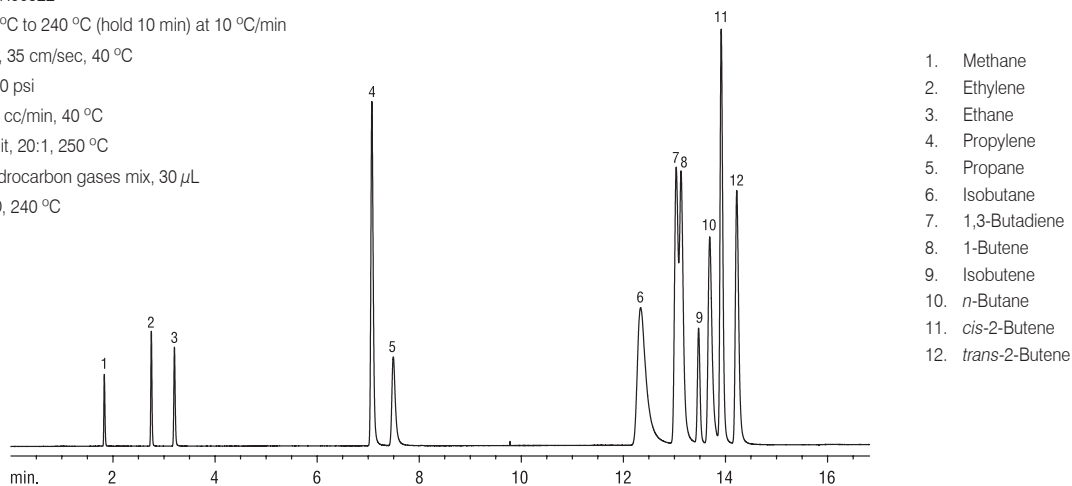

Petrochemicals

Petroleum Oxygenates

Column: DM-Wax, 30 m x 0.53 mm x 1.00 μ m

Cat. No.: 7551

Index: CSR00196

Oven Temp.: 45 °C (hold 4 min) to 220 °C at 6 °C/min


Carrier Gas: H₂, 40 cm/sec

Injection: Direct, 220 °C

Sample: Synthetic blend, 0.2 μ L, 15 - 30 ng/ μ L

Detector: FID, 16 x 10⁻¹¹ AFS, 220 °C

- | | | | |
|---------------------|------------------------------|------------------------------|------------------------------------|
| 1. Heptane | 7. <i>m</i> -Xylene | 13. <i>m</i> -Diethylbenzene | 19. Acetophenone |
| 2. C3 oxide | 8. Cumene | 14. α -Methylstyrene | 20. 2-Phenyl-2-propanol |
| 3. Benzene | 9. <i>o</i> -Xylene | 15. <i>o</i> -Diethylbenzene | 21. α -Methylbenzyl alcohol |
| 4. Toluene | 10. Styrene | 16. Phenylacetylene | 22. Benzyl alcohol |
| 5. Ethylbenzene | 11. 2-Methylpentanol | 17. Benzaldehyde | 23. Phenylethyl alcohol |
| 6. <i>p</i> -Xylene | 12. <i>p</i> -Diethylbenzene | 18. Monopropylene glycol | 24. Phenol |

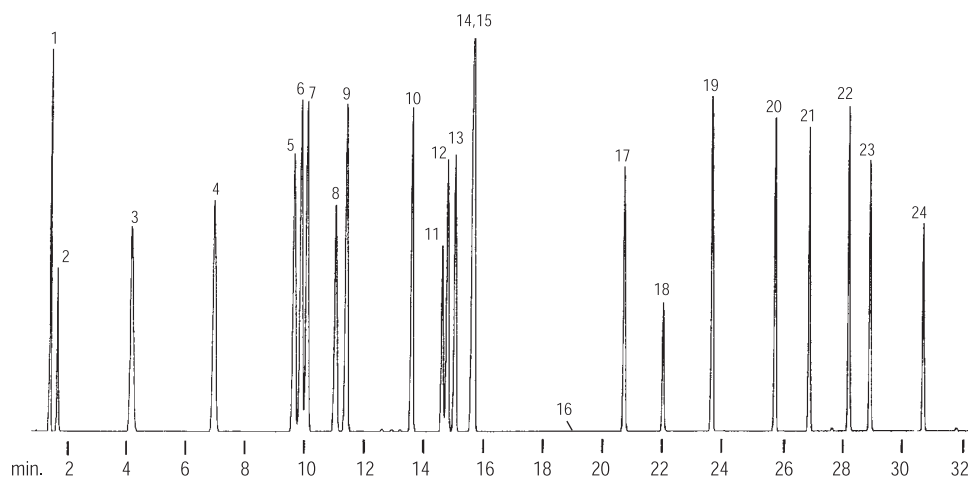

Applications

Petroleum Oxygenates

Column: DM-TCEP, 60 m x 0.25 mm x 0.40 μ m

Cat. No.: 7809

Index: CSR00195

Oven Temp.: 60 °C (hold 5 min) to 100 °C (hold 10 min) at 5 °C/min


Carrier Gas: He, 30 cm/sec, 80 °C

Injection: Split, 46 mL/min, 200 °C

Sample: 1.0 μ L, 500 ppm

Detector: FID, 6.4 x 10⁻¹¹ AFS, 200 °C


1. Methyl *tert*-butyl ether
2. *n*-Undecane
3. *tert*-Butanol
4. Methanol
5. Isopropyl alcohol
6. Ethanol
7. *n*-Dodecane
8. *n*-Tridecane
9. *n*-Butanol

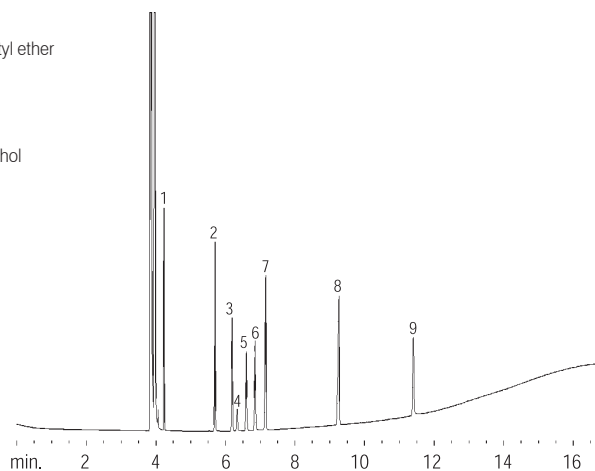

Petroleum Oxygenates

Column: DM-1, 30 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7155
 Index: CSR00194
 Oven Temp.: 60 °C
 Carrier Gas: He, 5 mL/min, 60 °C
 Injection: Split, 15:1, 200 °C
 Sample: Oxygenates blend 1 - 10 % wt in surrogate gasoline, 0.5 μ L
 Detector: FID, 250 °C


1. Methanol
2. Ethanol
3. Isopropanol
4. *tert*-butanol
5. *n*-Propanol
6. Methyl *tert*-butyl ether
7. *sec*-Butanol
8. DIPE
9. Isobutanol
10. Ethyl *tert*-butyl ether
11. *tert*-Amyl ether
12. Dimethoxyethane
13. *n*-Butanol
14. Benzene
15. TAME
16. Total heavy hydrocarbons

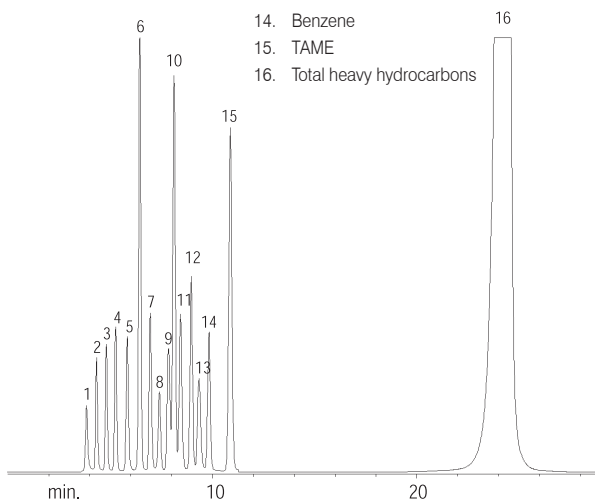

Oxygenates MTBE

Column: DM-1, 30 m x 0.53 mm x 5.00 μ m
 Cat. No.: 7157
 Index: CSR00197
 Oven Temp.: 40 °C (hold 8 min) to 200 °C at 5 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Direct, 200 °C
 Sample: Methyl *tert*-butyl ether, 0.1 μ L
 Detector: FID, 8 x 10⁻¹¹ AFS, 200 °C

1. Dimethylether
2. Methanol
3. C4s
4. *tert*-Butyl alcohol
5. Methyl *tert*-butyl ether
6. *sec*-Butyl methyl ether
7. Diisobutylene
8. 4-Vinyl cyclohexene-1
9. Triisobutylene

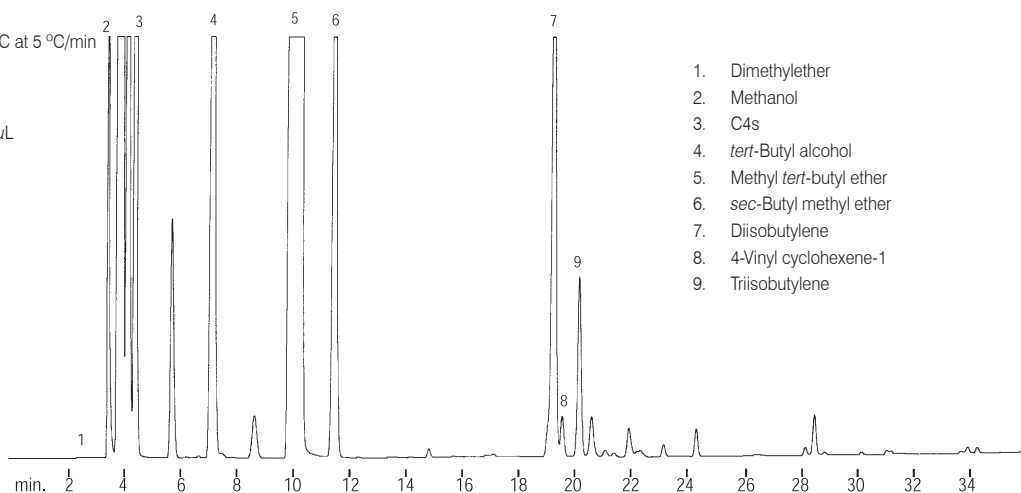


Applications

Petrochemicals

Sulfur in Gasoline

Column: DM-1, 30 m x 0.32 mm x 4.00 μ m
 Cat. No.: 7143
 Index: CSR00198
 Oven Temp.: 40 $^{\circ}$ C (hold 3 min) to 275 $^{\circ}$ C (hold 5 min) at 10 $^{\circ}$ C/min
 Carrier Gas: He, 70 cm/sec
 Injection: Split, 10:1, 275 $^{\circ}$ C
 Sample: Sulfur in gasoline, 1.0 μ L, 300 ppm
 Detector: SCD, 275 $^{\circ}$ C


1. Thiophene
2. 2-Methylthiophene
3. 3-Methylthiophene
4. 2-Ethylthiophene
5. Alkylthiophenes
6. Benzothiophene
7. Methylbenzothiophenes
8. Dimethylbenzothiophenes

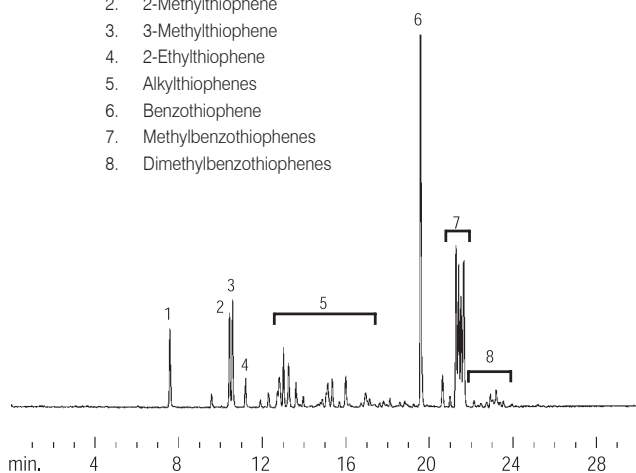

Sulfur in Naphtha

Column: DM-1, 30 m x 0.32 mm x 4.00 μ m
 Cat. No.: 7143
 Index: CSR00199
 Oven Temp.: 35 $^{\circ}$ C to 275 $^{\circ}$ C (hold 5 min) at 10 $^{\circ}$ C/min
 Carrier Gas: He, 24 cm/sec
 Injection: Split, 10:1, 275 $^{\circ}$ C
 Sample: Sulfur in naphtha, 1.0 μ L, 500 ppm
 Detector: AED, 181 nm, 275 $^{\circ}$ C

1. Hydrogen sulfide
2. Thiophene
3. 2-Methylthiophene
4. 3-Methylthiophene
5. 2-Ethylthiophene

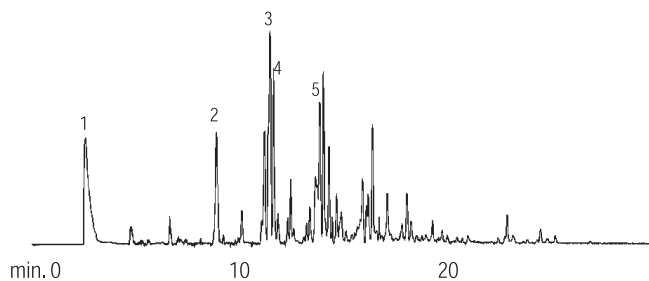


Applications

Sulfide


Column: DM-1, 60 m x 0.53 mm x 5.00 μ m
 Cat. No.: 7158
 Index: CSR00200
 Oven Temp.: 50 $^{\circ}$ C to 200 $^{\circ}$ C at 15 $^{\circ}$ C/min
 Carrier Gas: He, 30 cm/sec, 50 $^{\circ}$ C
 Injection: Direct, 50 $^{\circ}$ C
 Sample: Sulfide mix, 100 μ L
 Detector: FPD, 230 $^{\circ}$ C

1. Hydrogen sulfide
2. Sulfur dioxide + Carbonyl sulfide
3. Methanethiol
4. Ethanethiol
5. Carbon disulfide
6. Methyl sulfide
7. 2-Propylmercaptan
8. Allylmercaptan
9. 1-Propylmercaptan
10. Ethyl thioether
11. Butanethiol
12. Methyl disulfide
13. Diallylsulfide
14. Dipropyl sulfide
15. Butyl sulfide + Diallyl disulfide

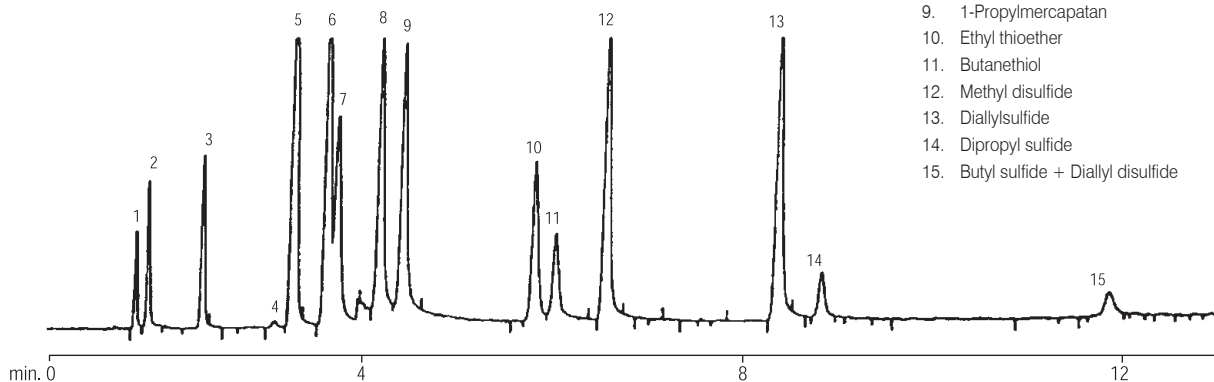


Bleed Profile

Column: DM-HT SimDist Metal, 5 m x 0.53 mm x 0.10 μ m
 Cat.No.: **7806**
 Index: CSR00527
 Oven Temp.: 40 °C to 430 °C (hold 30 min) at 10 °C/min
 Carrier Gas: He, 60 cm/sec
 Injection: On-column
 Flow Rate: 7.8 mL/min
 Head Pressure: 1.0 psi
 Detector: FID, 430 °C

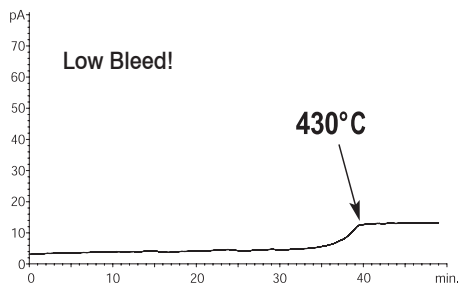


Glycerin in Biodiesel (ASTM D6584)

Column: DM-BDTG Metal, 14 m x 0.53 mm x 0.16 μ m (with 2 m Integra-Gap, total length 16 m)
 Cat. No.: **8864**
 Index: CSR00969
 Sample: Biodiesel (B100) in *n*-hexane
 Injection: 1 μ L cold on-column
 Oven Temp.: 50 °C (hold 1 min) to 180 °C at 15 °C/min to 230 °C at 7 °C/min, to 380 °C (hold 5 min) at 30 °C/min
 Carrier Gas: H₂, 4 mL/min
 Detector: FID, 380 °C

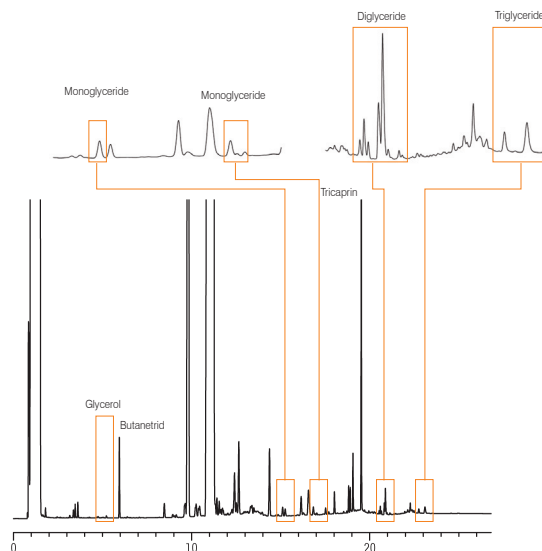


Hydrocarbons, C44 - C100

Column: DM-HT SimDist Metal, 5 m x 0.53 mm x 0.10 μ m
 Cat. No.: **7806**
 Index: CSR00543
 Solvent: Carbon disulfide
 Injection: On-column
 Oven Temp.: 40 °C to 430 °C (hold 30 min) at 60 °C/min
 Carrier Gas: H₂, 1.0 psi
 Sample: Polywax 1000, 0.2 μ L
 Detector: FID, 430 °C

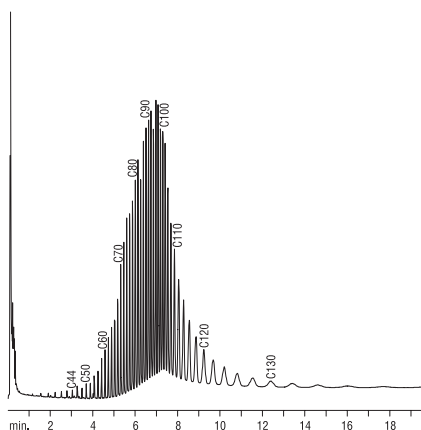


Hydrocarbons, C44 - C100

Column: DM-HT SimDist Metal, 5 m x 0.53 mm x 0.10 μ m
 Cat. No.: **7806**
 Index: CSR00531
 Injection: On-column, 0.2 μ L
 Oven Temp.: 40 °C to 430 °C (hold 25 min) at 60 °C/min
 Carrier Gas: He, 60 cm/sec, 1.0 psi
 Sample: Polywax 1000, 0.2 μ L
 Flow Rate: 7.8 mL/min
 Detector: FID, 430 °C

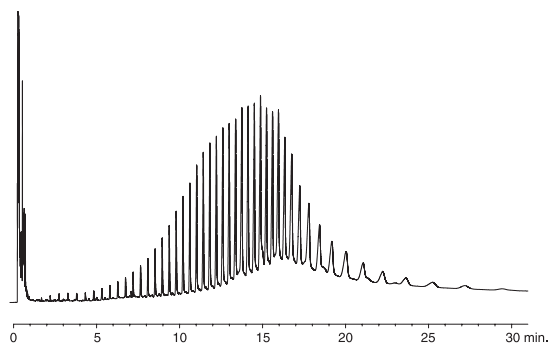


Simulated Distillation

Column: DM-2887, 10 m x 0.53 mm x 2.65 μ m
 Cat. No.: **7808**
 Index: CSR00227
 Oven Temp.: 35 °C to 360 °C (hold 5 min) at 15 °C/min
 Carrier Gas: N₂, 112 cm/sec
 Injection: Direct, 360 °C
 Sample: 0.1 - 0.01 wt% Hydrocarbon in CS₂ solvent, 1.0 μ L

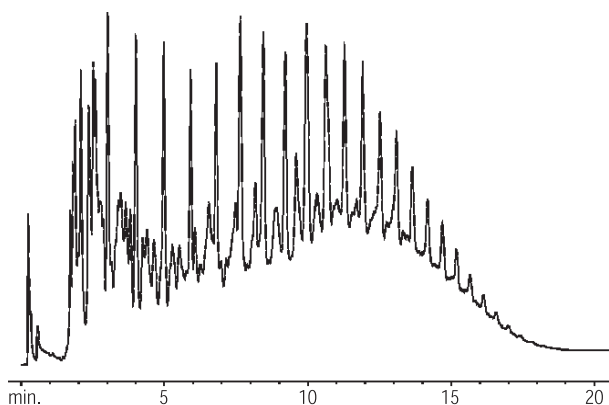


Simulated Distillation

Column: DM-2887, 10 m x 0.53 mm x 2.65 μ m
 Cat. No.: **7808**
 Index: CSR00226
 Oven Temp.: 35 °C to 360 °C (hold 5 min) at 15 °C/min
 Carrier Gas: N₂, 112 cm/sec
 Injection: Direct, 360 °C
 Sample: 0.1 - 0.01 wt% Hydrocarbon in CS₂ solvent, 1.0 μ L

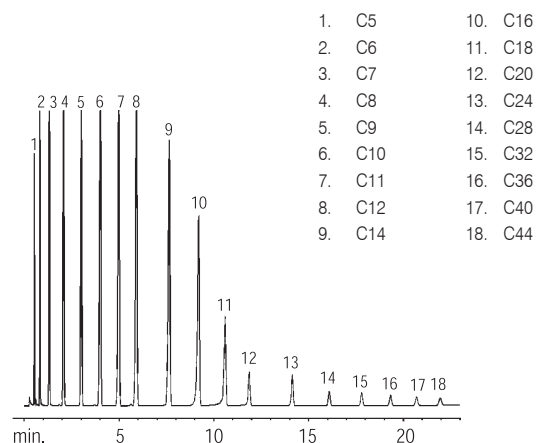


Hydrocarbons, C30 - C110

Column: DM-HT SimDist Metal, 5 m x 0.53 mm x 0.10 μ m
 Cat. No.: **7806**
 Index: CSR00530
 Oven Temp.: 40 °C to 430 °C (hold 30 min) at 10 °C/min
 Carrier Gas: He, 60 cm/sec
 Injection: On-column
 Flow Rate: 7.8 mL/min
 Head Pressure: 1.0 psi
 Solvent: CS₂
 Sample: Polywax 1000, 0.2 μ L
 Detector: FID, 430 °C

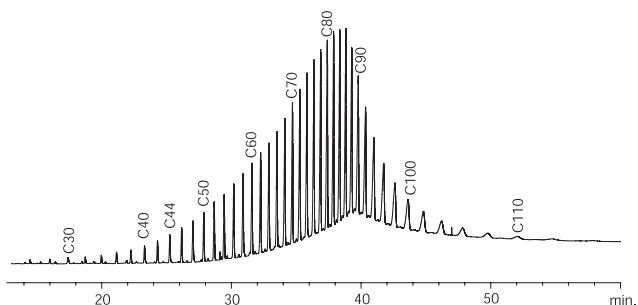

Hydrocarbons, C10 - C44


Column: DM-HT SimDist Metal, 5 m x 0.53 mm x 0.10 μ m
 Cat. No.: **7806**
 Index: CSR00529
 Oven Temp.: 40 °C to 430 °C (hold 30 min) at 10 °C/min
 Carrier Gas: He, 60 cm/sec
 Injection: On-column
 Flow Rate: 7.8 mL/min
 Head Pressure: 1.0 psi
 Solvent: CS₂
 Sample: Hydrocarbons, 0.2 μ L
 Detector: FID, 430 °C

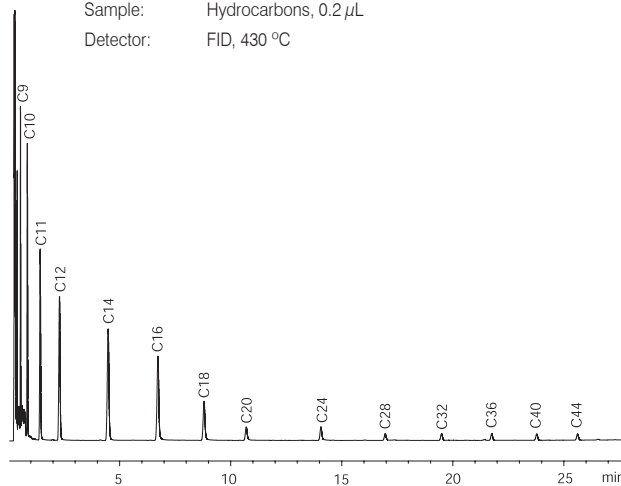

Detailed Hydrocarbons Analysis

Column: DM-PONA, 100 m x 0.25 mm x 0.50 μ m
 Cat. No.: 7805
 Index: CSR00209
 Oven Temp.: 35 °C (hold 13 min) to 45 °C (hold 15 min) at 10 °C/min
 to 60 °C (hold 15 min) at 1 °C/min to 200 °C (hold 5 min) at 1.9 °C/min
 Carrier Gas: He, 24 cm/sec, 35 °C
 Injection: Split, 100:1, 250 °C
 Sample: Reformulated gasoline, 0.5 μ L
 Detector: FID, 4 x 10⁻¹² AFS, 250 °C


- | | |
|----------------------------------|----------------------------|
| 1. Propane | 16. <i>p</i> -Xylene |
| 2. <i>iso</i> -Butane / Methanol | 17. 2,3-Dimethylheptane |
| 3. <i>n</i> -Butane | 18. <i>o</i> -Xylene |
| 4. <i>iso</i> -Pentane | 19. <i>n</i> -Nonane |
| 5. <i>n</i> -Pentane | 20. 1,3,5-Trimethylbenzene |
| 6. 3-Methylpentane | 21. 1,2,4-Trimethylbenzene |
| 7. <i>n</i> -Hexane | 22. <i>n</i> -Decane |
| 8. Benzene | 23. <i>n</i> -Undecane |
| 9. 2-Methylhexane | 24. Naphthalene |
| 10. <i>n</i> -Heptane | 25. <i>n</i> -Dodecane |
| 11. Toluene | 26. 2-Methylnaphthalene |
| 12. 2,3-Dimethylhexane | 27. <i>n</i> -Tridecane |
| 13. <i>n</i> -Octane | |
| 14. Ethylbenzene | |
| 15. <i>m</i> -Xylene | |

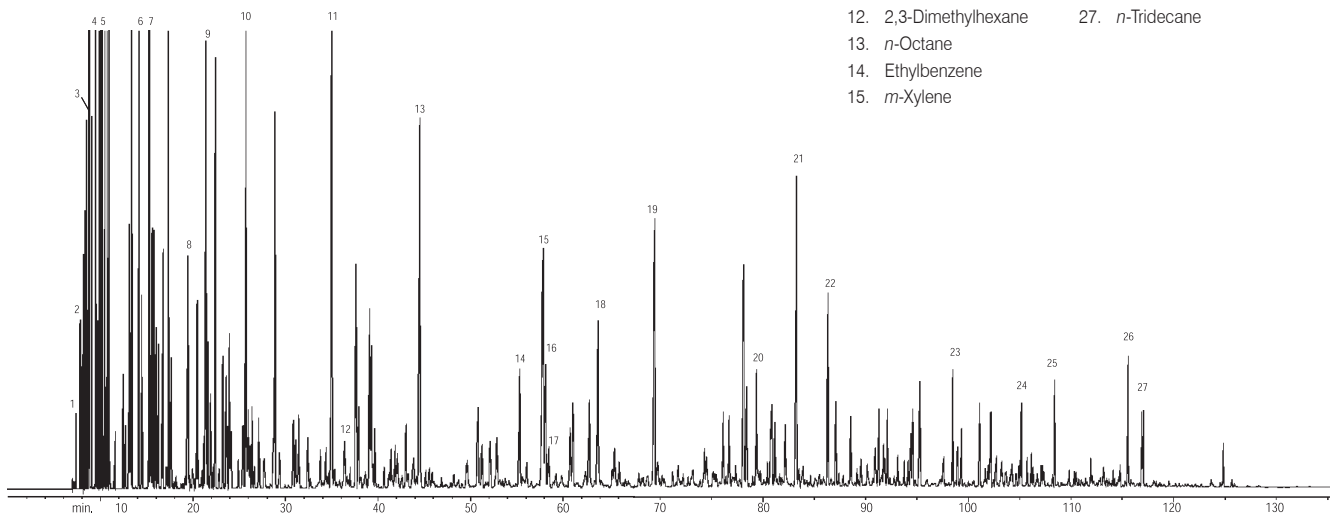

Hydrocarbons, C7 - C42

Column: DM-1, 30 m x 0.25 mm x 0.10 μ m
 Cat. No.: 7119
 Index: CSR00216
 Oven Temp.: 40 °C to 340 °C at 5 °C/min
 Carrier Gas: H₂, 40 cm/sec, 40 °C
 Injection: Direct, 340 °C
 Sample: 0.2 μ L Injection of a synthetic hydrocarbons mix, 0.1 mg/mL per component
 Detector: FID, 64 x 10⁻¹¹ AFS, 340 °C

- | | | | | |
|--------|---------|---------|---------|---------|
| 1. C7 | 6. C12 | 11. C17 | 16. C23 | 21. C30 |
| 2. C8 | 7. C13 | 12. C18 | 17. C24 | 22. C32 |
| 3. C9 | 8. C14 | 13. C19 | 18. C25 | 23. C34 |
| 4. C10 | 9. C15 | 14. C20 | 19. C26 | 24. C36 |
| 5. C11 | 10. C16 | 15. C22 | 20. C28 | 25. C38 |
| | | | | 26. C40 |
| | | | | 27. C42 |

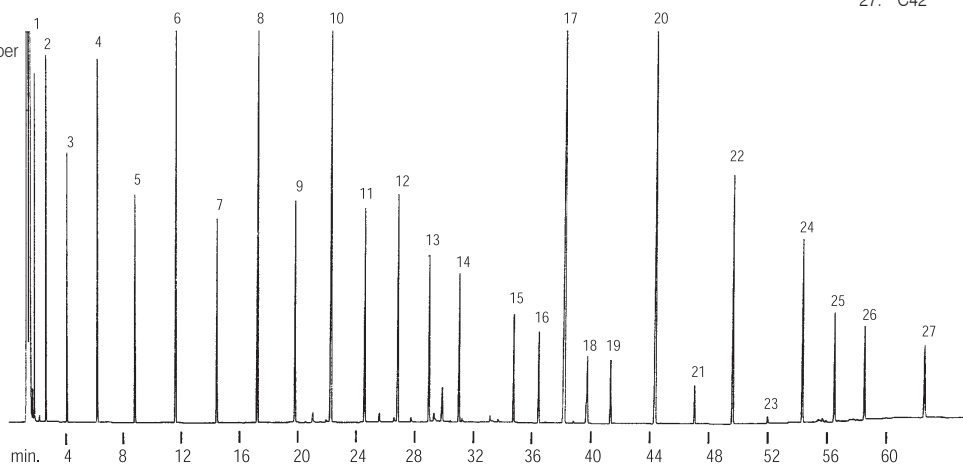



Applications

Petrochemicals

Gasoline Aromatics


Column: DM-1, 60 m x 0.25 mm x 1.00 μ m
Cat. No.: 7126
Index: CSR00215
Oven Temp.: 50 $^{\circ}$ C (hold 1 min) to 190 $^{\circ}$ C at 2 $^{\circ}$ C/min
Injection: Split, 200:1, 250 $^{\circ}$ C
Sample: Neat gasoline, 1.0 μ L
Detector: MS, 45 - 300 m/e, 1 scan/sec, 280 $^{\circ}$ C

1. Benzene
2. Toluene
3. Ethylbenzene
4. *m*-Xylene
5. *p*-Xylene
6. *o*-Xylene
7. Isopropyl benzene
8. *n*-Propylbenzene
9. 1-Methyl-3-ethylbenzene
10. 1-Methyl-4-ethylbenzene
11. 1,3,5-Trimethylbenzene
12. 1-Methyl-2-ethylbenzene
13. 1,2,4-Trimethylbenzene
14. 1,2,3-Trimethylbenzene
15. Indane
16. 1,4-Diethylbenzene
17. Butylbenzene
18. 1,2-Diethylbenzene
19. 1,2,4,5-Tetramethylbenzene
20. 1,2,3,5-Tetramethylbenzene
21. Pentamethylbenzene
22. Naphthalene
23. 2-Methylnaphthalene
24. 1-Methylnaphthalene

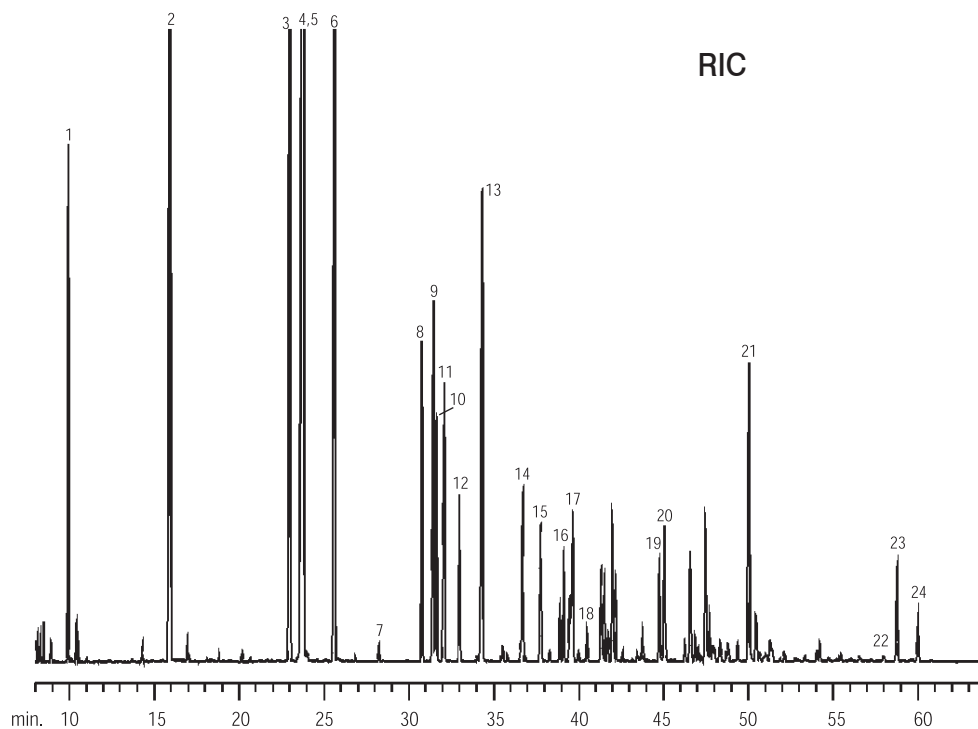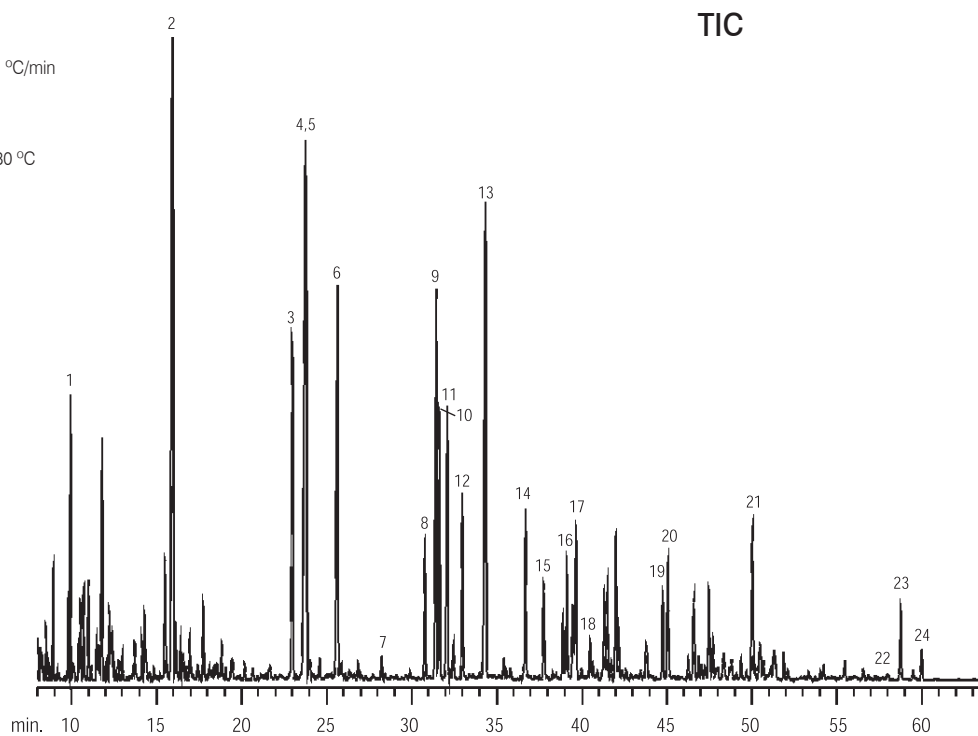

Aromatics (Benzene / Toluene / Xylene)


Column: DM-Wax, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7551
 Index: CSR00191
 Oven Temp.: 50 $^{\circ}$ C
 Carrier Gas: H₂, 40 cm/sec
 Injection: Direct, 250 $^{\circ}$ C
 Sample: Benzene, toluene, xylene, 0.1 μ L
 Detector: FID, 16 x 10⁻¹¹ AFS, 250 $^{\circ}$ C

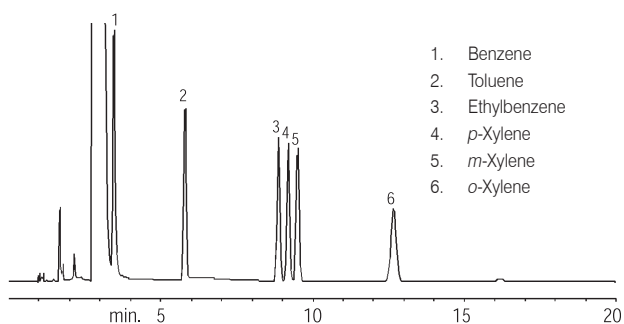

1. Benzene
2. Toluene
3. Ethylbenzene
4. *p*-Xylene
5. *m*-Xylene
6. *o*-Xylene

Aromatics (Benzene / Toluene / Xylene)


Column: DM-200, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 8347
 Index: CSR00189
 Oven Temp.: 60 $^{\circ}$ C
 Carrier Gas: He, 40 cm/sec
 Injection: Direct, 250 $^{\circ}$ C
 Sample: Benzene, toluene, xylene standard, 0.1 μ L
 Detector: FID, 4 X 10⁻¹¹ AFS, 250 $^{\circ}$ C

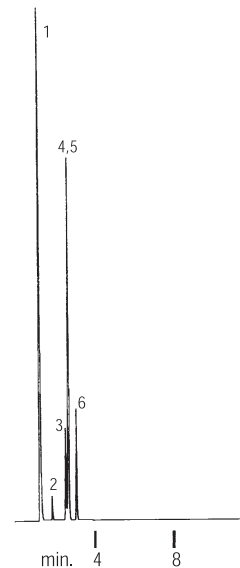

1. Benzene
2. Toluene
3. Ethylbenzene
4. *m*-Xylene
5. *p*-Xylene
6. *o*-Xylene

Aromatics


Column: DM-TCEP, 60 m x 0.25 mm x 0.40 μ m
 Cat. No.: 7809
 Index: CSR00211
 Oven Temp.: 60 $^{\circ}$ C (hold 5 min) to 100 $^{\circ}$ C (hold 10 min) at 5 $^{\circ}$ C/min
 Carrier Gas: He, 30 cm/sec, 80 $^{\circ}$ C
 Injection: Split, 46 mL/min, 200 $^{\circ}$ C
 Sample: 500 ppm (Ethylbenzene 1,000 ppm), 1.0 μ L
 Detector: FID, 6.4 x 10⁻¹¹ AFS, 200 $^{\circ}$ C

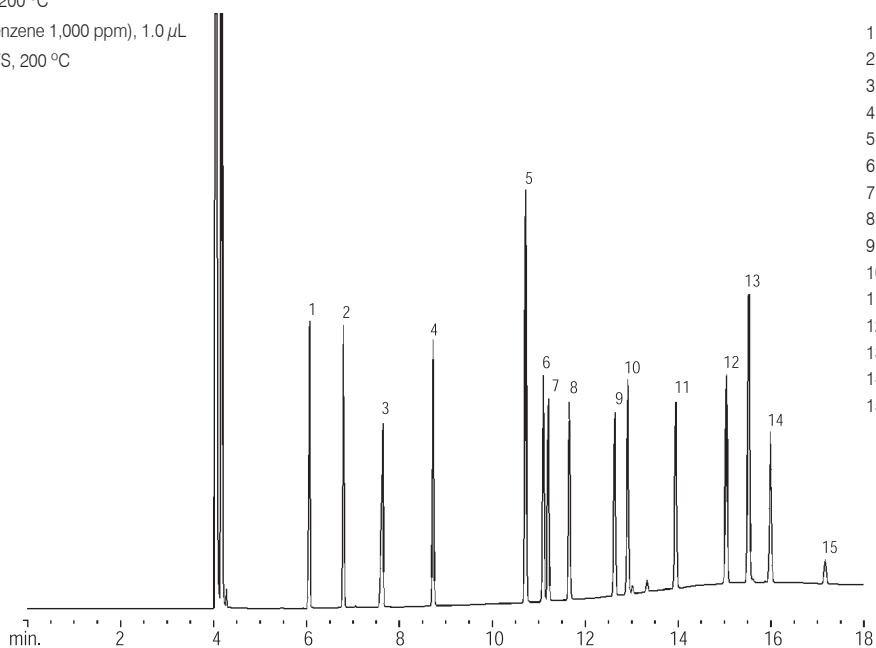

1. *n*-Undecane
2. Benzene
3. *n*-Dodecane
4. Toluene
5. Ethylbenzene
6. *p*-Xylene
7. *m*-Xylene
8. Cumene
9. *n*-Propylbenzene
10. *o*-Xylene
11. Mesitylene
12. 1-Ethyl-2-methylbenzene
13. *m*-Diethylbenzene
14. *p*-Diethylbenzene
15. *o*-Diethylbenzene


Petrochemicals

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7552
 Index: CCR00309
 Oven Temp.: 40 °C (hold 10 min) to 245 °C (hold 20 min) at 4 °C/min
 Carrier Gas: He, 50 cm/sec, 50 °C
 Injection: Split, 7:1, 250 °C
 Sample: Aromatics mixture, 1.0 μ L
 Detector: MS, 280 °C
 Ionization: EI

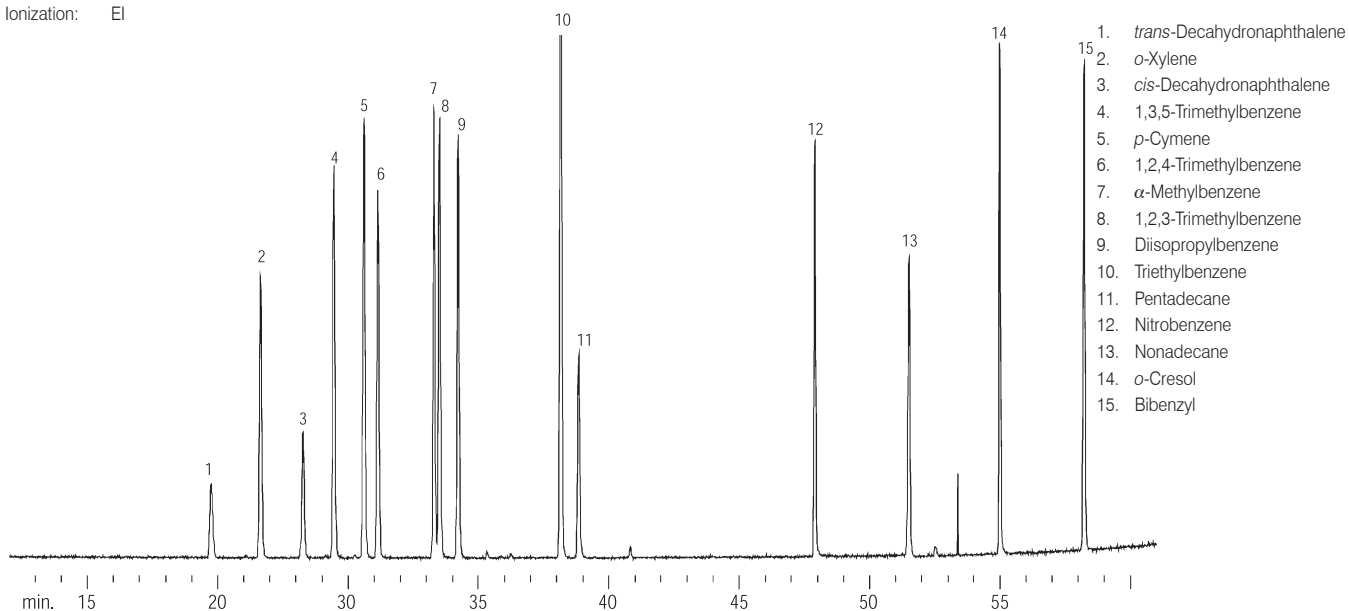


Aromatics

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7552
 Index: CCR00311
 Oven Temp.: 45 °C (hold 10 min) to 250 °C (hold 20 min) at 12 °C/min
 Carrier Gas: He, 50 cm/sec, 50 °C
 Injection: Split, 7:1, 250 °C
 Sample: Aromatics mixture, 1.0 μ L
 Detector: FID, 285 °C
 Ionization: EI, scan 10, range 300

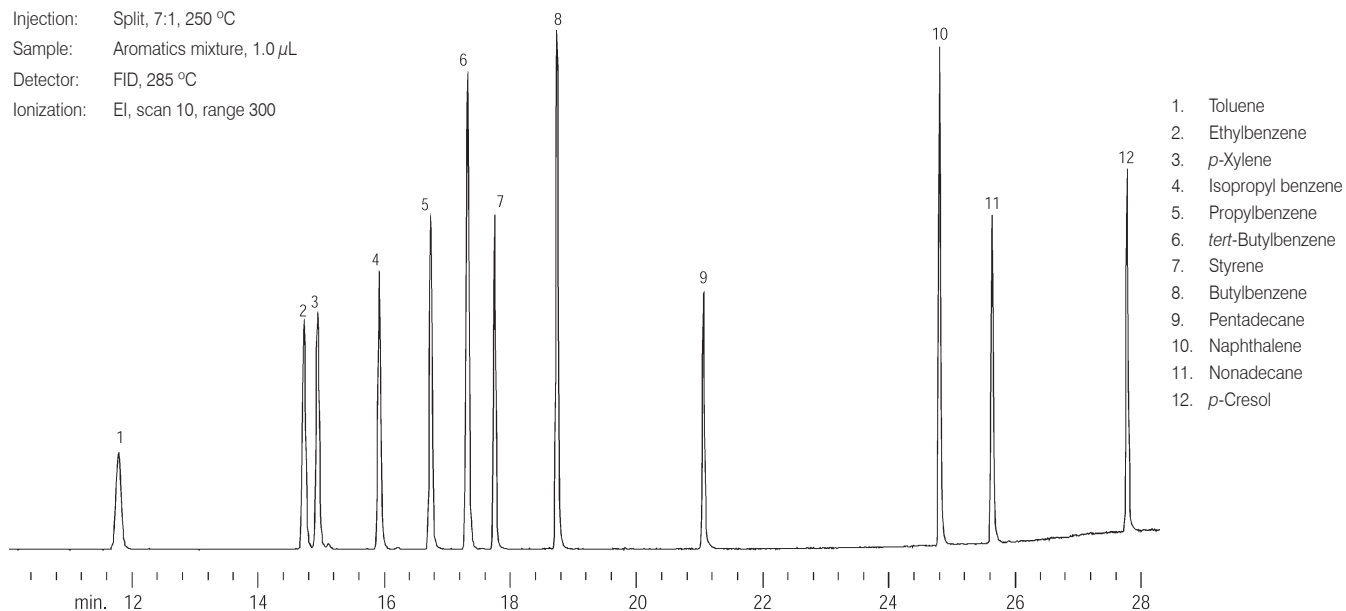


Primary Amines (Low MW)

Column: DM-Wax Amine, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7833
 Index: CCR00304
 Oven Temp.: 45 $^{\circ}$ C
 Carrier Gas: H₂, 40 cm/sec
 Injection: Direct, 1.0 μ L, 250 $^{\circ}$ C
 Sample: Amines in water, 1.0 μ L
 Detector: FID, 1 x 10⁻¹¹ AFS, 250 $^{\circ}$ C

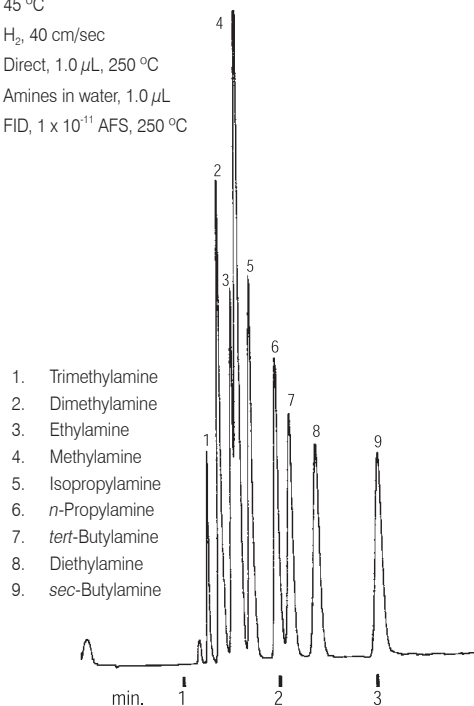


Amines (Low MW)

Column: DM-Wax Amine, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7833
 Index: CCR00305
 Oven Temp.: 50 $^{\circ}$ C
 Carrier Gas: H₂, 47 cm/sec
 Injection: Split, 40:1, 200 $^{\circ}$ C
 Sample: Methanol in water, 0.6 μ L, 500 ng/ μ L
 Detector: FID, 4 x 10⁻¹¹ AFS, 200 $^{\circ}$ C

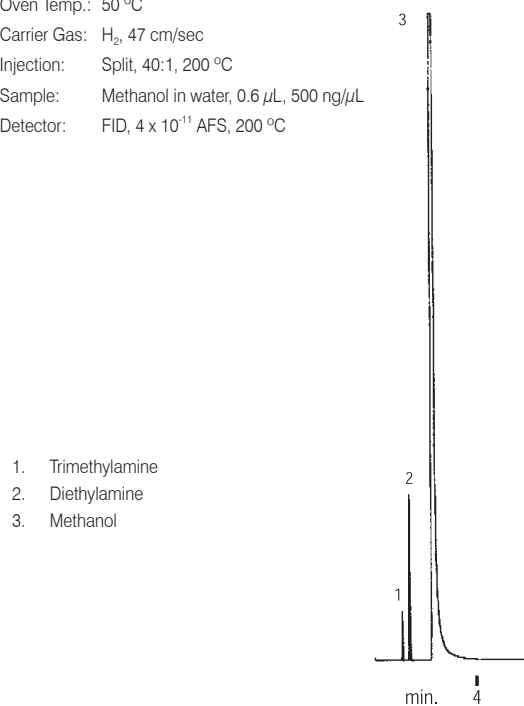


Primary Amines

Column: DM-35 Amine, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7825
 Index: CCR00578
 Oven Temp.: 35 $^{\circ}$ C (hold 5 min)
 Carrier Gas: He, 35.7 cm/sec constant pressure
 Injection: Split, 10:1
 Sample: Primary amines in water, 50 ppm, 1.0 μ L
 Detector: FID, 300 $^{\circ}$ C

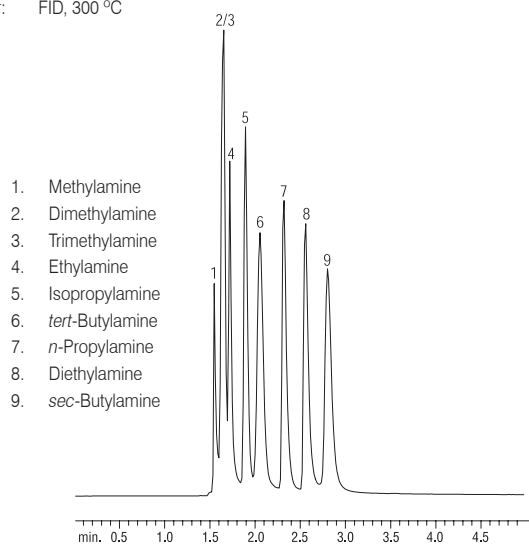

Short Chain Amines in Water


Column: DM-Volatile Amine, 60 m x 0.32 mm
 Cat. No.: 8857
 Index: CGN1154
 Sample: 200 - 1,000 ppm Short chain amines in water
 Injection: Split, 15:1, 1.0 μ L, 220 $^{\circ}$ C
 Oven Temp.: 40 $^{\circ}$ C (hold 10 min) to 250 $^{\circ}$ C (hold 10 min) at 20 $^{\circ}$ C/min
 Carrier Gas: H₂, 2.0 mL/min, 35 cm/sec, 40 $^{\circ}$ C
 Detector: FID, 250 $^{\circ}$ C

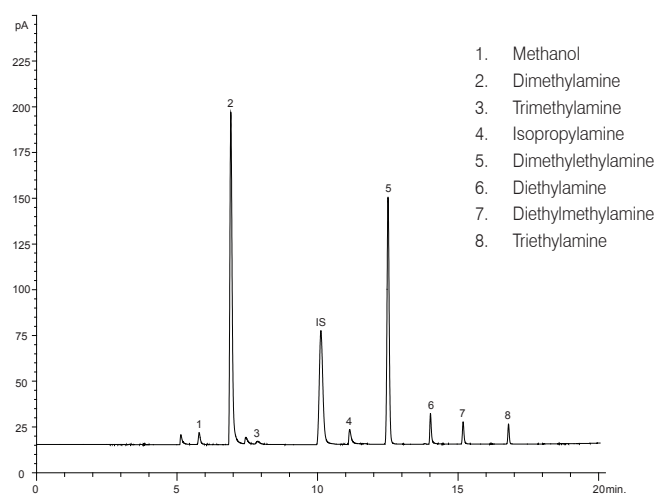

Amines

Ethylenediamines


Column: DM-5 Amine, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: 7815
 Index: CCR00298
 Oven Temp.: 40 °C (hold 4 min) to 315 °C (hold 5 min) at 10 °C/min
 Carrier Gas: H₂, 43 cm/sec, 40 °C
 Injection: Split, 20:1, 315 °C
 Sample: Ethylenediamines, 3.0 μ L, 5 – 80 ng
 Detector: FID, 6.4 x 10⁻¹¹ AFS, 315 °C

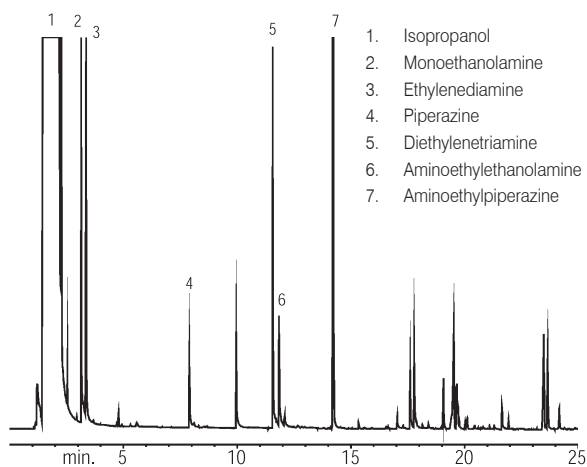

Ethanolamines

Column: DM-35 Amine, 30 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7823
 Index: CCR00585
 Oven Temp.: 50 °C (hold 0.5 min) to 280 °C at 15 °C/min
 Carrier Gas: He, 40 cm/sec constant pressure, 50 °C
 Injection: Split, 10:1, 300 °C
 Sample: 500 μ g/mL Ethanolamines standard in water, 1.0 μ L
 Detector: FID, 300 °C

1. Monoethanolamine
2. Diethanolamine
3. Triethylene glycol monomethylether
4. Triethanolamine


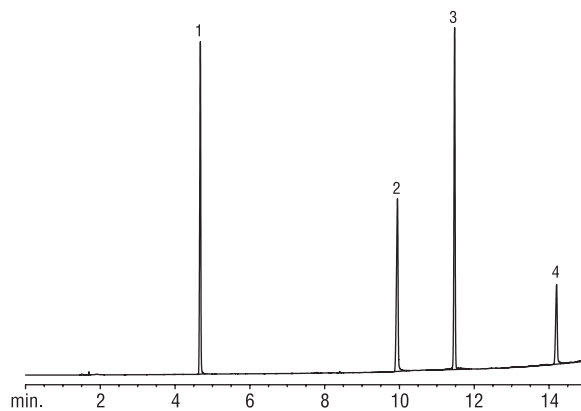


Hexamethylenediamine

Column: DM-Wax Amine, 30 m x 0.32 mm x 0.25 μ m
 Cat. No.: 7829
 Index: CCR00302
 Oven Temp.: 95 °C (hold 6 min) to 235 °C (hold 4 min) at 7 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Direct, 250 °C
 Sample: Hexamethylenediamine, 0.4 μ L, 10 - 100 ng
 Detector: FID, 2 x 10⁻¹¹ AFS, 250 °C


V.S.

Column: DM-Wax Amine, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7837
 Index: CCR00303
 Oven Temp.: 95 °C (hold 6 min) to 235 °C (hold 2 min) at 7 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Direct, 255 °C
 Sample: Hexamethylenediamine, 0.2 μ L
 Detector: FID, 64 x 10⁻¹¹, 255 °C

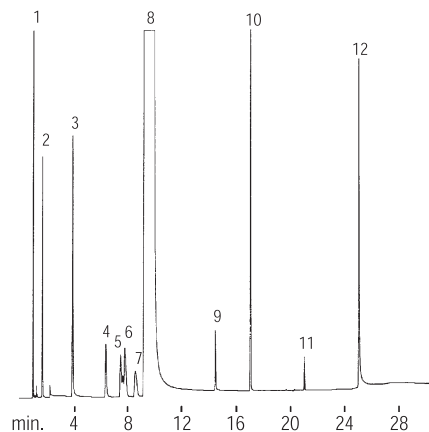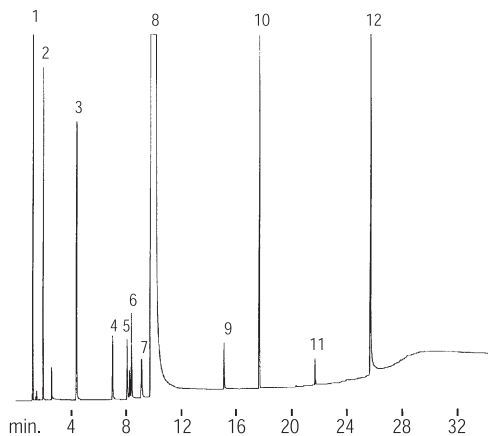


Nitrosamines

Column: DM-Wax Amine, 60 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7836
 Index: CCR00306
 Oven Temp.: 100 °C (hold 1 min) to 170 °C at 5 °C/min
 Carrier Gas: He, 100 cm/sec
 Injection: Direct, 200 °C
 Sample: Nitrosamines, 1.0 μ g/mL
 Detector: TSD, 200 °C

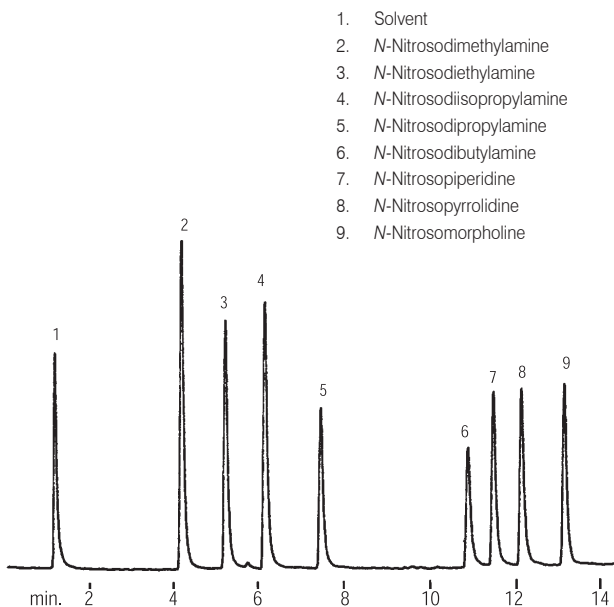


Amines / Alcohols / Chlorides

Column: DM-Wax, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7547
 Index: CCR00307
 Oven Temp.: 100 °C to 250 °C (hold 5 min) at 8 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 40:1, 250 °C
 Sample: Mix, 0.5 μ L
 Detector: FID, 128 x 10⁻¹¹ AFS, 250 °C

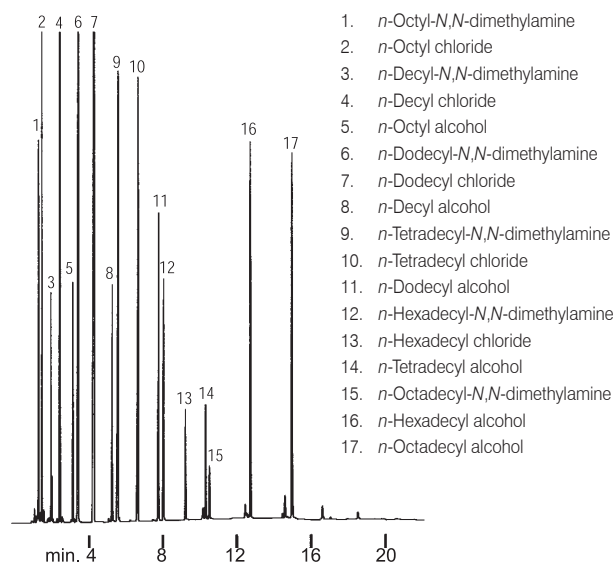

Amines / Phenols

Column: DM-5 Amine, 30 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7817
 Index: CCR00301
 Oven Temp.: 120 °C to 220 °C at 10 °C/min
 Carrier Gas: H₂, 38 cm/sec, 120 °C
 Injection: Split, 25:1, 305 °C
 Sample: Miscellaneous amines and phenols in water, 1.0 μ L, 22 ng
 Detector: FID, 6.4 x 10⁻¹¹ AFS, 305 °C


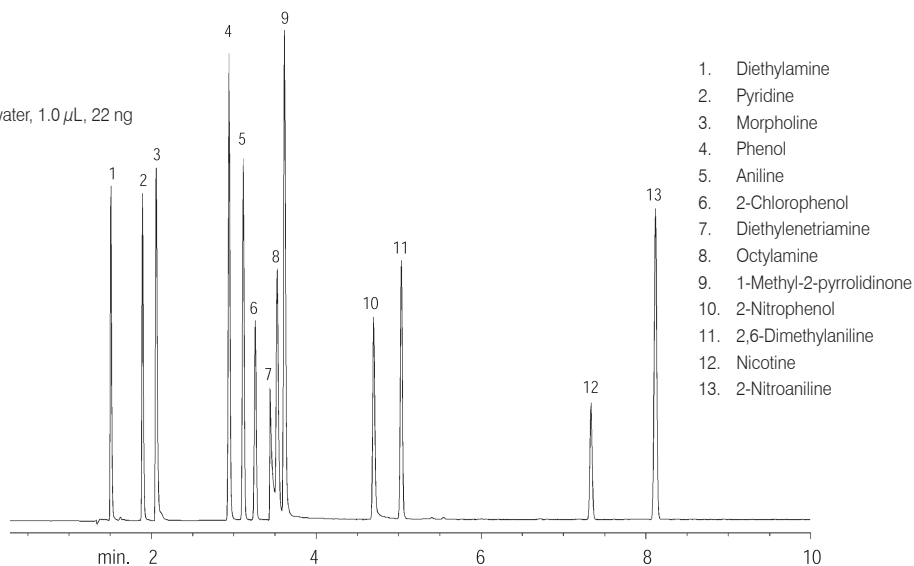


Alcohols

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7552
 Index: CCR00288
 Oven Temp.: 45 $^{\circ}$ C (hold 10 min) to 250 $^{\circ}$ C (hold 20 min) at 12 $^{\circ}$ C/min
 Carrier Gas: He, 51 cm/sec, 50 $^{\circ}$ C
 Injection: Split, 8:1, 250 $^{\circ}$ C
 Sample: Alcohols, 1.0 μ L
 Detector: MS, 250 $^{\circ}$ C
 Ionization: EI

- | | |
|---------------|-----------------|
| 1. Pentane | 11. Tetradecane |
| 2. Hexane | 12. 1-Heptanol |
| 3. Heptane | 13. 1-Octanol |
| 4. Ethanol | 14. Hexadecane |
| 5. Decane | 15. 1-Nonanol |
| 6. 1-Propanol | 16. 1-Decanol |
| 7. 1-Butanol | 17. 1-Undecanol |
| 8. Dodecane | 18. 1-Dodecanol |
| 9. 1-Pentanol | |
| 10. 1-Hexanol | |


- | | |
|---|--------------------------------|
| 1. Pentane | 12. 1-Pentanol |
| 2. Methanol | 13. 2-Methyl-1-pentanol |
| 3. 2-Methyl-2-propanol (<i>tert</i> -Butylalcohol) | 14. 2,2-Dimethyl-1-pentanol |
| 4. 2-Methyl-3-buten-2-ol | 15. Tetradecane |
| 5. 3-Buten-2-ol | 16. <i>trans</i> -2-Hexen-1-ol |
| 6. Undecane | 17. 1-Octanol |
| 7. 2,2-Dimethyl-1-propanol (Neopentanol) | 18. Ethylene glycol |
| 8. 1-Penten-3-ol | 19. 1-Undecanol |
| 9. 2-Methoxyethanol | 20. 1,4-Butanediol |
| 10. 2,2,2-Trifluoroethanol | |
| 11. 2-Ethoxyethanol | |

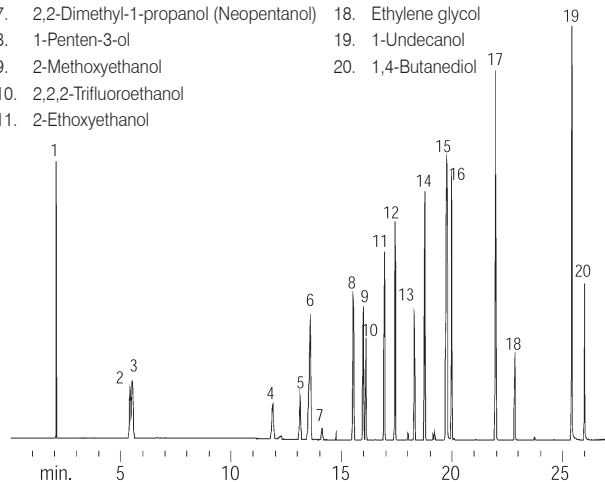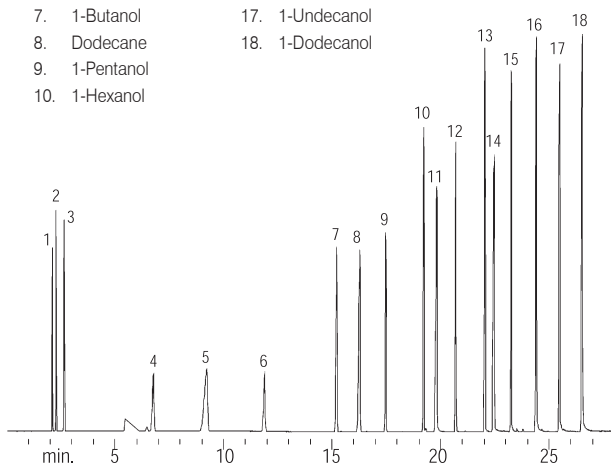

Applications

Alcohols


Column: DM-PLOT Q, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: 8818
 Index: CCR00495
 Oven Temp.: 100 $^{\circ}$ C to 240 $^{\circ}$ C (hold 10 min) at 5 $^{\circ}$ C/min
 Carrier Gas: He, 31 cm/sec, 100 $^{\circ}$ C
 Head Pressure: 18.0 psi
 Column Flow Rate: 1.1 cc/min, 100 $^{\circ}$ C
 Injection: Split, 70:1, 250 $^{\circ}$ C
 Sample: Alcohols, 1.0 μ L
 Detector: FID, 270 $^{\circ}$ C

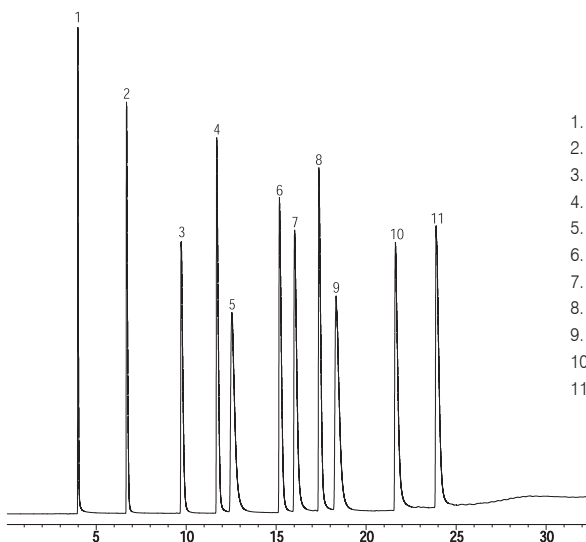

- | |
|-------------------------|
| 1. Methanol |
| 2. Ethanol |
| 3. 2-Propanol |
| 4. 1-Propanol |
| 5. <i>tert</i> -Butanol |
| 6. 2-Butanol |
| 7. Isobutyl alcohol |
| 8. 1-Butanol |
| 9. 2-Methyl-2-butanol |
| 10. 3-Methyl-1-butanol |
| 11. 4-Methyl-2-pentanol |


Glycols

Column: DM-Wax, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7551
 Index: CER00476
 Oven Temp.: 80 °C to 200 °C (hold 10 min) at 8 °C/min
 Solvent: H₂O:MeOH = 50:50
 septa purge 5.0 cc/min
 Carrier Gas: He, 50 cm/sec
 Injection: Direct
 Flow Rate: 6.9 mL/min
 Sample: Glycol mix, 1.0 μ L, 150 ppm
 Detector: FID, 270 °C

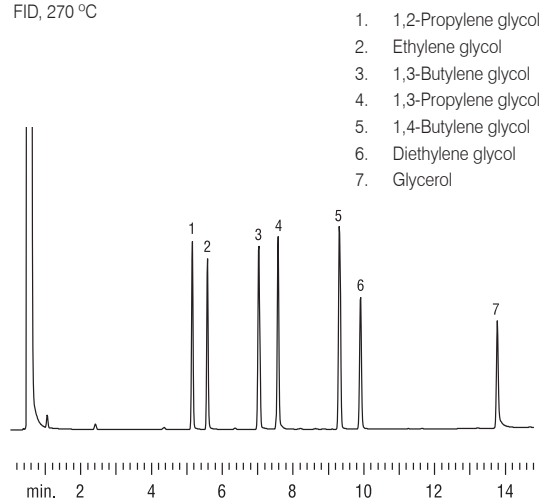


Alcohols

Column: DM-5, 60 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7236
 Index: CCR00292
 Oven Temp.: 25 °C (hold 4 min) to 80 °C (hold 5 min) at 8 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 40:1, 200 °C
 Sample: Alcohol mix, 0.03 μ L
 Detector: FID, 128 x 10⁻¹¹ AFS, 200 °C

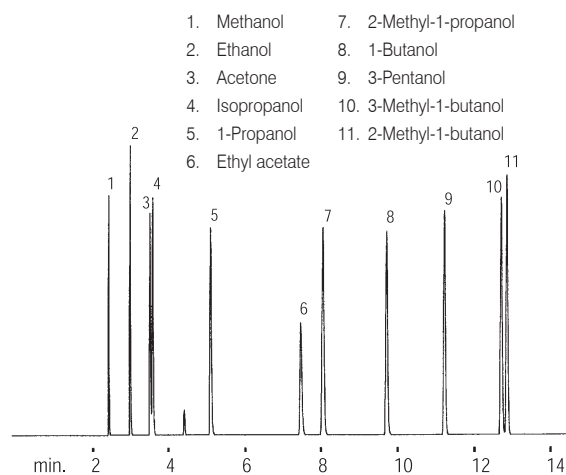


Glycols

Column: DM-200, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 8356
 Index: CCR00326
 Oven Temp.: 40 °C to 250 °C (hold 15 min) at 8 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 19:1, 200 °C
 Sample: Glycols, 1.0 μ L, 50 ng on-column
 Detector: FID, 6.4 x 10⁻¹¹ AFS, 250 °C

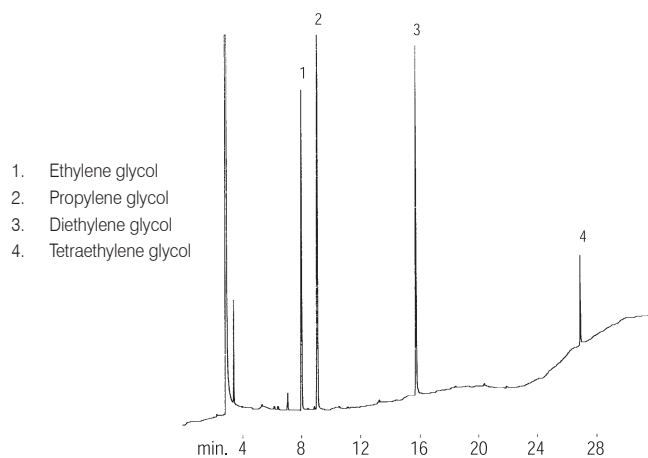

Glycols / Alcohols


Column: DM-5, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7249
 Index: CCR00327
 Oven Temp.: 40 °C to 185 °C (hold 5 min) at 15 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Direct, 150 °C
 Sample: Glycols and alcohols, 1.0 μ L, 100 ppm
 Detector: FID, 8 x 10⁻¹¹ AFS, 200 °C

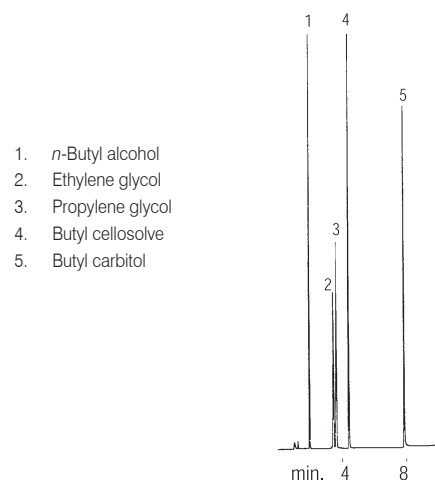

Aldehydes / Ketones


Alcohols / Aldehydes

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
Cat. No.: 7552
Index: CCR00295
Oven Temp.: 45 °C (hold 10 min) to 250 °C (hold 20 min) at 12 °C/min
Carrier Gas: He, 50 cm/sec, 50 °C
Injection: Split, 7:1, 250 °C
Sample: Alcohols and aldehydes, 1.0 μ L
Detector: FID, 285 °C
Ionization: EI, scan 10, range 300

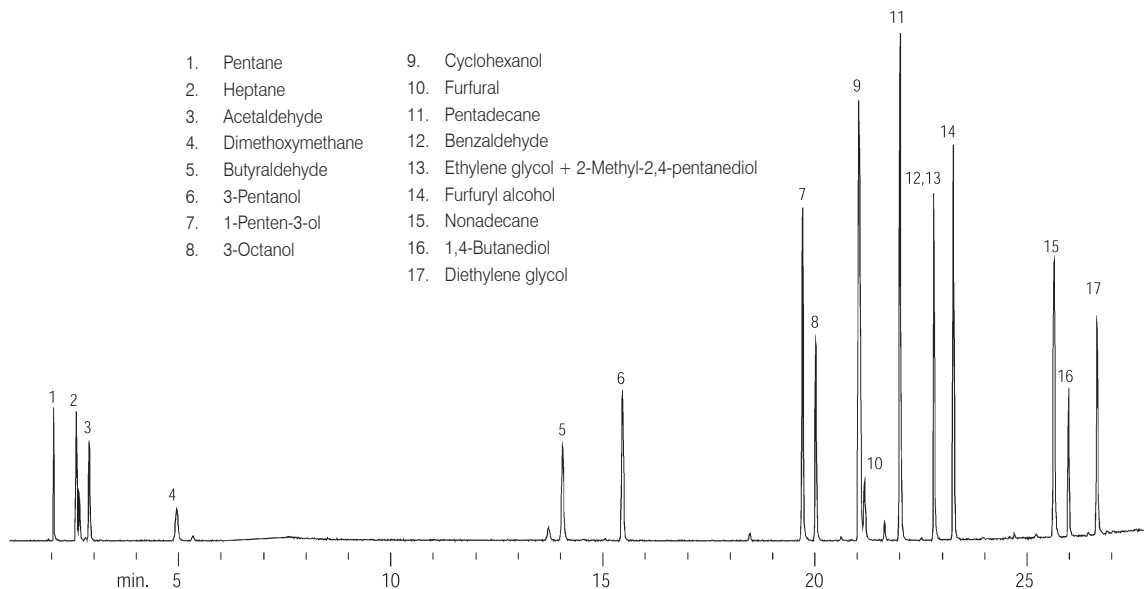


Aldehydes

Column: DM-InertWax, 30 m x 0.25 mm x 0.50 μ m
Cat. No.: 8523
Index: CCR00300
Oven Temp.: 40 °C (hold 5 min) to 200 °C at 10 °C/min
Carrier Gas: H₂, 35 cm/sec, 40 °C
Injection: Split, 100:1, 200 °C
Sample: C2-C11 Aldehydes mix, 250 ng on-column
Detector: FID, 82 x 10⁻¹¹ AFS, 200 °C

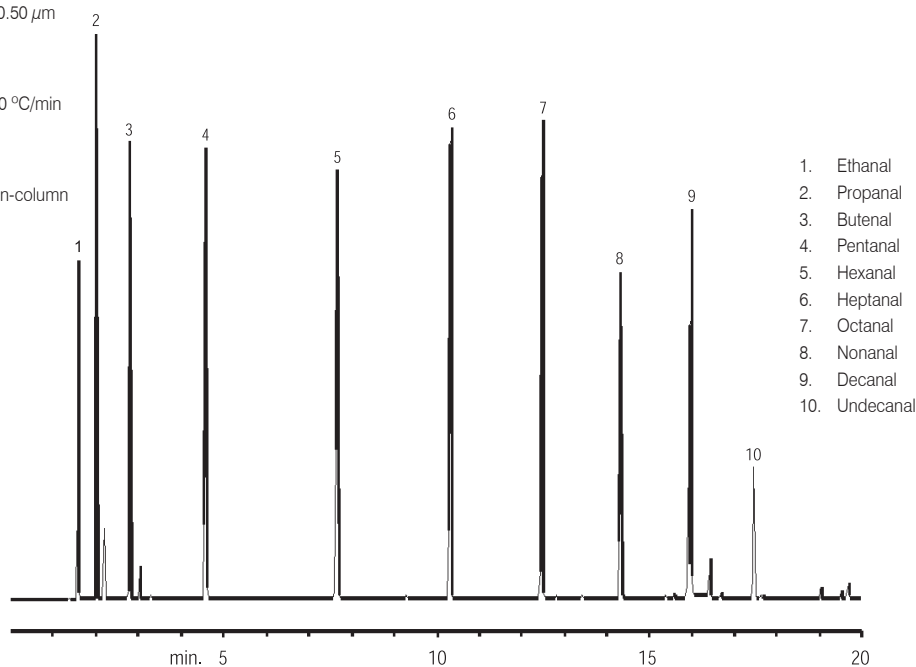


Formaldehyde

Column: DM-1701, 60 m x 0.25 mm x 1.00 μ m
 Cat. No.: 7324
 Index: CCR00313
 Oven Temp.: 40 °C constant
 Carrier Gas: He, 20 cm/sec
 Injection: Split, 30 mL/min, 150 °C
 Sample: Formaldehyde, 0.5 μ L
 Detector: TCD, 8 mV, 175 °C

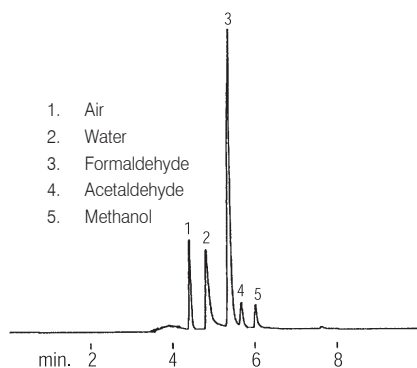

Ketones


Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7552
 Index: CCR00316
 Oven Temp.: 45 °C (hold 10 min) to 250 °C (hold 20 min) at 12 °C/min
 Carrier Gas: He, 51 cm/sec, 50 °C
 Injection: Split, 8:1, 250 °C
 Sample: Ketones, 1.0 μ L
 Detector: MSD, 250 °C
 Ionization: EI

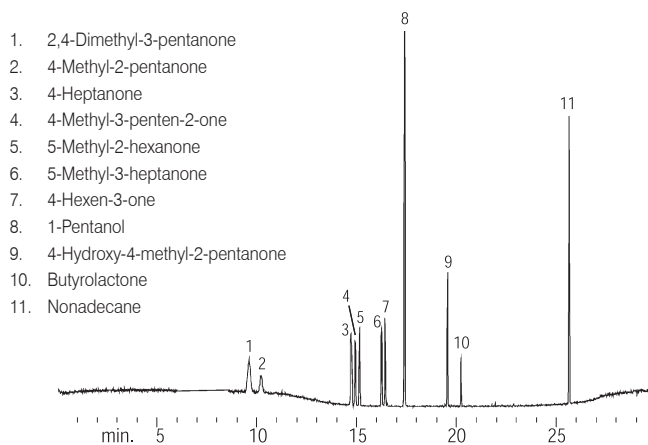

Aldehydes

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7552
 Index: CCR00315
 Oven Temp.: 45 °C (hold 10 min) to 250 °C (hold 20 min) at 12 °C/min
 Carrier Gas: He, 51 cm/sec, 50 °C
 Injection: Split, 8:1, 250 °C
 Sample: Aldehydes, 1.0 μ L
 Detector: MSD, 250 °C
 Ionization: EI

- | | |
|----------------------|---------------------------|
| 1. Pentane | 11. Heptanal |
| 2. Acetaldehyde | 12. 1-Pentanol |
| 3. Dimethoxymethane | 13. Octanal |
| 4. Propanal | 14. Tetradecane |
| 5. 2-Methyl propanal | 15. Nonanal |
| 6. Methanol | 16. 2-Furancarboxaldehyde |
| 7. Pentanal | 17. Decanal |
| 8. 2-Butenal | 18. Benzaldehyde |
| 9. Hexanal | 19. 1-Octanol |
| 10. Undecane | |

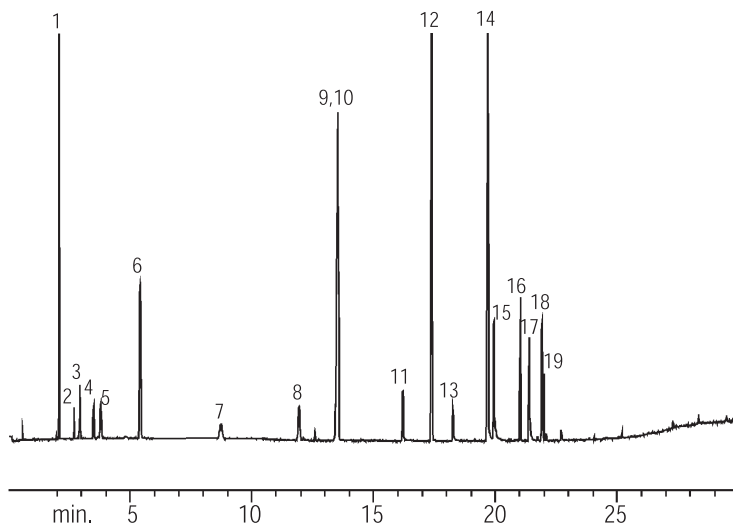

Esters

Esters

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m

Cat. No.: 7552

Index: CCR00314

Oven Temp.: 45 °C (hold 10 min) to 250 °C (hold 20 min) at 12 °C/min


Carrier Gas: He, 50 cm/sec, 50 °C

Injection: Split, 7:1, 250 °C

Sample: Esters, 1.0 μ L

Detector: MS, 285 °C

1. Pentane
2. Heptane
3. Methyl formate
4. Methyl acetate
5. Methyl propionate
6. Methyl butyrate
7. Methyl valerate
8. Methyl hexanoate
9. Methyl octanoate
10. Pentadecane
11. Methyl decanoate
12. Methyl benzoate
13. Nonadecane

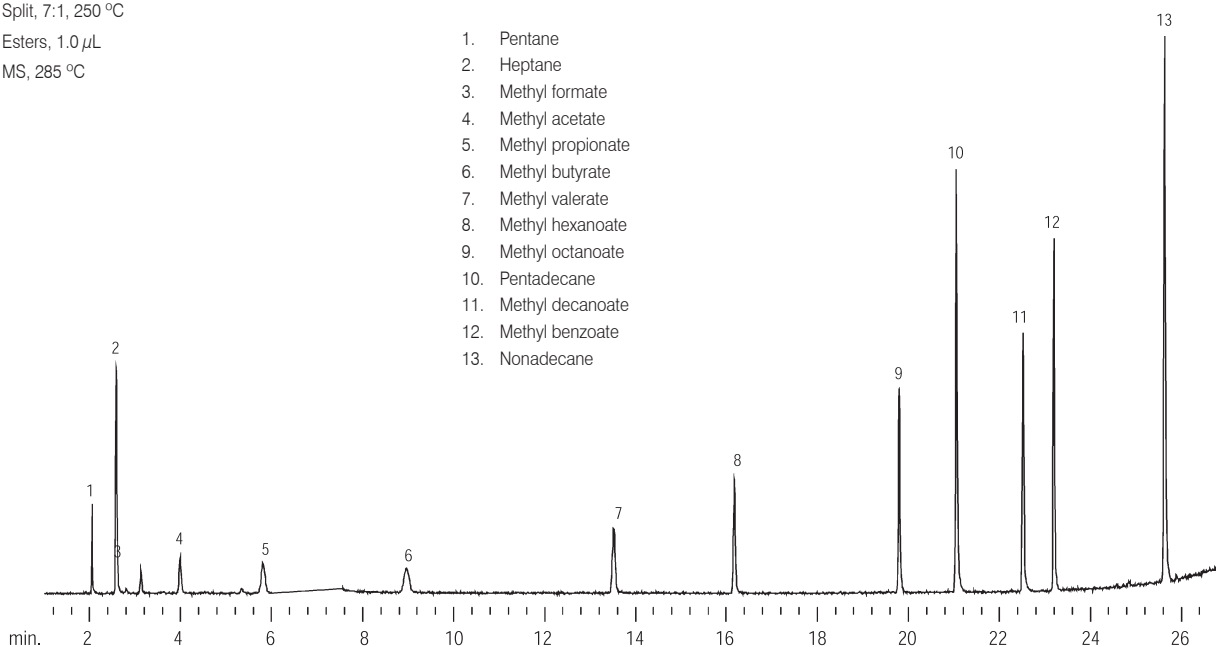

Esters

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m

Cat. No.: 7552

Index: CCR00318

Oven Temp.: 40 °C (hold 10 min) to 245 °C (hold 20 min) at 4 °C/min


Carrier Gas: He, 50 cm/sec, 50 °C

Injection: Split, 7:1, 250 °C

Sample: Esters, 1.0 μ L


Detector: MS, 280 °C

1. Tetrahydro-2-methyl furan
2. Butyraldehyde
3. Butyl ether
4. 1,3-Dioxolane
5. Ethyl acrylate
6. 1,4-Dioxane
7. 2-Methoxy ethyl ether
8. 2-Ethoxy ethyl ether
9. Pentadecane
10. 1,2-bis(2-Methoxyethoxy)ethane
11. Nonadecane
12. bis(2-(2-Methoxyethoxy)ethyl)ether
13. Benzyl ether

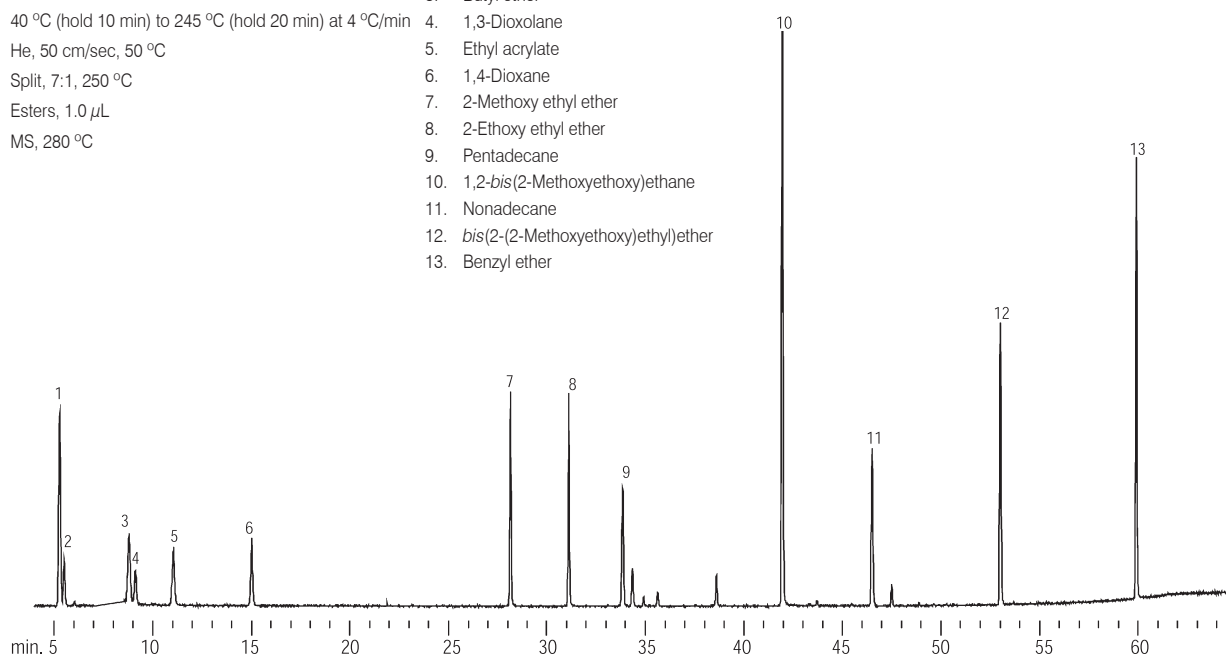


Acrylic Esters

Column: DM-1701, 30 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7333
 Index: CCR00312
 Oven Temp.: 70 °C (hold 10 min) to 120 °C at 5 °C/min to 250 °C at 15 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 56:1, 250 °C
 Sample: Acrylic esters, 0.5 μ L
 Detector: FID, 4 x 10⁻¹¹ AFS, 250 °C

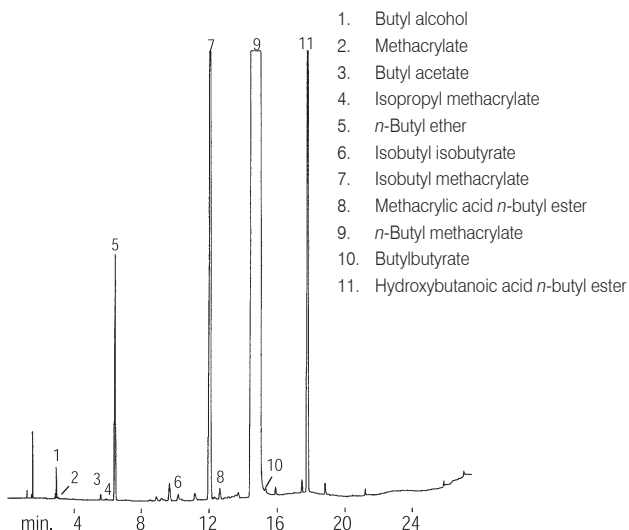


Silanes

Column: DM-200, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 8356
 Index: CCR00362
 Oven Temp.: 40 °C to 250 °C (hold 5 min) at 8 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 40 mL/min, 200 °C
 Sample: Silanes, 0.5 μ L
 Detector: FID, 1.02 x 10⁻⁹ AFS, 270 °C

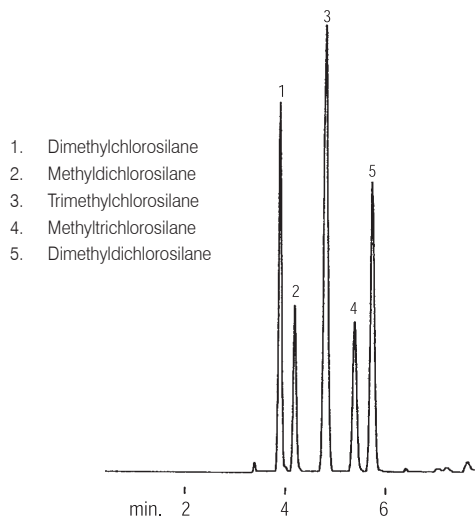


Styrene Impurities

Column: DM-Wax, 30 m x 0.53 mm x 0.50 μ m
 Cat. No.: 7547
 Index: CCR00356
 Oven Temp.: 40 °C (hold 10 min) to 150 °C (hold 15 min) at 10 °C/min
 Carrier Gas: He, 20 cm/sec, 40 °C
 Injection: Split, 40 cc/min, 150 °C
 Sample: 95% Styrene, 0.5 mL
 Detector: FID, 16 x 10⁻¹¹ AFS, 150 °C

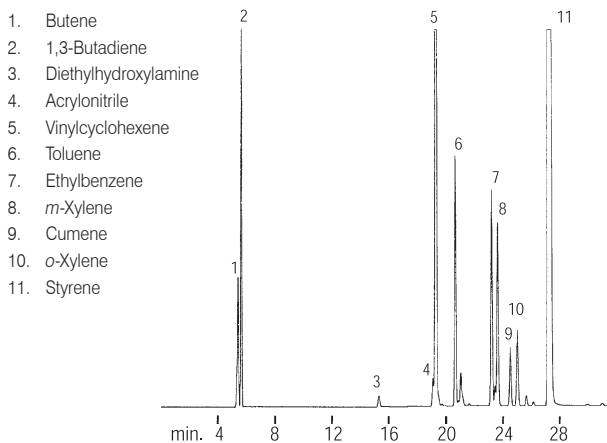

Styrene Impurities


Column: DM-1701, 30 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7355
 Index: CCR00357
 Oven Temp.: 40 °C (hold 10 min) to 150 °C (hold 15 min) at 12 °C/min
 Carrier Gas: He, 20 cm/sec, 40 °C
 Injection: Split, 40 cc/min, 150 °C
 Sample: 95% Styrene, 0.5 mL
 Detector: FID, 16 x 10⁻¹¹ AFS, 150 °C

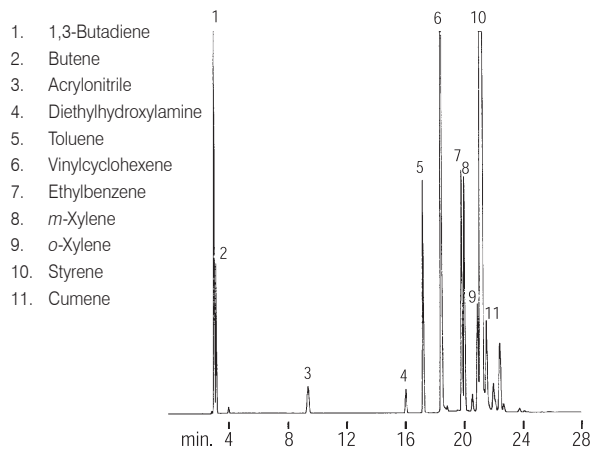

Solvents

USP Solvents


Column: DM-1, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7156
 Index: CER00463
 Oven Temp.: 35 $^{\circ}$ C (hold 4min) to 250 $^{\circ}$ C at 4 $^{\circ}$ C/min
 septa purge 5 mL/min
 Carrier Gas: He, 45.6 cm/sec, 35 $^{\circ}$ C
 Head Pressure: 11.0 psi constant pressure
 Injection: Split, 100 mL/min, ~1:13, 250 $^{\circ}$ C
 Sample: Solvents, ~1.3% each
 Detector: MS
 Scan Range: 10 AMU - 260 AMU

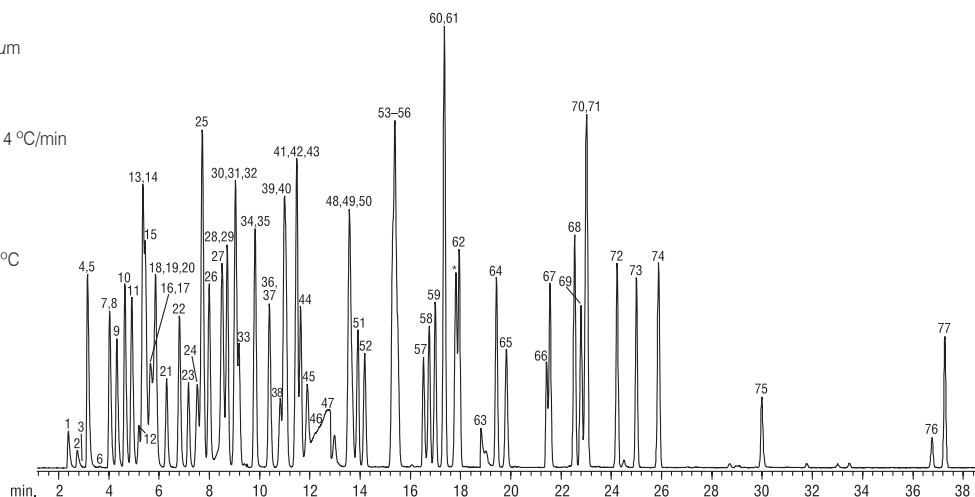

- | | | | | |
|---------------------|--------------------------------------|-----------------------------|---------------------------|-----------------------------------|
| 1. Formaldehyde | 17. Methylal | 33. Chloroform | 49. Trichloroethylene | 65. 1,1-Diethoxypropane |
| 2. Water | 18. 1,1-Dichloroethene | 34. Tetrahydrofuran | 50. Isooctane | 66. <i>N,N</i> -Dimethylacetamide |
| 3. Chloromethane | 19. Methyl acetate | 35. 2-Methoxyethanol | 51. 2-Ethoxyethanol | 67. Chlorobenzene |
| 4. Methanol | 20. Methylene chloride | 36. 1,2-Dichloroethane | 52. <i>n</i> -Heptane | 68. Ethylbenzene |
| 5. Acetaldehyde | 21. Nitromethane | 37. Methyl cyclopentane | 53. Isoamyl alcohol | 69. Isoamyl acetate |
| 6. Ethylene oxide | 22. 1-Propanol | 38. 1,1,1-Trichloroethane | 54. Hexanone | 70. <i>p</i> -Xylene |
| 7. Chloroethane | 23. <i>trans</i> -1,2-Dichloroethene | 39. 1,2-Dimethoxyethane | 55. Pyridine | 71. <i>m</i> -Xylene |
| 8. Ethanol | 24. Methyl <i>tert</i> -butyl ether | 40. Methyl isopropyl ketone | 56. Methyl cyclohexane | 72. <i>o</i> -Xylene |
| 9. Acetonitrile | 25. 2-Methylpentane (spiked at 9%) | 41. 2,2-Dimethoxypropane | 57. Dimethyl formamide | 73. Anisole |
| 10. Acetone | 26. 2-Butanone | 42. Isopropyl acetate | 58. 1,1,2-Trichloroethane | 74. Isopropyl benzene (Cumene) |
| 11. 2-Propanol | 27. 2-Butanol | 43. 1-Butanol | 59. 1-Pentanol | 75. 1-Methyl-2-pyrrolidinone |
| 12. 2-Chloropropane | 28. <i>cis</i> -1,2-Dichloroethene | 44. Benzene | 60. Isobutyl acetate | 76. Sulfolane |
| 13. Diethyl ether | 29. Acetic acid | 45. Carbon tetrachloride | 61. Toluene | 77. 1,2,3,4-Tetrahydronaphthalene |
| 14. Pentane | 30. Isopropyl ether | 46. Ethylene glycol | 62. 2-Hexanone | |
| 15. Ethyl formate | 31. Ethyl acetate | 47. Formamide | 63. Dimethyl sulfoxide | |
| 16. Formic acid | 32. Hexane | 48. 1,4-Dioxane | 64. Butyl acetate | |


USP Solvents

Column: DM-200, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 8356
 Index: CER00464
 Oven Temp.: 35 $^{\circ}$ C (hold 4 min) to 250 $^{\circ}$ C at 4 $^{\circ}$ C/min
 Head Pressure: 11.0 psi constant pressure
 Carrier Gas: He, 45.6 cm/sec, 35 $^{\circ}$ C
 Injection: Split, 100 mL/min, 1:13, 250 $^{\circ}$ C
 Sample: Solvents, ~1.3% each
 Detector: MS
 Scan Range: 10 AMU - 260 AMU

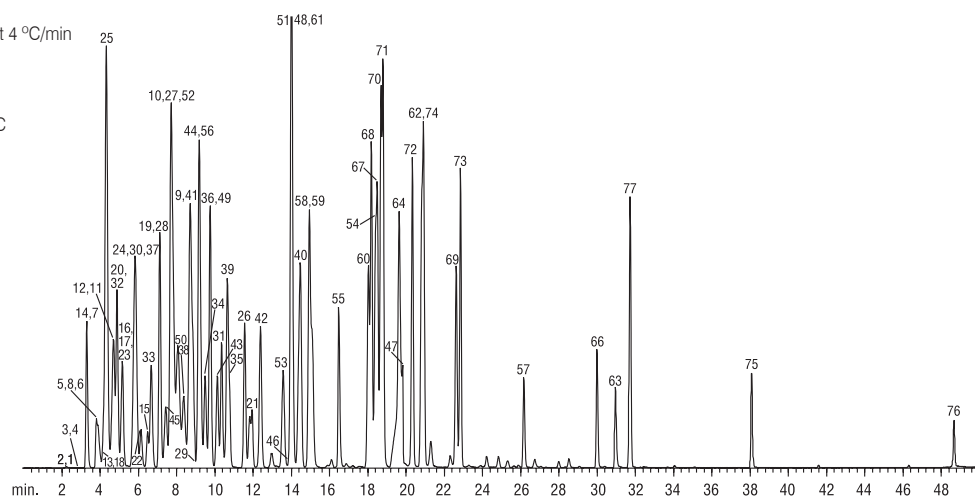

Solvents Mixture #1

Column: DM-1, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7156
 Index: CCR00335
 Oven Temp.: 40 °C (hold 5 min) to 285 °C at 5 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Split, 50 mL/min, 275 °C
 Sample: Solvents mixture #1, 1.0 μ L
 Detector: MS full scan, 285 °C

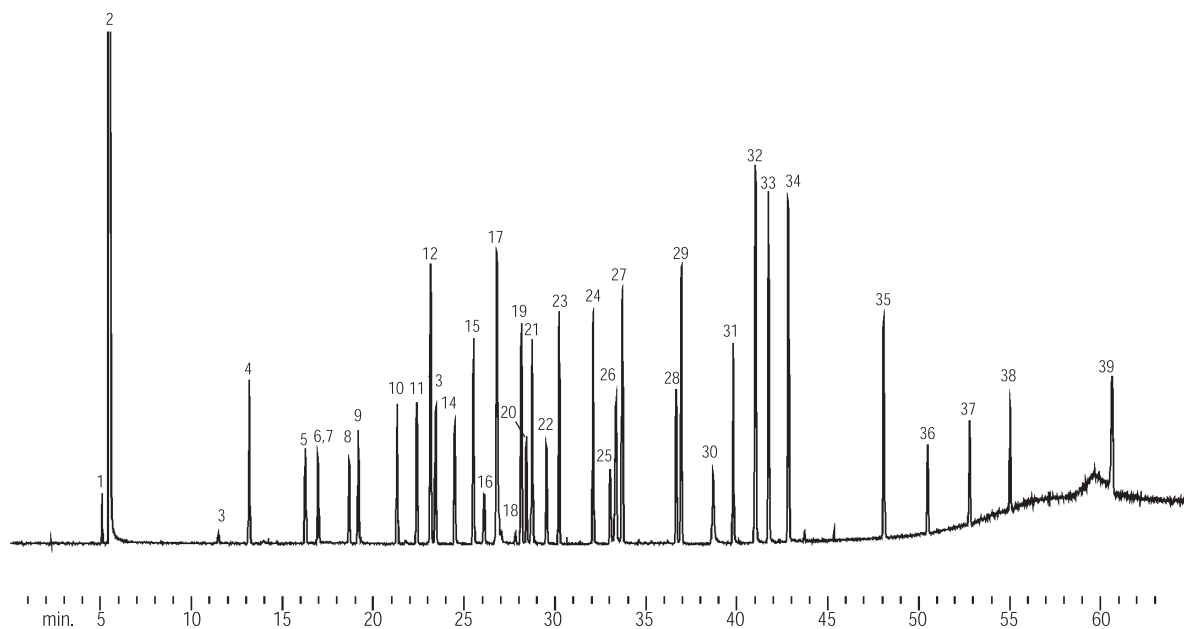


1. Pentane	22. Hexachloroethane	43. 1-Nitropropane	64. 1-Dodecanol	85. 2-Methyl-2,4-pentanediol
2. Methylene chloride	23. Undecane	44. Dimethyl formamide	65. Tetraethylene glycol	86. Butoxyethanol
3. Ethylene glycol	24. 1-Nonanol	45. 2-Methyl-3-pentanol	66. Dibenzyl	87. 1,2,3-Trichloropropane
4. Heptane	25. <i>p</i> -Methoxyphenol	46. Toluene	67. Diethyl phthalate	88. 1,4-Butanediol
5. Cyclopentanol	26. Triethylene glycol	47. Ethyl chloroacetate	68. Tributyl phosphate	89. Methyl hexanoate
6. 3-Hexanol	27. Dodecane	48. Dimethylacetamide	69. Diphenyl sulfone	90. 1,2,4-Trimethylbenzene
7. Acetamide	28. Undecanal	49. <i>p</i> -Xylene	70. Allyl alcohol	91. 2-Ethyl-1-hexanol
8. 2-Methyl-1-pentanol	29. Tridecane	50. <i>sec</i> -Tetrachloroethane	71. -	92. Dipentene
9. Furfuryl alcohol	30. -	51. Benzaldehyde	72. Isopropyl acetate	93. Tetrahydrofurfuryl acetate
10. Butyl ether	31. Dodecanal	52. <i>o</i> -Chlorotoluene	73. Benzene	94. -
11. Nonane	32. Dicyclohexylamine	53. 2,6-Dimethyl-4-heptanone	74. 2-Nitropropane	95. Decahydronaphthalene
12. Cume ne	33. <i>bis</i> (2,2-Methoxy)ethyl ether	54. 2-Octanone	75. Nitroethane	96. -
13. Ethyl amyl ketone	34. Pentadecane	55. <i>o</i> -Cresol	76. Pentanal	97. -
14. Heptanol	35. Heptadecane	56. α -Methylbenzyl alcohol	77. 2-Bromobutane	98. 2-Decanol
15. Butyl butanoate	36. Octadecane	57. 5-Nonanone	78. 1-Chloropentane	99. 1,2- <i>bis</i> (2-Methoxyethoxy)ethane
16. -	37. Nonadecane	58. Nonanal	79. Cyclopentanone	100. 2-Phenoxyethanol
17. Benzyl alcohol	38. Eicosane	59. Decanal	80. 2-Hexanol	101. -
18. Dipropylene glycol	39. Acetyl tributyl citrate	60. -	81. Butyl acetate	102. Benzyl ether
19. Diethylbenzene	40. 2-Buten-1-ol	61. 1-Decanol	82. 2-Ethyl-1-butanol	
20. -	41. Formamide	62. 1-Undecanol	83. 3-Ethyl-3-pentanol	
21. -	42. 3-Pentanol	63. 2-Dodecanone	84. 1,4-Dichlorobutane	

Solvents


Solvents Mixture #1

Column: DM-200, 60 m x 0.53 mm x 3.00 μ m
Cat. No.: 8356
Index: CCR00336
Oven Temp.: 40 $^{\circ}$ C (hold 5 min) to 285 $^{\circ}$ C at 5 $^{\circ}$ C/min
Carrier Gas: He, 40 cm/sec
Injection: Split, 50 mL/min, 275 $^{\circ}$ C
Sample: Solvents mixture #1, 1.0 μ L
Detector: MS, TIC mode, 285 $^{\circ}$ C

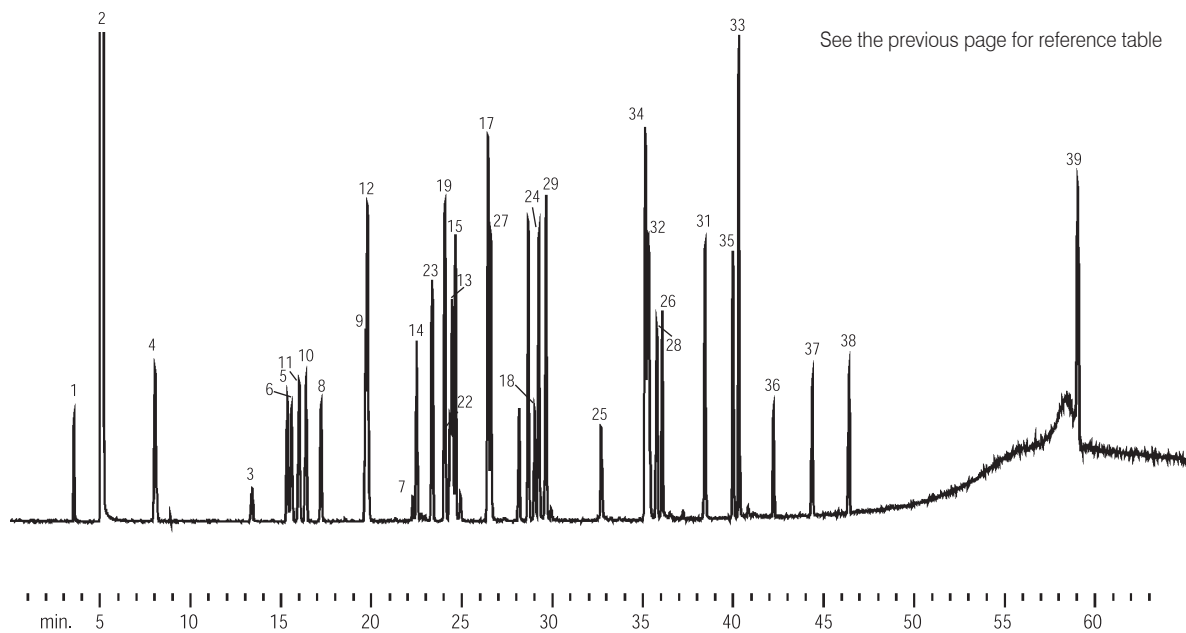


Solvents Mixture #1

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
Cat. No.: 7552
Index: CCR00337
Oven Temp.: 40 $^{\circ}$ C (hold 5 min) to 250 $^{\circ}$ C at 5 $^{\circ}$ C/min
Carrier Gas: He, 40 cm/sec
Injection: Split, 50 mL/min, 275 $^{\circ}$ C
Sample: Solvents mixture #1, 1.0 μ L
Detector: MS full scan, 285 $^{\circ}$ C

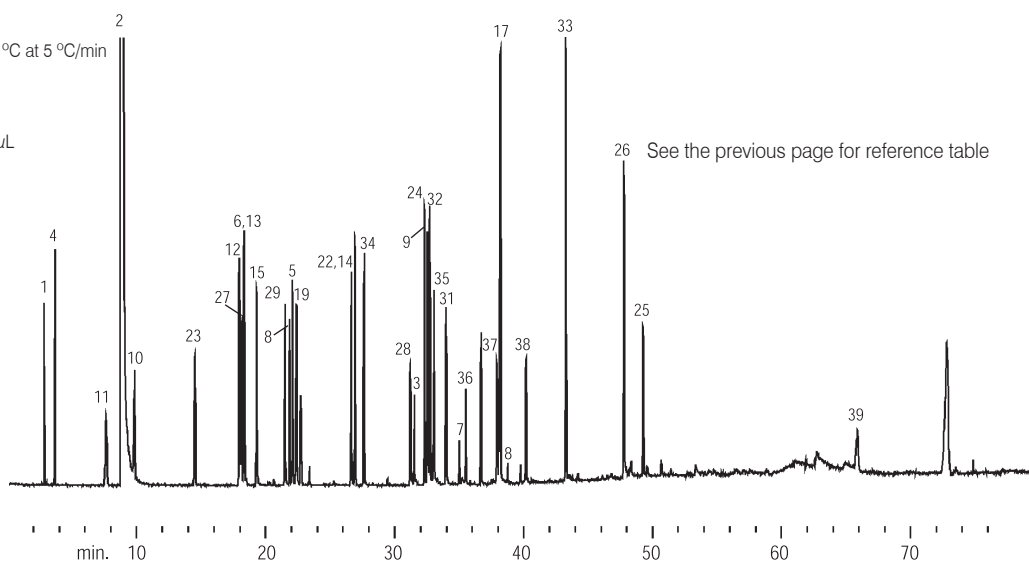

Solvents Mixture #2

Column: DM-1, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7156
 Index: CCR00338
 Oven Temp.: 40 °C (hold 5 min) to 250 °C at 5 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Split, 50 mL/min, 275 °C
 Sample: Solvents mixture #2, 1.0 μ L
 Detector: MS full scan, 285 °C

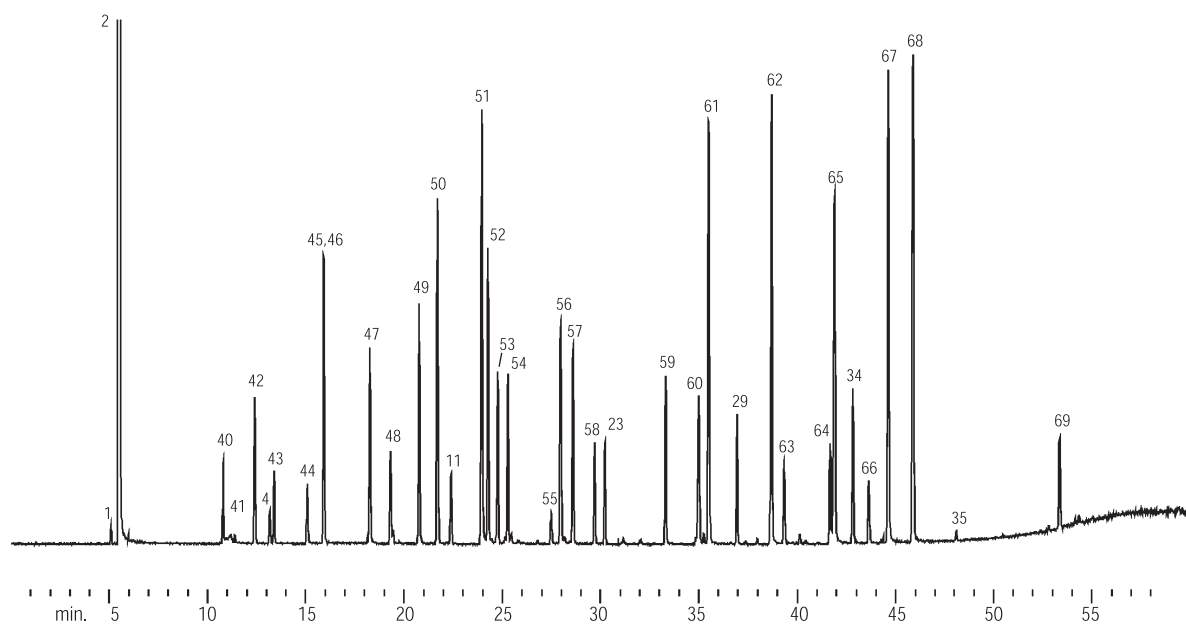


1. Pentane	22. Hexachloroethane	43. 1-Nitropropane	64. 1-Dodecanol	85. 2-Methyl-2,4-pentanediol
2. Methylene chloride	23. Undecane	44. Dimethyl formamide	65. Tetraethylene glycol	86. Butoxyethanol
3. Ethylene glycol	24. 1-Nonanol	45. 2-Methyl-3-pentanol	66. Dibenzyl	87. 1,2,3-Trichloropropane
4. Heptane	25. <i>p</i> -Methoxyphenol	46. Toluene	67. Diethyl phthalate	88. 1,4-Butanediol
5. Cyclopentanol	26. Triethylene glycol	47. Ethyl chloroacetate	68. Tributyl phosphate	89. Methyl hexanoate
6. 3-Hexanol	27. Dodecane	48. Dimethylacetamide	69. Diphenyl sulfone	90. 1,2,4-Trimethylbenzene
7. Acetamide	28. Undecanal	49. <i>p</i> -Xylene	70. Allyl alcohol	91. 2-Ethyl-1-hexanol
8. 2-Methyl-1-pentanol	29. Tridecane	50. <i>sec</i> -Tetrachloroethane	71. -	92. Dipentene
9. Furfuryl alcohol	30. -	51. Benzaldehyde	72. Isopropyl acetate	93. Tetrahydrofurfuryl acetate
10. Butyl ether	31. Dodecanal	52. <i>o</i> -Chlorotoluene	73. Benzene	94. -
11. Nonane	32. Dicyclohexylamine	53. 2,6-Dimethyl-4-heptanone	74. 2-Nitropropane	95. Decahydronaphthalene
12. Cumene	33. <i>bis</i> (2,2-Methoxy)ethyl ether	54. 2-Octanone	75. Nitroethane	96. -
13. Ethyl amyl ketone	34. Pentadecane	55. <i>o</i> -Cresol	76. Pentanal	97. -
14. Heptanol	35. Heptadecane	56. α -Methylbenzyl alcohol	77. 2-Bromobutane	98. 2-Decanol
15. Butyl butanoate	36. Octadecane	57. 5-Nonanone	78. 1-Chloropentane	99. 1,2- <i>bis</i> (2-Methoxyethoxy)ethane
16. -	37. Nonadecane	58. Nonanal	79. Cyclopentanone	100. 2-Phenoxyethanol
17. Benzyl alcohol	38. Eicosane	59. Decanal	80. 2-Hexanol	101. -
18. Dipropylene glycol	39. Acetyl tributyl citrate	60. -	81. Butyl acetate	102. Benzyl ether
19. Diethylbenzene	40. 2-Buten-1-ol	61. 1-Decanol	82. 2-Ethyl-1-butanol	
20. -	41. Formamide	62. 1-Undecanol	83. 3-Ethyl-3-pentanol	
21. -	42. 3-Pentanol	63. 2-Dodecanone	84. 1,4-Dichlorobutane	

Solvents

Solvents Mixture #2

Column: DM-200, 60 m x 0.53 mm x 3.00 μ m
Cat. No.: 8356
Index: CCR00339
Oven Temp.: 40 °C (hold 5 min) to 285 °C at 5 °C/min
Carrier Gas: He, 40 cm/sec
Injection: Split, 50 mL/min, 275 °C
Sample: Solvents mixture #2, 1.0 μ L
Detector: MS full scan, 285 °C


See the previous page for reference table

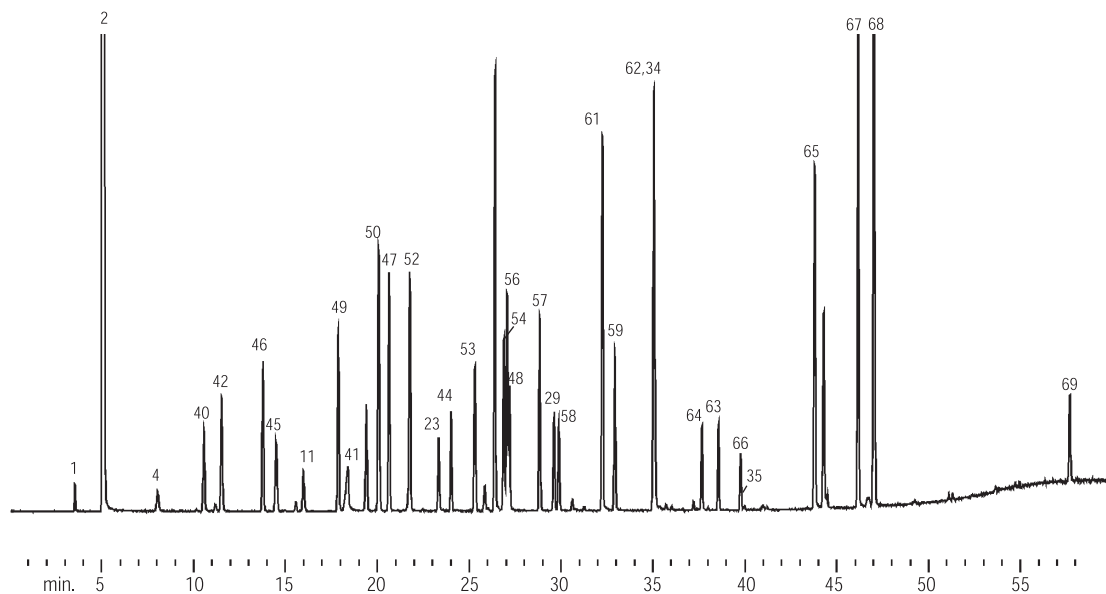

Solvents Mixture #2


Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
Cat. No.: 7552
Index: CCR00340
Oven Temp.: 40 °C (hold 5 min) to 250 °C at 5 °C/min
Carrier Gas: He, 40 cm/sec
Injection: Split, 50 mL/min, 275 °C
Sample: Solvents mixture #2, 1.0 μ L
Detector: MS full scan, 285 °C

See the previous page for reference table

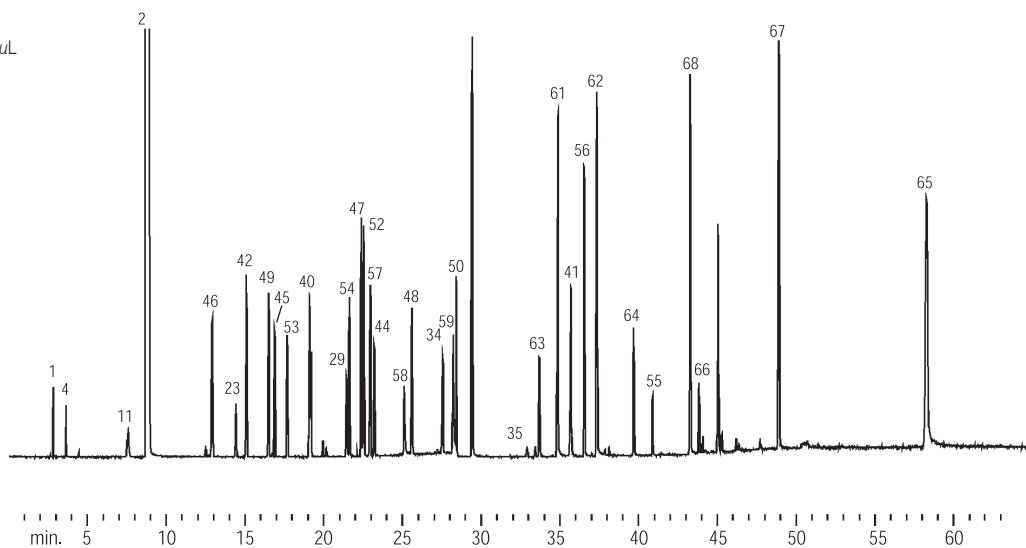

Solvents Mixture #3

Column: DM-1, 60 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7156
 Index: CCR00341
 Oven Temp.: 40 °C (hold 5 min) to 285 °C at 5 °C/min
 Carrier Gas: He, 40 cm/sec
 Injection: Split, 50 mL/min, 275 °C
 Sample: Solvents mixture #3, 1.0 μ L
 Detector: MS full scan, 285 °C

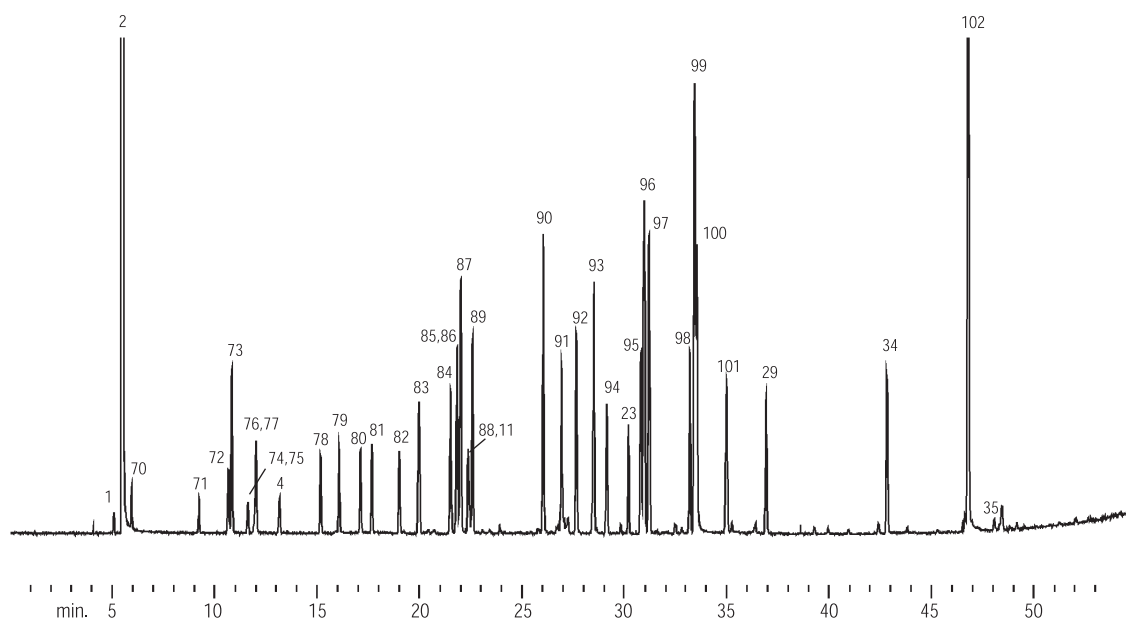


1. Pentane	22. Hexachloroethane	43. 1-Nitropropane	64. 1-Dodecanol	85. 2-Methyl-2,4-pentanediol
2. Methylene chloride	23. Undecane	44. Dimethyl formamide	65. Tetraethylene glycol	86. Butoxyethanol
3. Ethylene glycol	24. 1-Nonanol	45. 2-Methyl-3-pentanol	66. Dibenzyl	87. 1,2,3-Trichloropropane
4. Heptane	25. <i>p</i> -Methoxyphenol	46. Toluene	67. Diethyl phthalate	88. 1,4-Butanediol
5. Cyclopentanol	26. Triethylene glycol	47. Ethyl chloroacetate	68. Tributyl phosphate	89. Methyl hexanoate
6. 3-Hexanol	27. Dodecane	48. Dimethylacetamide	69. Diphenyl sulfone	90. 1,2,4-Trimethylbenzene
7. Acetamide	28. Undecanal	49. <i>p</i> -Xylene	70. Allyl alcohol	91. 2-Ethyl-1-hexanol
8. 2-Methyl-1-pentanol	29. Tridecane	50. <i>sec</i> -Tetrachloroethane	71. -	92. Dipentene
9. Furfuryl alcohol	30. -	51. Benzaldehyde	72. Isopropyl acetate	93. Tetrahydrofurfuryl acetate
10. Butyl ether	31. Dodecanal	52. <i>o</i> -Chlorotoluene	73. Benzene	94. -
11. Nonane	32. Dicyclohexylamine	53. 2,6-Dimethyl-4-heptanone	74. 2-Nitropropane	95. Decahydronaphthalene
12. Cume ne	33. <i>bis</i> (2,2-Methoxy)ethyl ether	54. 2-Octanone	75. Nitroethane	96. -
13. Ethyl amyl ketone	34. Pentadecane	55. <i>o</i> -Cresol	76. Pentanal	97. -
14. Heptanol	35. Heptadecane	56. α -Methylbenzyl alcohol	77. 2-Bromobutane	98. 2-Decanol
15. Butyl butanoate	36. Octadecane	57. 5-Nonanone	78. 1-Chloropentane	99. 1,2- <i>bis</i> (2-Methoxyethoxy)ethane
16. -	37. Nonadecane	58. Nonanal	79. Cyclopentanone	100. 2-Phenoxyethanol
17. Benzyl alcohol	38. Eicosane	59. Decanal	80. 2-Hexanol	101. -
18. Dipropylene glycol	39. Acetyl tributyl citrate	60. -	81. Butyl acetate	102. Benzyl ether
19. Diethylbenzene	40. 2-Buten-1-ol	61. 1-Decanol	82. 2-Ethyl-1-butanol	
20. -	41. Formamide	62. 1-Undecanol	83. 3-Ethyl-3-pentanol	
21. -	42. 3-Pentanol	63. 2-Dodecanone	84. 1,4-Dichlorobutane	

Solvents

Solvents Mixture #3

Column: DM-200, 60 m x 0.53 mm x 3.00 μ m
Cat. No.: 8356
Index: CCR00342
Oven Temp.: 40 $^{\circ}$ C (hold 5 min) to 285 $^{\circ}$ C at 5 $^{\circ}$ C/min
Carrier Gas: He, 40 cm/sec
Injection: Split, 50 mL/min, 275 $^{\circ}$ C
Sample: Solvents mixture #3, 1.0 μ L
Detector: MS full scan, 285 $^{\circ}$ C


See the previous page for reference table

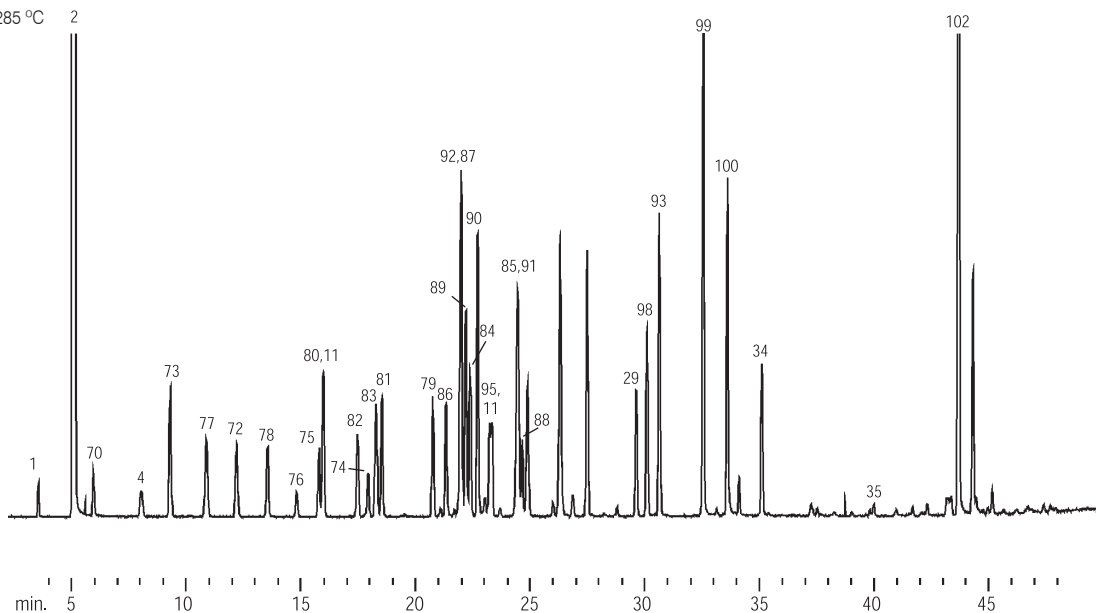

Solvents Mixture #3


Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m
Cat. No.: 7552
Index: CCR00343
Oven Temp.: 40 $^{\circ}$ C (hold 5 min) to 250 $^{\circ}$ C at 5 $^{\circ}$ C/min
Carrier Gas: He, 40 cm/sec
Injection: Split, 50 mL/min, 275 $^{\circ}$ C
Sample: Solvents mixture #3, 1.0 μ L
Detector: MS full scan, 285 $^{\circ}$ C

See the previous page for reference table

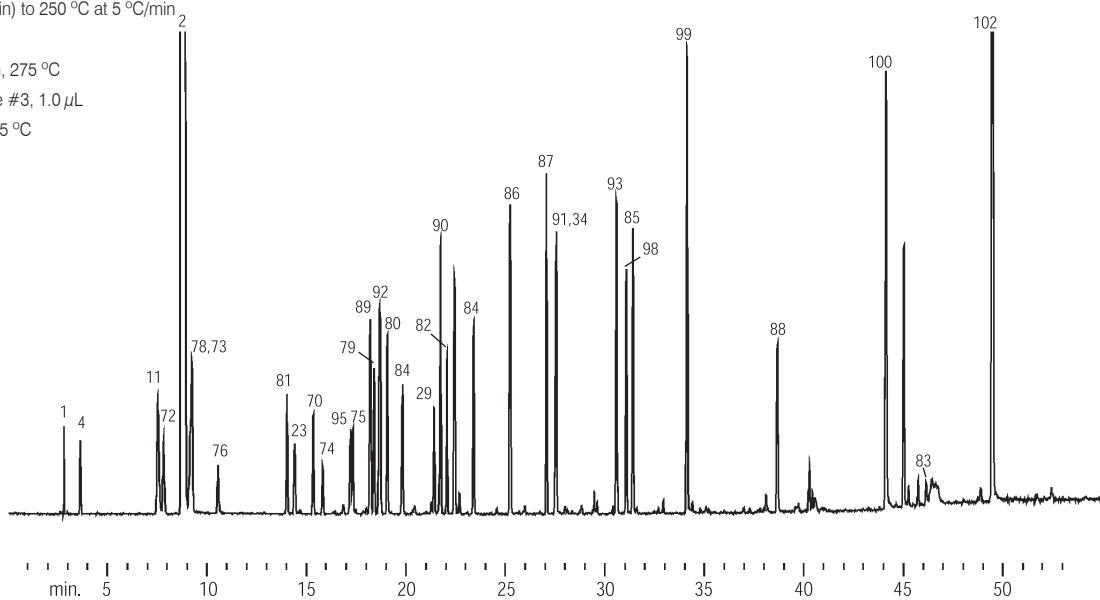


Polar Solvents

Column: DM-PLOT U, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: 8824
 Index: CSR00182
 Oven Temp.: 150 °C constant
 Carrier Gas: H₂
 Injection: Split, 20:1, 200 °C
 Sample: 50 ppm (w / v) each in He, 20 μ L
 Detector: FID, 200 °C

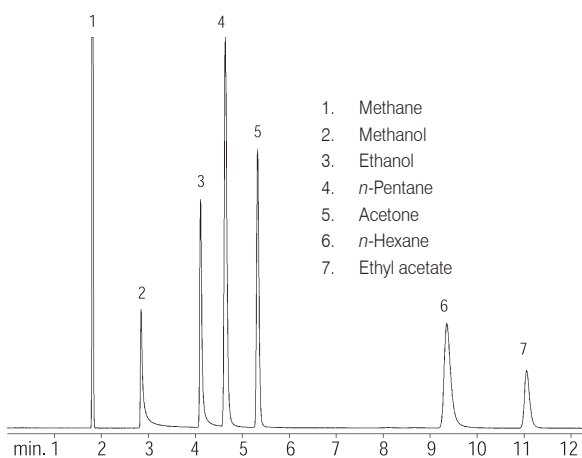


Polar Solvents

Column: DM-PLOT Q, 30 m x 0.32 mm x 10.00 μ m
 Cat. No.: 8818
 Index: CSR00181
 Oven Temp.: 150 °C constant
 Carrier Gas: H₂
 Injection: Split, 20:1, 200 °C
 Sample: 50 ppm (w / v) each in He, 20 μ L
 Detector: FID, 200 °C

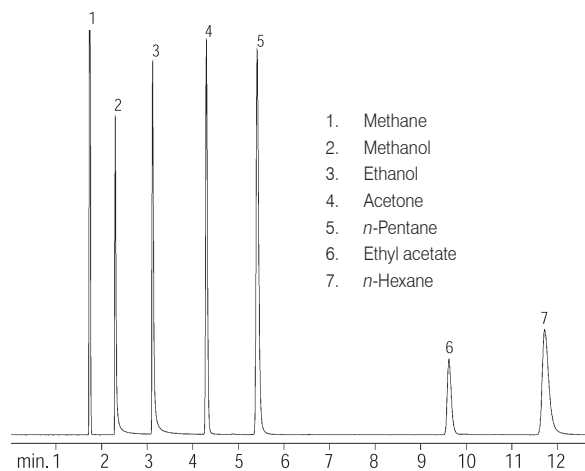


Solvents

Column: DM-5, 60 m x 0.32 mm x 3.00 μ m
 Cat. No.: 7242
 Index: CCR00346
 Oven Temp.: 50 °C (hold 4 min) to 120 °C (hold 20 min) at 5 °C/min
 Carrier Gas: H₂, 40 cm/sec, 50 °C
 Injection: Split, 300 °C
 Sample: in CS₂ solvent, 1.0 μ L
 Detector: FID, 128 x 10¹² AFS, 300 °C

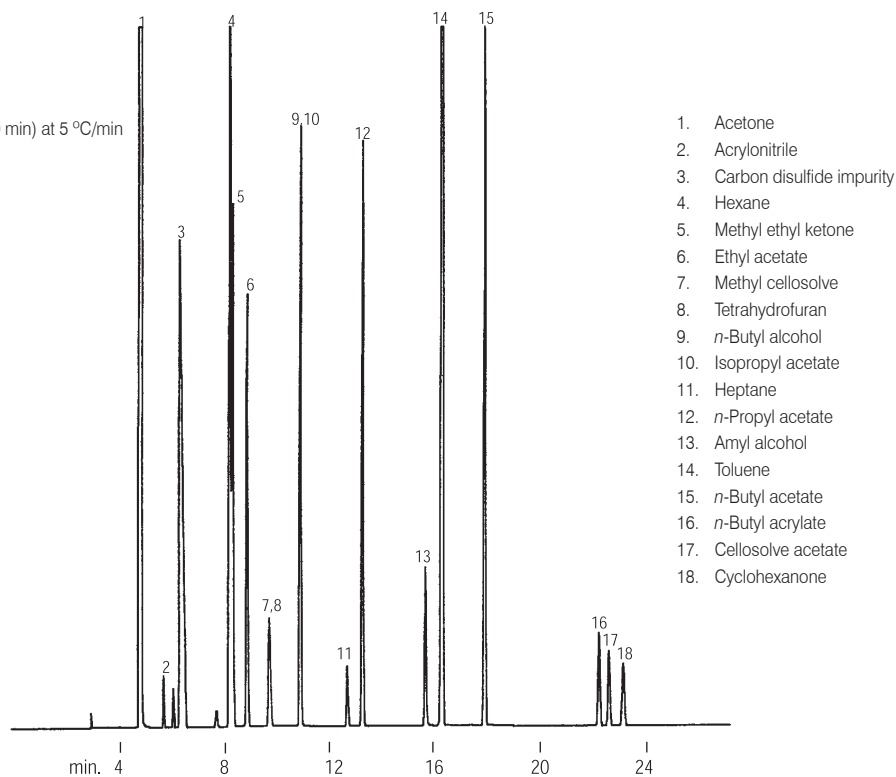


Fatty Acids (Free)

Column: DM-1, 30 m x 0.53 mm x 5.00 μ m
 Cat. No.: 7157
 Index: CCR00281
 Oven Temp.: 60 °C to 180 °C at 15 °C/min
 Carrier Gas: H₂, 50 cm/sec
 Injection: Direct, 250 °C
 Sample: Fatty acids (free), 0.2 μ L, 10 - 20 ng/ μ L
 Detector: FID, 4 x 10⁻¹¹ AFS, 250 °C

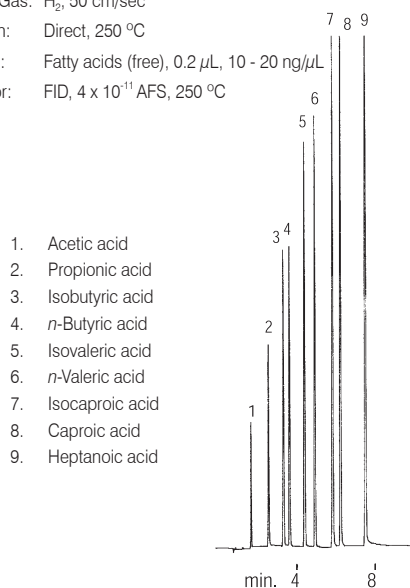


Fatty Acids (Free)

Column: DM-FFAP, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7621
 Index: CCR00280
 Oven Temp.: 145 °C, constant
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 50:1, 250 °C
 Sample: Fatty acids (free), 1.0 μ L, 10 - 20 ng/ μ L
 Detector: FID, 2 x 10⁻¹¹ AFS, 250 °C

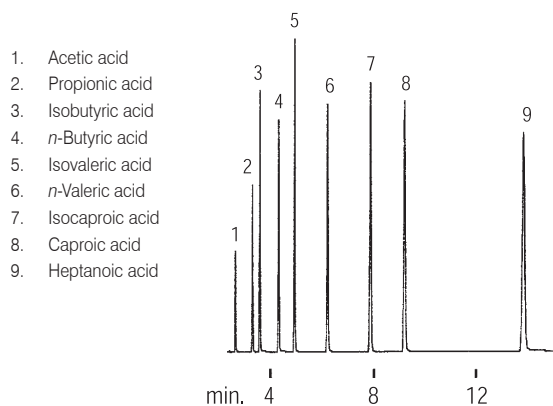

Fatty Acids (Free)


Column: DM-FFAP, 30 m x 0.32 mm x 0.25 μ m
 Cat. No.: 7631
 Index: CFR00653
 Oven Temp.: 40 °C to 250 °C (hold 15 min) at 10 °C/min
 Carrier Gas: H₂
 Injection: Splitless, 0.25 min, 250 °C
 Sample: Free fatty acid mix, 1.0 μ L
 Flow Rate: 6.0 mL/min
 Make up gas: 75 mL/min
 Solvent: H₂O
 Concentration: 5 mg/mL in MeOH
 Detector: FID, 250 °C

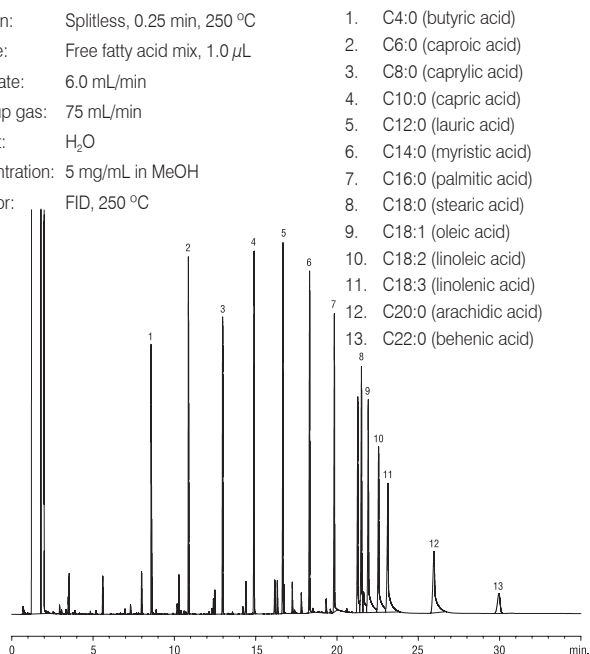

FAMES (*cis* / *trans* Isomers)


Column: DM-2560, 100 m x 0.25 mm x 0.20 μ m
 Cat. No.: 8858
 Index: CFR00652
 Sample: 10 mg/mL *cis* / *trans* FAMES mix in methylene chloride
 Injection: Split, 20:1, 1 μ L, 225 °C
 Oven Temp.: 100 °C (hold 4 min) to 240 °C (hold 10 min) at 3 °C/min
 Carrier Gas: H₂, 1.2 mL/min
 Detector: FID, 250 °C

1. C18:0 (methyl stearate)
 2. C18:1 (methyl petroselinate (*trans*-6))
 3. C18:1 (methyl elaidate (*trans*-9))
 4. C18:1 (methyl transvaccenate (*trans*-11))
 5. C18:1 (methyl petroselinate (*cis*-6))
 6. C18:1 (methyl oleate (*cis*-9))
 7. C18:1 (methyl vaccenate (*cis*-11))
 8. C18:2 (methyl linoleate (*cis*-9,12))

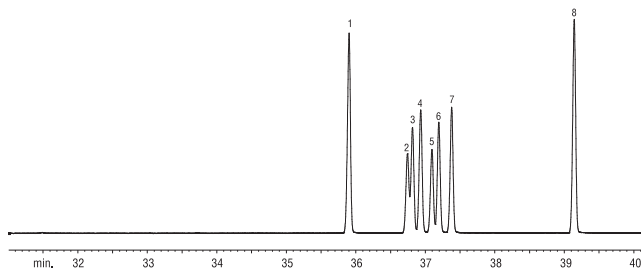


PUFA (Animal Source)

Column: DM-2330, 30 m x 0.32 mm x 0.20 μ m
 Cat. No.: 8633
 Index: CFR00119
 Oven Temp.: 160 °C to 250 °C (hold 10 min) at 2 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 260 °C
 Sample: PUFA (animal source) mix, 0.1 μ L
 Detector: FID, 8 x 10⁻¹¹ AFS, 260 °C

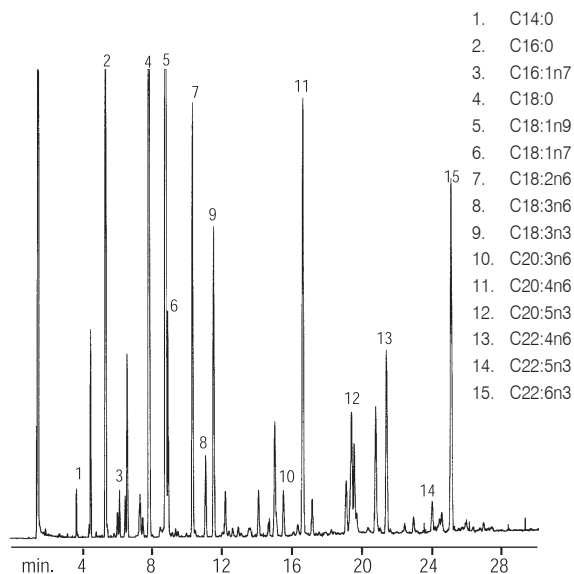


FAMES

Column: DM-InertWax, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 8521
 Index: CFR00538
 Oven Temp.: 120 °C (hold 3 min) to 220 °C (hold 12 min) at 20 °C/min
 Carrier Gas: He, 34 cm/sec, 1 mL/min
 Injection: Split, 100:1, 250 °C
 Sample: Saw palmetto, 1.0 μ L
 Detector: FID, 300 °C

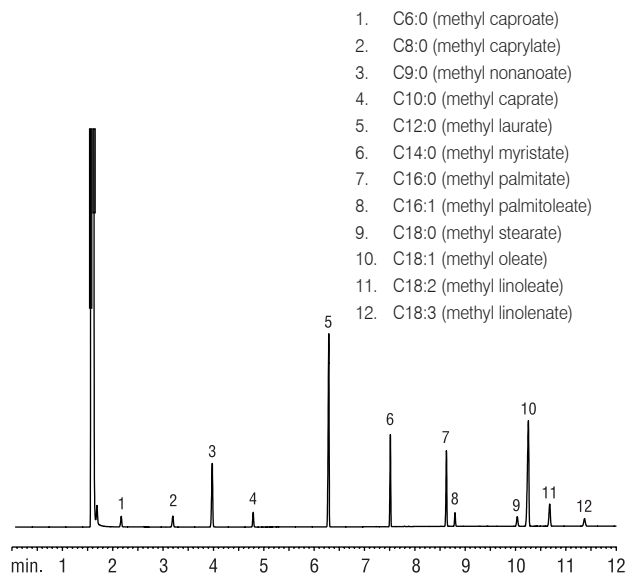


PUFA (Animal Source)

Column: DM-Wax, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7521
 Index: CFR00117
 Oven Temp.: 160 °C to 250 °C (hold 10 min) at 2 °C/min
 Carrier Gas: H₂, 40 cm/sec
 Injection: Split, 20:1, 260 °C
 Sample: PUFA mix, 0.1 μ L
 Detector: FID, 8 x 10⁻¹¹ AFS, 260 °C

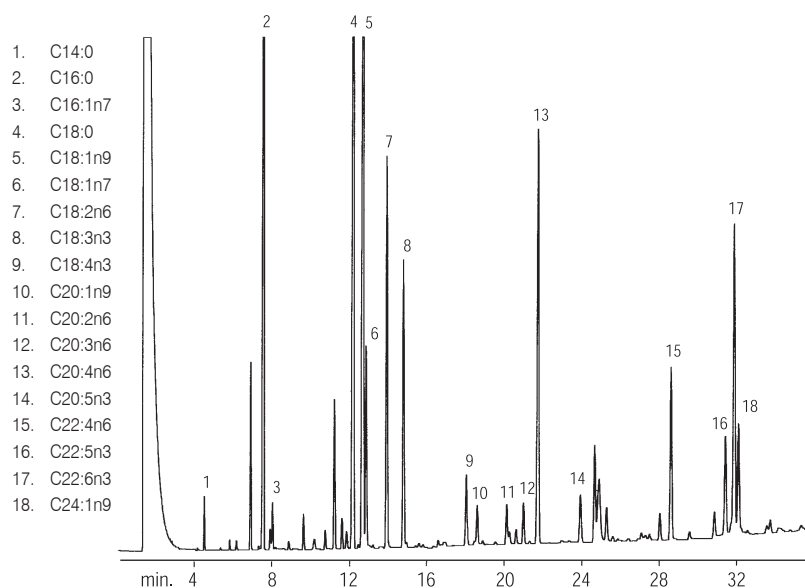

FAMES (Flax Seed Oil)


Column: DM-FAMEWAX, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: **7811**
 Index: CFR00364
 Oven Temp.: 165 $^{\circ}$ C (hold 30 min) to 220 $^{\circ}$ C (hold 15 min) at 1.5 $^{\circ}$ C/min
 Carrier Gas: He, 40 cm/sec
 Injection Temp.: 225 $^{\circ}$ C
 Detector: FID, 230 $^{\circ}$ C

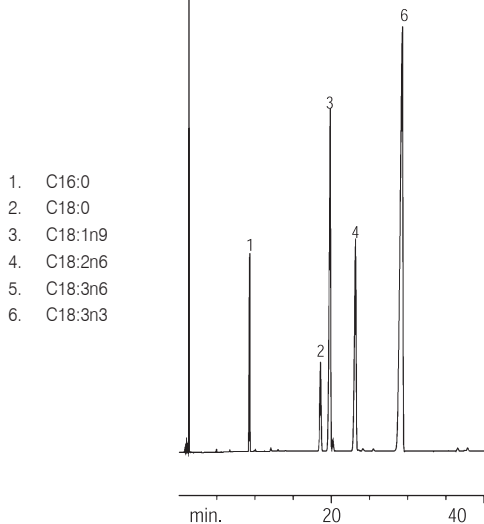

- 1. C16:0
- 2. C18:0
- 3. C18:1n9
- 4. C18:2n6
- 5. C18:3n6
- 6. C18:3n3

FAMES (Black Currant Seed Oil)

Column: DM-FAMEWAX, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: **7811**
 Index: CFR00365
 Oven Temp.: 165 $^{\circ}$ C (hold 30 min) to 220 $^{\circ}$ C (hold 15 min) at 1.5 $^{\circ}$ C/min
 Carrier Gas: He, 40 cm/sec
 Injection Temp.: 225 $^{\circ}$ C
 Detector: FID, 230 $^{\circ}$ C

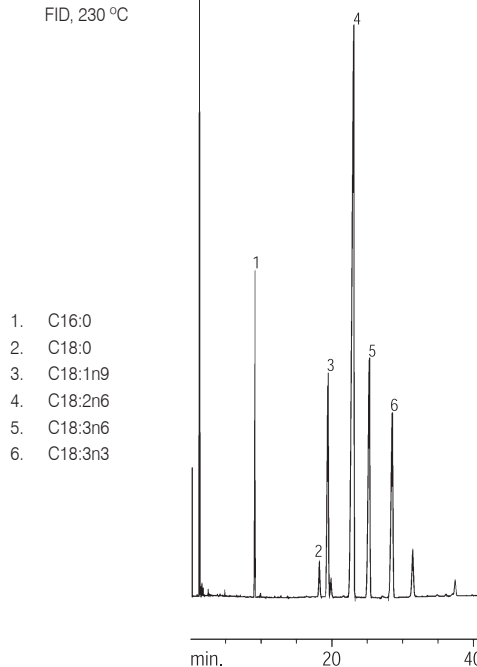


- 1. C16:0
- 2. C18:0
- 3. C18:1n9
- 4. C18:2n6
- 5. C18:3n6
- 6. C18:3n3

Applications

FAMES (Marine Oil Standard)

Column: DM-FAMEWAX, 30 m x 0.32 mm x 0.25 μ m
 Cat. No.: **7813**
 Index: CFR00568
 Oven Temp.: 195 $^{\circ}$ C to 240 $^{\circ}$ C (hold 1 min) at 5 $^{\circ}$ C/min
 Carrier Gas: H₂, 62 cm/sec
 Injection: Split, 150:1, 3 mm ID split liner, 250 $^{\circ}$ C
 Sample: 12 mg/mL total FAMES, 0.5 μ L
 Detector: FID, 250 $^{\circ}$ C

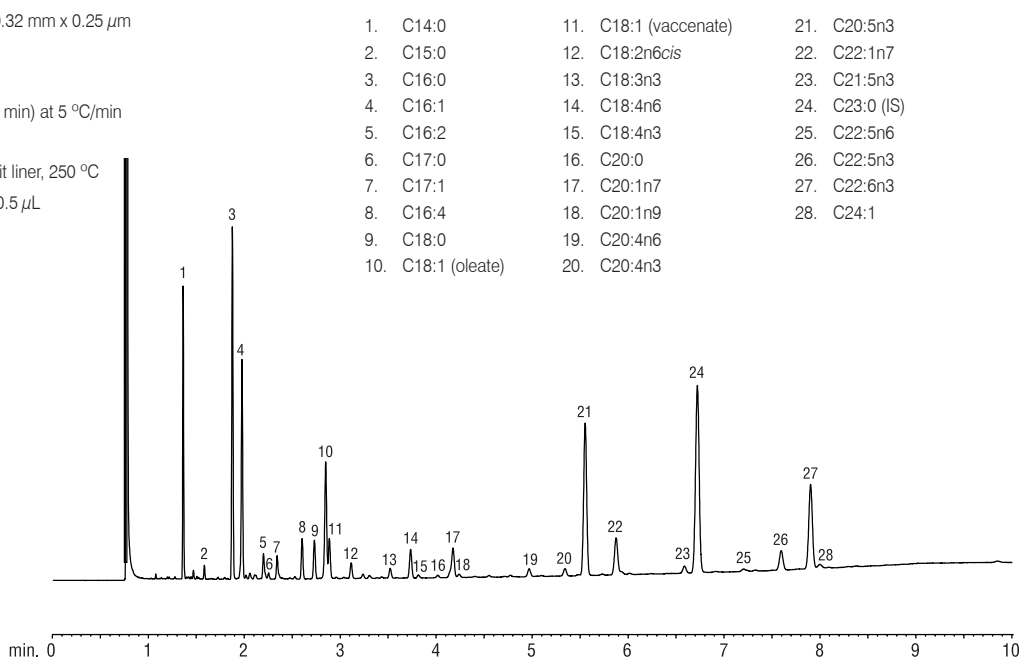

- | | | |
|--------------------|-----------------------|----------------|
| 1. C14:0 | 11. C18:1 (vaccenate) | 21. C20:5n3 |
| 2. C15:0 | 12. C18:2n6cis | 22. C22:1n7 |
| 3. C16:0 | 13. C18:3n3 | 23. C21:5n3 |
| 4. C16:1 | 14. C18:4n6 | 24. C23:0 (IS) |
| 5. C16:2 | 15. C18:4n3 | 25. C22:5n6 |
| 6. C17:0 | 16. C20:0 | 26. C22:5n3 |
| 7. C17:1 | 17. C20:1n7 | 27. C22:6n3 |
| 8. C16:4 | 18. C20:1n9 | 28. C24:1 |
| 9. C18:0 | 19. C20:4n6 | |
| 10. C18:1 (oleate) | 20. C20:4n3 | |

Flavor Volatiles

Column: DM-1, 60 m x 0.32 mm x 0.50 μ m

Cat. No.: 7148

Index: CFR00536


Oven Temp.: 70 °C (hold 15 min) to 190 °C (hold 5 min) at 2 °C/min

Carrier Gas: He, 20 cm/sec, 70 °C

Injection: Split, 20:1, 220 °C

Sample: Flavor volatiles mix, 0.8 μ LDetector: FID, 64 x 10⁻¹¹ AFS, 260 °C

- | | | | |
|-----------------------|-----------------------------|-----------------------------------|-------------------------------------|
| 1. Methanol | 11. Ethyl butyrate | 21. α -Phellandrene | 31. <i>trans</i> -Limonene monoxide |
| 2. Acetaldehyde | 12. Furfural | 22. α -Terpinene | 32. Citronellal |
| 3. Ethanol | 13. <i>trans</i> -2-Hexenal | 23. <i>p</i> -Cymene | 33. Terpinene-4-ol |
| 4. Acetone | 14. α -Thujene | 24. δ -Limonene | 34. α -Terpineol |
| 5. Isopropyl alcohol | 15. α -Pinene | 25. γ -Terpinene | 35. Decanal |
| 6. Methylene chloride | 16. Camphene | 26. Octanol | 36. <i>d/l</i> Carveol |
| 7. Hexane | 17. Sabinene | 27. Terpinolene | 37. Neral |
| 8. Ethyl acetate | 18. β -Pinene | 28. Nonanal | 38. Carvone |
| 9. Ethyl propionate | 19. Octanal | 29. Linalool | 39. Geranial |
| 10. <i>n</i> -Hexanal | 20. Myrcene | 30. <i>cis</i> -Limonene monoxide | 40. Neryl acetate |

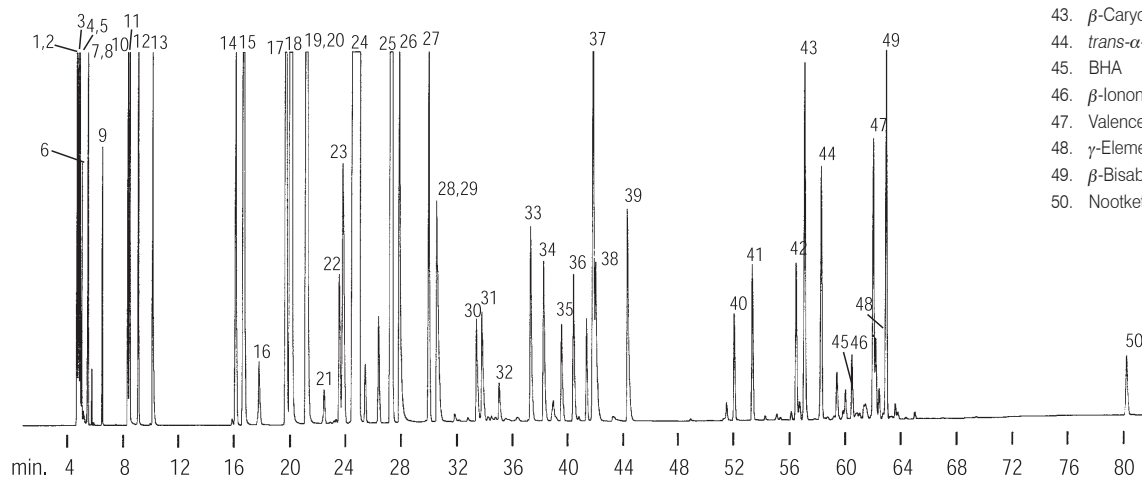

Flavor Volatiles

Column: DM-Wax, 60 m x 0.53 mm x 1.00 μ m

Cat. No.: 7552

Index: CFR00537


Oven Temp.: 70 °C (hold 15 min) to 190 °C (hold 5 min) at 2 °C/min

Carrier Gas: He, 20 cm/sec, 70 °C

Injection: Split, 20:1, 220 °C

Sample: Flavor volatiles mix, 0.8 μ LDetector: FID, 64 X 10⁻¹¹ AFS, 260 °C


- | | | | |
|-----------------------|-----------------------------|--|-------------------------|
| 1. Hexane | 12. <i>n</i> -Hexanal | 23. Nonanal | 34. Neral |
| 2. Acetaldehyde | 13. β -Pinene | 24. <i>cis</i> -Limonene monoxide | 35. α -Terpineol |
| 3. Acetone | 14. Sabinene | 25. <i>trans</i> -Limonene | 36. Neryl acetate |
| 4. Methanol | 15. Myrcene | 26. Furfural | 37. Valencene |
| 5. Ethyl acetate | 16. δ -Limonene | 27. Citronellal | 38. Geranial |
| 6. Isopropyl alcohol | 17. 1,8-Cineole | 28. Decanal | 39. Carvone |
| 7. Ethanol | 18. <i>trans</i> -2-Hexenal | 29. Linalool | 40. Geranyl acetate |
| 8. Methylene chloride | 19. γ -Terpinene | 30. Octanol | 41. <i>d/l</i> Carveol |
| 9. Ethyl propionate | 20. <i>p</i> -Cymene | 31. <i>trans</i> - α -Bergamotene | 42. α -Ionone |
| 10. α -Pinene | 21. Terpinolene | 32. β -Caryophyllene | 43. <i>d/l</i> Carveol |
| 11. Ethyl butyrate | 22. Octanal | 33. Terpinene-4-ol | 44. β -Ionone |

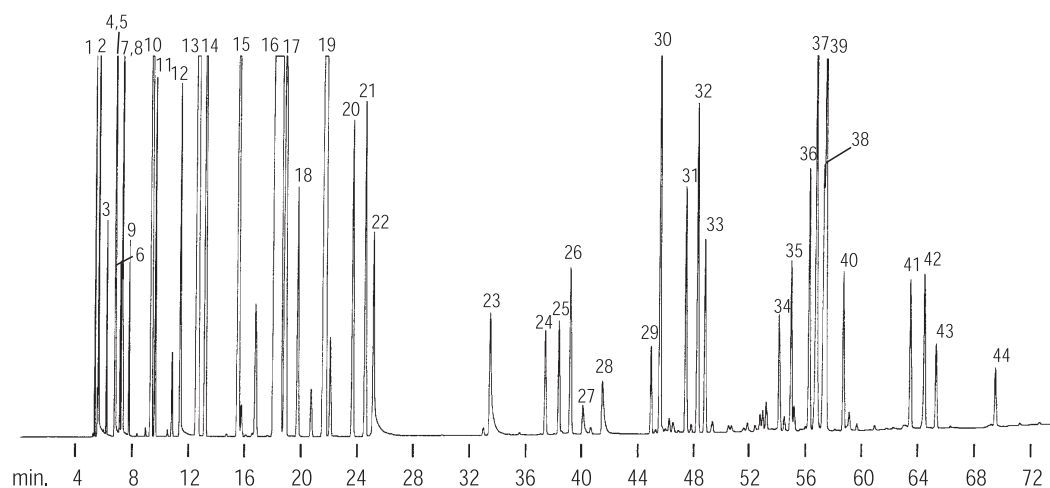

Concentrated Liquors


Column: DM-Wax, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7521
 Index: CFO00011
 Oven Temp.: 37 °C (hold 2 min) to 70 °C at 3 °C/min
 70 °C (hold 1 min) to 130 °C at 6 °C/min
 130 °C to 220 °C at 10 °C/min
 to 220 °C (hold 10 min)
 Carrier Gas: High purity nitrogen, 1 mL/min
 Injection: 260 °C, Split ratio 30:1
 Detector: FID, 260 °C

- | | | | |
|----------------------------|-------------------------------|------------------------|---------------------------------|
| 1. Acetaldehyde | 17. 2-Ethoxy butane | 33. <i>n</i> -Butanol | 49. Ethyl octanoate |
| 2. Propanal | 18. 2-Pentanone | 34. - | 50. - |
| 3. Isobutanol | 19. <i>sec</i> -Butyl alcohol | 35. - | 51. Acetic acid |
| 4. Acetone | 20. Ethyl butyrate | 36. Isoamyl alcohol | 52. Furfural |
| 5. Ethyl formate | 21. <i>n</i> -Propanol | 37. - | 53. - |
| 6. - | 22. - | 38. Ethyl caproate | 54. - |
| 7. - | 23. - | 39. - | 55. Benzaldehyde |
| 8. - | 24. - | 40. <i>n</i> -Pentanol | 56. Ethyl nonanoate |
| 9. Ethyl acetate + Acetal | 25. Ethyl isovalerate | 41. Acetoin | 57. Propionic acid |
| 10. Methanol | 26. Diethoxy isopentane | 42. - | 58. <i>L</i> -2,3-Butanediol |
| 11. 2-Butanone | 27. Diethoxy-3-methylbutane | 43. Propyl hexanoate | 59. Capryl alcohol |
| 12. 2-Methyl butyraldehyde | 28. - | 44. 2-Heptanol | 60. Isobutyric acid |
| 13. 3-Methyl butyraldehyde | 29. Isobutyl alcohol | 45. Ethyl heptanoate | 61. <i>meso</i> -2,3-Butanediol |
| 14. Ethanol | 30. Isoamyl acetate | 46. Ethyl lactate | 62. Hexyl hexanoate |
| 15. Ethyl propionate | 31. <i>sec</i> -Pentanol | 47. <i>n</i> -Hexanol | 63. Ethyl caprate |
| 16. Ethyl isobutyrate | 32. Ethyl valerate | 48. Butyl hexanoate | 64. <i>n</i> -Butanoic acid |

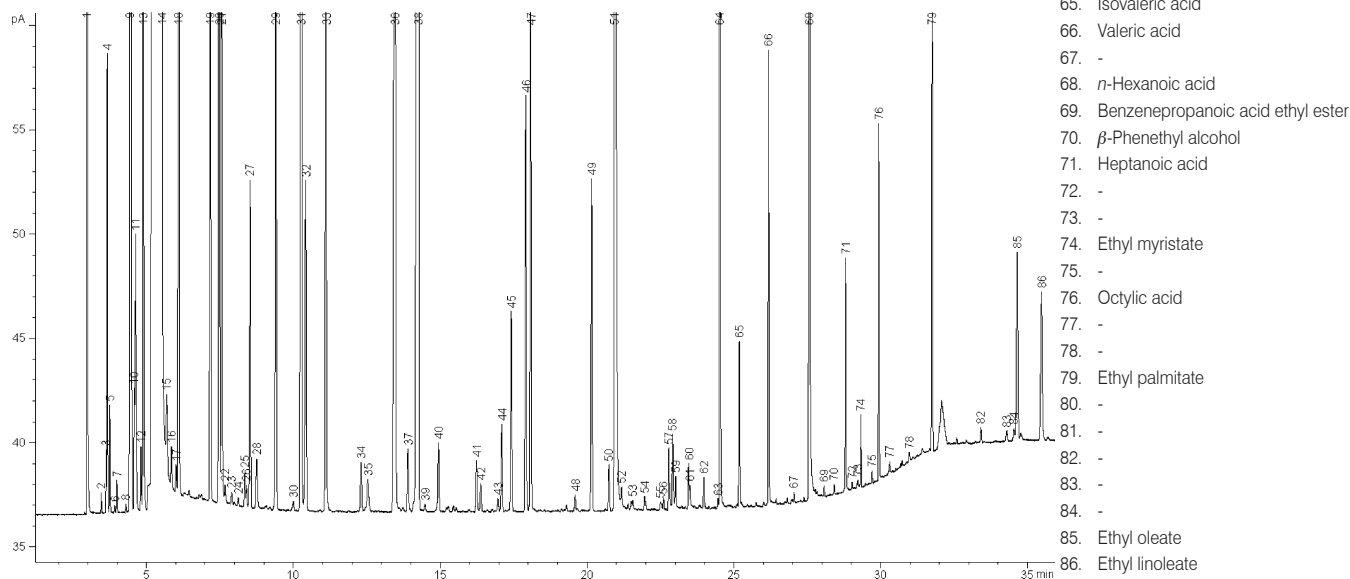

Alcoholic Standard: Acids and Esters

Column: DM-FFAP, 50 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7672
 Index: CFR00500
 Oven Temp.: 70 °C to 240 °C (hold 3 min) at 12 °C/min
 Carrier Gas: H₂, 28 psi, 240 °C
 Injection: Splitless, 1.0 μ L, constant 0.5 min, 240 °C
 Detector: FID

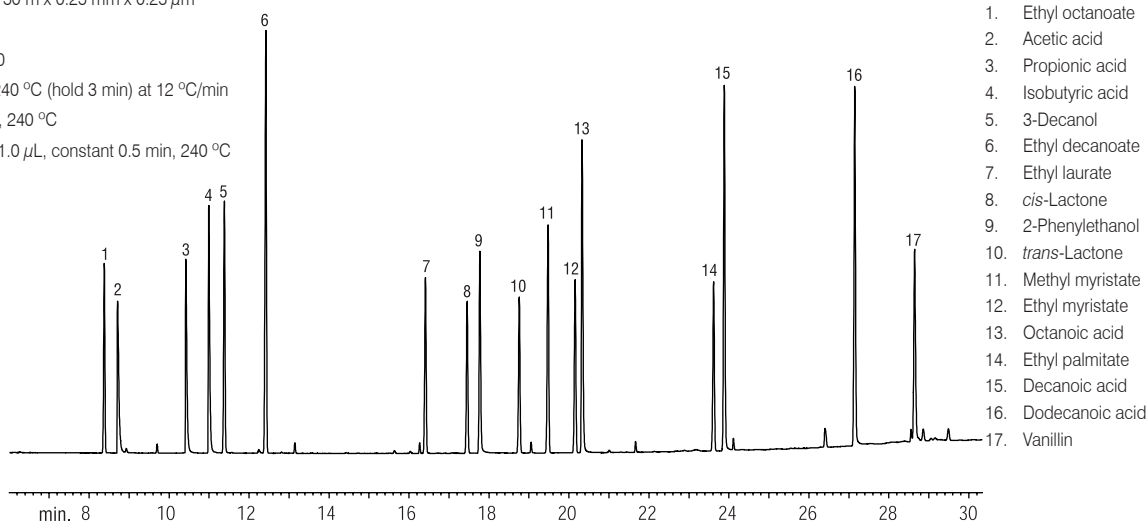

Peppermint Oil

Column: DM-Wax, 30 m x 0.25 mm x 0.50 μ m

Cat. No.: 7521

Index: CFR00141


Oven Temp.: 75 °C (hold 4 min) to 240 °C at 4 °C/min

Carrier Gas: H₂, 40 cm/sec, 75 °C

Injection: Split, 1.0 μ L, 50:1, 250 °C

Sample: Peppermint oil, 1.0 μ L

Detector: FID, 16 x 10⁻¹¹ AFS, 250 °C

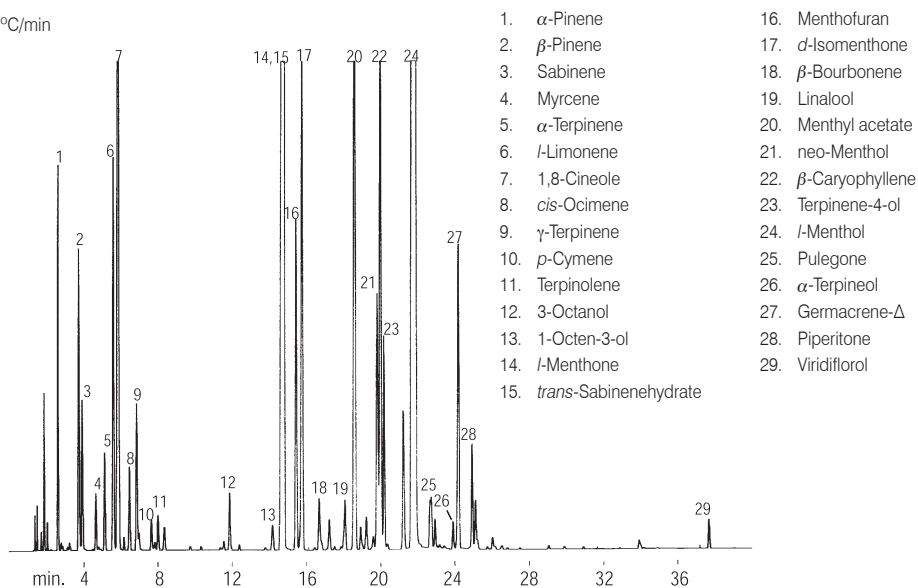

Citronella Java Oil

Column: DM-1, 60 m x 0.25 mm x 0.25 μ m

Cat. No.: 7122

Index: CFR00144


Oven Temp.: 100 °C to 260 °C (hold 1 min) at 4 °C/min

Carrier Gas: He, 30 cm/sec, 50 °C

Injection: Split, 100 cc/min, 250 °C

Sample: Citronella java oil, 1.0 μ L


Detector: MS, 280 °C

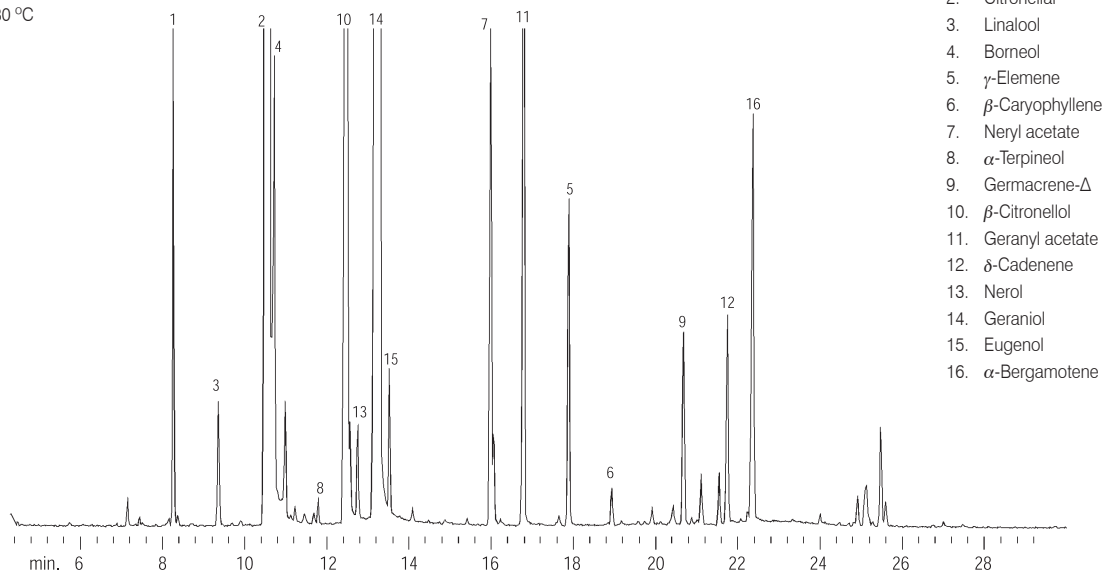

Fragrance

Column: DM-1, 60 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7122
 Index: CFR00657
 Oven Temp.: 50 °C to 270 °C at 3 °C/min
 Carrier Gas: He
 Injection: Split, 40:1, 285 °C
 Flow rate: 0.6 mL/min
 Sample: 5% FMA mix in acetone, 1.0 μ L
 Detector: FID, 300 °C


1. Ethyl butyrate
2. Limonene
3. Eucalyptol
4. Benzoic acid
5. Cinnamic aldehyde
6. Geraniol
7. Hydroxycitronellal
8. Thymol
9. Cinnamyl alcohol
10. Vanillin
11. Cinnamyl acetate
12. Benzyl salicylate

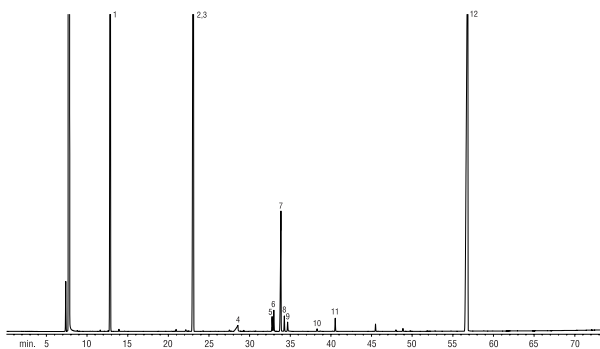

Fragrance


Column: DM-1701, 60 m x 0.25 mm x 0.25 μ m
 Cat. No.: 7322
 Index: CFR00658
 Oven Temp.: 50 °C to 270 °C at 3 °C/min
 Carrier Gas: He
 Injection: Split, 40:1, 285 °C
 Sample: 5% FMA mix in acetone, 1.0 μ L
 Detector: FID, 300 °C

1. Ethyl butyrate
2. Limonene
3. Eucalyptol
4. Geraniol
5. Benzoic acid
6. Cinnamic aldehyde
7. Hydroxycitronellal
8. Thymol
9. Cinnamyl alcohol
10. Cinnamyl acetate
11. Vanillin
12. Benzyl salicylate

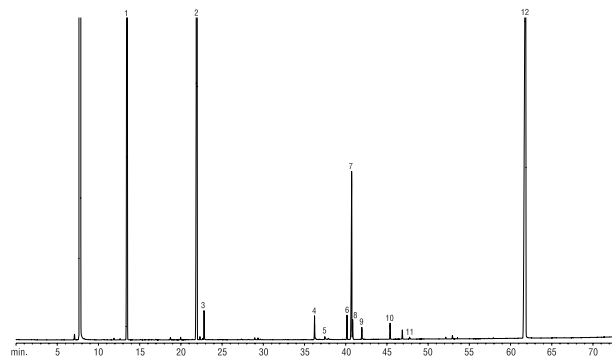

BHA / BHT

Column: DM-17, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7451
 Index: CFR00630
 Oven Temp.: 50 °C to 240 °C (hold 3 min) at 15 °C/min
 Carrier Gas: He, 60 cm/sec, 50 °C
 Injection: Direct, 280 °C
 Sample: 50 ppm BHA / BHT each in MeOH, 1.0 μ L
 Detector: FID, 280 °C

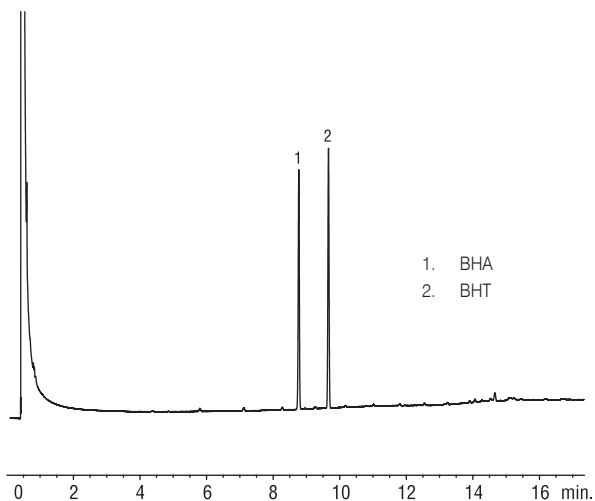


1. BHA
2. BHT

Food Packaging Volatiles

Column: DM-5MS, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: 8223
 Index: CFR00459
 Oven Temp.: 50 °C to 92 °C at 3 °C/min
 to 220 °C (hold 1 min) at 20 °C/min
 Carrier Gas: He, 36 cm/sec
 Injection: Purge and trap
 Desorb Temp.: 220 °C
 Detector: MSD, 280 °C
 Ionization: EI, 70 eV
 Scan Range: 35 - 260 AMU


1. Tetrahydrofuran
2. 1-Butanol
3. Toluene
4. Hexanal
5. Ethylbenzene
6. 4-Heptanone
7. Butyl ether
8. Styrene
9. 1-Methylethylbenzene
10. Propylbenzene
11. Benzaldehyde
12. Benzeneacetaldehyde
13. Acetophenone
14. Methyl benzoate
15. Decanal

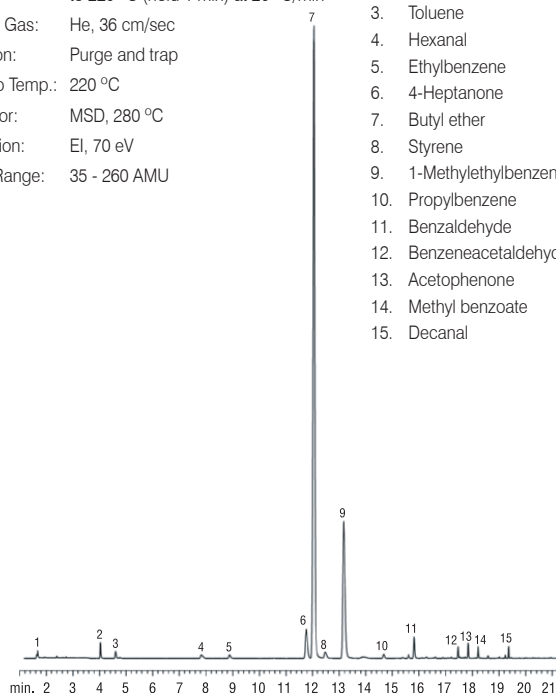

Neutral Sterols

Column: DM-225, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 8421
 Index: CFR00431
 Oven Temp.: 260 °C constant
 Carrier Gas: He, 45 cm/sec, 240 °C
 Injection: Split, 30:1, 260 °C
 Sample: Neutral sterols and phytosterols,
 1.5 μ L, 200 ng on-column
 Detector: FID, 8 x 10⁻¹¹ AFS, 260 °C


1. 5- α -Cholestane
2. Coprosterol
3. Cholesterol
4. Brassicasterol
5. Coprostanone
6. Campesterol
7. Stigmasterol
8. β -Sitosterol

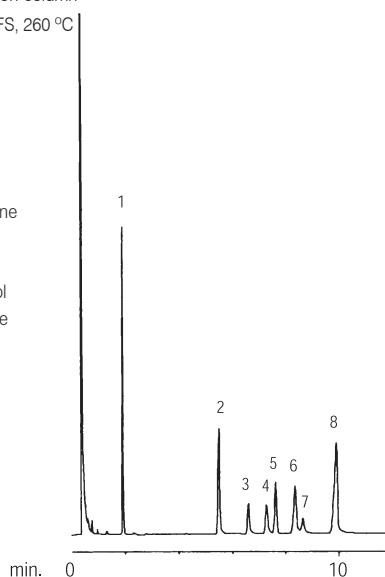

Sugars (Alditol Acetates)

Column: DM-225, 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: 8421
 Index: CFR00128
 Oven Temp.: 190 °C (hold 5 min) to 250 °C (hold 5 min) at 8 °C/min
 Carrier Gas: H₂, 42 cm/sec, 40 °C
 Injection: Split, 50:1, 260 °C
 Sample: Alditol acetates derivative, 0.5 μ L
 Detector: FID, 16 x 10⁻¹¹ AFS, 260 °C


1. Rhamnitol
2. Fucitol
3. Ribitol
4. Arabinitol
5. Mannitol
6. Galactitol
7. Glucitol
8. Inositol

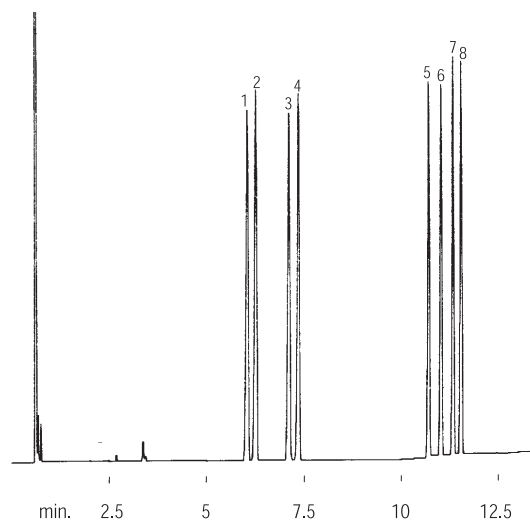

Sugars (Alditol Acetates)

Column: DM-2330, 30 m x 0.32 mm x 0.20 μ m
 Cat. No.: 8633
 Index: CFR00127
 Oven Temp.: 175 °C (hold 2 min) to 240 °C (hold 1 min) at 8 °C/min
 to 265 (hold 12 min) at 8 °C/min
 Carrier Gas: He, 80 cm/sec
 Injection: Split, 20:1, 275 °C
 Sample: Sugars, 0.6 μ L
 Detector: FID, 2 x 10⁻¹¹ AFS, 275 °C

1. Glyceraldehyde
2. Deoxyribitol
3. Rhamnitol
4. Fucitol
5. Ribitol
6. Arabinitol
7. Xylitol
8. Deoxyglucitol
9. Mannitol
10. Galactitol
11. Glucitol
12. Inositol
13. Glucoheptitol
14. *n*-Acetyl galactose amine
15. *n*-Acetyl glucose amine
16. 2-Keto-3-deoxyoctanate

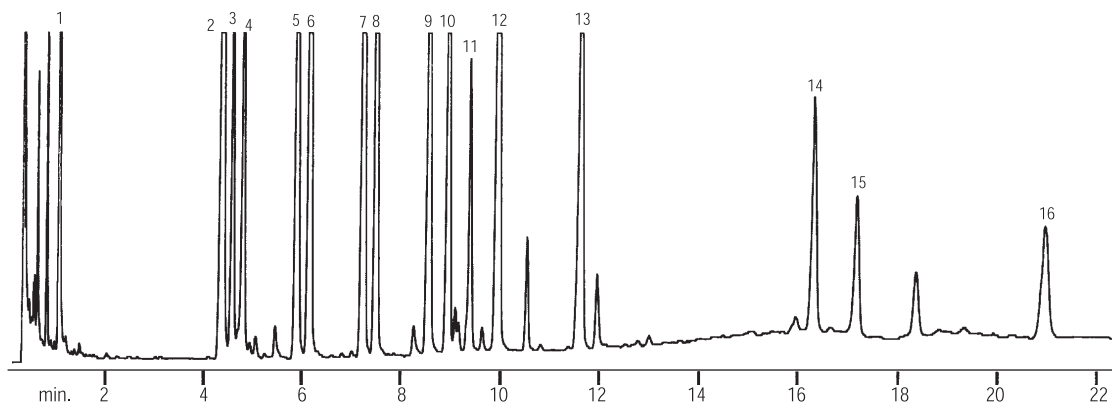


Basic Drugs (Underivatized)

Column: 30 m x 0.25 mm x 0.25 μ m
 Cat. No.: DM-35, #7921
 DM-5, #7221
 DM-200, #8321
 Oven Temp.: 100 °C to 325 °C (hold 10 min) at 4 °C/min
 Carrier Gas: He, 30 cm/sec, 100 °C
 Injection: Split, 50:1, 250 °C
 Sample: Basic drugs, 1.0 μ L, 1000 ng/ μ L
 Detector: FID, 1.28 x 10⁻¹⁰ AFS, 320 °C

DM-35


Index: CPR00236

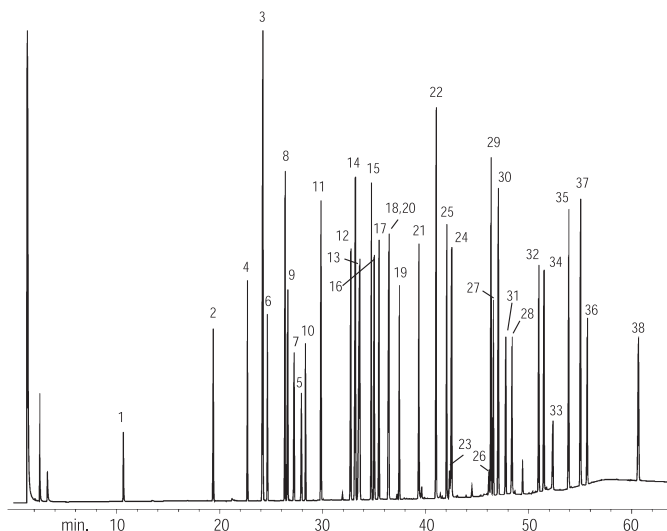

- | | |
|----------------------|--------------------|
| 1. Nicotine | 20. Bupivacaine |
| 2. Benzocaine | 21. Scopolamine |
| 3. Cotinine | 22. Codeine |
| 4. Meperidine | 23. Morphine |
| 5. Caffeine | 24. Diazepam |
| 6. Benzphetamine | 25. Chlorpromazine |
| 7. Ketamine | 26. Temazepam |
| 8. Diphenhydramine | 27. Flunitrazepam |
| 9. Lidocaine | 28. Bromazepam |
| 10. Phenyltoloxamine | 29. Prazepam |
| 11. Tripeleminamine | 30. Acetopromazine |
| 12. Phenothiazine | 31. Flurazepam |
| 13. Dextromethorphan | 32. Papaverine |
| 14. Methadone | 33. Clonazepam |
| 15. Amitriptyline | 34. Haloperidol |
| 16. Trimipramine | 35. Alprazolam |
| 17. Tetracaine | 36. Triazolam |
| 18. Pyrilamine | 37. Thioridazine |
| 19. Medazepam | 38. Trazodone |


DM-5

Index: CPR00235

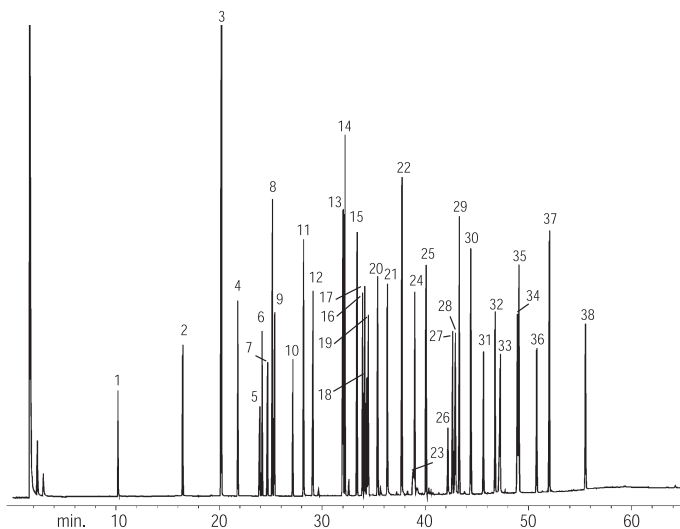

DM-200


Index: CPR00237

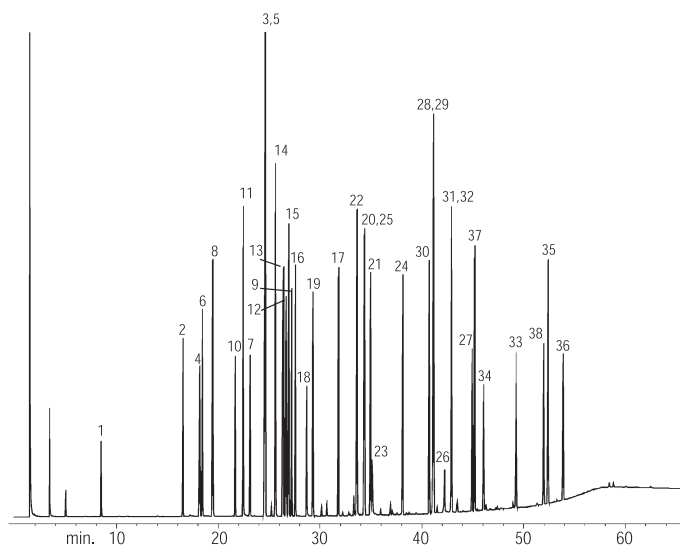

Acidic / Neutral Drugs (Underivatized)

Column: DM-35, 30 m x 0.53 mm x 1.00 μ m
 Cat. No.: 7951
 Index: CPR00262
 Oven Temp.: 100 $^{\circ}$ C to 280 $^{\circ}$ C (hold 5 min) at 10 $^{\circ}$ C/min
 Carrier Gas: He, 40 cm/sec, 100 $^{\circ}$ C
 Injection: Splitless, 0.5 min, 250 $^{\circ}$ C
 Sample: Acidic / Neutral drugs, 1.0 μ L, 50 μ g/mL
 Detector: FID, 5.12 x 10⁻¹⁰ AFS, 250 $^{\circ}$ C


1. Ethosuximide
2. Barbitol
3. Methypylon
4. Aprobarbital
5. Butalbital
6. Amobarbital
7. Pentobarbital
8. Secobarbital
9. Meprobamate
10. Carisoprodal
11. Glutethimide
12. Phenobarbital
13. Methaqualone
14. Primidone
15. Carbamazepine
16. Diphenylhydantoin

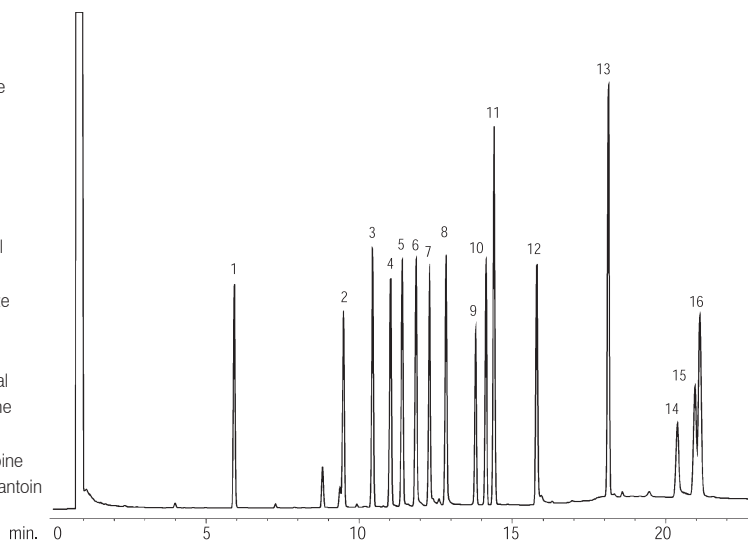

Sympathomimetic Amines Drugs

Column: DM-35 Amine, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: 7821
 Index: CPR00574
 Oven Temp.: 150 $^{\circ}$ C to 240 $^{\circ}$ C at 7 $^{\circ}$ C/min
 Carrier Gas: He, 30 cm/sec
 Injection: Split, 250 $^{\circ}$ C
 Sample: Sympathomimetic amines drugs, 1.0 μ L, 1,000 ng/ μ L
 Detector: MS
 Scan Range: 40 - 450 AMU
 Ionization: EI, scan


1. Amphetamine
2. Methamphetamine
3. N-Ethylamphetamine
4. PMA
5. PMMA
6. MDA
7. MDMA
8. MDEA
9. HMMA
10. MBDB

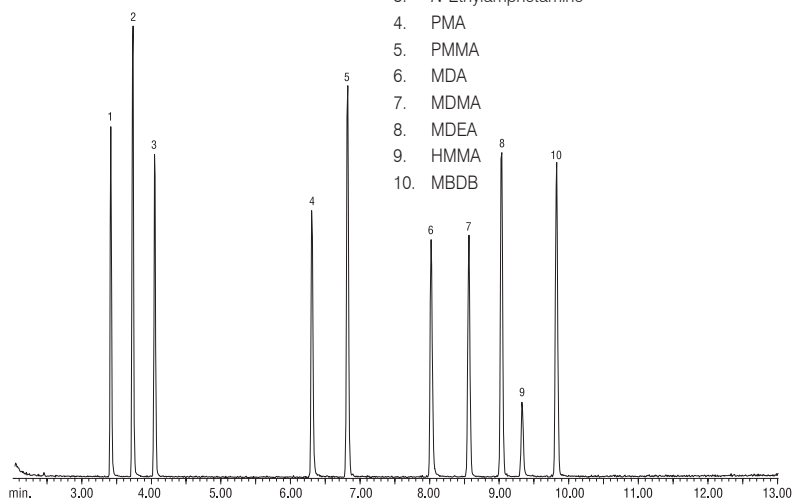

Sympathomimetic Amines Drugs

Column: DM-5 Amine, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: 7815
 Index: CPR00438
 Oven Temp.: 100 $^{\circ}$ C to 310 $^{\circ}$ C at 10 $^{\circ}$ C/min
 Injection: Split, 45 mL/min
 Detector: MS

- | | |
|------------------------|---------------------------------------|
| 1. Phenylethylamine | 12. Pseudoephedrine |
| 2. Amphetamine | 13. Phenmetrazine |
| 3. Phentermine | 14. Phendimetrazine |
| 4. Methamphetamine | 15. Methylenedioxyamphetamine |
| 5. Fenfluramine | 16. Diethylpropion |
| 6. Mephentermine | 17. Methylenedioxymethamphetamine |
| 7. Cathinone | 18. Methylenedioxyethylamphetamine |
| 8. Phenylpropanolamine | 19. 4-Methyl-2,5-dimethoxyamphetamine |
| 9. Methcathinone | 20. Phenylephrine |
| 10. Nicotine | 21. Caffeine |
| 11. Ephedrine | 22. Benzphetamine |

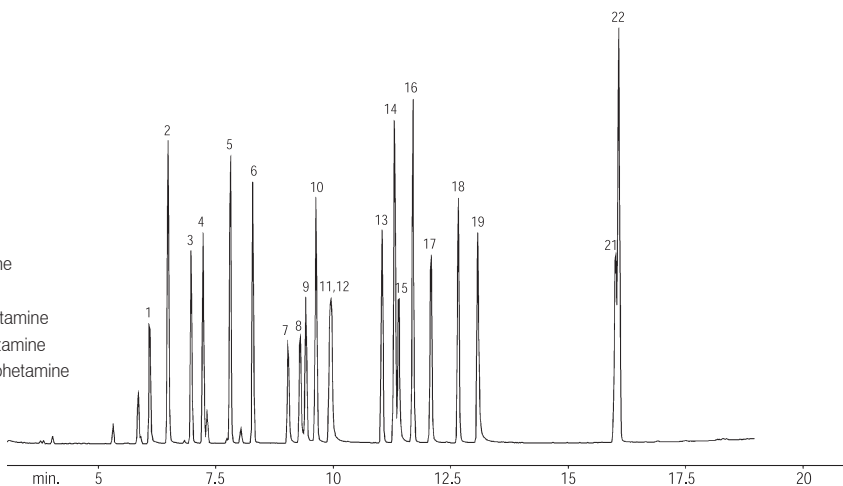


Applications

Steroids, Anabolic


Column: DM-5, 30 m x 0.25 mm x 0.10 μ m
 Cat. No.: 7219
 Index: CPR00255
 Oven Temp.: 180 °C to 340 °C (hold 3 min) at 10 °C/min
 Carrier Gas: He, 35 cm/sec, 180 °C
 Injection: Split, 50:1, 280 °C
 Sample: Anabolic steroids, 0.5 μ L, 1,000 ng/ μ L
 Detector: FID, 1.28 x 10⁻¹⁰ AFS, 340 °C

- | | |
|---|--|
| 1. 5-Androstene-3 β ,17 β -diol | 11. Bolasterone |
| 2. 17 α -Methyl-5-androstene-3 β ,17 β -diol | 12. Oxymethalone |
| 3. 5 α -Androstan-17 β -ol-3-one | 13. 19-Nortestosterone-17-propionate |
| 4. 19-Nortestosterone | 14. Testosterone propionate |
| 5. 17 α -Methylandrostan-17 β -ol-3-one | 15. Fluoxymesterone |
| 6. Mesterolone | 16. 4-Chlorotestosterone-17-acetate |
| 7. Testosterone | 17. Testosterone-17 β -cypionate |
| 8. 17 α -Methyltestosterone | 18. 1-Dehydrotestosterone benzoate |
| 9. 1-Dehydrotestosterone | 19. 1-Dehydrotestosterone undecylenate |
| 10. 1-Dehydro-17 α -methyltestosterone | |

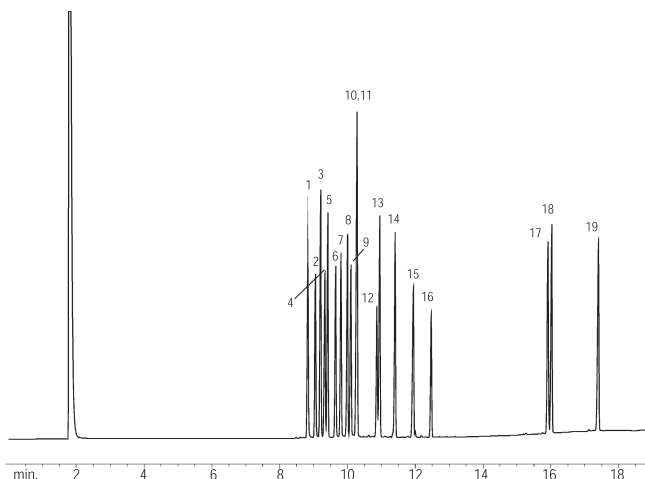

Cold Medicine

Column: DM-35 Amine, 30 m x 0.25 mm x 0.50 μ m
 Cat. No.: 7821
 Index: CPR00575
 Oven Temp.: 250 °C to 300 °C (hold 7 min) at 7 °C/min
 Carrier Gas: He, 30 cm/sec
 Injection: Split, 250 °C
 Sample: Underivatized cold medicine, 1.0 μ L, 1,000 ng/ μ L
 Detector: MS
 Scan Range 40 - 450 AMU
 Ionization EI, scan

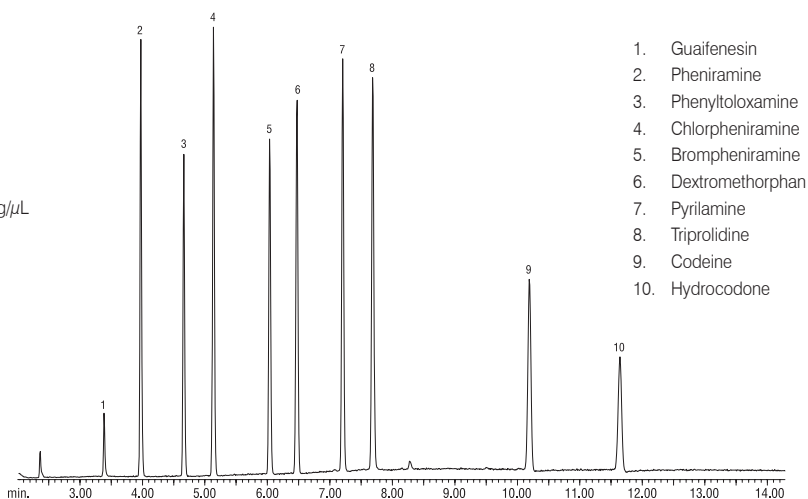


1. Guaifenesin
2. Pheniramine
3. Phenyltoloxamine
4. Chlorpheniramine
5. Brompheniramine
6. Dextromethorphan
7. Pyrilamine
8. Triprolidine
9. Codeine
10. Hydrocodone

Antihistamines

Column: DM-5 Amine, 30 m x 0.32 mm x 1.00 μ m
 Cat. No.: 7817
 Index: CPR00247
 Oven Temp.: 130 °C (hold 5 min) to 305 °C (hold 5 min) at 10 °C/min
 Carrier Gas: H₂, 43 cm/sec, 130 °C
 Injection: Split, 50:1, 305 °C
 Sample: Antihistamines, 1.0 μ L, 1,000 ng/ μ L
 Detector: FID, 6.4 x 10⁻¹¹ AFS, 305 °C


1. Phenylpropranolamine
2. Ephedrine
3. Pseudoephedrine
4. Pheniramine
5. Diphenhydramine
6. Doxylamine
7. Phenyltoloxamine
8. Methapyrilene
9. Chlorpheniramine
10. Brompheniramine
11. Triprolidine

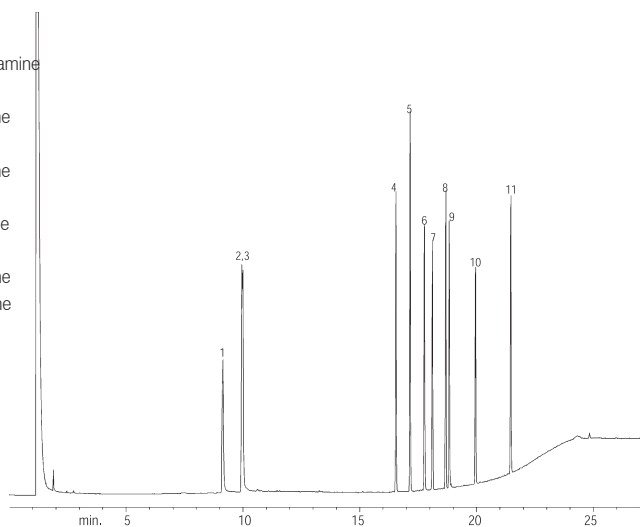

Organic Volatile Impurities (USP 467)

Column: DM-624, 30 m x 0.53 mm x 3.00 μ m + 5 m Guard column
 Cat. No.: 7751
 Index: CPR00259
 Oven Temp.: 40 °C (hold 20 min) to 240 °C (hold 10 min) at 35 °C/min
 Carrier Gas: He, 35 cm/sec, 35 °C
 Injection: Split, 2:1, 180 °C
 Detector: FID, 1.25 x 10⁻¹⁰ AFS, 260 °C


1. Methylene chloride
2. Chloroform
3. Benzene
4. Trichloroethylene
5. 1,4-Dioxane

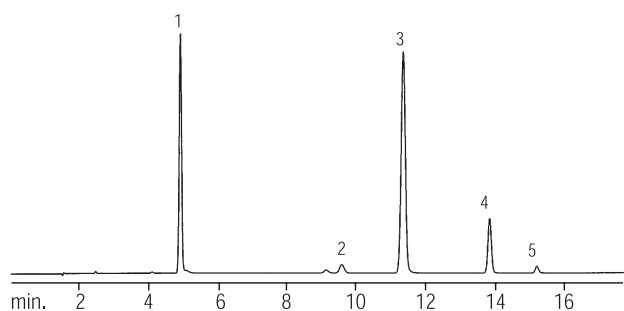

Organic Volatile Impurities

Column: DM-624, 30 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7751
 Index: CPR00261
 Oven Temp.: 35 °C (hold 10 min) to 100 °C at 5 °C/min
 to 240 °C (hold 5 min) at 25 °C/min
 Carrier Gas: He, 35 cm/sec, 35 °C
 Injection: Split, 2:1, 220 °C
 Detector: FID, 1.05 x 10⁻¹¹ AFS, 240 °C


- | | | |
|-----------------------|---------------------------|------------------------|
| 1. Ethylene oxide | 10. -Hexane | 19. 1,2-Dichloroethane |
| 2. Methanol | 11. <i>n</i> -Propanol | 20. Heptane |
| 3. Ethanol | 12. Methyl ethyl ketone | 21. Trichloroethylene |
| 4. Diethyl ether | 13. Ethyl acetate | 22. <i>n</i> -Butanol |
| 5. 1,1-Dichloroethene | 14. Tetrahydrofuran | 23. 1,4-Dioxane |
| 6. Acetone | 15. Chloroform | 24. Pyridine |
| 7. Isopropanol | 16. 1,1,1-Trichloroethane | 25. Toluene |
| 8. Acetonitrile | 17. Carbon tetrachloride | |
| 9. Methylene chloride | 18. Benzene | |

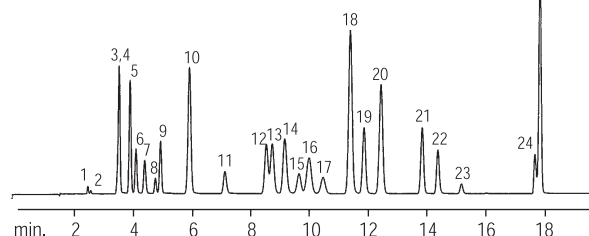

EP Class 1 and Class 2 Solvents

Column: DM-624, 30 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7751
 Index: CPR00553
 Oven Temp.: 40 °C (hold 20 min) to 240 °C (hold 20 min) at 10 °C/min
 Carrier Gas: H₂, 35 cm/sec
 Injection: 1 mL Headspace injection, using samples shaken and heated
 at 80 °C for 15 min, 200 °C
 Split Ratio: 2:1
 Detector: FID, 1.1 x 10⁻¹¹ AFS, 250 °C


- | | | |
|-----------------------------------|---------------------------|-----------------------------------|
| 1. Methanol | 10. 1,1,1-Trichloroethane | 19. Toluene |
| 2. 1,1-Dichloroethene | 11. Carbon tetrachloride | 20. 2-Hexanone |
| 3. Acetonitrile | 12. Benzene | 21. Chlorobenzene |
| 4. Dichloromethane | 13. 1,2-Dimethoxyethane | 22. DMF |
| 5. Hexane | 14. 1,2-Dichloroethane | 23. Ethylbenzene |
| 6. <i>cis</i> -1,2-Dichloroethene | 15. 1,1,2-Trichloroethene | 24. <i>m</i> -Xylene |
| 7. Nitromethane | 16. Methyl cyclohexane | 25. <i>p</i> -Xylene |
| 8. Chloroform | 17. 1,4-Dioxane | 26. <i>o</i> -Xylene |
| 9. Cyclohexane | 18. Pyridine | 27. <i>N,N</i> -Dimethylacetamide |
| | | 28. 1,2,3,4-Tetrahydronaphthalene |

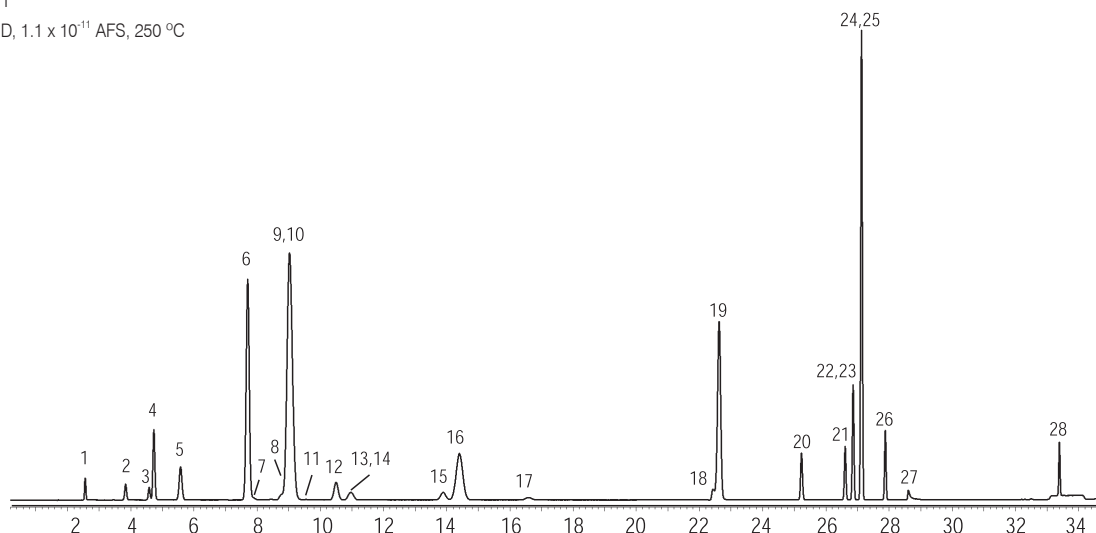

Residual Solvents

Column: DM-624, 30 m x 0.53 mm x 3.00 μ m
 Cat. No.: 7751
 Index: CPR00257
 Oven Temp.: 35 $^{\circ}$ C (hold 8 min) to 240 $^{\circ}$ C at 20 $^{\circ}$ C/min
 Carrier Gas: He, 25 cm/sec, 35 $^{\circ}$ C
 Injection: Split, 30:1, 180 $^{\circ}$ C
 Sample: Residual solvents, 0.5 μ L
 Detector: FID, 1.28×10^{-10} AFS, 260 $^{\circ}$ C

1. Methanol
2. Ethanol
3. Ether
4. Acetone
5. Isopropanol
6. Acetonitrile
7. Methylene chloride
8. *tert*-Butanol
9. Hexane
10. *n*-Propanol
11. Methyl ethyl ketone
12. Ethyl acetate
13. Tetrahydrofuran
14. *sec*-Butanol
15. Chloroform
16. Cyclohexane
17. Benzene
18. Heptane
19. Trichloroethylene
20. 1,4-Dioxane
21. Pyridine
22. Toluene
23. Dimethyl formamide

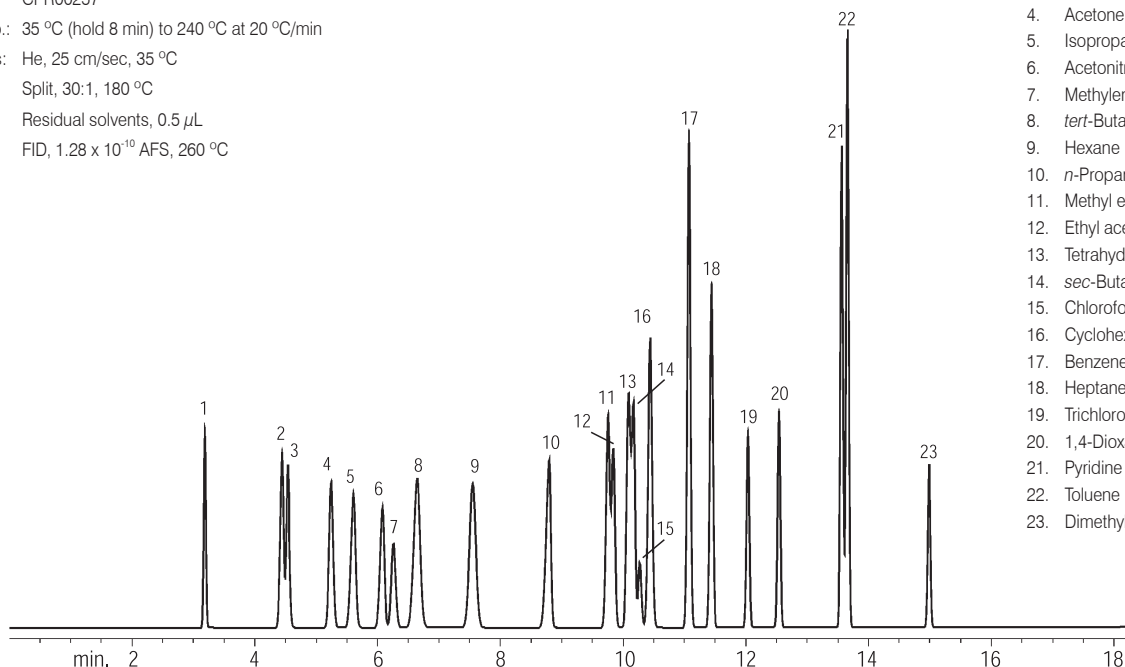


Applications

Primary, Second and Tertiary Amines

Column: DM-624MS, 30 m x 0.32 mm x 1.80 μ m
 Cat. No.: 8838
 Index: CPR1162
 Oven Temp.: 50 $^{\circ}$ C (hold 1 min) to 200 $^{\circ}$ C (hold 5 min) at 20 $^{\circ}$ C/min
 Carrier Gas: He, 37 cm/sec
 Injection: Split, 20:1, 1.0 μ L, 250 $^{\circ}$ C
 Sample: Primary, second and tertiary amines in DMSO, 100 μ g/mL
 Detector: FID, 250 $^{\circ}$ C

1. Isopropylamine 100 μ g/mL
2. Diethylamine 100 μ g/mL
3. Triethylamine 100 μ g/mL

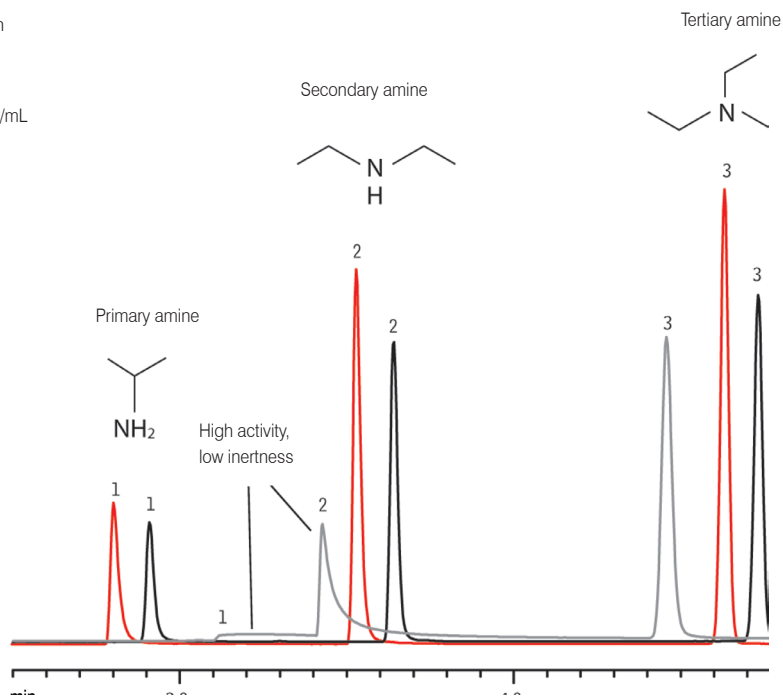

Industry Index

Food	214
Environmental.....	229
Pharmaceutical	231
Others.....	232

Product Index

ProElut™ BaP

Determination of Benzopyrene Originating from Vegetable Oil.....	224
--	-----

ProElut™ PLS

Determination of Phenols in Water.....	229
Determination of Sulfonamides in Animal Tissue	218
Determination of Tetracyclines in Animal Tissue.....	225
Determination of Tetracyclines in Milk and Dairy Products.....	228
Determination of Tetracyclines in Serum.....	231

ProElut™ PLS GLASS

Determination of Migration of Bisphenol A (BPA) from Plastic Baby Bottles.....	232
Determination of Phthalate Esters (PAEs) in Water.....	230

ProElut™ PXC

Determination of β -Agonist Drugs in Animal Tissue	222
Determination of Fungicides in Fruit Juice.....	226
Determination of Histamine Originating from Aquatic Products.....	214
Determination of Melamine in Milk and Dairy Products.....	216
Determination of Sulfonamides in Milk and Milk Powder.....	220

Determination of Histamine Originating from Aquatic Products

1. Scope of application

For determination of histamine in aquatic products

2. Sample preparation / extraction

2.1. Weighing

Smoked fish and other dried samples: Weigh 2.5 g of sample (accurate to 0.01 g) in 50 mL centrifuge tube.

Tuna and other wet samples: Weigh 5.0 g of sample (accurate to 0.01 g) in 50 mL centrifuge tube.

2.2. Extraction of histamine

Add 20 mL histamine extract* to centrifuge tube, vortex 1 min, shock in thermostatic water bath for 30 min at 60 °C, centrifuge at 4,000 rpm for 10 min. Take 6 mL of supernatant and adjust the pH to be between 2 - 3 with 50% H₃PO₄ as the sample solution to be purified.

*Histamine extract: MeOH:50 mM KH₂PO₄ = 1:1

3. Sample purification

ProElut™ PXC 150 mg / 6 mL (**Cat#68204**)

Condition: 6 mL MeOH / 6 mL H₂O

Load: 6 mL supernatant

Wash 1: 6 mL 0.1 M HCl

Wash 2: 6 mL solution of NH₄OH:MeOH:H₂O = 5:5:90

Elute: 6 mL solution of NH₄OH:MeOH:H₂O = 5:60:35

Reconstitute: Reconstitute to 6 mL with elution solvent

4. HPLC method

Column: Inspire™ 5 μm C18, 150 x 4.6 mm (**Cat#81001**)

Mobile Phase: A: MeOH, B: Phosphoric acid - triethylamine buffer*, A:B = 40:60

Flow Rate: 1.0 mL/min

Temperature: 30 °C

Detection: FLD Ex: 345 nm, Em: 445 nm


Injection Volume: 10 μL

Injection Procedure: 7.5 μL *o*-Phthalaldehyde (OPA) + 10 μL sample + 7.5 μL OPA

*Phosphoric acid - triethylamine buffer: Add 12.5 mL triethylamine and 25.7 mL phosphoric acid to 1 L deionized water


5.1. Recovery

Compounds	Spike Level (mg/kg)	Recovery
Histamine	10	89.96
	10	90.04
	20	73.04
	20	71.50
	40	59.98
	40	53.63

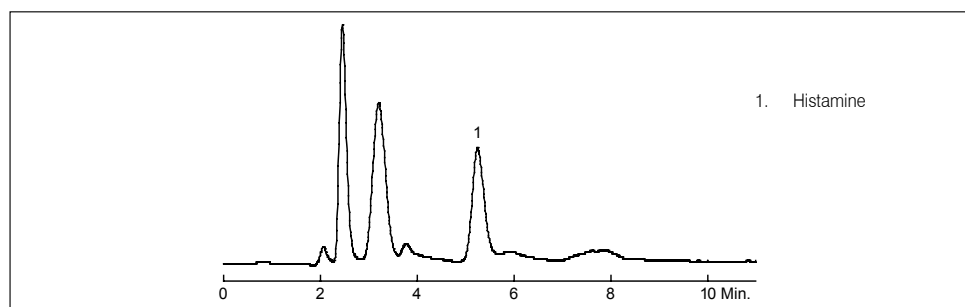


Chromatogram of aquatic products extracts - spiked histamine in aquatic products (10 mg/kg)

5.2. Recovery rate comparison

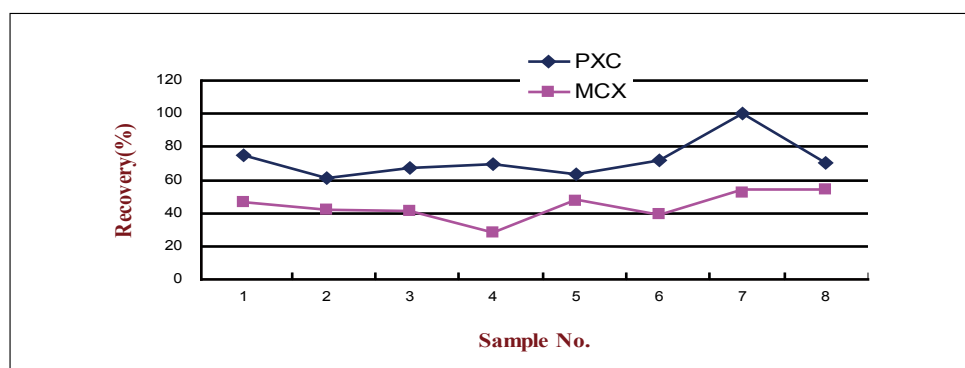

Samples No. 1 - 6 show the internal standard added in sample. Samples No. 7 and No. 8 show the internal standard added in sample extracting solution. Both methods exhibit stable recovery, the recovery of PXC treatment is better than that of MCX treatment.

5.3. Purification comparison

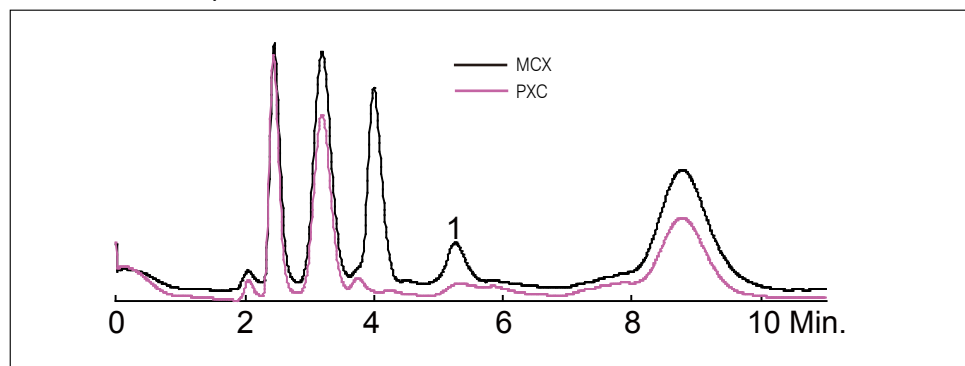

Applications

Determination of Melamine in Milk and Dairy Products

1. Scope of application

For determination of melamine in milk and dairy products

2. Sample preparation

2.1. Milk and milk powder

Dilute milk (2 mL) or milk powder (1 g) with 5 mL of trichloroacetic acid aqueous solution (10 g/L) in a 15 mL centrifuge tube, add 0.5 mL lead acetate aqueous solution (22 g/L) and 2 mL chloroform, vortex and centrifuge for 2 min at 3,000 rpm, collect supernatant, add 5 mL trichloroacetic acid aqueous solution (10 g/L) to residue, vortex and centrifuge for 2 min at 3,000 rpm, collect and combine supernatants.

2.2. Cream candy and cookies

Grind 1 g sample with sand into powder in a mortar, add powder to a 50 mL centrifuge tube, rinse the mortar with 15 mL of trichloroacetic acid aqueous solution (10 g/L), transfer solution to centrifuge tube then shake, add 1 mL lead acetate aqueous solution (22 g/L) and 5 mL chloroform, vortex and centrifuge for 2 min at 3,000 rpm, collect supernatant, add 15 mL trichloroacetic acid aqueous solution (10 g/L) to residue, vortex and centrifuge for 2 min at 3,000 rpm, collect and combine supernatants.

3. Sample purification

ProElut™ PXC 60 mg / 3mL (**Cat#68203**)

Condition: 3 mL MeOH / 3 mL H₂O

Load*: supernatant

Wash 1: 3 mL deionized water

Wash 2: 3 mL MeOH

Elute: 3 mL 5 % NH₄OH in MeOH

Reconstitute: Evaporate at 50 °C by N₂, reconstitute to 1 mL with MeOH:H₂O (20:80, V / V) solution

*12 mL reservoir (**Cat#4810**) and adaptor (**Cat#4803**) is available for large volume sample

4. HPLC method

Column: Inspire™ 5 μm C18, 150 x 4.6 mm (**Cat#81001**)

Mobile Phase : Buffer:MeCN = 92:8

Flow Rate: 1.0 mL/min

Temperature: 30 °C


Detection: UV 240 nm

Injection Volume: 20 μL

Buffer: dilute 2.02 g sodium 1-heptanesulfonate and 2.10 g citric acid with water to total volume 1,000 mL


5. Recovery

5.1. Milk powder sample recovery

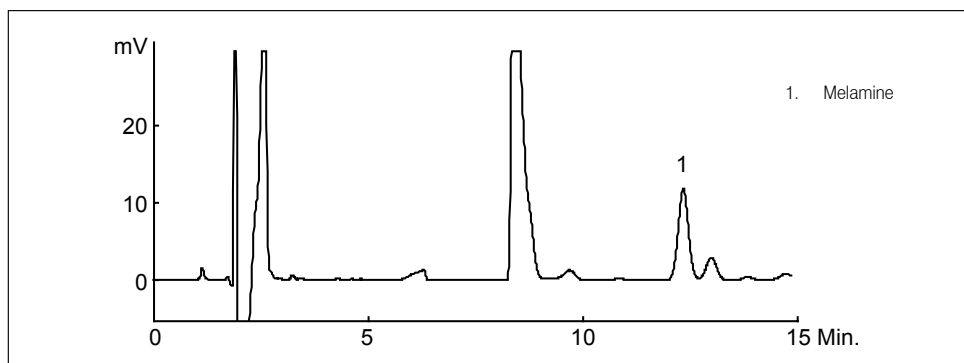


Chromatogram of milk powder extracts - spiked melamine in milk powder, 0.5 mg/kg

5.2. Cookies sample recovery

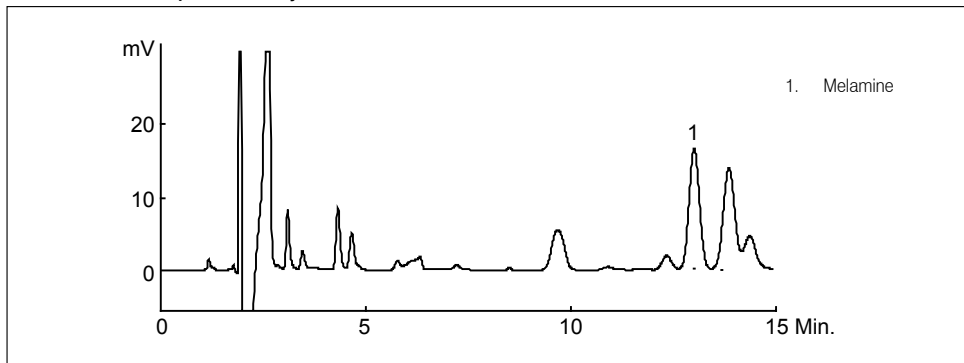

Chromatogram of cookies extracts - spiked melamine in cookies, 0.5 mg/kg, recovery: 85.9%

5.3. Cream candy sample recovery

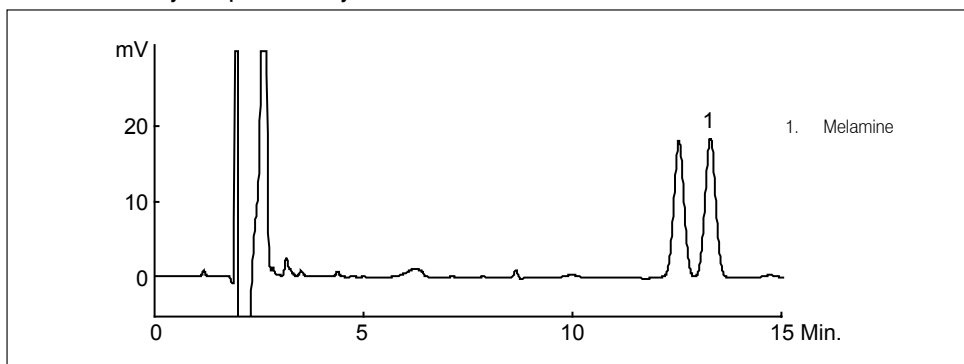

Chromatogram of cream candy extracts - spiked melamine in cream candy, 0.5 mg/kg, recovery: 95.9%

Determination of Sulfonamides in Animal Tissue

1. Scope of application

Used for determination of sulfonamides in poultry, meat and aquatic product

2. Sample preparation

Weigh 5 g sample, add 5 g anhydrous sodium sulfate and 25 mL ethyl acetate, homogenize at 10,000 rpm for 2 min, centrifuge at 4,000 rpm for 2 min, collect ethyl acetate layer. Repeat 25 mL ethyl acetate extraction, combined ethyl acetate extracts, and vacuum distillation at 30 °C to near dry. Add 1 mL methanol, 2 mL 1% acetic acid and 3 mL *n*-hexane to the distillation flask, vortex for 1 min, then transfer to 15 mL centrifuge tube. Repeat the dissolution process, add mixture to the centrifuge tube, vortex for 1 min, centrifuge for 1 min at 4,000 rpm, discard the hexane. Add 6 mL *n*-hexane and repeat the operation. Finally, add 6 mL deionized water to the lower layer.

3. Sample purification

ProElut™ PLS 60 mg / 3mL (Cat#68003)

Condition: 3 mL MeOH / 3 mL H₂O

Load: Add sample

Wash 1: 3 mL H₂O

Wash 2: 3 mL MeOH:H₂O = 5:95

Elute: 5 mL MeOH

Reconstitute: Evaporate at 30 °C by N₂, reconstitute to 1 mL with mobile phase

4. HPLC method

Column: Inspire™ 5 μm C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: A: MeCN, B: 2 % CH₃COOH in H₂O

Flow Rate: 1.0 mL/min

Temperature: 35 °C

Detection: UV 270 nm


Injection Volume: 20 μL

Gradient:

Time / Min.	0	30	40	41	50
A	12	25	25	12	12
B	88	75	75	88	88

5. Recovery

Compounds	Spike Level (mg/kg)	Recovery (%)	RSD (%) (n = 4)
Sulfapyridine	0.1	79.8	5.5
	1.0	81.3	2.8
Sulfamerazine	0.1	89.5	6.4
	1.0	91.3	4.7
Sulfadimidine	0.1	94.3	5.2
	1.0	92.7	2.9
Sulfamethoxypridazine	0.1	88.5	5.1
	1.0	86.2	3.9
Sulfamethoxazole	0.1	84.6	5.3
	1.0	82.9	3.2
Sulfisoxazole	0.1	94.1	4.7
	1.0	92.7	3.9
Sulfaquinoxaline	0.1	88.9	3.1
	1.0	91.3	4.5
Sulphadimethoxine	0.1	82.7	4.9
	1.0	94.2	2.6

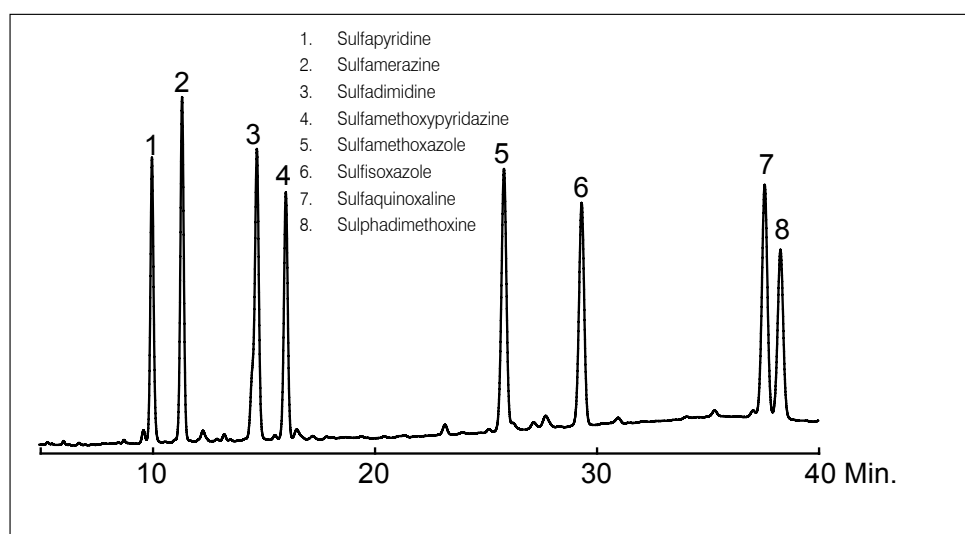

Chromatogram of sulfonamides - spiked 8 sulfonamides in animal tissue (0.1 mg/kg)

Determination of Sulfonamides in Milk and Milk Powder

1. Scope of application

Used for determination of sulfonamides in milk and milk powder

2. Sample preparation

To 15 mL milk (or 3 g milk powder in 15 mL H₂O), add 15 mL acetonitrile, vortex for 2 min, centrifuge at 6,000 rpm for 5 min, transfer 20 mL supernatant to another centrifuge tube, and add 15 mL *n*-hexane, vortex for 2 min, centrifuge at 6,000 rpm for 2 min, then discard the *n*-hexane. Repeat 15 mL *n*-hexane extraction. Add 15 mL ethyl acetate to the lower layer, vortex for 2 min, centrifuge at 6,000 rpm for 2 min, and collect supernatant. Repeat 15 mL ethyl acetate extraction, and combine supernatants. Vacuum evaporate the ethyl acetate layer to near dry at 30 °C, reconstitute with 10 mL 2% phosphoric acid.

3. Sample purification

ProElut™ PXC 200 mg / 6 mL (Cat#68212)

Condition: 6 mL MeOH / 6 mL H₂O

Load: Add sample

Wash 1: 6 mL H₂O

Wash 2: 6 mL MeOH

Elute: 6 mL MeOH (5 % NH₄OH)

Reconstitute: Vacuum evaporation at 30 °C, reconstitute to 1 mL with mobile phase

4. HPLC method

Column: Inspire™ 5 μm C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: A: MeCN, B: 2 % CH₃COOH in H₂O

Flow Rate: 1.0 mL/min

Temperature: 35 °C

Detection: UV 270 nm


Injection Volume: 20 μL

Gradient:

Time / Min.	0	30	38	39	45
A	12	25	25	12	12
B	88	75	75	88	88

5. Recovery

Compounds	Spike Level (mg/kg)	Recovery (%)	RSD (%) (n = 4)
Sulfapyridine	0.1	78.4	4.1
	0.5	97.0	2.9
Sulfamerazine	0.1	82.3	4.6
	0.5	96.0	2.3
Sulfadimidine	0.1	83.5	4.8
	0.5	96.0	2.5
Sulfamethoxy pyridazine	0.1	82.0	3.2
	0.5	98.0	2.3
Sulfamethoxazole	0.1	84.3	3.9
	0.5	101.5	2.5
Sulfisoxazole	0.1	75.4	3.4
	0.5	91.8	3.8
Sulfaquinoxaline	0.1	77.8	4.2
	0.5	96.2	3.1
Sulphadimethoxine	0.1	77.5	5.2
	0.5	97.0	2.6

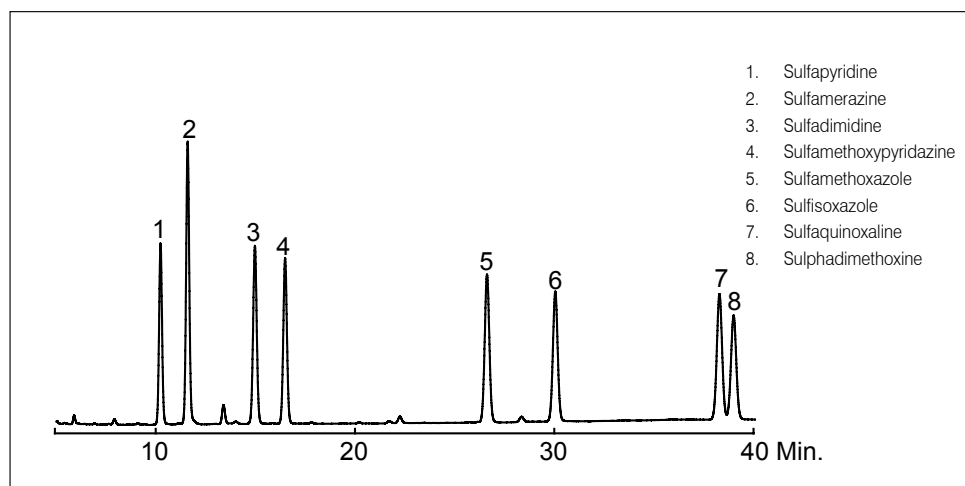

Chromatogram of milk extracts - spiked 8 sulfonamides in milk (0.1 mg/kg)

Determination of β - Agonist Drugs in Animal Tissue

1. Scope of application

Used for determination of clenbuterol hydrochloride, salbutamol, cimaterol, and ractopamine hydrochloride in animal muscle and liver

2. Sample preparation

Weigh 5 g sample, add 15 mL ethyl acetate and 3 mL 10% sodium carbonate, homogenize at 10,000 rpm for 2 min, centrifuge at 6,000 rpm for 2 min, transfer the supernatant to the centrifuge tube, extract residues using 15 mL ethyl acetate, combine ethyl acetate layers. Add 5 mL 0.1 M hydrochloric acid to the ethyl acetate extract, vortex for 1 min, centrifuge for 1 min at 6,000 rpm, collect the lower aqueous phase. Repeat the extraction and combine lower aqueous phase, adjust to pH 5.2 with 2.5 mol/L sodium hydroxide.

3. Sample purification

ProElut™ PXC 60 mg / 3 mL (Cat#68203)

Condition: 3 mL MeOH / 3 mL H₂O / 3 mL 30 mM HCl

Load: Add sample

Wash 1: 3 mL deionized water

Wash 2: 3 mL MeOH

Elute: 5 mL MeOH (4% NH₄OH), evaporate to near dry at 50 °C by N₂

4. Derivatization

Add 100 μ L toluene and 100 μ L *bis*-trimethylsilyl trifluoroacetamide (BSTFA), vortex for 20 sec, seal, heat for 1 h at 80 °C, add 300 μ L of toluene after cooling as the sample solution.

5. GC-MS method

GC conditions

Column: DM-5MS 30 m x 0.25 mm x 0.25 μ m (Cat#8221)

Inlet Temperature: 220 °C

Injection Mode: Splitless

Injection Volume: 1 μ L

Temperature Program: Heating to 70 °C in 0.6 min, then heating to 200 °C with 25 °C/min in 6 min, finally heating to 280 °C with 25 °C/min in 5 min

Carrier Gas: He > 99.999%, flow rate: 0.9 mL/min

MS conditions

Interface Temperature: 280 °C

Solvent Delay: 8 min


EI Temperature: 230 °C

Quadrupole Temperature: 160 °C

Ion Monitoring: Qualitative ion 86, 243, 262, 277, quantitative ion 86

5. Recovery

Compounds	Spike Level ($\mu\text{g}/\text{kg}$)					
	1.0		10.0		100	
	Recovery (%)	RSD (%) (n = 3)	Recovery (%)	RSD (%) (n = 3)	Recovery (%)	RSD (%) (n = 3)
Clenbuterol	75.37	5.93	83.21	5.39	90.05	2.86
Salbutamol	72.40	6.12	84.45	5.72	88.27	4.16
Cimaterol	76.73	4.90	85.95	4.68	91.15	3.86
Ractopamine	70.09	7.85	87.46	3.59	89.53	5.93

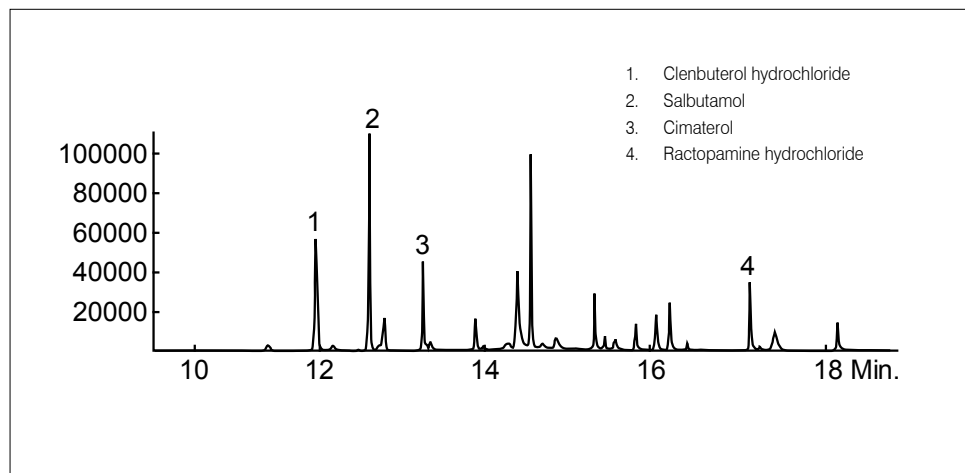

The total ion chromatogram (TIC) of pig liver extracts - spiked 4 β -agonist drugs in pig liver (0.1 mg/kg)

Determination of Benzopyrene Originating from Vegetable Oil

1. Scope of application

Used for determination of benzopyrene originating from vegetable oil

2. Sample preparation

Weigh 0.4 g sample, accurate to 0.001 g, dilute with 5 mL *n*-hexane.

3. Sample purification

ProElut™ BaP 22 g / 60 mL (Grade IV activity) (Cat#65351)

Condition: 30 mL *n*-hexane

Load: Add sample

Elute: 50 mL *n*-hexane

Reconstitute: Vacuum evaporation at 30 °C, reconstitute to 1 mL with MeCN:THF (9:1, V / V) solution

4. HPLC method

Column: Inspire™ 5 μm C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: MeCN:H₂O = 97:3

Flow Rate: 1.0 mL/min


Temperature: 30 °C

Detection: FLD Ex: 384 nm, Em: 406 nm

Injection Volume: 5 μL

5. Recovery

Compounds	Spike Level (mg/kg)	Recovery (%)	RSD (%) (n = 4)
Benzopyrene	0.1	96.8	2.30
Benzopyrene	0.01	98.5	4.50

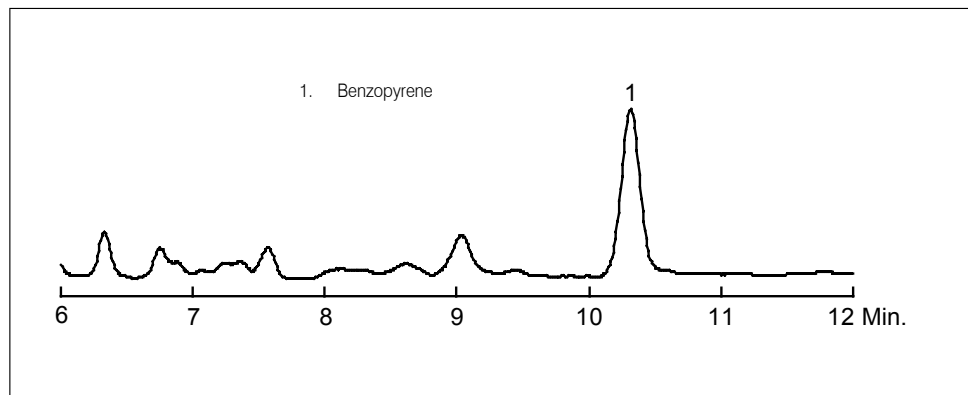

Chromatogram of vegetable oil extracts - spiked benzopyrene in vegetable oil (0.01 mg/kg)

Determination of Tetracyclines in Animal Tissue

1. Scope of application

Used for determination of oxytetracycline, tetracycline, chlortetracycline and doxycycline in animal tissue

2. Sample preparation

To 5.0 g of homogenized sample, add 20 mL of Mcllvaine buffer*, vortex 2 min, centrifuge at 4000 rpm for 5 min, collect supernatant. Wash lower residue with 20 mL, and then 10 mL Mcllvaine buffer. Repeat wash and combine extracts, and set the volume to 50 mL. Filter extract with fast filter paper, collect filtrate and take 10 mL as the sample solution.

*Mcllvaine buffer: Disodium hydrogen phosphate ($\text{Na}_2\text{HPO}_4 \cdot 12\text{H}_2\text{O}$) 27.6 g, citric acid ($\text{C}_6\text{H}_8\text{O}_7 \cdot \text{H}_2\text{O}$) 12.9 g, EDTA disodium salt 37.2 g, dissolved in water and diluted to 1,000 mL.

3. Sample purification

ProElut™ PLS 60 mg / 3 mL (Cat#68003)

Condition: 3 mL MeOH / 3 mL H_2O

Load*: 10 mL sample

Wash 1: 3 mL H_2O

Wash 2: 3 mL 5 % MeOH in H_2O

Elute: 3 mL MeOH

Reconstitute: Evaporate to near dry, reconstitute to 1 mL with mobile phase

*20 mL reservoir (Cat#4811) and adaptor (Cat#4803) is available for large volume sample

4. HPLC method

Column: Spursil™ 5 μm C18, 150 x 4.6 mm (Cat#82001)

Mobile Phase: A: 0.01 M Oxalic acid in H_2O , B: MeOH:MeCN = 1:1

Flow Rate: 1.0 mL/min

Temperature: 30 °C

Detection: UV 365 nm


Injection Volume: 20 μL

Gradient:

Time / Min.	0	10	10.5	20
A	70	50	70	70
B	30	50	30	30

5. Recovery

Compounds	Spike Level (mg/kg)	Recovery (%)	RSD (%) (n = 3)
Oxytetracycline	0.2	95.31	2.80
	1.0	90.30	2.00
Tetracycline	0.2	83.17	0.54
	1.0	81.84	2.38
Chlortetracycline	0.2	102.70	2.75
	1.0	90.83	3.21
Doxycycline	0.2	83.16	3.12
	1.0	81.30	1.43

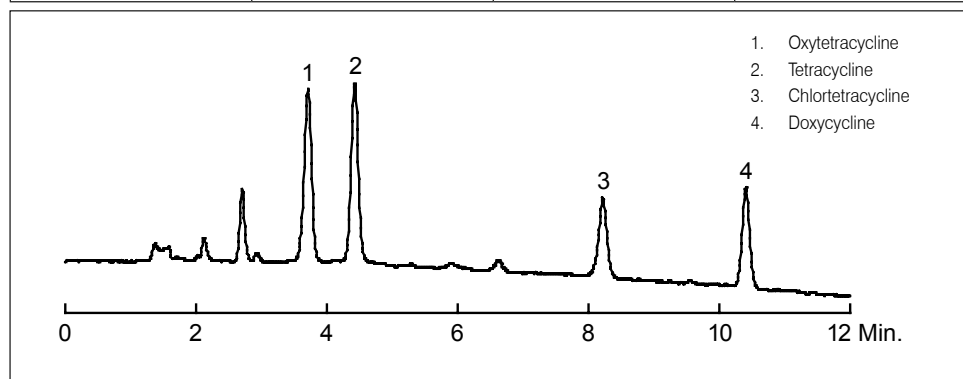

Chromatogram of tetracyclines - spiked tetracyclines in pork tissue (1.0 mg/kg)

Determination of Fungicides in Fruit Juice

1. Scope of application

Used for determination of carbendazim and thiabendazole in fruit juice

2. Sample preparation

2.1 Juice drinks and pure fruit juice

Start with 10 mL sample, adjust to pH 10 - 11 with 0.1 M NaOH, add 15 mL ethyl acetate, shake 1 min, centrifuge 1 min at 4,000 rpm, collect ethyl acetate layer. Repeat 15 mL ethyl acetate extraction, and combine organic phases, vacuum distillation at 30 °C to near dry. Dissolve residue with 0.1 M HCl (6 mL) twice.

2.2 Fruit juice concentrate

Start with 2 mL sample mixed with 8 mL H₂O, adjust to pH 10 - 11 with 0.1 M NaOH, and then follow the above steps.

3. Sample purification

ProElut™ PXC 60 mg / 3 mL (Cat#68203)

Condition: 3 mL MeOH / 3 mL H₂O

Load: Adding sample

Wash: 3 mL H₂O / 3 mL MeOH

Elute: 3 mL MeOH (5 % NH₄OH)

Reconstitute: Evaporate to near dry at 30 °C, reconstitute to 1 mL with mobile phase

4. HPLC method

Column: Inspire™ 5 μm C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: Phosphate buffer:MeCN = 75:25

Flow Rate: 1.0 mL/min

Temperature: 30 °C

Detection: UV 288 nm


Injection Volume: 20 μL

Phosphate buffer: 1.38 g sodium dihydrogen phosphate, 1.41 g disodium hydrogen phosphate, dissolve in 1,000 mL water

5. Recovery

5.1. Grape juice


Compounds	Spike Level (mg/L)	Recovery (%)	RSD (%) (n = 3)
Carbendazim	0.1	87.0	8.0
	0.5	99.7	3.5
Thiabendazole	0.1	83.1	7.8
	0.5	102.6	3.8

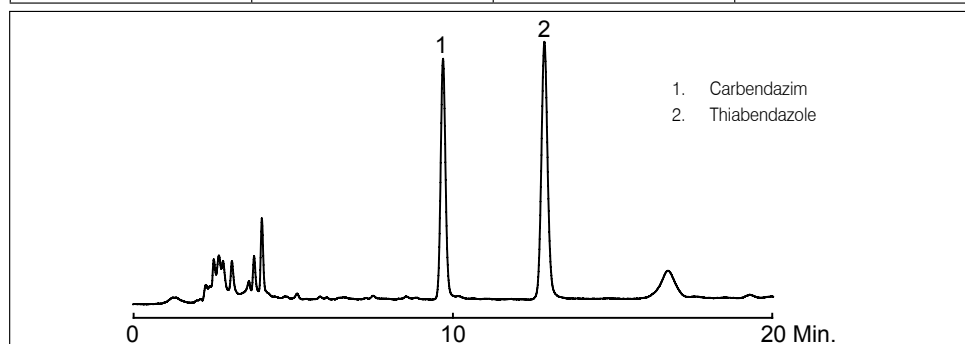

Chromatography of fungicides - spiked fungicides in grape juice (0.1 mg/L)

5.2. Orange juice


Compounds	Spike Level (mg/L)	Recovery (%)	RSD (%) (n = 3)
Carbendazim	0.1	100.4	2.6
	0.5	94.4	4.5
Thiabendazole	0.1	98.1	3.1
	0.5	98.3	1.9

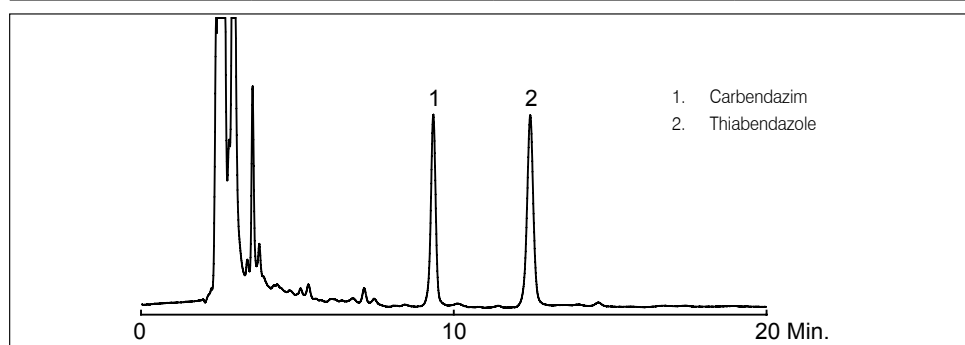

Chromatography of fungicides - spike fungicides in orange juice (0.1 mg/L)

5.3. Peach juice

Compounds	Spike Level (mg/L)	Recovery (%)	RSD (%) (n = 3)
Carbendazim	0.1	89.9	2.4
	0.5	92.3	5.5
Thiabendazole	0.1	90.0	1.6
	0.5	92.6	2.9

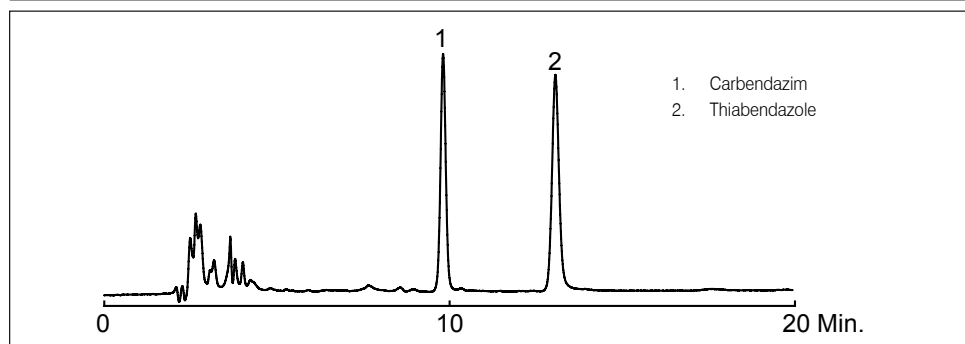

Chromatography of fungicides - spike fungicides in peach juice (0.5 mg/L)

Determination of Tetracyclines in Milk and Dairy Products

1. Scope of application

Used for determination of oxytetracycline, tetracycline, chlortetracycline and doxycycline in milk and dairy products

2. Sample preparation

Dilute milk sample (20 mL) or 2 g solid dairy product with 20 mL H₂O, add 20 mL Mcllvaine buffer*, vortex for 2 min, centrifuge at 4,000 rpm for 10 min, take 20 mL supernatant as the sample solution.

*Mcllvaine buffer: Disodium hydrogen phosphate (Na₂HPO₄•12H₂O) 27g, citric acid (C₆H₈O₇•H₂O) 12 g, EDTA disodium salt 37 g, dissolved in water and diluted to 1,000 mL.

3. Sample purification

ProElut™ PLS 150 mg / 6 mL (Cat#68004)

Condition: 6 mL MeOH / 6 mL H₂O

Load*: 20 mL sample

Wash 1: 6 mL H₂O

Wash 2: 6 mL 10 % MeOH in H₂O

Elute: 6 mL MeOH

Reconstitute: Evaporate to near dry at 40 °C, reconstitute to 1 mL with mobile phase

*20 mL reservoir (Cat#4811) and adaptor (Cat#4803) is available for large volume sample

4. HPLC method

Column: Spursil™ 5 μm C18, 150 x 4.6 mm (Cat#82001)

Mobile Phase: A: 0.01 M Oxalic acid in H₂O, B: MeOH:MeCN = 1:1

Flow Rate: 1.0 mL/min

Temperature: 30 °C

Detection: UV 365 nm


Injection Volume: 20 μL

Gradient:

Time / Min.	0	10	10.5	20
A	70	50	70	70
B	30	50	30	30

5. Recovery

Compounds	Spike Level (mg/kg)	Recovery (%)	RSD (%) (n = 3)
Oxytetracycline	0.1	88.17	4.01
	0.5	83.95	2.35
Tetracycline	0.1	89.46	0.69
	0.5	90.06	3.68
Chlortetracycline	0.1	96.54	2.92
	0.5	100.86	0.69
Doxycycline	0.1	90.48	0.99
	0.5	88.26	0.81

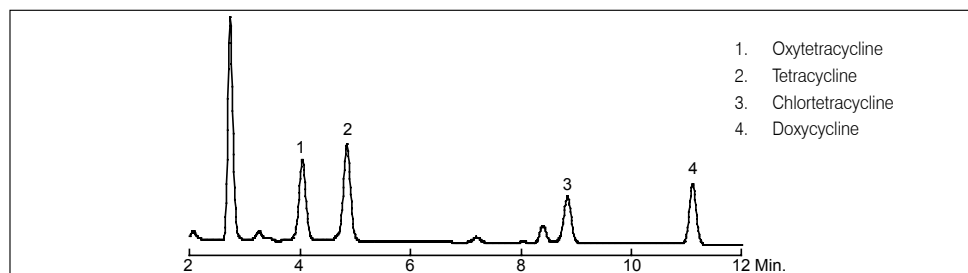

Chromatogram of tetracyclines - spiked tetracyclines in milk (0.1 mg/kg)

Determination of Phenols in Water

1. Scope of application

Used for determination of phenols in natural water, drinking water

2. Sample preparation

100 mL sample, adjust to pH 2 with H₃PO₄

3. Sample purification

ProElut™ PLS 60 mg / 3 mL (Cat#68003)

Condition: 3 mL MeOH:MTBE = 10:90 / 3 mL MeOH / 3 mL H₂O

Load: 100 mL sample, flow rate ≤ 5 mL/min

Wash: 3 mL H₂O

Elute: 3 mL MeOH:MTBE = 10:90

Reconstitute: Evaporate at 40 °C by N₂, reconstitute to 1 mL with MeCN:H₂O (50:50, V / V) solution

4. HPLC method

Column: Inspire™ 5 μm C18, 150 x 4.6 mm (Cat#81001)

Mobile Phase: A: 1% CH₃COOH in H₂O, B: 1% CH₃COOH in MeCN

Flow Rate: 1.0 mL/min


Temperature: Ambient

Detection: UV 280 nm

Injection Volume: 20 μL

Gradient:

Time / Min.	0	25	30	35	37
A	80	30	0	0	80
B	20	70	100	100	20

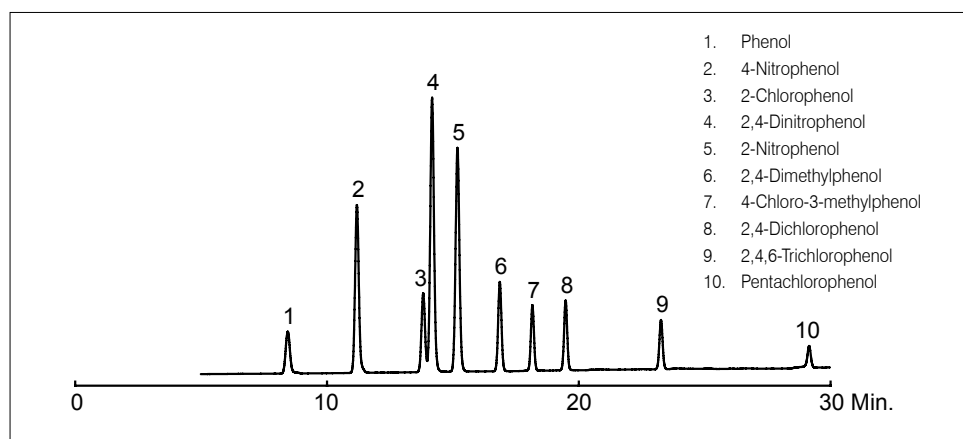

Environmental

Determination of Phthalate Esters (PAEs) in Water

1. Scope of application

Used for determination of dimethyl phthalate (DMP), diethyl phthalate (DEP), dipropyl phthalate (DPrP), butyl benzyl phthalate (BBP), dibutyl phthalate (DBP), diamyl phthalate (DPP), dicyclohexyl phthalate (DCHP), di-*n*-hexyl phthalate (DHP), and di-(2-ethylhexyl)phthalate (DEHP) in natural water and drinking water.

2. Sample purification

ProElut™ PLS GLASS 200 mg / 6 mL (Cat#68012G)

Condition: 6 mL methyl *tert*-butyl ether / 6 mL MeOH / 6 mL H₂O

Load: Up to 500 mL sample, flow rate ≤15 mL/min

Wash: 3 mL 5 % MeOH / H₂O

Elute: 3 mL MeOH / 6 mL methyl *tert*-butyl ether

Reconstitute: Evaporate to near dry at 30 °C, reconstitute to 1 mL with acetonitrile

3. HPLC method

Column: Inspire™ 5 μm C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: A: H₂O, B: MeCN

Flow Rate: 1.0 mL/min

Temperature: 30 °C

Detection: UV 230 nm


Injection Volume: 20 μL

Gradient:

Time / Min.	0	10	15	23	24	33
A	50	10	0	0	50	50
B	50	90	100	100	50	50

4. Recovery

Compounds	Spike Level (μg/L)	Recovery (%)	RSD (%) (n = 3)
DMP	2	110.3	5.6
	10	90.9	3.8
DEP	2	99.4	2.9
	10	88.9	1.3
DPrP	2	98.7	1.5
	10	89.1	1.0
BBP	2	82.6	1.5
	10	76.3	3.0
DBP	2	98.4	1.6
	10	97.1	2.2
DPP	2	74.7	6.4
	10	68.3	5.6
DCHP	2	82.8	1.7
	10	76.2	5.8
DHP	2	70.4	3.0
	10	69.3	3.8
DEHP	2	74.3	1.9
	10	71.9	2.5

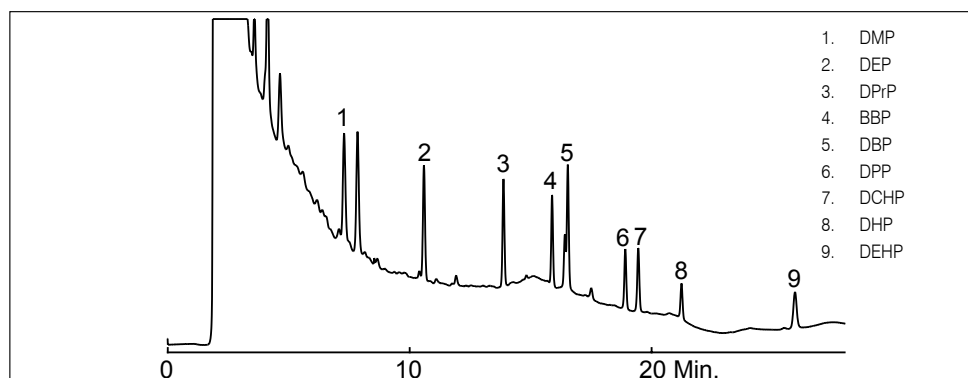

Chromatography of PAEs - spiked PAEs in water (2 μg/L)

Determination of Tetracyclines in Serum

1. Scope of application

Used for determination oxytetracycline, tetracycline and chlortetracycline in human and animal serum

2. Sample preparation

2 mL serum, add 40 μ L H₃PO₄

3. Sample purification

ProElut™ PLS 60 mg / 3 mL (Cat#68003)

Condition: 3 mL MeOH / 3 mL H₂O

Load: 2 mL sample

Wash: 3 mL 5 % MeOH in H₂O

Elute: 3 mL MeOH

Reconstitute: Evaporate to near dry at 30 °C, reconstitute to 1 mL with mobile phase

4. HPLC method

Column: Inspire™ 5 μ m C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: MeOH:MeCN:10 mM oxalic acid in H₂O = 15:15:70

Flow Rate: 1.0 mL/min


Temperature: 30 °C

Detection: UV 365 nm

Injection Volume: 20 μ L

5. Recovery

Compounds	Spike Level (mg/L)	Recovery (%)	RSD (%) (n = 3)
Oxytetracycline	0.5	92.6	2.1
	2.0	95.8	0.5
Tetracycline	0.5	97.3	2.4
	2.0	95.8	0.8
Chlortetracycline	0.5	102.70	3.1
	2.0	97.3	1.4

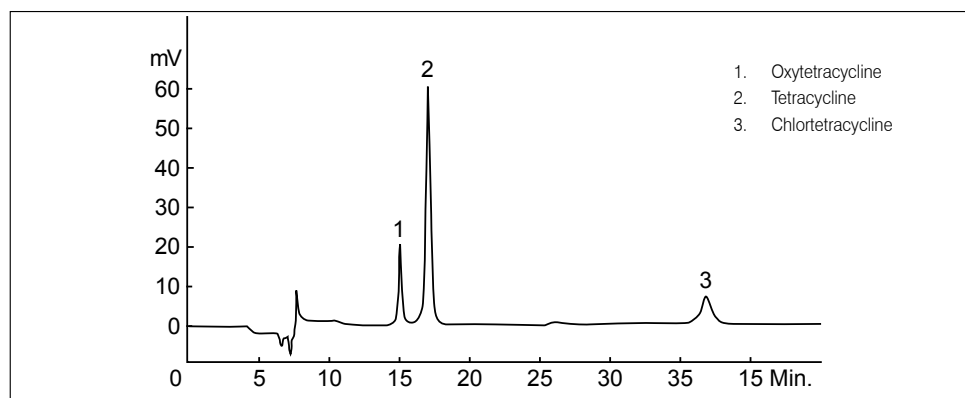

Chromatogram of tetracyclines - spiked tetracyclines in serum (0.5 mg/L)

Others

Determination of Migration of Bisphenol A (BPA) from Plastic Baby Bottles

1. Scope of application

Used for determination of migration of bisphenol A (BPA) from plastic baby bottles

2. Sample purification

Wash bottles, dry completely. Add distilled water so that each 8 m² of plastic contact area corresponds to 10 mL of simulant immersion. Sealed with aluminum foil, place in oven at 100 °C for 1 h. Cool to room temperature, then transfer to glass bottles, and seal until detection.

3. Sample purification

ProElut™ PLS GLASS 200 mg / 6 mL (Cat#68012G)

Condition: 6 mL MeOH / 6 mL H₂O

Load: Adding sample

Wash: 6 mL 5 % MeOH in H₂O

Elute: 6 mL MeOH

Reconstitute: Evaporate to near dry at 40 °C, reconstitute to 1 mL with mobile phase

4. HPLC method

Column: Inspire™ 5 μm C18, 250 x 4.6 mm (Cat#81006)

Mobile Phase: MeCN:2% CH₃COOH in H₂O = 40:60

Flow Rate: 1.0 mL/min


Temperature: 30 °C

Detection: FLD Ex: 227 nm, Em: 313 nm

Injection Volume: 20 μL

5. Recovery

Compounds	Spike Level (μg/L)	Recovery (%)	RSD (%) (n = 3)
Bisphenol A	0.4	94.54	5.1
	1.6	97.30	3.7

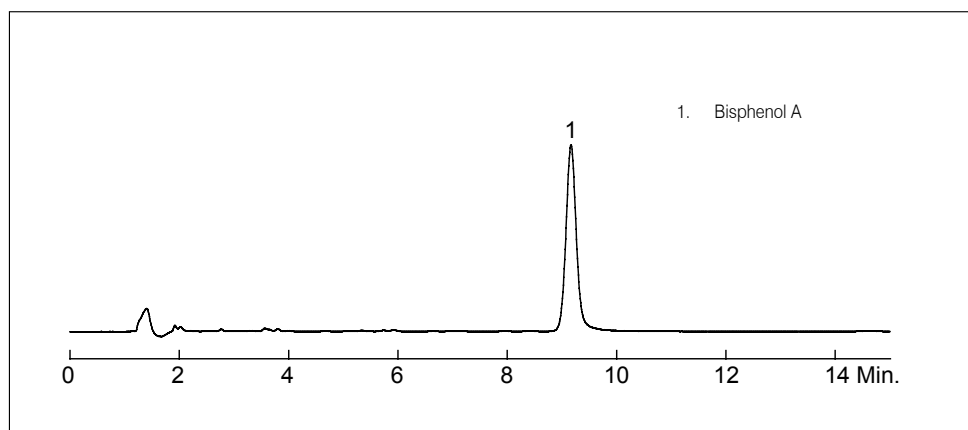

Chromatography of bisphenol A - immersion concentration (0.4 μg/L)

HPLC

A

Acebutolol	10, 17, 21, 134
Acenaphthene	6
Acesulfame K	147, 148
Acetaldehyde-DNPH	143
Acetaminophen	7, 131
Acetanilide	7, 34
Acetic acid	28, 144, 145
Acetone-DNPH	143
Acetophenone	5, 15, 32
Acetylacetone	8
Acetylsalicylic acid	7, 12, 14, 19, 34, 131, 141
Acid orange II	143
Acid red 2G	143
Acid yellow 36	143
Acrolein-DNPH	143
Adenine	34
ADP	44
Alicyclic acid	14
Aloe emodin	54
Alprazolam	27, 44, 139
Alprenolol	10, 21, 38, 134
Amaranth	143
<i>p</i> -Aminobenzoic acid	12, 14, 19, 131, 141, 146, 147
Amitriptyline	6, 11, 18, 24, 25, 37, 45, 50, 139, 140
Amoxicillin	138
AMP	44
Ampicillin	138
Amylbenzene	5
Ancy red	143
Aniline	8, 15, 16, 23
<i>L</i> -Ascorbic acid	7, 12, 19, 36, 40, 131, 140, 141
Aspartame	23, 147, 148
ATP	44
Auramine	143
Azorubine	143

B

Basic orange	143
BBP	146
Benzaldehyde-DNPH	143
Benzene	8, 16, 22, 33
Benzoic acid	14, 131, 141, 142
Benzoyl peroxide	142
Berberine	131
Betamethasone	16
BHA	149
BHT	149
Bibenzyl	39
Bisoprolol	38
Bovine insulin	52
Brilliant black	143
Brilliant blue	143
Brompheniramine	24, 133
Butylbenzene	5
Butyl paraben	6, 9, 39, 145, 146
Butyraldehyde-DNPH	143

C

Caffeic acid	29, 138
Caffeine	5
Capsaicin	56
Carbadox	13, 19, 26, 132
Carmine	143
Catechin	29, 138
Catechol	49, 143
Cefaclor	26, 41, 42, 43, 135, 136, 137
Cefadroxil	26, 41, 42, 43, 135, 136, 137
Cefazolin	26, 41, 42, 43, 135, 136, 137
Cefoxitin	26, 41, 43, 135, 136, 137
Cefradine	26, 41, 43, 135, 136, 137
Ceftazidime	26, 41, 42, 43, 135, 136, 137
Cefuroxime	26, 41, 43, 136
Cephalexin	26, 41, 42, 43, 135, 136, 137
Chlorbenzuron	142
Chlorfluazuron	142
<i>p</i> -Chlorobenzoic acid	12, 147
4-Chloro-3-methylphenol	46, 146, 150
2-Chlorophenol	46, 146, 150
4-Chlorophenol	46, 146
Chlorpheniramine	24, 54, 133
Chrysophanol	54
Cimetidine	11, 131, 132

Ciprofloxacin	139
Citric acid	28, 144, 145
Citrulline	36
Clomipramine	11, 18, 24, 44, 50, 139, 140
Clonazepam	27, 44, 139
Cloxacillin	138
CMP	44
Codeine	6
Cortisone	23, 35, 150
Cortisone 21-acetate	16
<i>p</i> -Coumaric acid	29, 138
Crotonaldehyde-DNPH	143
CTP	44
Cytochrome C	52, 149
Cytosine	34

D

2,4-D	29, 143
Dalapon	29, 143
DBP	146
DEHP	146
Desipramine	11, 24, 25, 37, 140
Dexamethasone	14, 35, 150
Dextromethorphan	34
Dextromethorphan hydrobromide	54
Diazepam	27, 44, 139
2,4-Dichlorophenol	46, 146, 150
Diclofenac	35, 133
Dicloxacillin	138
DIDP	146
Difloxacin	139
Diflubenzuron	142
Dihydrocapsaicin	56
<i>N,N</i> -Dimethylaniline	15, 23, 39
2,4-Dimethylphenol	150
2,5-Dimethylresorcinol	49, 143
1,3-Dimethyluric acid	40, 142
1,7-Dimethylxanthine	40, 142
2,4-Dinitrophenol	150
DINP	146
Dioctyl phthalate	23
Diphenhydramine	6, 24, 34, 59, 133
Dipropyl phthalate	6
Diuron	144
DNOP	146
DNPH	143
Dopamine	9, 48, 135
Doxepin	11, 18, 24, 25, 44, 50, 139, 140
Doxylamine	7, 24, 34, 133

E

Emodin	54
Enrofloxacin	139
Epinephrine	9, 48, 135
Erythrosine	143
Estazolam	139
Ethylbenzene	15, 23, 39, 45
Ethyl benzoate	15, 23, 57
Ethyl paraben	9, 39, 145, 146

F

Famotidine	11, 131, 132
Fenoprofen	13, 35, 133
Fenuron	144
Flufenoxuron	142
Flumequine	139
Flurbiprofen	13, 35, 133
Formaldehyde-DNPH	143
Fumaric acid	28, 144, 146
Furazolidone	13, 19, 26, 132

G

Gallic acid	29, 138
Gatifloxacin	139
GDP	44
GMP	44
GTP	44

H

Hexaflumuron	142
Hexaldehyde-DNPH	143
Homovanillic acid	12, 18, 19, 59, 131, 141, 146, 147
Human insulin	52
Hydrastine	131
Hydrocortisone 21-acetate	14, 35, 150
11- α -Hydroprogesterone	14, 16, 150
<i>p</i> -Hydroxybenzoic acid	34
<i>o</i> -Hydroxyhippuric acid	59

11- α -Hydroxyprogesterone	14, 16, 150
-----------------------------------	-------------

I

Ibuprofen	13, 35, 133
Imipramine	24, 25, 37, 50
Indigotin	143
Insulin	52, 149
Ionox 100	149
Isovaleraldehyde-DNPH	143

K, L

Ketoprofen	13, 35, 133
Labeltolol	10, 17, 21, 38, 60, 134
Lactic acid	28, 144, 145
Lauryl gallate	149
Linoleic acid	148
Linolenic acid	148
Linuron	144
Lissamine green B	143
Lle-Val-Pro-Phe-Lyl-Pro-Leu-Thr-Amide	52
Lysozymes	52, 149

M

Maleic acid	24, 34, 133
Malic acid	28, 144, 145
Marbofloxacin	139
Melamine	144
Methionine	36
Methoxyfenozide	142
Methyl benzoate	5, 15, 32, 57
3-Methylcatechol	49, 143
4-Methylcatechol	49, 143
Methyl paraben	9, 39, 145, 146
2-Methylresorcinol	49, 143
1-Methyluric acid	40, 142
3-Methylxanthine	40, 142
7-Methylxanthine	40, 142
Metoprolol	10, 17, 21, 38, 60, 134
Monuron	144
Myricetin	29, 138

N

Nadolol	10, 17, 21, 38, 60, 134
Nalidixic acid	59, 139
Naphazoline hydrochloride	54
Naphthalene	5, 6, 8, 15, 32
NDGA	149
<i>N</i> -Formyl-Nle-Leu-Phe-Nle-Tyr-Lys	52
Nicotinamide	7, 36, 40, 140
<i>p</i> -Nitrobenzoic acid	12, 18, 146, 147
2-Nitrobenzyl alcohol	56
4-Nitrobenzyl alcohol	56
4-Nitrocatechol	49, 143
1-Nitronaphthalene	8
2-Nitrophenol	46, 146, 150
4-Nitrophenol	46, 146, 150
Nitrozepam	27, 139
Nizatidine	11, 131, 132
Norclozapine	59, 139, 140
Nordoxepin	24, 25, 27, 50
Norepinephrine	9, 48, 135
Norfloroxacin	139
Nortriptyline	6, 11, 18, 24, 25, 27, 37, 50, 139, 140

O

Octyl gallate	149
Ofloxacin	139
Oleic acid	148
Orotic acid	36, 40
Oxacillin	138
Oxalic acid	28, 144, 145
Oxazepam	27, 139
Oxolinic acid	13, 19, 26, 132, 139

P, Q

Pazufloxacin	139
Penicillin G	138
Pentachlorophenol	150
Phenacetin	13, 35, 133
Pheniramine	24, 133
Phenol	5, 8, 15, 16, 22, 23, 33, 46, 47, 146, 150
Physcion	54
Pindolol	10, 17, 21, 38, 60, 134
Piperacilin	138
Porcine insulin	52
Prednisolone	14, 16, 35, 150
Prednisone	14, 16, 35, 150
Procainamide	34
Propranolol	10, 17, 21, 38, 60, 134

Compound Index for HPLC / GC

Propylbenzene39
 Propyl gallate149
 Propyl paraben9, 39, 145, 146
 Protriptyline18, 50, 139
 Pseudoephedrine hydrochloride54
 Pyridine6, 22, 33, 47
 Pyridoxal7, 36, 40, 140
 Pyridoxamine7, 36, 40, 140
 Pyridoxol36, 40, 140
 Quercitrin29, 138
 Quinine6, 131
 Quinizarin45

R
 Ranitidine11, 131, 132
 Reserpine23
 Resorcinol49, 143
 Rhein54
 Riphenylene5

S
 Salicylic acid7, 12, 18, 19, 59, 141, 147
 Sarafloxacin139
 Sodium saccharin147, 148
 Sorbic acid12, 18, 19, 59, 131, 141, 142, 146, 147
 Sparfloxacin139
trans-Stilbene39
 Succinic acid28, 144, 145
 Sulfadimethoxine13, 19, 132
 Sulfamerazine13, 19, 26, 132
 Sulfamethazine19, 132
 Sulfamethoxazole13, 19, 26, 132
 Sulfamethoxyipyridazine13, 19, 26, 132
 Sulfanilamide13, 19, 26, 132
 Sulfapyridine26, 132
 Sulfaquinoxaline13, 132
 Sulfisoxazole13, 19, 26, 132
 Sunset yellow143

T
 2,4,5-T29, 143
 Tartaric acid28, 144, 145
 Tartrazine143
 TBHQ149
 Tebufenozide142
 Teflubenzuron142
o-Terphenyl5
 THBP149
 Theobromine40, 131, 142
 Theophylline40, 142
 Thiamine36, 40
 Thiamphenicol26, 132
 Thiourea15, 23, 34
 α -Tocopherol36
 γ -Tocopherol36
 δ -Tocopherol36
 Tolmetin13, 35, 133
m-Tolualdehyde-DNPH143
o-Tolualdehyde-DNPH143
p-Tolualdehyde-DNPH143
o-Toluamide34
 Toluene5, 8, 15, 16, 23, 32, 45, 56
p-Toluic acid18, 146, 147
o,m,p-Toluidine15, 23
 Triazolam27, 44, 139
 2,4,6-Trichlorophenol46, 146, 150
 Triflumuron142
 Trimipramine11, 18, 24, 25, 27, 37, 44, 50, 139, 140
 Tyrosine36

U
 Uracil5, 6, 8, 15, 16, 22, 32, 33, 45
 Uric acid40, 142
 Uridine34

V, X
 Valeraldehyde-DNPH143
 Valine36
 Vanillic acid29, 138
 Verapamil59
 Xanthine40, 142

GC

A

Acenaphthene69, 99, 156, 157, 159
 Acenaphthene-d10158, 159
 Acenaphthylene69, 99, 156, 157, 159
 Acetal204
 Acetaldehyde188, 189, 192, 203, 204
 Acetamide193, 195, 197
 Acetic acid192, 200, 204
 Acetochlor158
 Acetoin204
 Acetone187, 192, 199, 203, 204, 211, 212
 Acetonitrile192, 211, 212
 Acetophenone159, 174, 206
 Acetopromazine208
 Acetylene82, 169, 170, 171, 172, 173
n-Acetyl galactose amine207
n-Acetyl glucose amine207
 Acetyl tributyl citrate193, 195, 197
 Acrylonitrile191, 199
 Adiponitrile184
 Air168, 189
 Aldrin162, 164
 Alkylthiophenes176
 Allyl alcohol193, 195, 197
 Allylmercaptan176
 Alprazolam208
 Ametryne165
 6-Aminocapronitrile184
 2-Amino-4,6-dinitrotoluene167
 4-Amino-2,6-dinitrotoluene167
 Aminoethylethanolamine184
 Aminoethylpiperazine184
 Aminomethylcyclopentylamine184
 2-Amino-4-nitrotoluene167
 2-Amino-6-nitrotoluene167
 Amitriptyline208
 Amobarbital209
 Amphetamine209
 Amyl alcohol199
tert-Amyl ether175
 5 α -Androstan-17 β -ol-3-one210
 5-Androstene-3 β ,17 β -diol210
 Aniline159, 185
 Anisole192
 Anisoxide155
 Anthracene66, 69, 156, 157, 159
 Aprobital209
 Arabinitol207
 Aramite159
 Argon84, 168, 169
 Aspon162
 Atraton165
 Atrazine163, 165
 Azinphos-ethyl162
 Azinphos-methyl162
 Azobenzene158, 159

B
 Balan163
 Barbitol209
 BBP160
 BEEP160
 Benzaldehyde174, 188, 189, 193, 195, 197, 204, 206
 Benzene87, 97, 98, 154, 155, 166, 174, 175,179, 180, 181, 192, 193, 195, 197, 211, 212
 Benzeneacetalddehyde206
 Benzenepropanoic acid ethyl ester204
 Benzidine159, 161
 Benzo[a]anthracene69, 99, 156, 157, 159
 Benzo[a]pyrene69, 99, 156, 157, 159
 Benzo[b]fluoranthene69, 99, 156, 157, 159
 Benzo[ghi]perylene69, 99, 156, 157, 159
 Benzoic acid159, 206
 Benzo[j]fluoranthene99, 156
 Benzo[k]fluoranthene69, 99, 156, 157, 159
 Benzothioephene176
 Benzotrifluoride97, 166
 1,2-Benzophenanthrene69, 156, 157
 Benzphetamine208, 209
 Benzyl alcohol159, 174, 193, 195, 197
 Benzyl butyl phthalate159
 Benzyl ether190, 193, 195, 197

Benzyl ethyl phthalate167
 Benzyl salicylate206
 α -Bergamotene205
trans- α -Bergamotene203
 BHA203, 206
 α -BHC162, 164
 β -BHC162, 164
 γ -BHC162, 164
 δ -BHC162, 164
 BHT206
 Bibenzyl182
 β -Bisabolene203
 BMPP160
 Bolasterone210
 Bolstar162
 Borneol205
 β -Bourbonene205
 Brassicasterol207
 Bromacil163
 Bromazepam208
 Bromobenzene97, 155, 166
 2-Bromobutane193, 195, 197
 Bromochloroacetone166
 Bromochloromethane166
 Bromodichloromethane97, 155, 166
 4-Bromofluorobenzene97, 166
 Bromoform97, 155, 166
 Bromomethane97, 154, 155, 166
 4-Bromophenyl phenyl ether159
 Brompheniramine210
 Bupivacaine208
 1,3-Butadiene82, 170, 171, 172, 173, 191
 Butalbital209
 1,4-Butanediol186, 188, 193, 195, 197
L-2,3-Butanediol204
meso-2,3-Butanediol204
iso-Butane179
n-Butane83, 87, 170, 171, 172, 173, 179
 Butanethiol176
n-Butanoic acid204
 1-Butanol (*n*-Butanol)88, 174, 175, 186,187, 192, 204, 206, 211
 2-Butanol (*sec*-Butanol)175, 186, 192, 212
tert-Butanol88, 174, 175, 186, 212
 2-Butanone192, 204
 2-Buten-1-ol193, 195, 197
 3-Buten-2-ol186
 Butenal188
 2-Butenal189
 Butene191
 1-Butene82, 83, 170, 171, 172, 173
cis-2-Butene82, 170, 171, 172, 173
trans-2-Butene82, 83, 170, 171, 172, 173
 Butoxyethanol193, 195, 197
 Butyl acetate98, 154, 191, 192, 193, 195, 197
n-Butyl acetate199
n-Butyl acrylate199
 Butyl alcohol191
n-Butyl alcohol187, 199
sec-Butyl alcohol204
tert-Butyl alcohol175
sec-Butylamine95, 183
tert-Butylamine95, 183
 Butylbenzene180, 182
n-Butylbenzene155
sec-Butylbenzene155
tert-Butylbenzene155, 182
 Butyl butanoate193, 195, 197
 Butylbutyrate191
 Butyl carbitol187
 Butyl cellosolve187
 1,3-Butylene glycol187
 1,4-Butylene glycol187
 Butyl ether190, 193, 195, 197, 206
n-Butyl ether191
 Butyl hexanoate204
n-Butyl methacrylate191
sec-Butyl methyl ether175
di-n-Butylphthalate159
 Butyl sulfide176
 Butyraldehyde188, 190
n-Butyric acid200
 Butyrolactone189

C			
C3 oxide	174	C22:5n3	100, 201, 202
C4:0 (butyric acid)	200	C22:5n6	100, 202
C4s	175	C22:6n3	100, 201, 202
C5	90, 178	C23	179
C6	90, 178	C23:0 (IS)	100, 202
C6:0 (caproic acid)	200	C24	90, 178, 179
C6:0 (methyl caproate)	201	C24:1	100, 202
C7	90, 178, 179	C24:1n9	201
C8	90, 178, 179	C25	179
C8:0 (caprylic acid)	200	C26	179
C8:0 (methyl caprylate)	201	C28	90, 178, 179
C9	90, 178, 179	C30	179
C9:0 (methyl nonanoate)	201	C32	90, 178, 179
C10	90, 178, 179	C34	179
C10:0 (capric acid)	200	C36	90, 178, 179
C10:0 (methyl caprate)	201	C38	179
C11	90, 178, 179	C40	90, 178, 179
C12	90, 178, 179	C42	179
C12:0 (lauric acid)	200	C44	90, 178
C12:0 (methyl laurate)	201	δ -Cadenene	205
C13	179	Caffeine	208, 209
C14	90, 178, 179	Campesterol	207
C14:0	100, 201, 202	Camphene	203
C14:0 (methyl myristate)	201	Caproic acid	200
C14:0 (myristic acid)	200	Capryl alcohol	204
C15	179	Carbamazepine	209
C15:0	100, 202	Carbofenthoion	162
C16	90, 178, 179	Carbon dioxide	168
C16:0	100, 201, 202	Carbon disulfide	176, 199
C16:0 (methyl palmitate)	201	Carbon monoxide	168, 169
C16:0 (palmitic acid)	200	Carbon tetrachloride	154, 166, 192, 211
C16:1	100, 202	Carbonyl sulfide	176
C16:1 (methyl palmitoleate)	201	Carisoprodal	209
C16:1n7	201	<i>d/l</i> Carveol	203
C16:2	100, 202	Carvone	203
C16:4	100, 202	β -Caryophyllene	203, 205
C17	179	Cathinone	209
C17:0	100, 202	Cellosolve acetate	199
C17:1	100, 202	Chloral hydrate	166
C18	90, 178, 179	Chlorbenzilate	159
C18:0	100, 201, 202	α -Chlordane	162, 164
C18:0 (methyl stearate)	80, 200, 201	γ -Chlordane	162, 164
C18:0 (stearic acid)	200	Chlorfenvinphos	162
C18:1 (methyl elaidate (<i>trans</i> -9))	80, 200	Chlorneb	162
C18:1 (methyl oleate)	201	4-Chloroaniline	159
C18:1 (methyl oleate (<i>cis</i> -9))	80, 200	Chlorobenzene	97, 154, 155, 166, 192, 211
C18:1 (methyl petroselaidate (<i>trans</i> -6))	80, 200	Chlorobenzilate	162
C18:1 (methyl petroselinate (<i>cis</i> -6))	80, 200	Chlorobromomethane	97, 155
C18:1 (methyl transvaccenate (<i>trans</i> -11))	80, 200	Chlorodibromomethane	97
C18:1 (methyl vaccenate (<i>cis</i> -11))	80, 200	Chlorodifluoromethane (CFC-22)	86, 170
C18:1n7	201	Chloroethane	97, 154, 155, 166, 192
C18:1n9	201, 202	<i>bis</i> (2-Chloroethoxy)methane	159
C18:1 (oleate)	100, 202	<i>bis</i> (2-Chloroethyl)ether	159
C18:1 (oleic acid)	200	Chloroform	97, 154, 155, 166, 192, 211, 212
C18:1 (vaccenate)	100, 202	1-Chlorohexane	97, 166
C18:2 (linoleic acid)	200	<i>bis</i> (2-Chloroisopropyl)ether	159
C18:2 (methyl linoleate)	201	Chloromethane	154, 155, 192
C18:2 (methyl linoleate (<i>cis</i> -9,12))	80, 200	4-Chloro-3-methylphenol	158, 159, 161
C18:2n6	201, 202	2-Chloronaphthalene	159, 160
C18:2n6 <i>cis</i>	100, 202	Chloropentafluoroethane (CFC-115)	86, 170
C18:3 (linolenic acid)	200	1-Chloropentane	193, 195, 197
C18:3 (methyl linolenate)	201	2-Chlorophenol	93, 158, 159, 161, 185
C18:3n3	100, 201, 202	2-Chlorophenol-d4	159
C18:3n6	201, 202	2-Chlorophenol-3,4,5,6-d4	158
C18:4n3	100, 201, 202	4-Chlorophenyl phenyl ether	159
C18:4n6	100, 202	Chloropicrin	166
C19	179	2-Chloropropane	192
C20	90, 178, 179	3-Chloropropane	154
C20:0	100, 202	4-Chlorotestosterone-17-acetate	210
C20:0 (arachidic acid)	200	Chlorothalnil	162
C20:1n7	100, 202	<i>m</i> -Chlorotoluene	97, 166
C20:1n9	100, 201, 202	<i>o</i> -Chlorotoluene	97, 155, 166, 193, 195, 197
C20:2n6	201	<i>p</i> -Chlorotoluene	97, 155, 166
C20:3n6	201	Chlorpheniramine	210
C20:4n3	100, 202	Chlorpromazine	208
C20:4n6	100, 201, 202	Chlorpyrifos	162
C20:5n3	100, 201, 202	Chlorpyrifos methyl	162
C21:5n3	100, 202	5- α -Cholestane	207
C22	179	Cholesterol	207
C22:0 (behenic acid)	200	Chrysene	99, 156, 158, 159
C22:1n7	100, 202	Chrysene-d12	159
C22:4n6	201	1,8-Cineole	203, 205
		Cinnamic aldehyde	206
		Cinnamyl acetate	206
		Cinnamyl alcohol	206
		Citronellal	203, 205
		β -Citronellol	205
		Clonazepam	208
		Codeine	208, 210
		Coprostanone	207
		Coprosterol	207
		Cotinine	208
		Coumaphos	162
		<i>o</i> -Cresol	182, 193, 195, 197
		<i>p</i> -Cresol	182
		<i>tri-o</i> -Cresyl phosphate	162
		Crotoxyphos	162
		Cyanazine	158
		Cyclohexane	184, 211, 212
		Cyclohexanol	188
		Cyclohexanone	199
		Cyclohexyl phthalate	167
		Cyclopentanone	193, 195, 197
		Cyclopropanone	193, 195, 197
		Cyclopropane	171, 172, 173
		<i>p</i> -Cymene	182, 203, 205
		D	
		Dalapon	165
		Dalapon methyl ester	165
		DBEP	160
		2,4-DB methyl ester	165
		DBOB (IS)	165
		DBP	160
		DCAA (SS)	165
		DCB	162
		DCHP	160
		DCCA	162
		4,4'-DDD	162, 164
		4,4'-DDE	164
		4,4'-DDT	162, 164
		Decachlorobiphenyl	164
		Decahydronaphthalene	193, 195, 197
		<i>cis</i> -Decahydronaphthalene	182
		<i>trans</i> -Decahydronaphthalene	182
		Decanal	188, 189, 193, 195, 197, 203, 206
		Decane	186
		<i>n</i> -Decane	87, 179
		Decanoic acid	204
		1-Decanol (<i>n</i> -Decyl alcohol)	185, 186, 193, 195, 197
		2-Decanol	193, 195, 197
		3-Decanol	204
		<i>n</i> -Decyl chloride	185
		<i>n</i> -Decyl- <i>N,N</i> -dimethylamine	185
		DEHP	160
		1-Dehydro-17 α -methyltestosterone	210
		1-Dehydrotestosterone	210
		1-Dehydrotestosterone benzoate	210
		1-Dehydrotestosterone undecylenate	210
		Demeton-O	162
		Demeton-S	162
		Deoxyglucitol	207
		Deoxyribitol	207
		DEP	160
		Dextromethorphan	208, 210
		Diallyl disulfide	176
		Diallylsulfide	176
		1,4-Diaminobutane	184
		1,2-Diaminocyclohexane	184
		1,5-Diamino-2-methylpentane	184
		2,6-Diamino-4-nitrotoluene	167
		2,3-Diaminotoluene	167
		2,4-Diaminotoluene	167
		2,6-Diaminotoluene	167
		Diazepam	208
		Diazinon	158, 162
		Dibenzo[<i>a,h</i>]acridine	99, 156
		Dibenzo[<i>a,i</i>]acridine	99, 156
		Dibenzo[<i>a,h</i>]anthracene	69, 99, 156, 157, 159
		7H-Dibenzo[<i>c,g</i>]carbazole	99, 156
		Dibenzo[<i>a,e</i>]pyrene	99, 156
		Dibenzo[<i>a,h</i>]pyrene	156
		Dibenzo[<i>a,i</i>]pyrene	99, 156
		Dibenzofuran	159
		Dibenzyl	193, 195, 197
		DIBP	160
		Dibromoacetonitrile	166

Compound Index for GC

Dibromochloromethane	155, 166
1,2-Dibromo-3-chloropropane	97, 155, 166
1,2-Dibromoethane	97, 154, 155, 166
Dibromomethane	97, 155, 166
Dibromooctafluorobiphenyl methyl ester	165
Dibutyl phthalate	167
Dibutyltin	165, 167
Dicamba	165
Dicamba methyl ester	165
Dichloroacetonitrile	166
1,2-Dichlorobenzene	97, 154, 155, 159, 160, 166
1,3-Dichlorobenzene	97, 154, 155, 159, 160, 166
1,4-Dichlorobenzene	97, 154, 155, 159, 160, 166
1,2-Dichlorobenzene-d4	159
1,4-Dichlorobenzene-d4	159
3,3'-Dichlorobenzidine	159, 161
1,4-Dichlorobutane	193, 195, 197
Dichlorodifluoromethane	154, 155
Dichlorodifluoromethane (CFC-12)	86, 170
1,1-Dichloroethane	97, 154, 155, 166, 192, 211
1,2-Dichloroethane	97, 154, 155, 166, 192, 211
<i>cis</i> -1,2-Dichloroethene	154, 192, 211
<i>trans</i> -1,2-Dichloroethene	192
1,1-Dichloroethylene	97, 166
<i>cis</i> -1,2-Dichloroethylene	97, 155, 166
<i>trans</i> -1,2-Dichloroethylene	97, 155, 166
Dichlorofenthion	162
Dichloromethane	97, 166, 211
2,4-Dichlorophenol	158, 159, 161
2,6-Dichlorophenol	159
2,4-Dichlorophenylacetic acid methyl ester	165
1,1-Dichloropropane	155
1,2-Dichloropropane	154, 155, 166
1,3-Dichloropropane	97, 155, 166
2,2-Dichloropropane	97, 155, 166
1,1-Dichloro-2-propanone	166
1,1-Dichloropropene	97, 155
<i>cis</i> -1,3-Dichloropropene	97, 154, 155
<i>trans</i> -1,3-Dichloropropene	154, 155
<i>cis</i> -1,3-Dichloropropylene	166
<i>trans</i> -1,3-Dichloropropylene	166
1,2-Dichlorotetrafluoroethane	154
Dichloroprop	165
Dichlorvos	162
Dicrotophos	162
Dicyclohexylamine	193, 195, 197
Dieldrin	162, 164
Diethanolamine	94, 184
Diethoxy isopentane	204
Diethoxy-3-methylbutane	204
1,1-Diethoxypropane	192
Diethylamine	93, 95, 96, 183, 185, 212
Diethylbenzene	193, 195, 197
1,2-Diethylbenzene (<i>o</i> -Diethylbenzene)	174, 180, 181
1,3-Diethylbenzene (<i>m</i> -Diethylbenzene)	174, 181
1,4-Diethylbenzene (<i>p</i> -Diethylbenzene)	74, 180, 181
Diethylene glycol	187, 188
Diethylenetriamine	93, 184, 185
Diethyl ether	192, 211
Diethylhydroxylamine	191
Diethylmethylamine	92, 183
Diethyl phthalate	159, 167, 193, 195, 197
Diethylpropion	209
Diheptyl phthalate	167
Dihexyl phthalate	167
Diisobutylene	175
Diisopropylbenzene	182
Dimethoate	162
Dimethoxyethane	175
1,2-Dimethoxyethane	192, 211
Dimethoxymethane	188, 189
2,2-Dimethoxypropane	192
2,3-Dimethylheptane	87, 179
2,6-Dimethyl-4-heptanone	193, 195, 197
2,3-Dimethylhexane	87, 179
1,3-Dimethyl-2-nitrobenzene	158
1,2-Dimethyl-3-nitrobenzene	158
2,2-Dimethyl-1-propanol (Neopentanol)	186
2,4-Dimethyl-3-pentanone	189
Dimethylacetamide	193, 195, 197
<i>N,N</i> -Dimethylacetamide	192, 211
Dimethylamine	92, 95, 183
2,6-Dimethylaniline	93, 185
Dimethylbenzothiofenenes	176
Dimethylchlorosilane	191
Dimethyldichlorosilane	191
Dimethylether	175
Dimethylethylamine	183
Dimethyl formamide	192, 193, 195, 197, 212
2,4-Dimethylphenol	158, 161
2,4-Dimethylphenol-3,5,6-d3	158
Dimethyl phthalate	159, 167
Dimethyl sulfoxide	192
1,3-Dinitrobenzene	159, 167
1,4-Dinitrobenzene	167
2,2'-Dinitrobiphenyl	167
4,6-Dinitro-2-methylphenol	159
1,3-Dinitronaphthalene	167
2,4-Dinitrophenol	158, 159, 161
2,3-Dinitrotoluene	167
2,4-Dinitrotoluene	159, 167
2,6-Dinitrotoluene	159, 167
3,4-Dinitrotoluene	167
Dinoseb	159, 165
Dinoseb methyl ester	165
Diocetyl phthalate	167
1,4-Dioxane	190, 192, 211, 212
Dioxathion	162
1,3-Dioxolane	190
DIPE	175
Dipentene	193, 195, 197
Dipentyl phthalate	167
Diphenhydramine	208, 210
Diphenylamine	159
Diphenylhydantoin	209
Diphenyl sulfone	193, 195, 197
Dipropylene glycol	193, 195, 197
Dipropyl sulfide	176
Disulfoton	158, 162
DMEP	160
2,4-D methyl ester	165
DMF	211
DMP	160
DNHP	160
DNNP	160
DNOP	160
Dodecanal	193, 195, 197
Dodecane	186, 193, 195, 197
<i>n</i> -Dodecane	87, 88, 174, 179, 181
Dodecanoic acid	204
1-Dodecanol (<i>n</i> -Dodecyl alcohol)	185, 186, 193, 195, 197
2-Dodecanone	193, 195, 197
<i>n</i> -Dodecyl chloride	185
<i>n</i> -Dodecyl- <i>N,N</i> -dimethylamine	185
DOP	160
Doxylamine	210
DPP	160
Dual	163
E	
Eicosane	193, 195, 197
γ -Elemene	203, 205
Endosulfan	164
Endosulfan I	162, 164
Endosulfan II	162
Endosulfan sulfate	162, 164
Endrin	162, 164
Endrin aldehyde	162, 164
Endrin ketone	164
Ephedrine	209, 210
EPN	162
Eptam	163
Ethanal	188
Ethane	82, 83, 169, 170, 171, 172, 173
Ethanethiol	176
Ethanol	88, 174, 175, 186, 187, 192, 199, 203, 204, 211, 212
Ethene	171
Ether	212
Ethion	162
Ethoprop	162
Ethosuximide	209
2-Ethoxy butane	204
2-Ethoxyethanol	186, 192
2-Ethoxy ethyl ether	190
Ethyl acetate	187, 192, 199, 203, 204, 211, 212
Ethyl acrylate	190
Ethylamine	95, 183
<i>N</i> -Ethylamphetamine	209
Ethyl amyl ketone	193, 195, 197
Ethylbenzene	87, 97, 98, 154, 155, 166, 174, 179, 180, 181, 182, 191, 192, 206, 211
2-Ethyl-1-butanol	193, 195, 197
Ethyl <i>tert</i> -butyl ether	175
Ethyl butyrate	203, 204, 206
Ethyl caprate	204
Ethyl caproate	204
Ethyl chloroacetate	193, 195, 197
Ethyl decanoate	204
Ethylene	82, 169, 170, 171, 172, 173
Ethylenediamine	184
Ethylene glycol	186, 187, 188, 192, 193, 195, 197
Ethylene oxide	192, 211
Ethyl formate	192, 204
Ethyl heptanoate	204
2-Ethyl-1-hexanol	193, 195, 197
2-Ethylhexyl phthalate	167
<i>bis</i> (2-Ethylhexyl)phthalate	159
Ethyl isobutyrate	204
Ethyl isovalerate	204
Ethyl lactate	204
Ethyl linoleate	204
Ethyl methanesulfonate	159
1-Ethyl-2-methylbenzene	181
Ethyl myristate	204
Ethyl nonanoate	204
Ethyl octanoate	204
Ethyl oleate	204
Ethyl palmitate	204
3-Ethyl-3-pentanol	193, 195, 197
Ethyl propionate	203, 204
Ethyl thioether	176
2-Ethylthiophene	176
Ethyl valerate	204
Etridiazole	162
Eucalyptol	206
Eugenol	205
F	
Famphur	162
Fenfluramine	209
Fenitrothion	162
Fensulfotihion	162
Fenthion	162
Flunitrazepam	208
Fluoranthene	69, 99, 156, 157, 159
Fluorene	69, 99, 156, 157, 159
2-Fluorobiphenyl	159
2-Fluorophenol	159
Fluoxymesterone	210
Flurazepam	208
Fonofos	158
Fonophos	162
Formaldehyde	189, 192
Formamide	192, 193, 195, 197
Formic acid	192
Fucitol	207
2-Furancarboxaldehyde	189
Furfural	188, 203, 204
Furfuryl alcohol	188, 193, 195, 197
G	
Galactitol	207
Geraniol	203
Geraniol	205, 206
Geranyl acetate	203, 205
Germacrene- Δ	205
Glucitol	207
Glucoshepitol	207
Glutethimide	209
Glyceraldehyde	207
Glycerol	187
GOAL	163
Guaifenesin	210
H	
Haloperidol	208
Helium	168, 169
Heptachlor	162, 164
Heptachlor epoxide	162, 164
Heptadecane	193, 195, 197
Heptanal	188, 189

Heptane.....	174, 186, 188, 190, 193, 195, 197, 199, 211, 212
<i>n</i> -Heptane.....	87, 179, 192
Heptanoic acid.....	200, 204
Heptanol.....	193, 195, 197
1-Heptanol.....	186
2-Heptanol.....	204
4-Heptanone.....	189, 206
Hexachlorobenzene.....	159, 160, 162
Hexachlorobutadiene.....	154, 155, 159, 160
1,1,2,3,4,4-Hexachloro-1,2-butadiene.....	97, 166
Hexachlorocyclopentadiene.....	159, 160
Hexachloroethane.....	159, 160, 193, 195, 197
Hexachloropropene.....	159
Hexadecane.....	186
<i>n</i> -Hexadecyl alcohol.....	185
<i>n</i> -Hexadecyl chloride.....	185
<i>n</i> -Hexadecyl- <i>N,N</i> -dimethylamine.....	185
Hexamethylenediamine.....	184
Hexamethyleneimine.....	184
<i>bis</i> -Hexamethylenetriamine.....	184
Hexamethylphosphoramide.....	162
Hexanal.....	188, 189, 206
<i>n</i> -Hexanal.....	203
Hexane.....	173, 186, 192, 199, 203, 211, 212
<i>n</i> -Hexane.....	87, 171, 179, 199, 211
Hexanes.....	82, 170
<i>n</i> -Hexanoic acid.....	204
1-Hexanol (<i>n</i> -Hexanol).....	186, 204
2-Hexanol.....	193, 195, 197
3-Hexanol.....	193, 195, 197
Hexanone.....	192
2-Hexanone.....	192, 211
Hexazinone.....	163
<i>trans</i> -2-Hexenal.....	203
Hexenes.....	170
<i>trans</i> -2-Hexen-1-ol.....	186
4-Hexen-3-one.....	189
Hexyl hexanoate.....	204
HMMA.....	209
Hydrocodone.....	210
Hydrogen.....	84, 169
Hydrogen sulfide.....	176
Hydroxybutanoic acid <i>n</i> -butyl ester.....	191
Hydroxycitronellal.....	206
4-Hydroxy-4-methyl-2-pentanone.....	189
I	
Indane.....	180
Indeno[1,2,3- <i>cd</i>]pyrene.....	99, 156, 157, 159
Inositol.....	207
α -Ionone.....	203
β -Ionone.....	203
Isoamyl acetate.....	192, 204
Isoamyl alcohol.....	192, 204
Isobutanol.....	204
Isobutane.....	82, 83, 87, 170, 171, 172, 173
Isobutanol.....	175
Isobutene.....	171, 173
Isobutyl acetate.....	192
Isobutyl alcohol.....	186, 204
Isobutylene.....	82, 83, 170, 172
Isobutyl isobutyrate.....	191
Isobutyl methacrylate.....	191
Isobutyl phthalate.....	167
Isobutyric acid.....	200, 204
Isodrin.....	159
<i>d</i> -Isomenthone.....	205
Isocitane.....	192
Isopentane.....	82, 170, 171, 172, 173
Isophorone.....	159
Isopropanol.....	175, 184, 187, 211, 212
Isopropyl acetate.....	192, 193, 195, 197, 199
Isopropyl alcohol.....	88, 174, 203
Isopropylamine.....	95, 96, 183, 212
Isopropyl benzene (cumene).....	174, 180, 181, 182, 191, 192, 193, 195, 197
Isopropyl ether.....	192
Isopropyl methacrylate.....	191
<i>p</i> -Isopropyl toluene.....	155
Isosafrole.....	159
Isovaleric acid.....	200, 204
K, L	
Kepon.....	159
Ketamine.....	208
2-Keto-3-deoxyoctanate.....	207
<i>cis</i> -Lactone.....	204
<i>trans</i> -Lactone.....	204
Leptophos.....	162
Lidocaine.....	208
Limonene.....	205, 206
δ -Limonene.....	203
<i>l</i> -Limonene.....	205
<i>trans</i> -Limonene.....	203
<i>cis</i> -Limonene monoxide.....	203
<i>trans</i> -Limonene monoxide.....	203
Linalool.....	203, 205
M	
Malathion.....	162
Mannitol.....	207
MBDB.....	209
MCPA.....	165
MCPP.....	165
MDA.....	209
MDEA.....	209
MDMA.....	209
Medazepam.....	208
Menthofuran.....	205
<i>l</i> -Menthofuran.....	205
neo-Menthol.....	205
<i>l</i> -Menthone.....	205
Menthyl acetate.....	205
Meperidine.....	208
Mephentermine.....	209
Meprobamate.....	209
Merphos.....	162
Merphos oxone.....	162
Mesitylene.....	181
Mesterolone.....	210
Methacrylate.....	191
Methacrylic acid <i>n</i> -butyl ester.....	191
Methadone.....	208
Methamphetamine.....	209
Methane.....	82, 83, 168, 169, 170, 171, 172, 173, 199
Methanol.....	87, 88, 92, 98, 154, 174, 175, 179, 183, 186, 187, 189, 192, 199, 203, 204, 211, 212
Methanthiol.....	176
Methapyrilene.....	210
Methaqualone.....	209
Methcathinone.....	209
Methoxychlor.....	162, 164
2-Methoxyethanol.....	186, 192
1,2- <i>bis</i> -(2-Methoxyethoxy)ethane.....	190, 193, 195, 197
<i>bis</i> -(2-(2-Methoxyethoxy)ethyl)ether.....	190
2-Methoxy ethyl ether.....	190
<i>bis</i> -(2-Methoxy)ethyl ether.....	195, 197
<i>p</i> -Methoxyphenol.....	193, 195, 197
Methyl acetate.....	190, 192
Methylal.....	192
Methylamine.....	95, 183
17 α -Methylandrostan-17 β -ol-3-one.....	210
17 α -Methyl-5-androstene-3 β ,17 β -diol.....	210
α -Methylbenzene.....	182
Methyl benzoate.....	190, 206
Methylbenzothiofenenes.....	176
α -Methylbenzyl alcohol.....	174, 193, 195, 197
2-Methyl-1-butanol.....	187
2-Methyl-2-butanol.....	186
3-Methyl-1-butanol.....	186, 187
2-Methyl-2-butene.....	82, 170
2-Methyl-3-buten-2-ol.....	186
Methyl <i>tert</i> -butyl ether.....	88, 174, 175, 192
2-Methyl butyraldehyde.....	204
3-Methyl butyraldehyde.....	204
Methyl butyrate.....	190
Methyl cellosolve.....	199
3-Methylcholanthrene.....	156, 159
Methyl cyclohexane.....	192, 211
Methyl cyclopentane.....	192
Methyl decanoate.....	190
Methyldichlorosilane.....	191
4-Methyl-2,5-dimethoxyamphetamine.....	209
2-Methyl-4,6-dinitrophenol.....	158, 161
Methyl disulfide.....	176
Methylene chloride.....	154, 155, 192, 193, 195, 197, 203, 211, 212
Methylenedioxyamphetamine.....	209
Methylenedioxyethylamphetamine.....	209
Methylenedioxyethylamphetamine.....	209
Methylethylamine.....	92
1-Methylethylbenzene.....	206
1-Methyl-2-ethylbenzene.....	180
1-Methyl-3-ethylbenzene.....	180
1-Methyl-4-ethylbenzene.....	180
Methyl ethyl ketone.....	199, 211, 212
Methyl formate.....	190
5-Methyl-3-heptanone.....	189
2-Methylhexane.....	87, 179
Methyl hexanoate.....	190, 193, 195, 197
5-Methyl-2-hexanone.....	189
Methyl isopropyl ketone.....	192
Methyl methanesulfonate.....	159
Methyl myristate.....	204
1-Methylnaphthalene.....	99, 156, 159, 180
2-Methylnaphthalene.....	87, 99, 156, 159, 179, 180
Methyl octanoate.....	190
2-Methylpentane.....	192
3-Methylpentane.....	87, 179
2-Methyl-2,4-pentanediol.....	188, 193, 195, 197
2-Methylpentanol.....	174
2-Methyl-1-pentanol.....	186, 193, 195, 197
2-Methyl-3-pentanol.....	193, 195, 197
4-Methyl-2-pentanol.....	186
4-Methyl-2-pentanone.....	189
4-Methyl-3-penten-2-one.....	189
2-Methylphenol.....	158, 159
3-Methylphenol.....	159
4-Methylphenol.....	159
2-Methyl propanal.....	189
2-Methyl-1-propanol.....	187
2-Methyl-2-propanol (<i>tert</i> -Butylalcohol).....	186
Methyl propionate.....	190
α -Methylstyrene.....	174
Methyl sulfide.....	176
17 α -Methyltestosterone.....	210
2-Methylthiophene.....	176
3-Methylthiophene.....	176
4-Methylthiophene.....	154
Methyltrichlorosilane.....	191
Methyl valerate.....	190
Methypyrion.....	209
Mevinphos.....	162
Monobutyltin.....	165, 167
Monocrotophos.....	162
Monoethanolamine.....	94, 184
Monopropylene glycol.....	174
Morphine.....	93, 208
Morpholine.....	185
Myrcene.....	203, 205
N	
Naled.....	162
Naphthalene.....	69, 87, 99, 155, 156, 157, 159, 179, 180, 182
Naphthalene- <i>d</i> 8.....	159
1,4-Naphthoquinone.....	159
Neral.....	203
Nerol.....	205
Neryl acetate.....	203, 205
Nicotine.....	93, 185, 209
2-Nitroaniline.....	93, 159, 185
3-Nitroaniline.....	159
4-Nitroaniline.....	159
Nitrobenzene.....	158, 159, 182
Nitrobenzene- <i>d</i> 5.....	159
3-Nitrobiphenyl.....	167
Nitroethane.....	193, 195, 197
Nitrogen.....	168, 169
Nitromethane.....	192, 211
2-Nitrophenol.....	93, 158, 159, 161, 185
4-Nitrophenol.....	158, 159, 161
1-Nitropropane.....	193, 195, 197
2-Nitropropane.....	193, 195, 197
4-Nitroquinoline-1-oxide.....	159
<i>N</i> -Nitrosoazetidine.....	161
<i>N</i> -Nitrosodibutylamine.....	185
<i>N</i> -Nitrosodiethylamine.....	161, 185
<i>N</i> -Nitrosodisopropylamine.....	185
<i>N</i> -Nitrosodimethylamine.....	159, 161, 185
<i>N</i> -Nitrosodipropylamine.....	185
<i>N</i> -Nitrosohexamethyleneimine.....	161

Compound Index for GC

N-Nitrosomethylethylamine.....	161	Phenylephrine.....	209	1,4,7,8-TCDD.....	155
N-Nitrosomorpholine.....	161, 185	2-Phenylethanol (Phenylethyl alcohol).....	174, 204	2,3,7,8-TCDD.....	155
N-Nitrosopiperidine.....	161, 185	Phenylethylamine.....	209	Temazepam.....	208
N-Nitroso- <i>di-n</i> -propylamine.....	159	2-Phenyl-2-propanol.....	174	TEPP.....	162
N-Nitrosopyrrolidine.....	161, 185	Phenylpropanolamine.....	209, 210	Terbacil.....	163
2-Nitrotoluene.....	167	Phenyltoloxamine.....	208, 210	Terbufos.....	158, 162
3-Nitrotoluene.....	167	Phorate.....	162	Terbutryne.....	165
4-Nitrotoluene.....	167	Phosmet.....	162	Terbutylazine.....	165
Nonadecane.....	182, 188, 189, 190, 193, 195, 197	Phosphamidon.....	162	<i>p</i> -Terphenyl-d14.....	159
Nonanal.....	188, 189, 193, 195, 197, 203	Phosphamidon isomer.....	162	α -Terpinene.....	203, 205
Nonane.....	193, 195, 197	Picloram methyl ester.....	165	γ -Terpinene.....	203, 205
<i>n</i> -Nonane.....	87, 179	β -Pinene.....	203, 205	Terpinene-4-ol.....	203, 205
1-Nonanol.....	186, 193, 195, 197	α -Pinene.....	203, 205	α -Terpineol.....	203, 205
5-Nonanone.....	193, 195, 197	Piperazine.....	184	Terpinolene.....	203, 205
Nootketone.....	203	Piperitone.....	205	Testosterone.....	210
19-Nortestosterone.....	210	PMA.....	209	Testosterone-17 β -cypionate.....	210
19-Nortestosterone-17-propionate.....	210	PMMA.....	209	Testosterone propionate.....	210
O		Prazepam.....	208	Tetrabutyltin.....	165, 167
<i>cis</i> -Ocimene.....	205	Primidone.....	209	Tracacaine.....	208
Octadecane.....	193, 195, 197	Prometon.....	158, 165	1,2,4,5-Tetrachlorobenzene.....	159
<i>n</i> -Octadecyl alcohol.....	185	Prometryne.....	165	1,1,1,2-Tetrachloroethane.....	97, 155, 166
<i>n</i> -Octadecyl- <i>N,N</i> -dimethylamine.....	185	Propachlor.....	163	1,1,2,2-Tetrachloroethane.....	97, 154, 155, 166
Octanal.....	188, 189, 203	Propadiene.....	82, 170, 171, 172, 173	<i>sec</i> -Tetrachloroethane.....	193, 195, 197
<i>n</i> -Octane.....	87, 179	Propanal.....	188, 189, 204	Tetrachloroethene.....	154
Octanoic acid.....	204	Propane.....	82, 83, 87, 169, 170, 171, 172, 173, 179	Tetrachloroethylene.....	97, 155, 166
Octanol.....	203	1-Propanol (<i>n</i> -Propanol).....	175, 186, 187, 192	Tetrachloromethane.....	97, 155, 166
1-Octanol (<i>n</i> -Octyl alcohol).....	185, 186, 189	2-Propanol.....	186, 192	2,3,4,5-Tetrachlorophenol.....	158
3-Octanol.....	188, 205	Propazine.....	163, 165	2,3,4,6-Tetrachlorophenol.....	159
2-Octanone.....	193, 195, 197	Propene.....	171	2,4,5,6-Tetrachloro- <i>m</i> -xylene.....	164
1-Octen-3-ol.....	205	Propionic acid.....	200, 204	Tetradecane.....	186, 189
Octylamine.....	93, 185	<i>n</i> -Propyl acetate.....	199	<i>n</i> -Tetradecyl alcohol.....	185
<i>n</i> -Octyl chloride.....	185	<i>n</i> -Propylamine.....	95, 183	<i>n</i> -Tetradecyl chloride.....	185
<i>n</i> -Octyl- <i>N,N</i> -dimethylamine.....	185	Propylbenzene.....	155, 182, 206	<i>n</i> -Tetradecyl- <i>N,N</i> -dimethylamine.....	185
Octylic acid.....	204	<i>n</i> -Propylbenzene.....	180, 181	Tetraethylene glycol.....	187, 193, 195, 197
<i>di-n</i> -Octyl phthalate.....	159	Propylene.....	82, 169, 170, 171, 172, 173	1,1,1,2-Tetrafluoroethane (CFC-134a).....	86, 170
Ordram.....	163	Propylene glycol.....	187	Tetrahydrofuran.....	192, 199, 206, 211, 212
Oxadiazon.....	163	1,2-Propylene glycol.....	187	Tetrahydrofurfuryl acetate.....	193, 195, 197
Oxygen.....	84, 168, 169	1,3-Propylene glycol.....	187	Tetrahydro-2-methyl furan.....	190
Oxymethalone.....	210	Propyl hexanoate.....	204	1,2,3,4-Tetrahydronaphthalene.....	192, 211
P		1-Propylmercaptan.....	176	1,2,3,5-Tetramethylbenzene.....	180
Paarlan.....	163	2-Propylmercaptan.....	176	1,2,4,5-Tetramethylbenzene.....	180
Papaverine.....	208	Propyne.....	171, 172, 173	Tetrapropyltin.....	165, 167
Parathion-ethyl.....	162	Prowl.....	163	Thionazin.....	162
Parathion-methyl.....	162	Pseudoephedrine.....	209, 210	Thiophene.....	176
PCNB.....	162	Pulegone.....	205	Thioridazine.....	208
PCNB (IS).....	162	Pyrene.....	69, 156, 157, 159	α -Thujene.....	203
Pentachlorobenzene.....	159	Pyridine.....	93, 159, 185, 192, 211, 212	Thymol.....	206
Pentachloronitrobenzene.....	159	Pyrimamine.....	208, 210	Tillam.....	163
Pentachlorophenol.....	158, 159, 161, 165	R		2,4,5-T methyl ester.....	165
Pentadecane.....	182, 188, 190, 193, 195, 197	Rhamnitol.....	207	Tokuthion.....	162
Pentamethylbenzene.....	180	Ribitol.....	207	Tolban.....	163
Pentamethylenediamine.....	184	Ro-Neet.....	163	Toluene.....	87, 97, 98, 154, 155, 166, 174, 179, 180, 181, 182, 191, 192, 193, 195, 197, 199, 206, 211, 212
Pentanal.....	188, 189, 193, 195, 197	Ronnel.....	162	Total heavy hydrocarbons.....	175
Pentane.....	186, 188, 189, 190, 192, 193, 195, 197	S		2,4,5-TP.....	165
<i>iso</i> -Pentane.....	87, 179	Sabinene.....	203, 205	2,4,5-TP (silvex) methyl ester.....	165
<i>n</i> -Pentane.....	82, 87, 170, 171, 172, 173, 179, 199	<i>trans</i> -Sabinenehydrate.....	205	Trazodone.....	208
1-Pentanol (<i>n</i> -Pentanol).....	186, 189, 192, 204	Safrole.....	159	Treflan.....	163
3-Pentanol.....	187, 188, 193, 195, 197	Scopolamine.....	208	Triazolam.....	208
<i>sec</i> -Pentanol.....	204	Secbumeton.....	165	2,4,6-Tribromophenol.....	158, 159
2-Pentanone.....	204	Secobarbital.....	209	Tributyl phosphate.....	162, 193, 195, 197
1-Pentene.....	82, 170	Sencor.....	163	Tributyltin.....	165, 167
<i>cis</i> -2-Pentene.....	82, 170	Simazine.....	163, 165	1,1,2-Trichlorethene.....	211
<i>trans</i> -2-Pentene.....	82, 170	Simetryne.....	165	Trichlorfon.....	162
1-Penten-3-ol.....	186, 188	β -Sitosterol.....	207	Trichloroacetone nitrile.....	166
Pentobarbital.....	209	Solvent.....	185	1,2,3-Trichlorobenzene.....	97, 155, 166
<i>cis</i> -Permethrin.....	162	Stigmasterol.....	207	1,2,4-Trichlorobenzene.....	97, 154, 155, 159, 160, 166
<i>trans</i> -Permethrin.....	162	Stirofos.....	162	1,1,1-Trichloroethane.....	97, 154, 155, 166, 192, 211
Perylene-d12.....	159	Styrene.....	154, 174, 182, 191, 206	1,1,2-Trichloroethane.....	97, 154, 155, 166, 192
α -Phellandrene.....	203	Styrol.....	155	Trichloroethylene.....	97, 154, 155, 166, 192, 211, 212
Phenacetin.....	159	Sulfolane.....	192	Trichloroethane.....	97, 154, 155, 166
Phenanthrene.....	69, 99, 156, 157, 159	Sulfotepp.....	162	Trichlorofluoromethane.....	97, 154, 155, 166
Phenanthrene-d10.....	158, 159	Sulfur dioxide.....	176	Trichloronate.....	162
Phendimetrazine.....	209	Sutan.....	163	2,4,5-Trichlorophenol.....	159
β -Phenethyl alcohol.....	204	T		2,4,6-Trichlorophenol.....	158, 159, 161
Pheniramine.....	210	2,4,5-T.....	165	1,2,3-Trichloropropane.....	97, 155, 166, 193, 195, 197
Phenmetrazine.....	209	TAME.....	175	1,1,1-Trichloro-2-propanone.....	166
Phenobarbital.....	209	1,2,3,4-TCDD.....	155	1,1,2-Trichloro-1,2,2-trifluoroethane.....	154
Phenol.....	93, 158, 159, 161, 174, 185	1,2,3,7-TCDD.....	155	Tridecane.....	193, 195, 197
Phenol-d6.....	159	1,2,3,8-TCDD.....	155	<i>n</i> -Tridecane.....	87, 88, 174, 179
Phenothiazine.....	208	1,2,6,7-TCDD.....	155	Triethanolamine.....	94, 184
2-Phenoxyethanol.....	193, 195, 197	1,2,7,8-TCDD.....	155	Triethylamine.....	92, 96, 183, 212
Phentermine.....	209	1,3,7,8-TCDD.....	155	Triethylbenzene.....	182
Phenylacetylene.....	174			Triethylene glycol.....	193, 195, 197

Triethylene glycol monomethylether.....	94, 184
2,2,2-Trifluoroethanol.....	186
Trifluralin.....	162
Triisobutylene.....	175
Trimethylamine.....	92, 95, 183
1,2,3-Trimethylbenzene.....	180, 182
1,2,4-Trimethylbenzene.....	87, 154, 155, 179, 180, 182, 193, 195, 197
1,3,5-Trimethylbenzene.....	87, 154, 155, 179, 180, 182
Trimethylchlorosilane.....	191
Trimipramine.....	208
2,3,4-Trinitrotoluene.....	167
2,4,5-Trinitrotoluene.....	167
2,4,6-Trinitrotoluene.....	167
Tripelennamine.....	208
Triptylitin.....	165, 167
Triphenylene.....	99, 156
Triphenyl phosphate.....	158, 162
Triprolidine.....	210
U	
Undecanal.....	188, 193, 195, 197
Undecane.....	98, 154, 186, 189, 193, 195, 197
<i>n</i> -Undecane.....	87, 88, 174, 179, 181
1-Undecanol.....	186, 193, 195, 197
V	
Valencene.....	203
<i>n</i> -Valeramide.....	184
Valeric acid.....	204
<i>n</i> -Valeric acid.....	200
Vanillin.....	204, 206
Vernam.....	163
Vinyl benzene.....	98, 154
Vinyl chloride.....	154, 155
Vinylcyclohexene.....	191
4-Vinyl cyclohexene-1.....	175
Viridiflorol.....	205
W, X	
Water.....	189, 192
<i>m</i> -Xylene.....	87, 97, 98, 154, 155, 166, 174, 179, 180, 181, 191, 192, 211
<i>o</i> -Xylene.....	87, 97, 98, 154, 155, 166, 174, 179, 180, 181, 182, 191, 192, 211
<i>p</i> -Xylene.....	87, 97, 98, 154, 155, 166, 174, 179, 180, 181, 182, 192, 193, 195, 197, 211
Xylitol.....	207

SPE

B	
BBP.....	230
Benzopyrene.....	224
Bisphenol A.....	232
C	
Carbendazim.....	227
4-Chloro-3-methylphenol.....	229
2-Chlorophenol.....	229
Chlortetracycline.....	225, 228, 231
D	
DBP.....	230
DCHP.....	230
DEHP.....	230
DEP.....	230
DHP.....	230
2,4-Dichlorophenol.....	229
2,4-Dimethylphenol.....	229
2,4-Dinitrophenol.....	229
DMP.....	230
Doxycycline.....	225, 228
DPP.....	230
DPrP.....	230
M, N	
Melamine.....	217
2-Nitrophenol.....	229
4-Nitrophenol.....	229
O, P	
Oxytetracycline.....	225, 228, 231
Pentachlorophenol.....	229
Phenol.....	229
S	
Sulfadimidine.....	219, 221
Sulfamerazine.....	219, 221
Sulfamethoxazole.....	219, 221
Sulfamethoxyipyridazine.....	219, 221
Sulfapyridine.....	219, 221
Sulfaquinoxaline.....	219, 221
Sulfisoxazole.....	219, 221
Sulphadimethoxine.....	219, 221
T	
Tetracycline.....	225, 228, 231
2,4,6-Trichlorophenol.....	229

Product Index

G

GC Columns

DikmaCap™ DM	
DM-1	67
DM-1HT	70
DM-1HT SimDist Metal	89
DM-1MS	67
DM-1 SimDist Metal	89
DM-5	68
DM-5Amine	93
DM-5HT	70
DM-5MS	68
DM-5MS / LB	69
DM-17	73
DM-17MS	73
DM-35	71
DM-35 Amine	94
DM-35MS	71
DM-200	74
DM-200MS	74
DM-225	75
DM-500 SimDist Metal	89
DM-624	96
DM-624MS	96
DM-1701	72
DM-2330	79
DM-2560	80
DM-2887	90
DM-2887 Metal	90
DM-AQUA	97
DM-BDTG Metal	91
DM-FAMEWAX	100
DM-FFAP	78
DM-InterWax	77
DM-PAH	99
DM-PLOT Alumina (Al ₂ O ₃)	81
DM-PLOT Alumina / KCl	83
DM-PLOT Alumina / Na ₂ SO ₄	82
DM-PLOT CFC	86
DM-PLOT MS 5A	84
DM-PLOT Q / QS / S / U	85
DM-PONA	87
DM-TCEP	88
DM-TVOC	98
DM-Volatile Amine	92
DM-Wax	76
DM-Wax Amine	95
Guard Columns	66

H

HPLC Columns

Bio-Bond™	52
Endeavorsil™	5
Inspire™	21
Leapsil™	15
Platisil™	54
Spursil™	31
HPLC Guard Columns	
EasyGuard™	55

P

Preparative Columns

Bio-Bond™	62
Inspire™	61
Luster™	62
Spursil™	61

S

Sample Preparation

Filters	
ProMax™ Syringe Filters	124

SPE Tubes

ProElut™ SPE	
ProElut™ AL-A	117
ProElut™ AL-B	117
ProElut™ AL-N	117
ProElut™ CARB	117
ProElut™ CARB / NH ₂	117
ProElut™ CN	111
ProElut™ C2	110
ProElut™ C8	110
ProElut™ C18	109
ProElut™ C18-U	109
ProElut™ Florisil	117
ProElut™ GLASS	118
ProElut™ LLE+	123
ProElut™ NH ₂	112
ProElut™ PH	111
ProElut™ PLS	115
ProElut™ PSA	112
ProElut™ PWA	116
ProElut™ PWC	116
ProElut™ PXA	115
ProElut™ PXC	115
ProElut™ QuEChERS	119
ProElut™ SAX	113
ProElut™ SCX	113
ProElut™ Silica	111

V

Vials

2 mL Autosampler Vials	
Crimp Top Vials	127
Screw Thread Vials	126
Accessory	
Vials Rack	127



About Dikma

Dikma Technologies Inc., established in 1993, is a global technology leader committed to developing novel separation and purification solutions for life sciences and related industries. Our core technology portfolio includes products for liquid chromatography, gas chromatography, sample preparation, and bulk purification chromatographic media. We also provide related chromatography accessories.

Quality

Dikma Technologies Inc. is an ISO 9001:2000 Standard Quality Assessed Company to ensure the quality and reliability of our products and services. We are dedicated to the highest standards of production, quality assurance and quality control.

Value

Dikma Technologies Inc. is committed to bringing maximum value to its customers.

DIKMA[®]
A reliable partner for your lab

©Dikma Technologies Inc.
Literature No. 3010A

USA

11 Orchard Road, Suite 106
Lake Forest, CA 92630, USA
Tel: 949-716-5810
Fax: 949-716-5811
Toll-Free: 1-877-328-8348
Email: sale@dikmatech.com
www.dikmatech.com

Canada

40 Vogell Road, Unit 57
Richmond Hill, ON L4B 3N6, Canada
Tel: 905-737-8066
Fax: 905-770-0181
Toll-Free: 1-866-889-9072
Email: sales@dimaglass.com
www.dikmatech.com

